
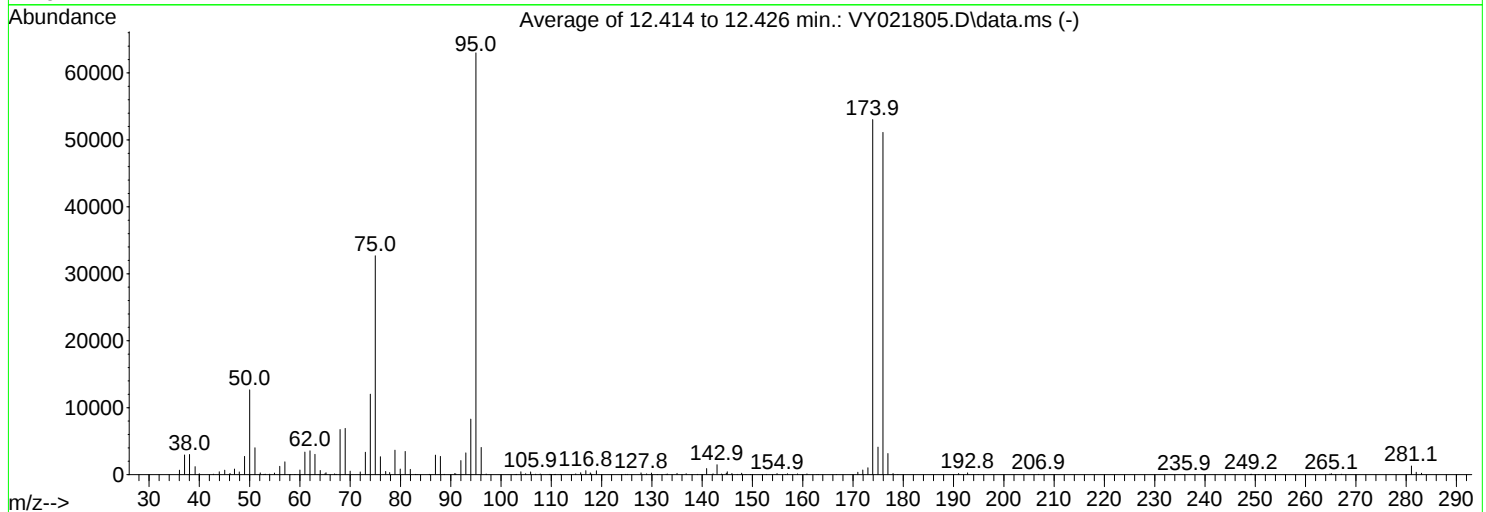


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040925\
Data File : VY021805.D
Acq On : 09 Apr 2025 08:47
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
Title : SW846 8260
Last Update : Fri Mar 28 02:30:29 2025

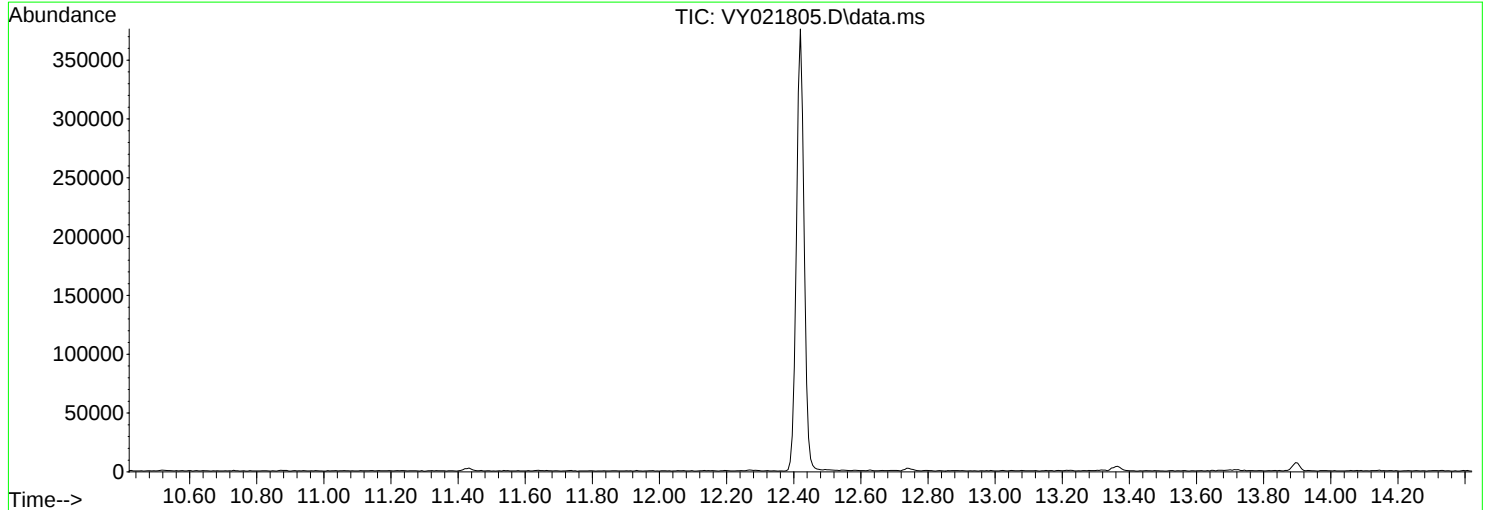

AutoFind: Scans 1754, 1755, 1756; Background Corrected with Scan 1746

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.1	12663	PASS
75	95	30	60	51.9	32693	PASS
95	95	100	100	100.0	63003	PASS
96	95	5	9	6.5	4070	PASS
173	174	0.00	2	2.0	1036	PASS
174	95	50	100	84.2	53040	PASS
175	174	5	9	7.8	4118	PASS
176	174	95	101	96.4	51115	PASS
177	176	5	9	6.2	3161	PASS