
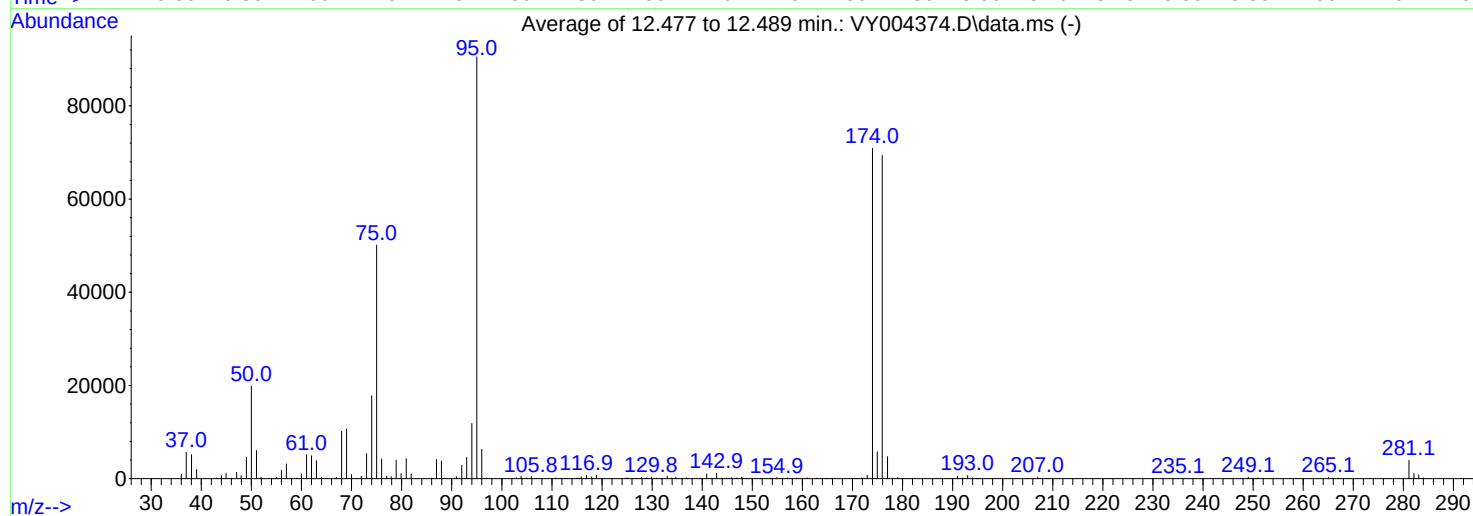


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY041221\  
 Data File : VY004374.D  
 Acq On : 12 Apr 2021 09:42  
 Operator : SY/MD  
 Sample : BFB  
 Misc : 5.00G/5ML/MSVOA\_Y/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y041221S.M  
 Title : SW846 8260  
 Last Update : Tue Apr 13 03:38:02 2021

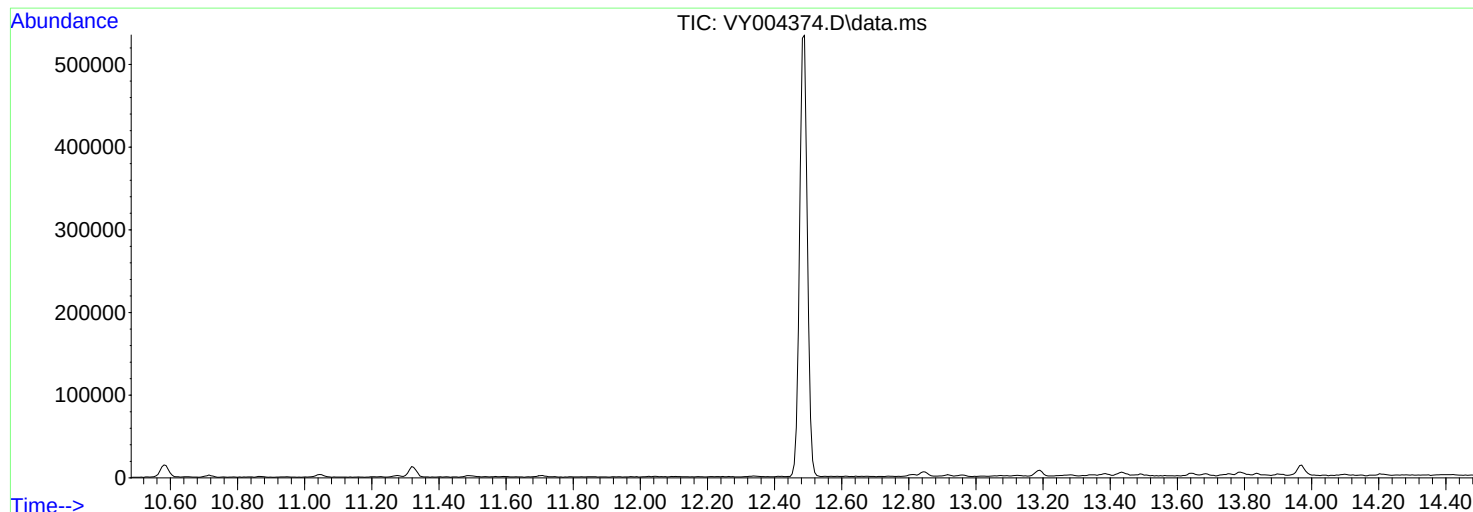

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1741

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 21.9         | 19845      | PASS                |
| 75             | 95              | 30              | 60              | 55.4         | 50115      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 90523      | PASS                |
| 96             | 95              | 5               | 9               | 7.0          | 6318       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.1          | 770        | PASS                |
| 174            | 95              | 50              | 100             | 78.3         | 70896      | PASS                |
| 175            | 174             | 5               | 9               | 8.1          | 5764       | PASS                |
| 176            | 174             | 95              | 101             | 97.8         | 69338      | PASS                |
| 177            | 176             | 5               | 9               | 6.8          | 4710       | PASS                |