
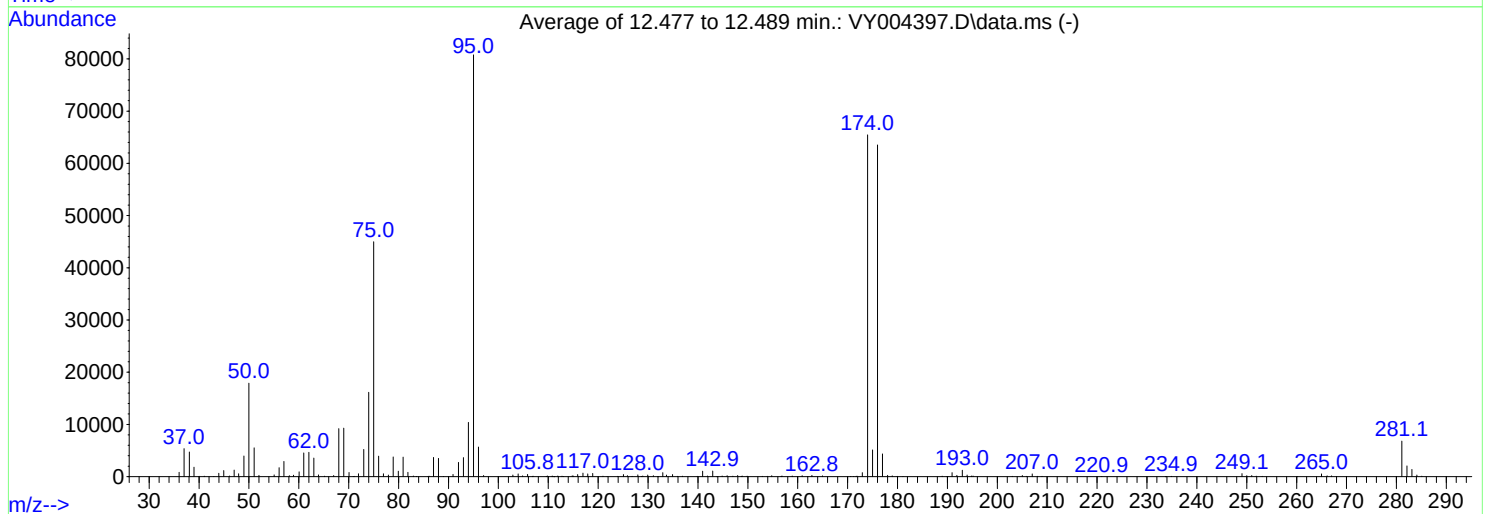


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041321\
Data File : VY004397.D
Acq On : 13 Apr 2021 09:06
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041221S.M
Title : SW846 8260
Last Update : Tue Apr 13 03:38:02 2021

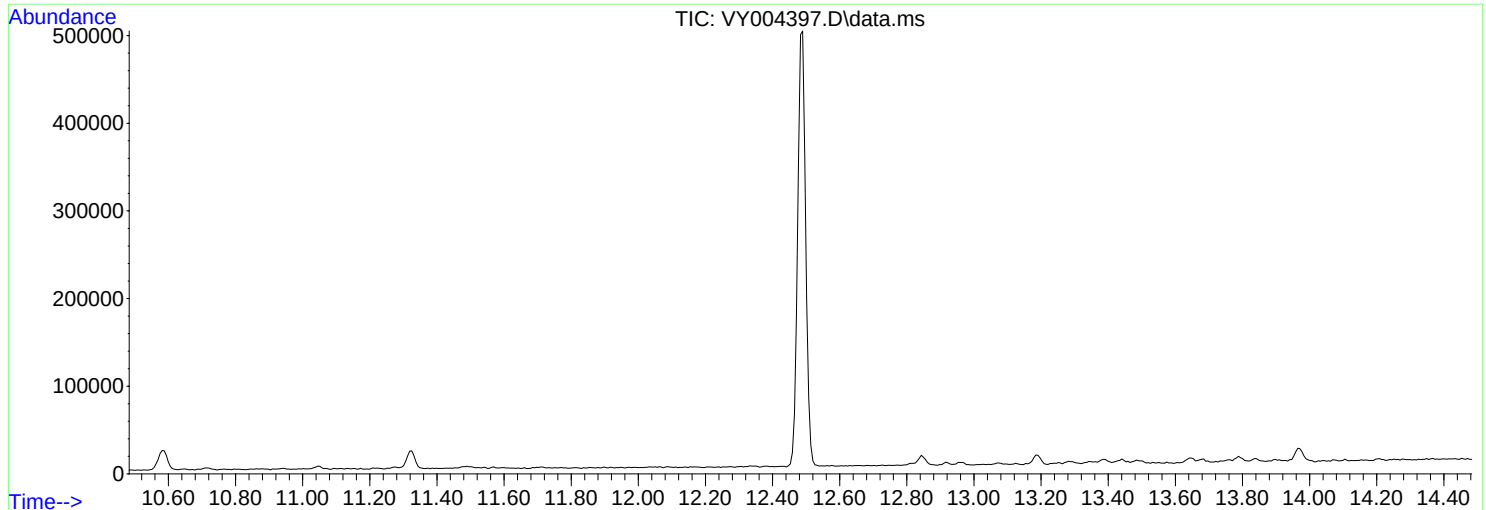

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	17889	PASS
75	95	30	60	55.7	44983	PASS
95	95	100	100	100.0	80781	PASS
96	95	5	9	7.0	5679	PASS
173	174	0.00	2	1.2	774	PASS
174	95	50	100	81.0	65440	PASS
175	174	5	9	7.8	5114	PASS
176	174	95	101	97.1	63520	PASS
177	176	5	9	6.9	4357	PASS