

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041323\
 Data File : VY013287.D
 Acq On : 13 Apr 2023 11:45
 Operator : KP/MD
 Sample : 02283-09
 Misc : 4.91g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 20230235-11-1

Quant Time: Apr 14 02:58:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041223S.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 13 05:55:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.783	168	173315	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	289122	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	264881	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	116638	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	123366	59.229	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 118.460%	
35) Dibromofluoromethane	7.710	113	100789	53.847	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 107.700%	
50) Toluene-d8	10.179	98	352831	50.643	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 101.280%	
62) 4-Bromofluorobenzene	12.477	95	103823	45.865	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 91.720%	
Target Compounds						
					Qvalue	
13) Acrolein	3.729	56	2193	8.571	ug/l #	54
16) Acetone	3.954	43	18454	25.769	ug/l	91
17) Carbon Disulfide	4.192	76	52121	9.707	ug/l	99
18) Methyl Acetate	4.485	43	3520	1.520	ug/l #	70
31) Cyclohexane	7.783	56	4854	1.541	ug/l #	42
84) 1,2,4-Trimethylbenzene	13.117	105	8287	1.271	ug/l	95
95) Naphthalene	15.233	128	2193	3.606	ug/l #	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041323\
Data File : VY013287.D
Acq On : 13 Apr 2023 11:45
Operator : KP/MD
Sample : 02283-09
Misc : 4.91g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
20230235-11-1

Quant Time: Apr 14 02:58:42 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041223S.M
Quant Title : SW846 8260
QLast Update : Thu Apr 13 05:55:16 2023
Response via : Initial Calibration




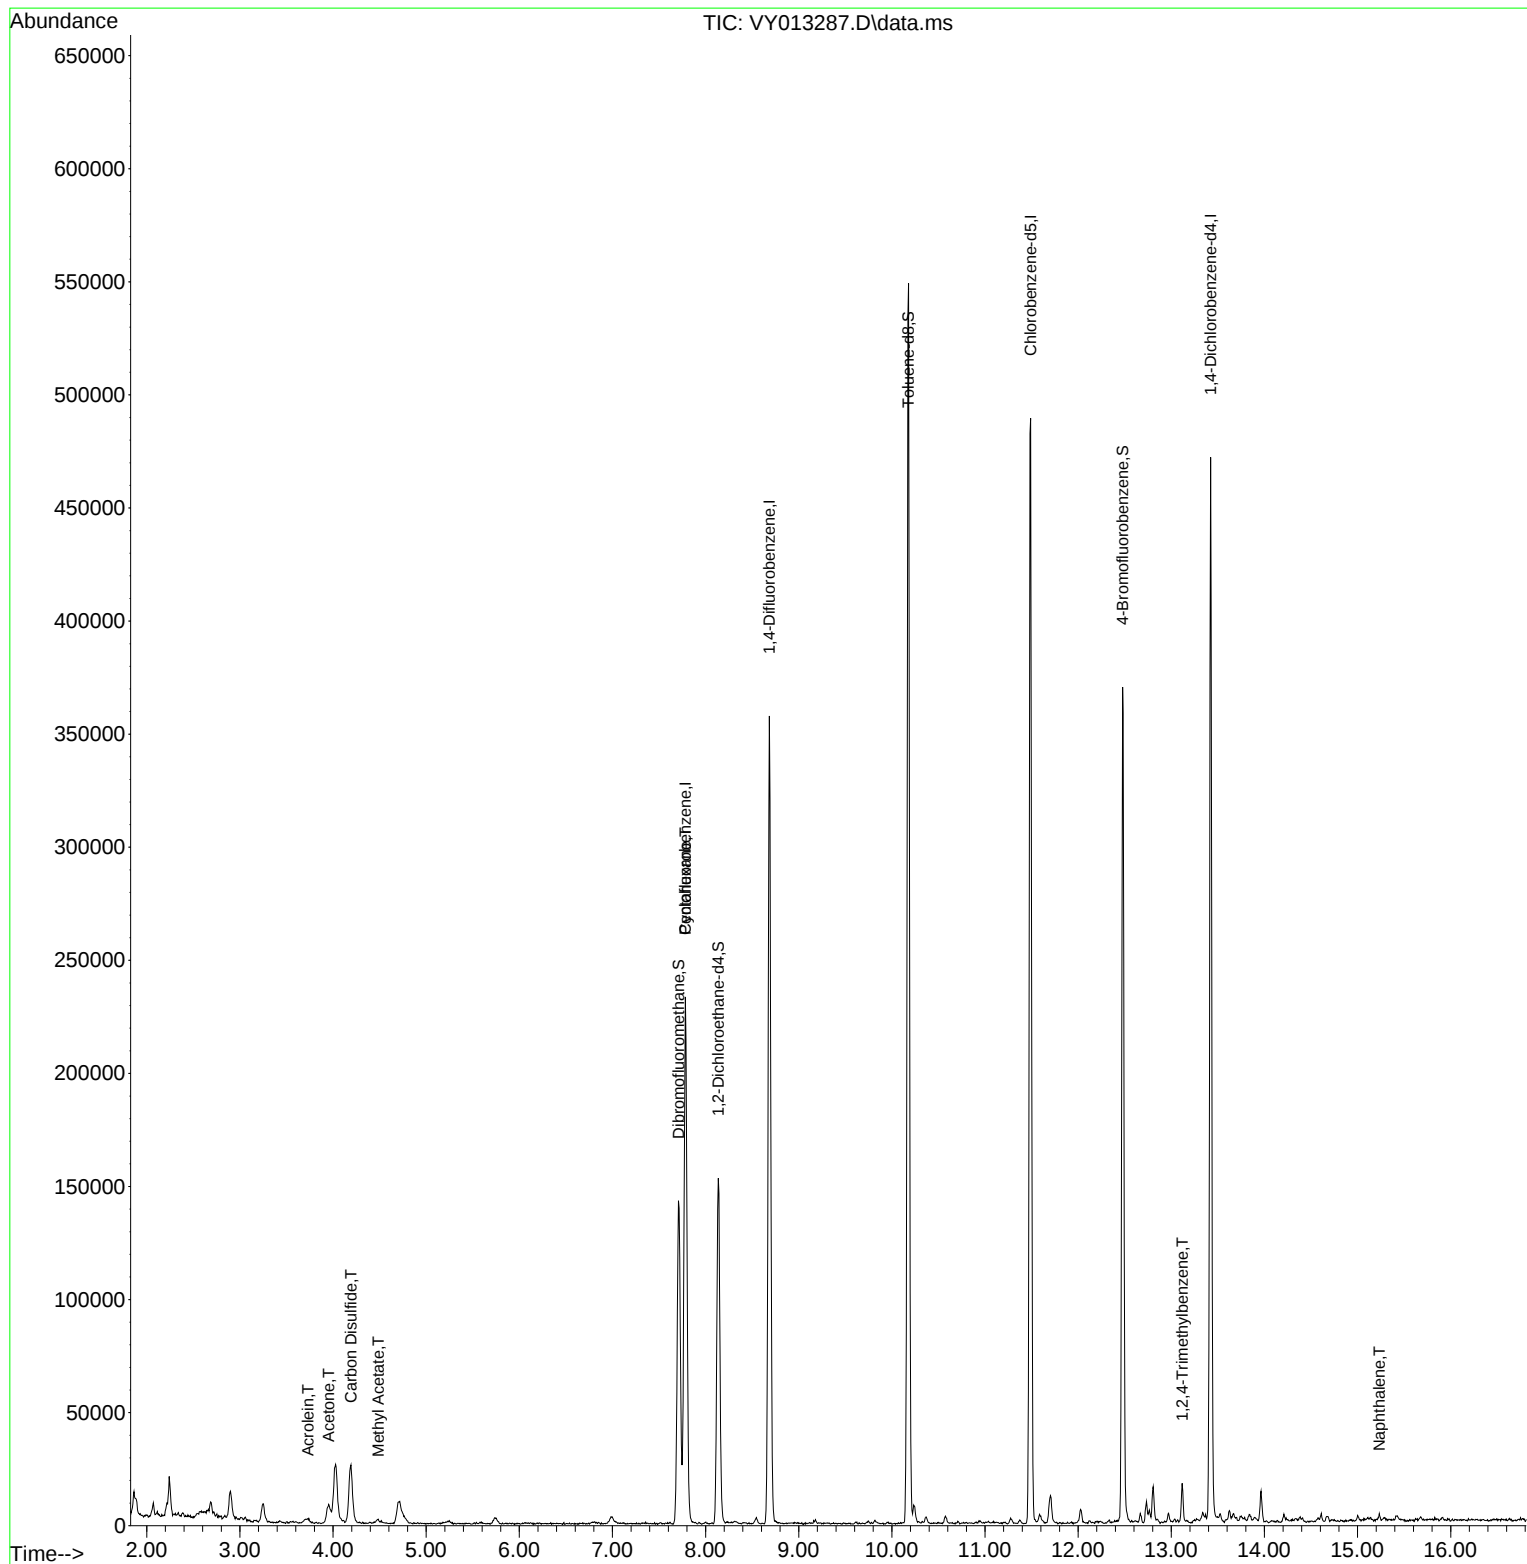




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY013287.D
Acq: 13 Apr 2023 11:45




Instrument :
MSVOA_Y
ClientSampleId :
20230235-11-1


Tgt Ion:168 Resp: 173315
Ion Ratio Lower Upper
168 100
99 52.8 41.7 62.5

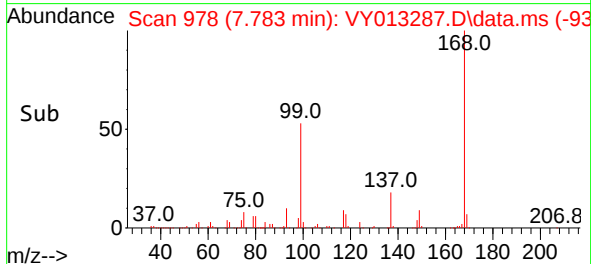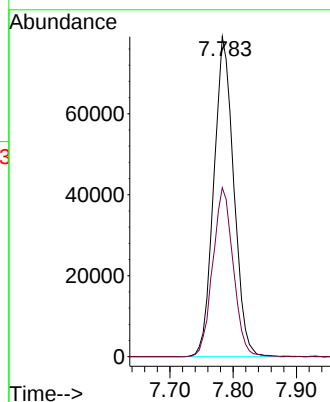

#13
Acrolein
Concen: 8.571 ug/l
RT: 3.729 min Scan# 313
Delta R.T. -0.000 min
Lab File: VY013287.D
Acq: 13 Apr 2023 11:45

Tgt Ion: 56 Resp: 2193
Ion Ratio Lower Upper
56 100
55 109.1 56.8 85.2#


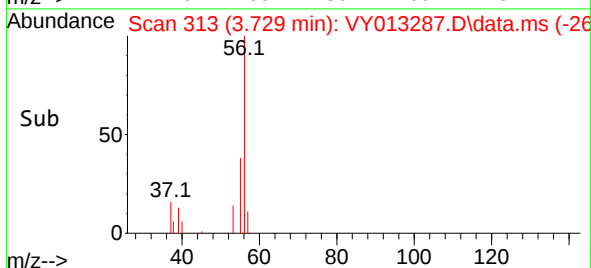
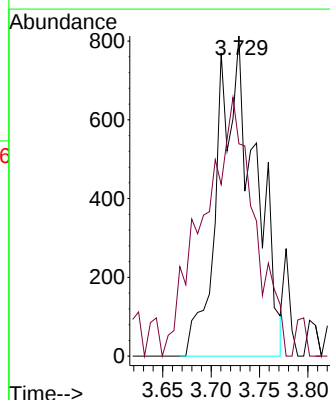
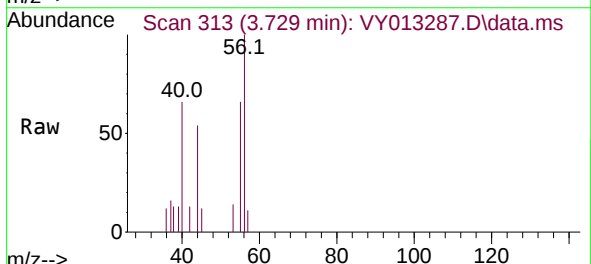




#16
Acetone
Concen: 25.769 ug/l
RT: 3.954 min Scan# 31
Delta R.T. 0.006 min
Lab File: VY013287.D
Acq: 13 Apr 2023 11:45




Instrument :
MSVOA_Y
ClientSampleId :
20230235-11-1


Tgt Ion: 43 Resp: 18454
Ion Ratio Lower Upper
43 100
58 25.2 24.2 36.2

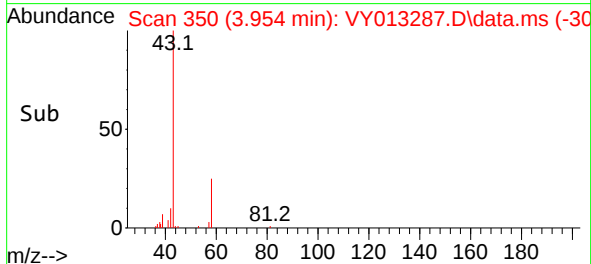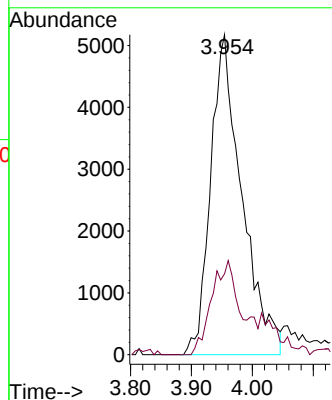

#17
Carbon Disulfide
Concen: 9.707 ug/l
RT: 4.192 min Scan# 389
Delta R.T. -0.000 min
Lab File: VY013287.D
Acq: 13 Apr 2023 11:45

Tgt Ion: 76 Resp: 52121
Ion Ratio Lower Upper
76 100
78 8.6 7.1 10.7


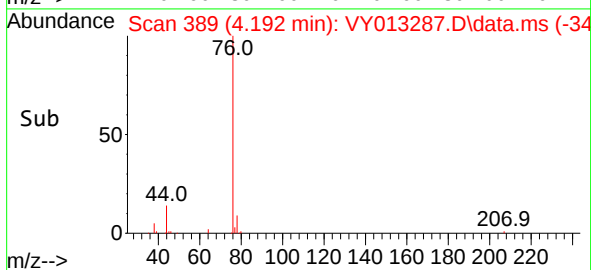
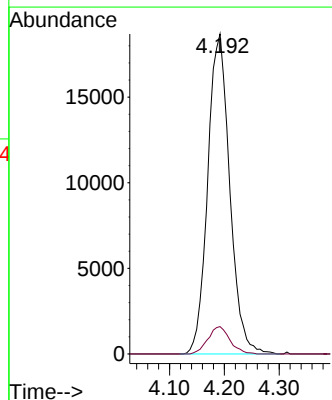
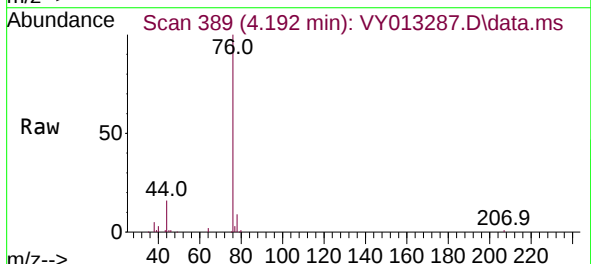




#18
Methyl Acetate
Concen: 1.520 ug/l
RT: 4.485 min Scan# 41
Delta R.T. 0.012 min
Lab File: VY013287.D
Acq: 13 Apr 2023 11:45




Instrument :
MSVOA_Y
ClientSampleId :
20230235-11-1


Tgt Ion: 43 Resp: 3520
Ion Ratio Lower Upper
43 100
74 7.6 17.4 26.0#

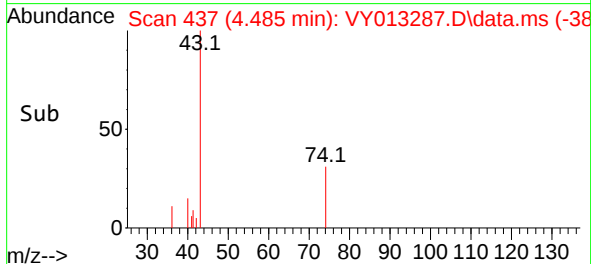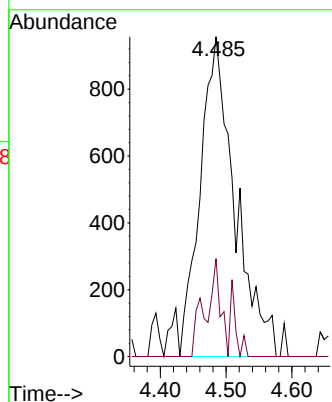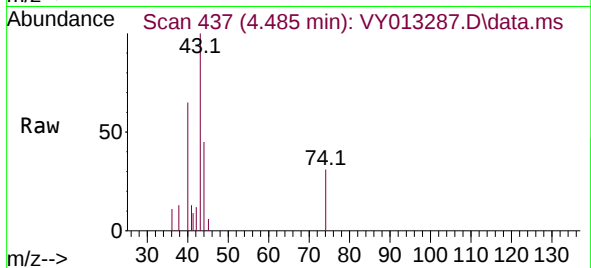

#31
Cyclohexane
Concen: 1.541 ug/l
RT: 7.783 min Scan# 978
Delta R.T. -0.000 min
Lab File: VY013287.D
Acq: 13 Apr 2023 11:45

Tgt Ion: 56 Resp: 4854
Ion Ratio Lower Upper
56 100
69 124.4 25.7 38.5#
84 93.8 64.3 96.5

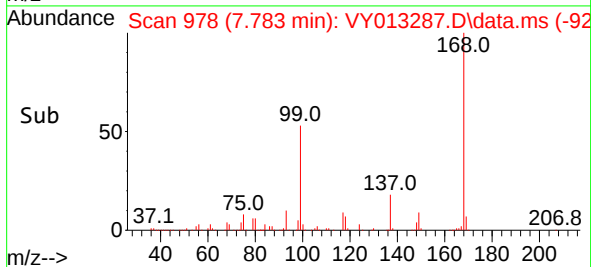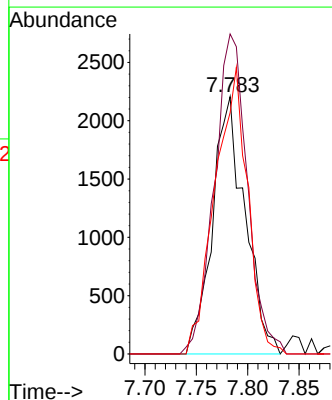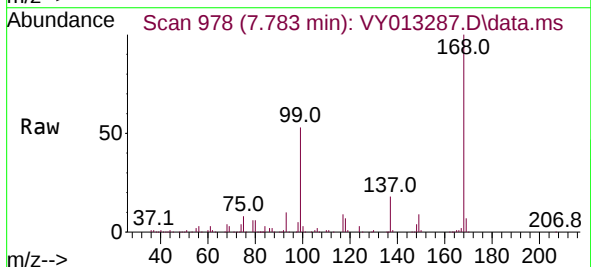



#33

1,2-Dichloroethane-d4

Concen: 59.229 ug/l

RT: 8.136 min Scan# 1036

Delta R.T. -0.000 min

Lab File: VY013287.D

Acq: 13 Apr 2023 11:45

Instrument :

MSVOA_Y

ClientSampleId :





20230235-11-1

Tgt Ion: 65 Resp: 123366

Ion Ratio Lower Upper

65 100

67 52.1 0.0 104.0

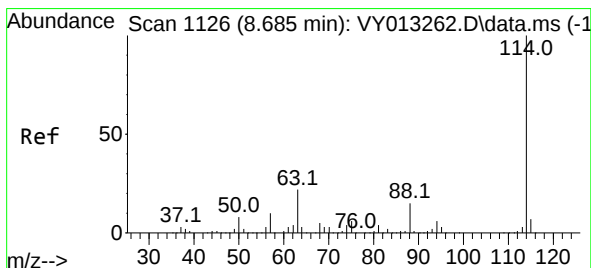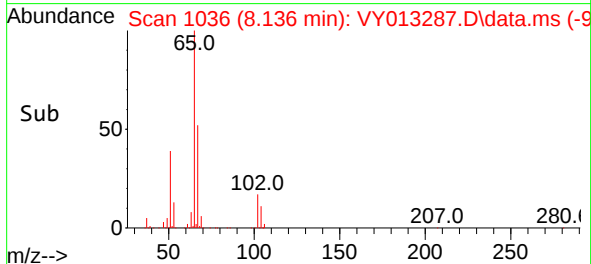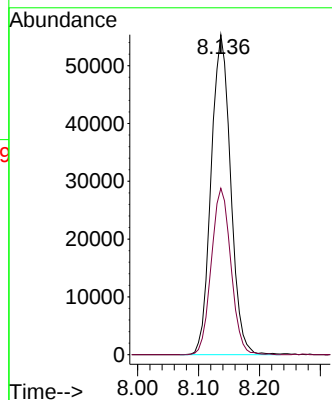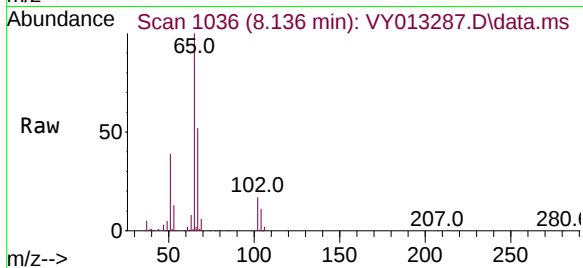

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.000 min

Lab File: VY013287.D

Acq: 13 Apr 2023 11:45




Tgt Ion: 114 Resp: 289122


Ion Ratio Lower Upper

114 100

63 21.7 0.0 37.4


88 15.7 0.0 28.6

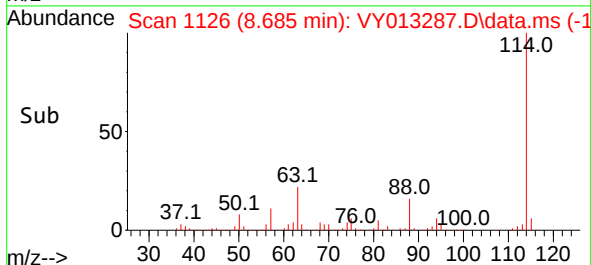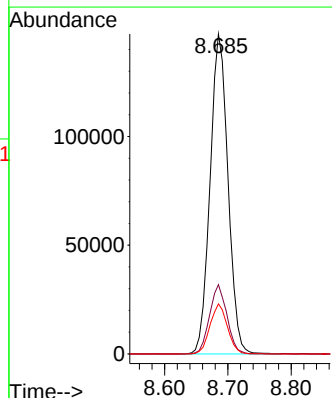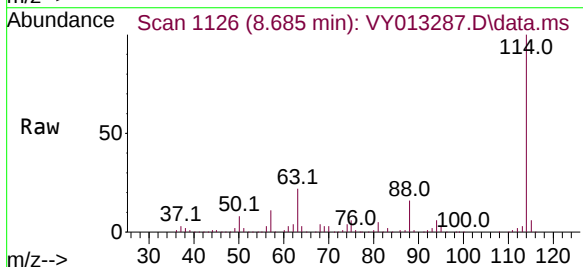






#35
Dibromofluoromethane
Concen: 53.847 ug/l
RT: 7.710 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY013287.D
Acq: 13 Apr 2023 11:45

Instrument :
MSVOA_Y
ClientSampleId :
20230235-11-1



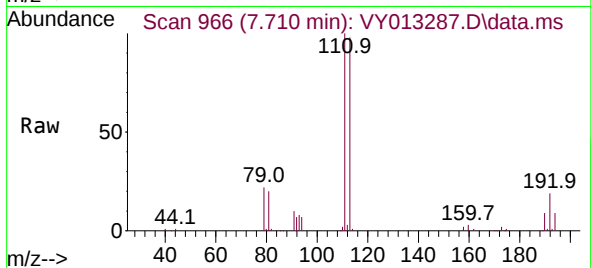



Tgt Ion:113 Resp: 100789
Ion Ratio Lower Upper
113 100
111 102.4 82.2 123.2
192 19.6 16.8 25.2

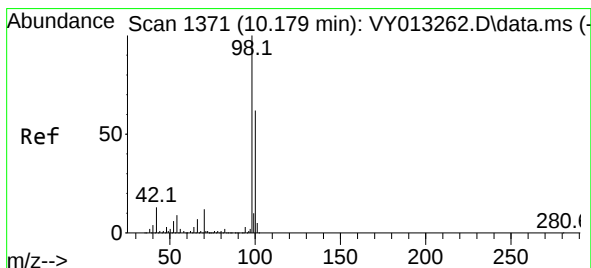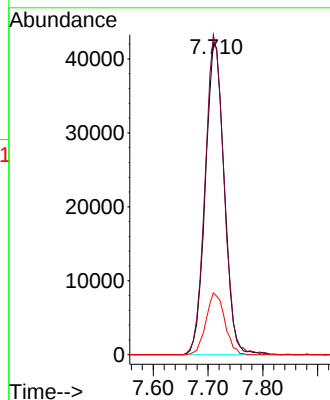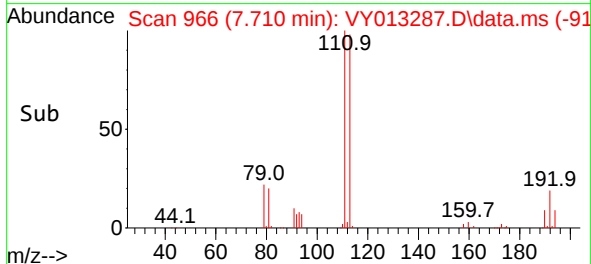

#50
Toluene-d8
Concen: 50.643 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY013287.D
Acq: 13 Apr 2023 11:45

Tgt Ion: 98 Resp: 352831
Ion Ratio Lower Upper
98 100
100 63.0 50.9 76.3


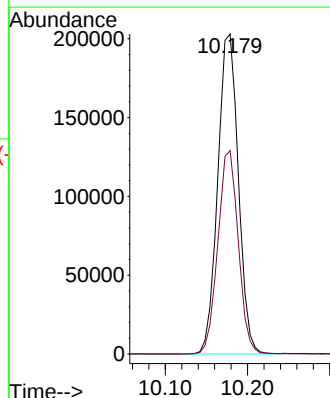
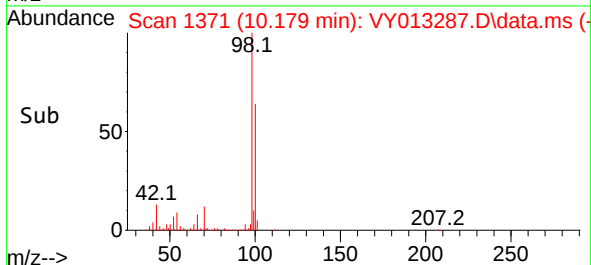
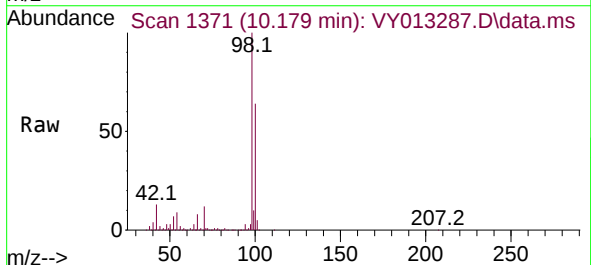


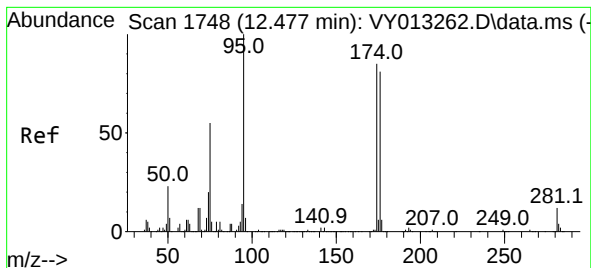

#62
4-Bromofluorobenzene
Concen: 45.865 ug/l
RT: 12.477 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY013287.D
Acq: 13 Apr 2023 11:45




Instrument :
MSVOA_Y
ClientSampleId :
20230235-11-1


Tgt Ion: 95 Resp: 103823
Ion Ratio Lower Upper
95 100
174 89.4 0.0 176.6
176 85.8 0.0 170.2

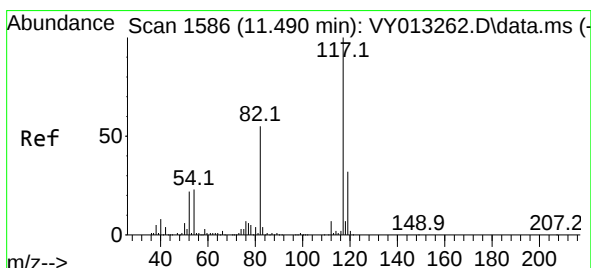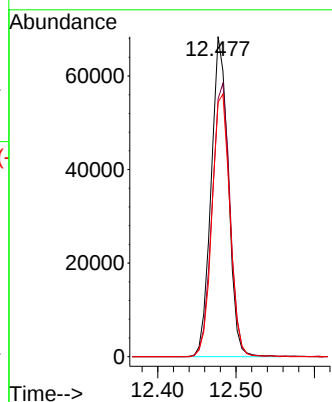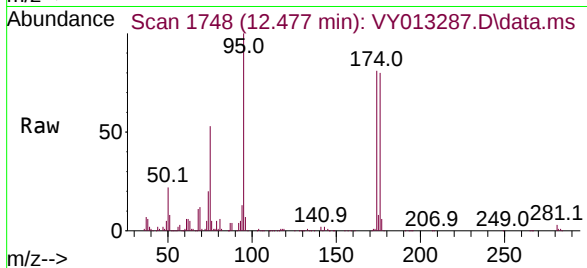

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 1586
Delta R.T. -0.000 min
Lab File: VY013287.D
Acq: 13 Apr 2023 11:45

Tgt Ion: 117 Resp: 264881
Ion Ratio Lower Upper
117 100
82 55.6 45.4 68.0
119 31.7 25.6 38.4


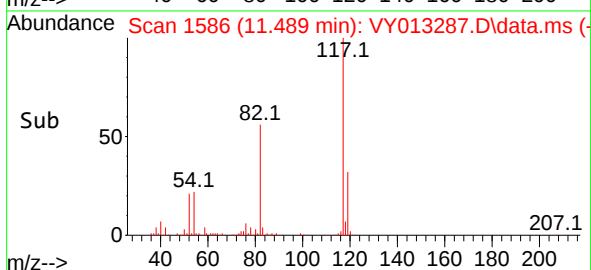
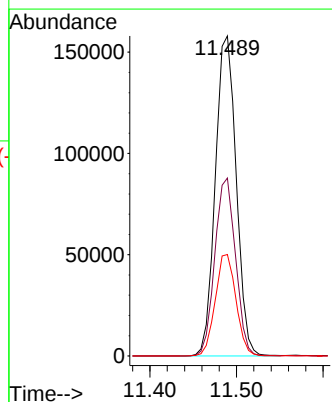
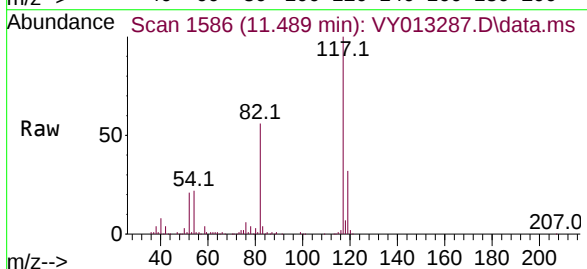


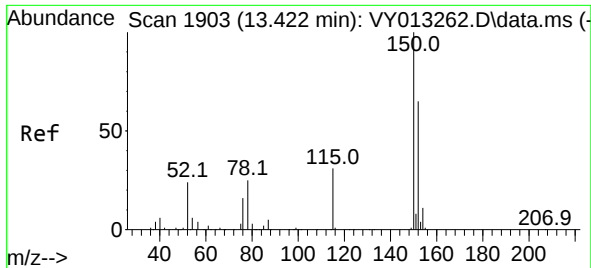

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.422 min Scan# 1903
 Delta R.T. -0.000 min
 Lab File: VY013287.D
 Acq: 13 Apr 2023 11:45




Instrument :
 MSVOA_Y
 ClientSampleId :
 20230235-11-1


Tgt Ion:152 Resp: 116638
 Ion Ratio Lower Upper
 152 100
 115 55.4 27.1 81.3
 150 155.8 0.0 347.8

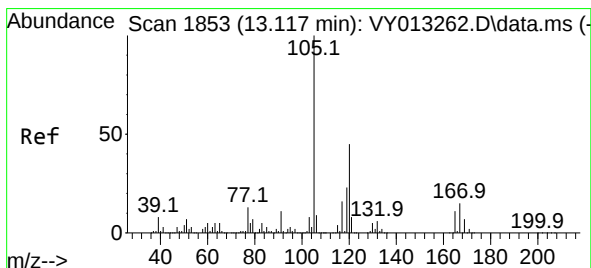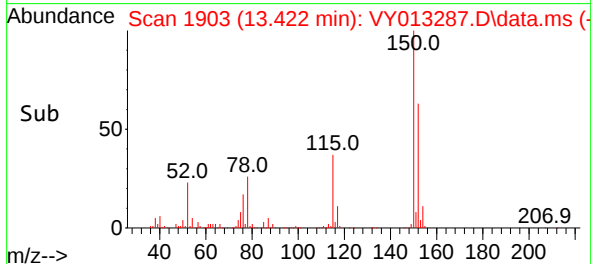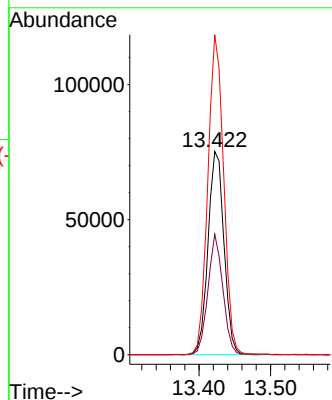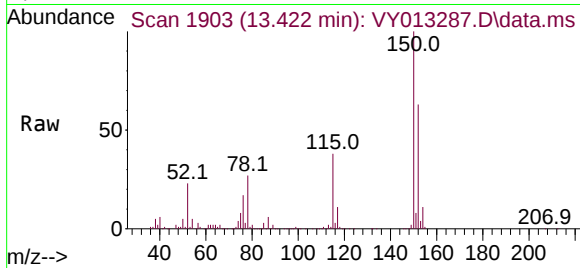

#84
 1,2,4-Trimethylbenzene
 Concen: 1.271 ug/l
 RT: 13.117 min Scan# 1853
 Delta R.T. -0.000 min
 Lab File: VY013287.D
 Acq: 13 Apr 2023 11:45


Tgt Ion:105 Resp: 8287
 Ion Ratio Lower Upper
 105 100
 120 42.7 23.0 69.0

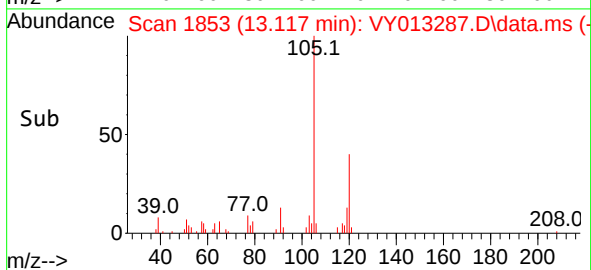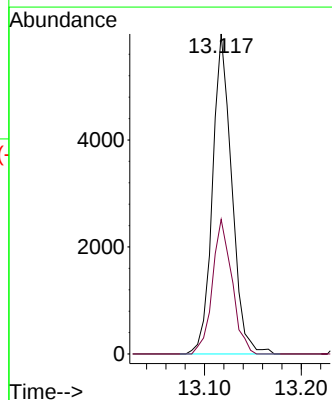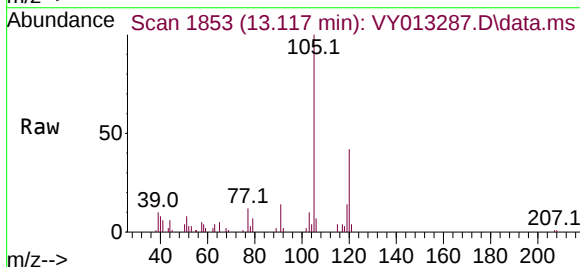

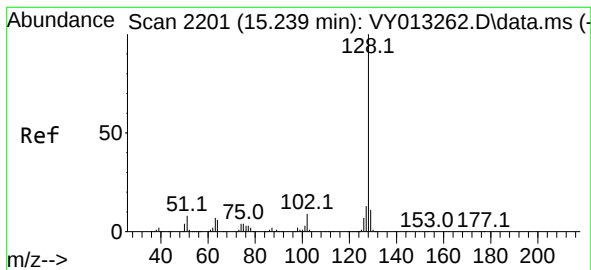

#95
Naphthalene
Concen: 3.606 ug/l
RT: 15.233 min Scan# 21
Delta R.T. -0.006 min
Lab File: VY013287.D
Acq: 13 Apr 2023 11:45

Instrument :
MSVOA_Y
ClientSampleId :
20230235-11-1

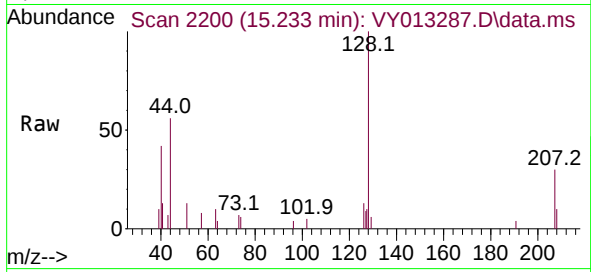

Tgt Ion:128 Resp: 2193
Ion Ratio Lower Upper
128 100
127 15.8 10.3 15.5#
129 9.5 8.6 13.0

