

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY041520\
 Data File : VY002349.D
 Acq On : 15 Apr 2020 19:48
 Operator : SY/MD
 Sample : L2281-08
 Misc : 4.38G/5ML/MSVOA Y/SOIL
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-43

Quant Time: Apr 16 06:48:36 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y040820S.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 08 15:15:02 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-7.80
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-8.70
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-11.49
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-13.43

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	0.00	95	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY041520\
Data File : VY002349.D
Acq On : 15 Apr 2020 19:48
Operator : SY/MD
Sample : L2281-08
Misc : 4.38G/5ML/MSVOA Y/SOIL
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TP-43

Quant Time: Apr 16 06:48:36 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y040820S.M
Quant Title : SW846 8260
QLast Update : Wed Apr 08 15:15:02 2020
Response via : Initial Calibration

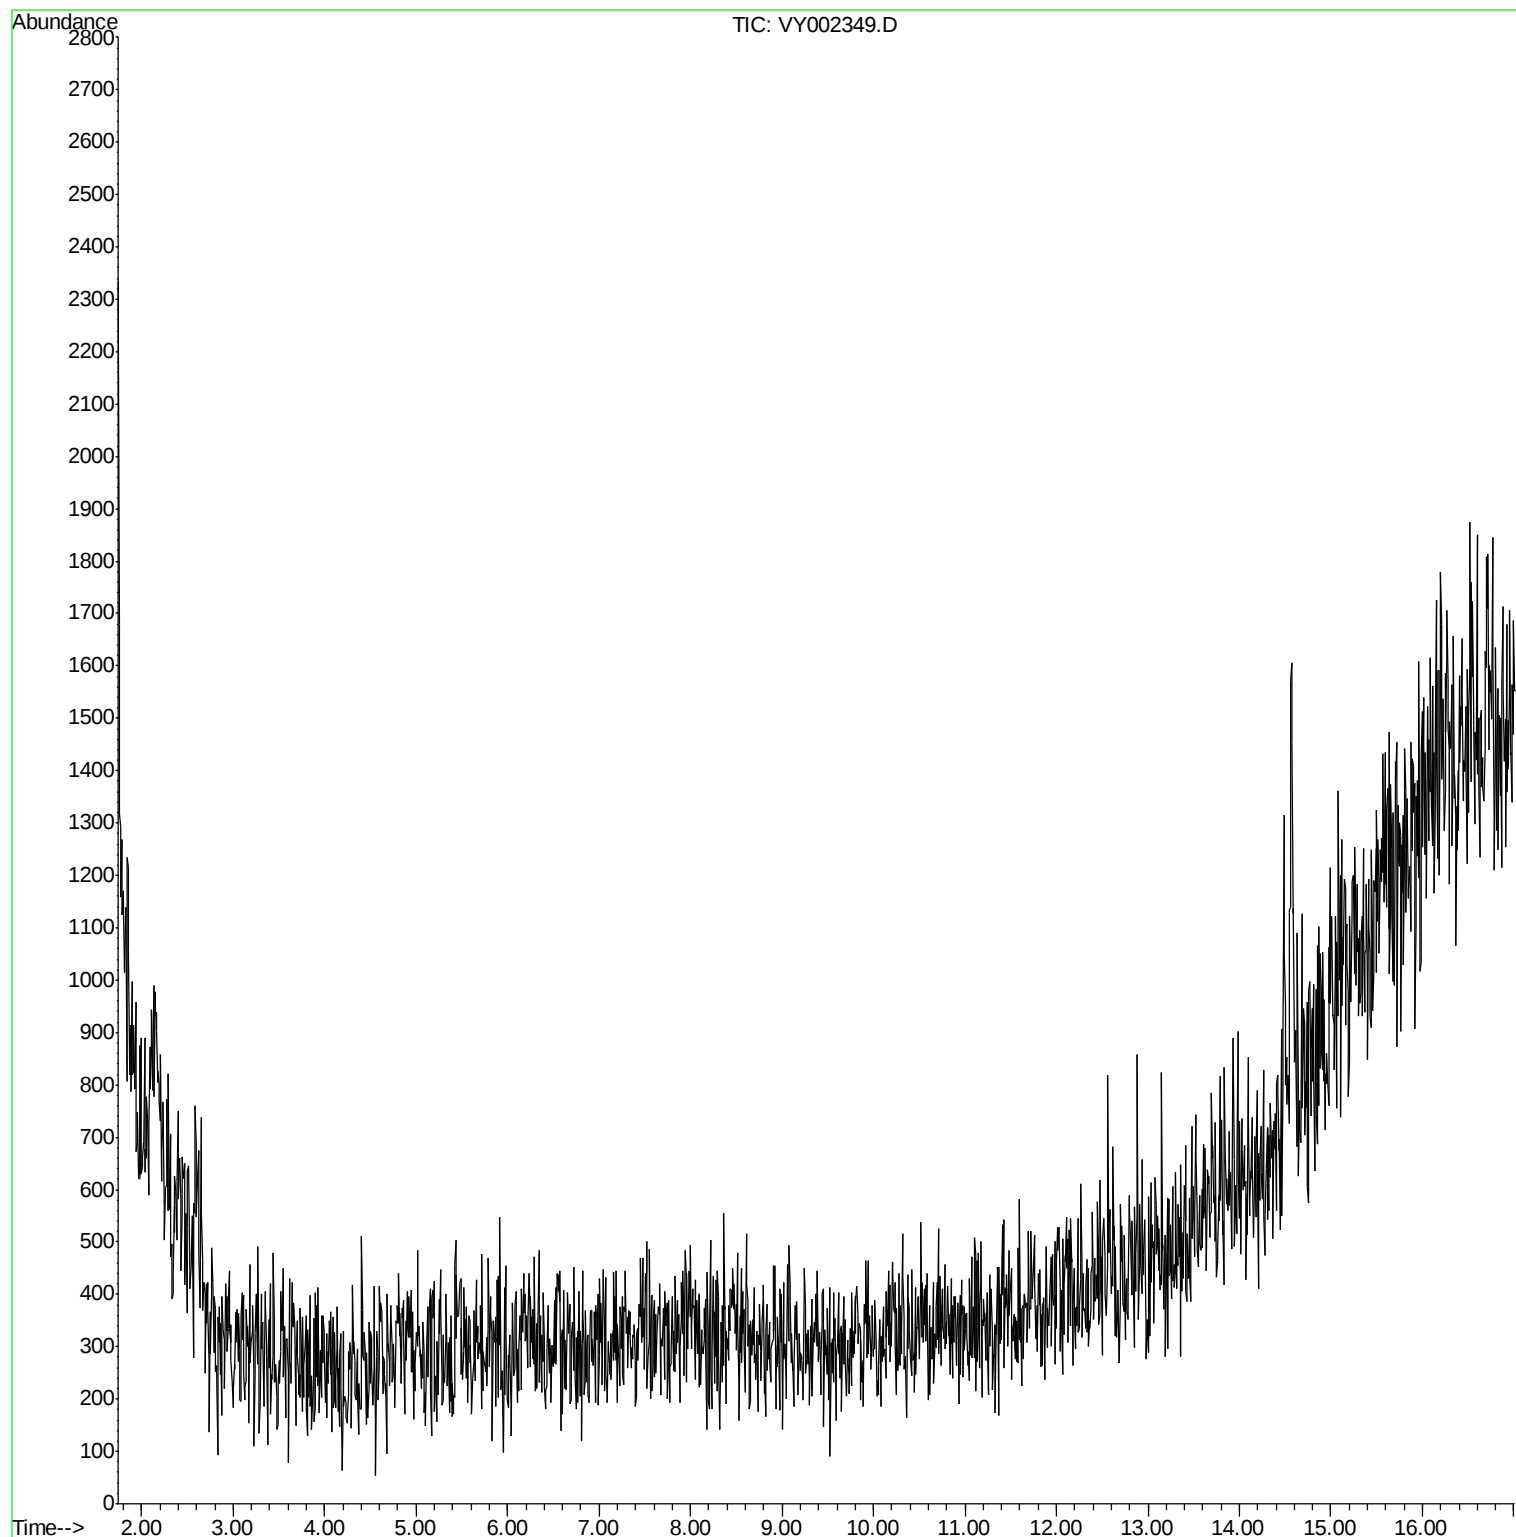

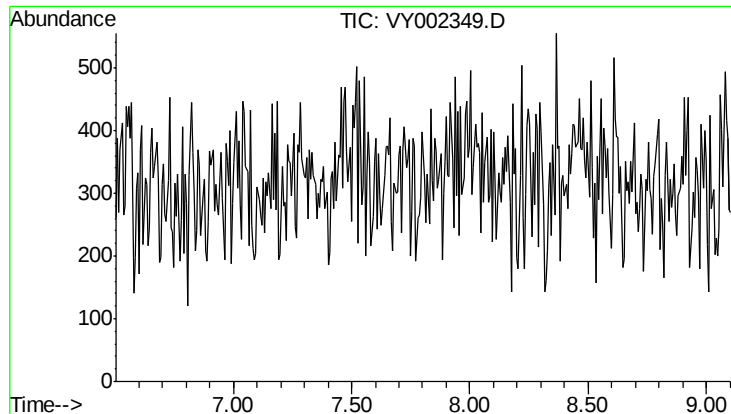

#1

Pentafluorobenzene

Concen: 0.000 ug/l

Expected RT: 7.80 min

Lab File: VY002349.D

Acq: 15 Apr 2020 19:48

Tot Ion: 168

Sig Exp Ratio

168 100



99 60.0

Instrument :

MSVOA_Y

ClientSampleId :

TP-43

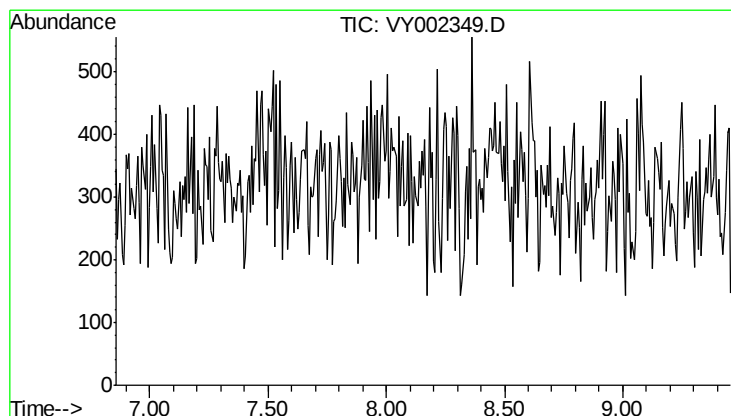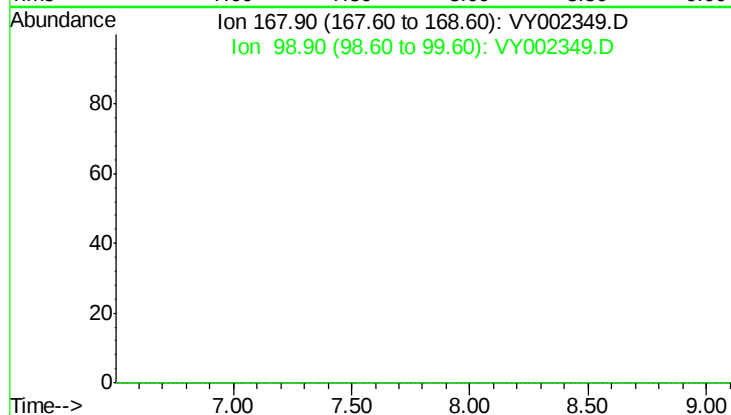

#33

1,2-Dichloroethane-d4

Concen: 0.000 ug/l

Expected RT: 8.16 min

Lab File: VY002349.D


Acq: 15 Apr 2020 19:48


Tgt Ion: 65

Sig Exp Ratio

65 100

67 57.0


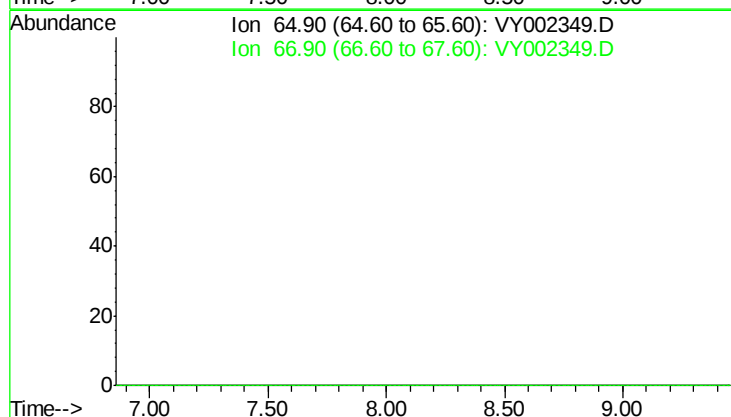


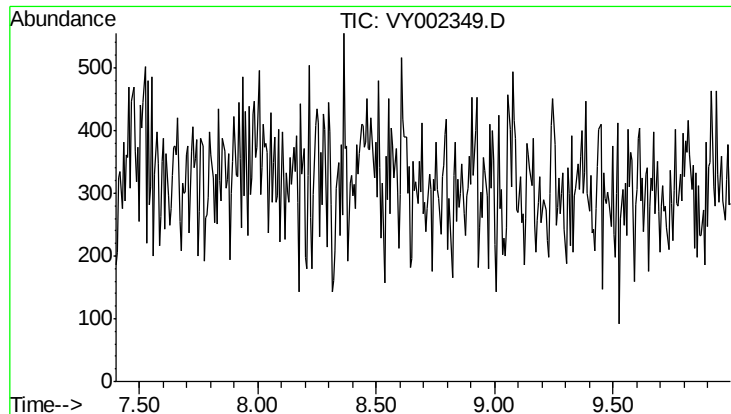

#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 8.70 min
 Lab File: VY002349.D
 Acq: 15 Apr 2020 19:48


Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-43


Tot Ion	114
Sig	Exp Ratio
114	100
63	19.5
88	15.5

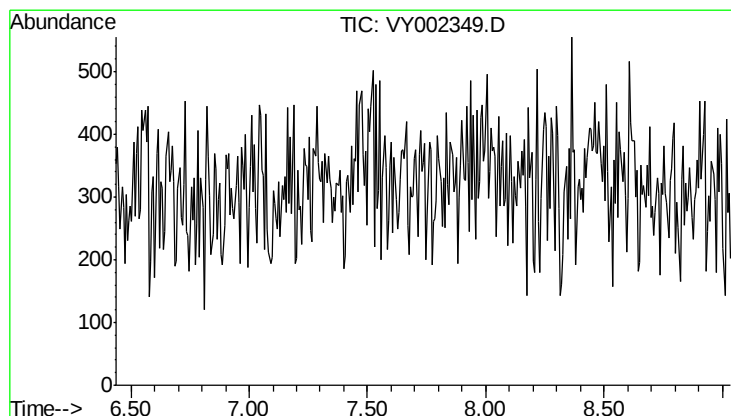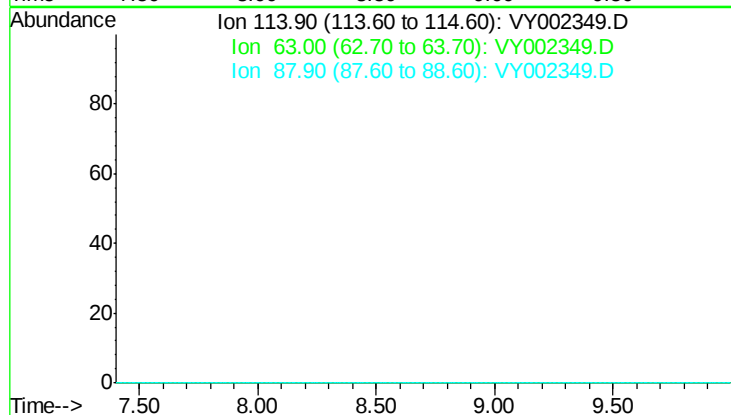

#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 7.74 min
 Lab File: VY002349.D
 Acq: 15 Apr 2020 19:48

Tgt Ion	113
Sig	Exp Ratio
113	100
111	104.4
192	18.4

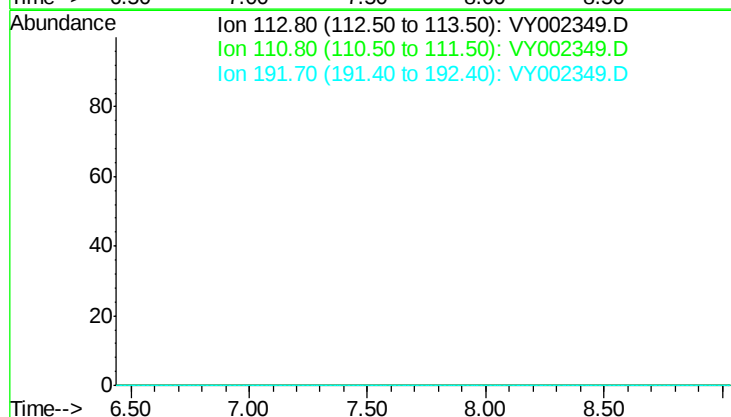


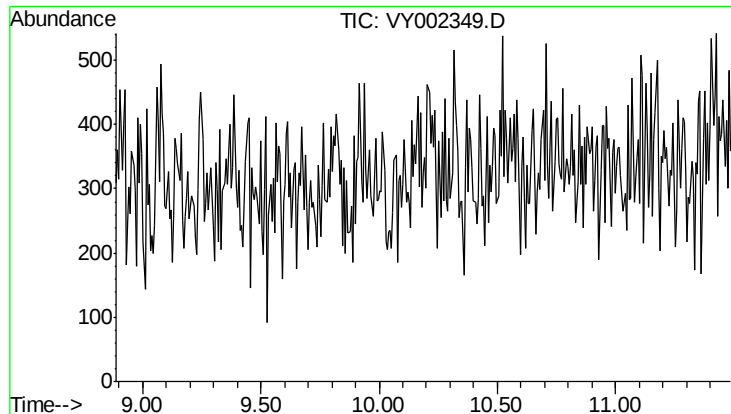


#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 10.19 min

Lab File: VY002349.D
Acq: 15 Apr 2020 19:48

Instrument :
MSVOA_Y
ClientSampleId :
TP-43


Tot Ion	98
Sig	Exp Ratio
98	100
100	65.7

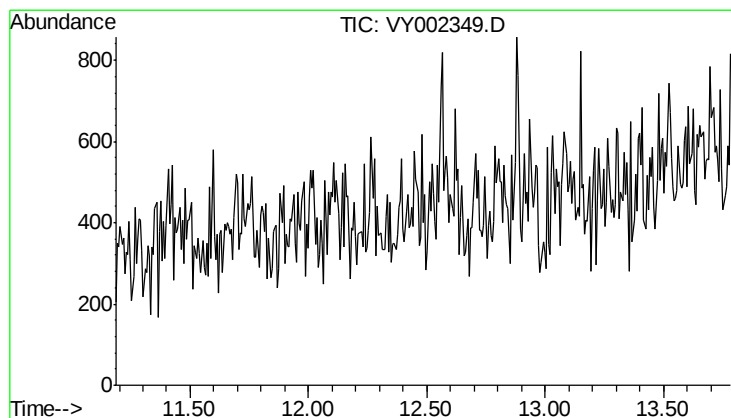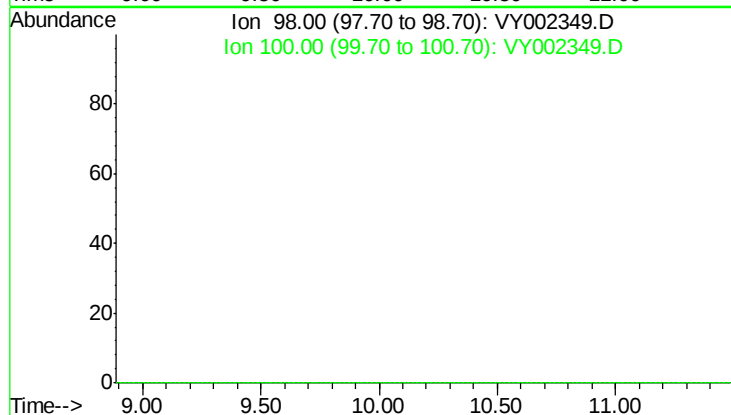


#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
Expected RT: 12.49 min

Lab File: VY002349.D
Acq: 15 Apr 2020 19:48

Tgt Ion	95
Sig	Exp Ratio
95	100
174	75.3
176	70.7


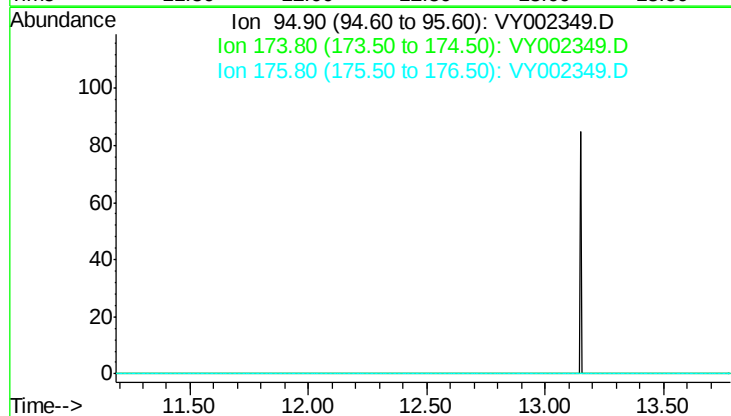


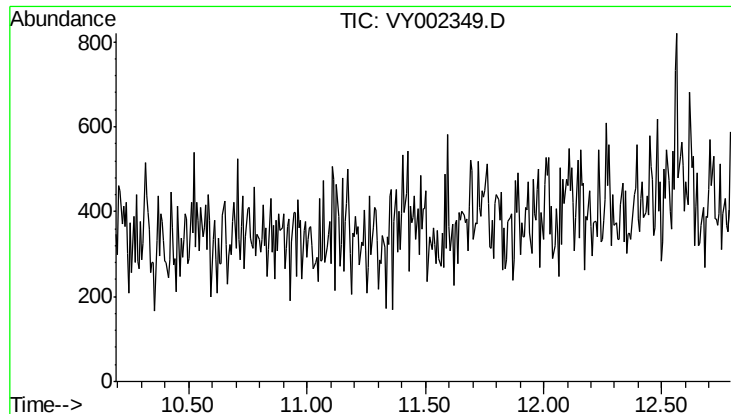

#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 11.49 min
 Lab File: VY002349.D
 Acq: 15 Apr 2020 19:48

Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-43

Tot Ion	117
Sig	Exp Ratio
117	100
82	55.3
119	31.4

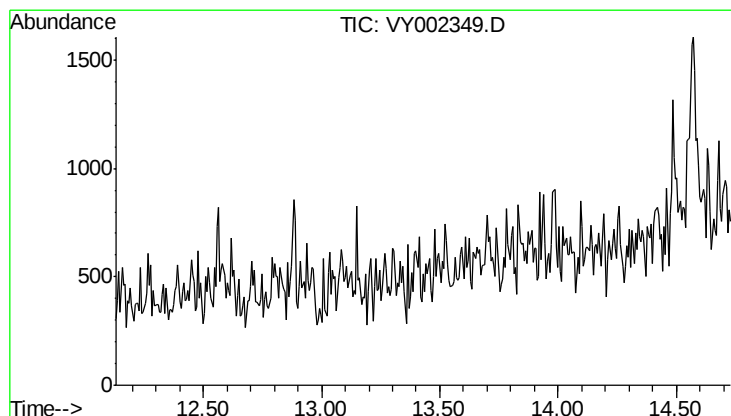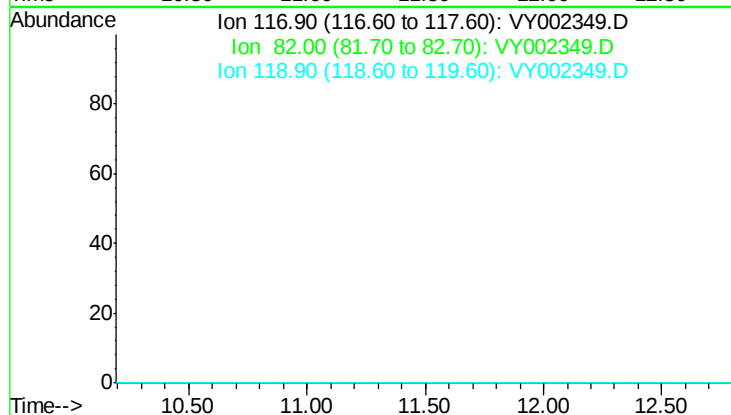

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 13.43 min
 Lab File: VY002349.D
 Acq: 15 Apr 2020 19:48

Tgt Ion	152
Sig	Exp Ratio
152	100
115	61.4
150	175.3

