

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041521\
 Data File : VY004452.D
 Acq On : 15 Apr 2021 19:37
 Operator : SY/MD
 Sample : M2048-16
 Misc : 5.02G/5ML/MSVOA_Y/SOIL
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-06-0-2.0

Quant Time: Apr 16 05:06:49 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041221S.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 13 03:38:02 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.795	168	2321	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	4085	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	3822	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	1363	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	1625	63.01	ug/l	-0.01
Spiked Amount 50.000	Range 50 - 163		Recovery = 126.02%			
35) Dibromofluoromethane	7.728	113	707	31.19	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 62.38%			
50) Toluene-d8	10.185	98	4705	48.79	ug/l	0.00
Spiked Amount 50.000	Range 49 - 140		Recovery = 97.58%			
62) 4-Bromofluorobenzene	12.483	95	1666	50.91	ug/l	0.00
Spiked Amount 50.000	Range 25 - 144		Recovery = 101.82%			
Target Compounds						Qvalue
4) Vinyl Chloride	2.229	62	19835	603.98	ug/l #	43
12) 1,1-Dichloroethene	3.912	96	29	1.29	ug/l #	1
16) Acetone	3.948	43	231	24.89	ug/l #	44
20) Methylene Chloride	4.728	84	44	1.77	ug/l #	54
21) trans-1,2-Dichloroethene	5.149	96	52	2.04	ug/l #	1
27) cis-1,2-Dichloroethene	6.996	96	50	1.75	ug/l #	1
36) 1,1-Dichloropropene	7.911	75	70	1.72	ug/l #	42
38) Carbon Tetrachloride	7.807	117	215	6.13	ug/l #	12
41) Methacrylonitrile	7.258	41	20	1.26	ug/l #	100
51) 4-Methyl-2-Pentanone	10.069	43	51	2.00	ug/l #	38
52) Toluene	10.246	92	277	3.75	ug/l	79
54) cis-1,3-Dichloropropene	9.886	75	49	1.01	ug/l #	32
59) 2-Hexanone	10.740	43	20	1.17	ug/l #	27
67) Ethyl Benzene	11.587	91	624	4.28	ug/l #	71
68) m/p-Xylenes	11.715	106	239	4.41	ug/l	96
73) Isopropylbenzene	12.325	105	157	1.49	ug/l #	49
74) N-amyl acetate	12.123	43	56	1.58	ug/l #	46
76) 1,2,3-Trichloropropane	12.636	75	220	15.04	ug/l #	100
78) n-propylbenzene	12.666	91	302	2.43	ug/l #	53
79) 2-Chlorotoluene	12.666	91	302	4.44	ug/l #	41
80) 1,3,5-Trimethylbenzene	12.812	105	160	1.87	ug/l #	28
81) trans-1,4-Dichloro-2-b...	12.361	75	93	11.37	ug/l #	12
82) 4-Chlorotoluene	12.666	91	302	4.20	ug/l #	41
84) 1,2,4-Trimethylbenzene	13.117	105	845	9.78	ug/l	75
85) sec-Butylbenzene	13.257	105	342	3.35	ug/l #	56
89) n-Butylbenzene	13.702	91	117	1.32	ug/l #	48
90) Hexachloroethane	13.983	117	139	11.14	ug/l #	13
92) 1,2-Dibromo-3-Chloropr...	14.336	75	71	19.86	ug/l #	2
95) Naphthalene	15.233	128	511	9.08	ug/l #	86
96) 1,2,3-Trichlorobenzene	15.690	180	24	1.05	ug/l #	12


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041521\
Data File : VY004452.D
Acq On : 15 Apr 2021 19:37
Operator : SY/MD
Sample : M2048-16
Misc : 5.02G/5ML/MSVOA_Y/SOIL
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SB-06-0-2.0

Quant Time: Apr 16 05:06:49 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041221S.M
Quant Title : SW846 8260
QLast Update : Tue Apr 13 03:38:02 2021
Response via : Initial Calibration




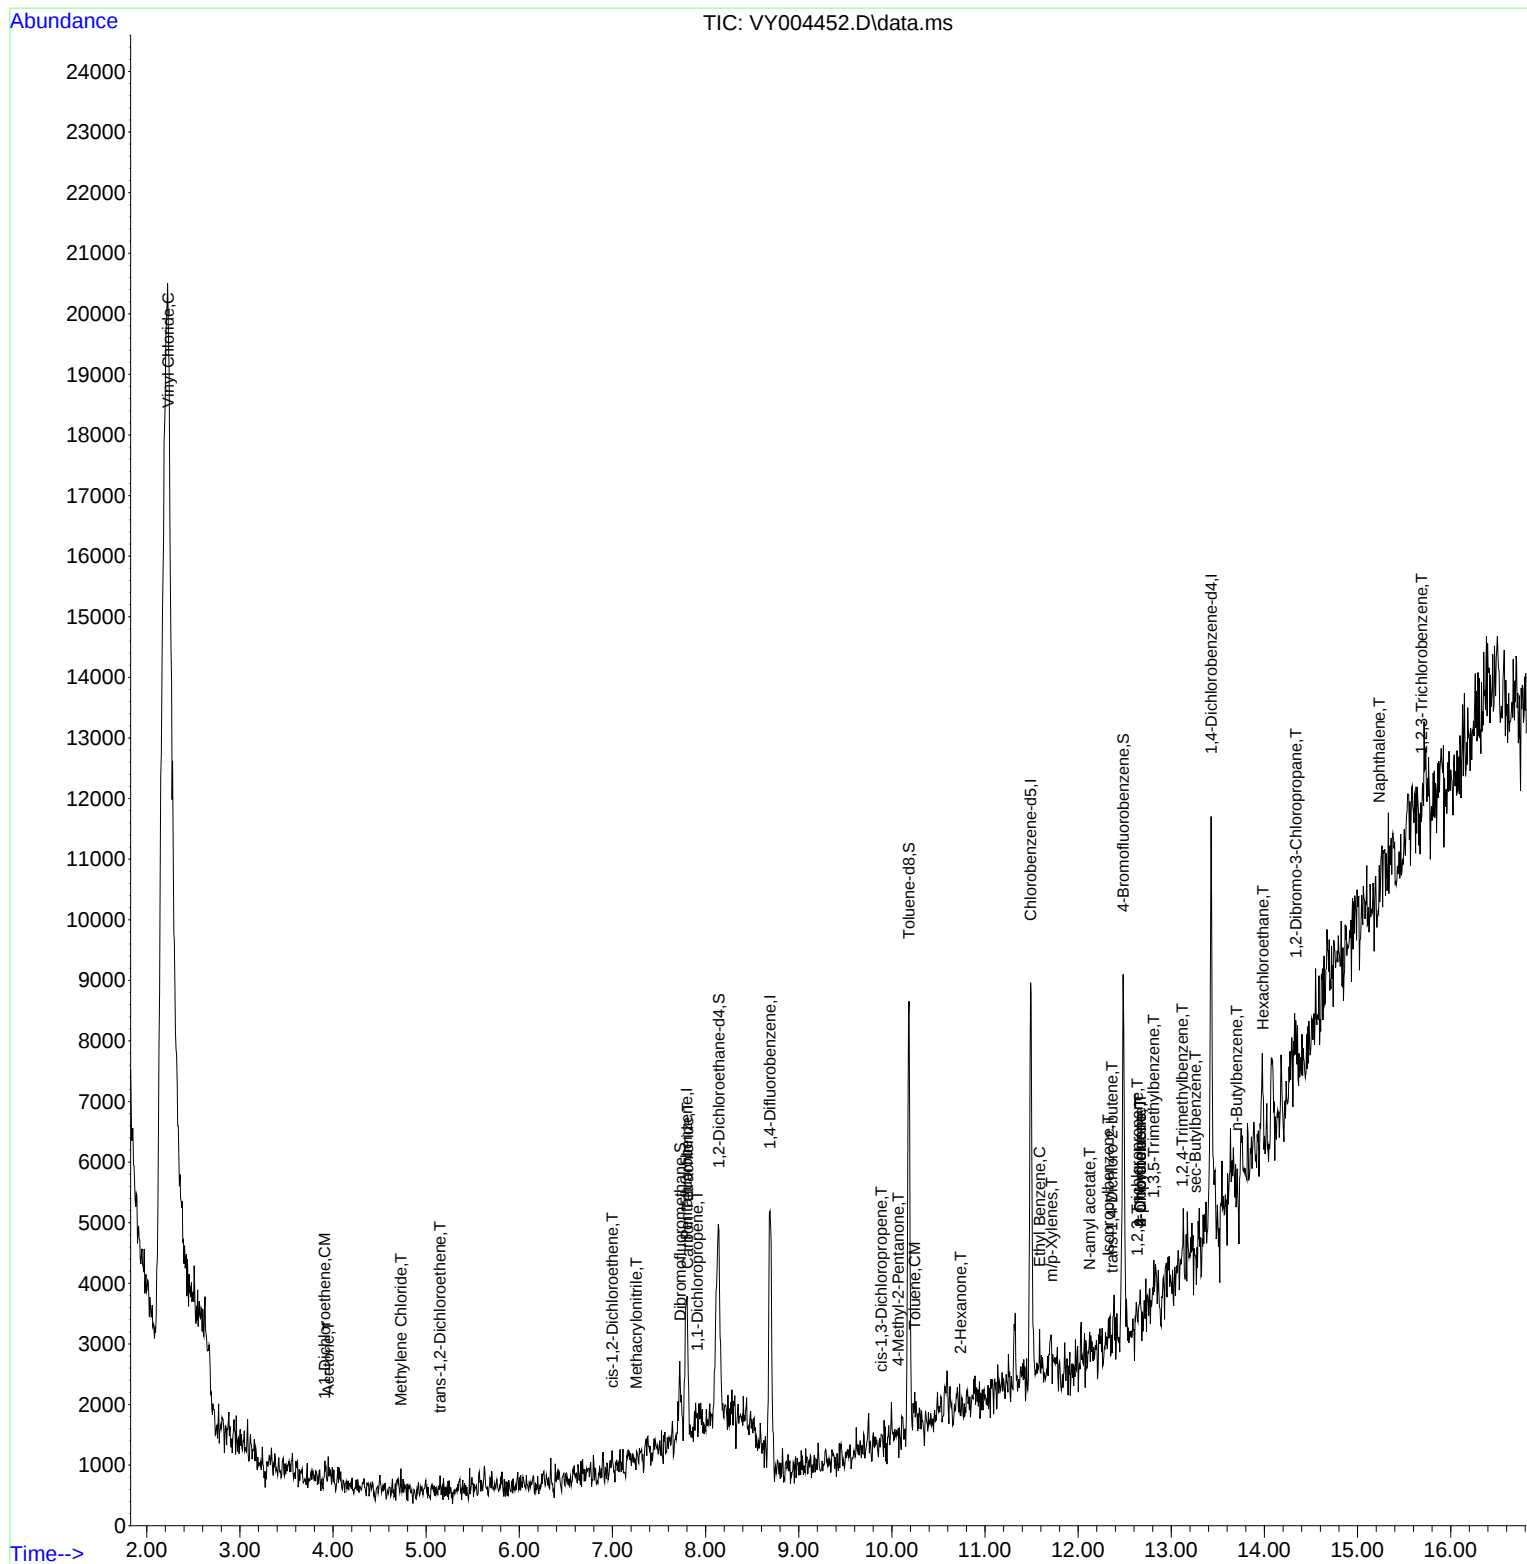




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.795 min Scan# 980
Delta R.T. -0.006 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37




Instrument :
MSVOA_Y
ClientSampleId :
SB-06-0-2.0


Tgt Ion:168 Resp: 2321
Ion Ratio Lower Upper
168 100
99 58.0 45.5 68.3

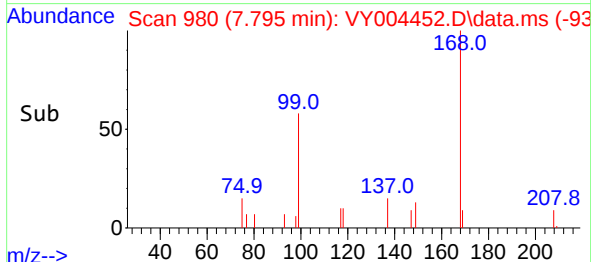

#4
Vinyl Chloride
Concen: 603.98 ug/l
RT: 2.229 min Scan# 67
Delta R.T. -0.030 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37

Tgt Ion: 62 Resp: 19835
Ion Ratio Lower Upper
62 100
64 0.0 25.1 37.7#

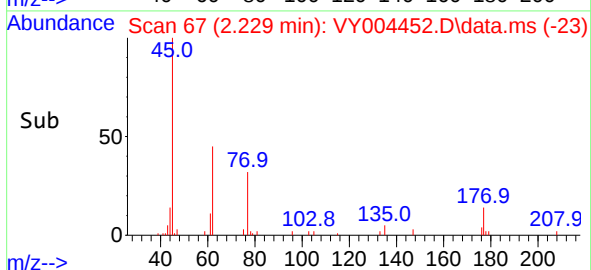



#12

1,1-Dichloroethene

Concen: 1.29 ug/l

RT: 3.912 min Scan# 343

Delta R.T. 0.025 min

Lab File: VY004452.D

Acq: 15 Apr 2021 19:37





Tgt Ion: 96 Resp: 29

Ion Ratio Lower Upper

96 100

61 0.0 132.1 198.1#

98 0.0 48.2 72.2#



#16

Acetone

Concen: 24.89 ug/l

RT: 3.948 min Scan# 349

Delta R.T. -0.012 min

Lab File: VY004452.D




Acq: 15 Apr 2021 19:37


Tgt Ion: 43 Resp: 231

Ion Ratio Lower Upper

43 100

58 0.0 24.6 37.0#



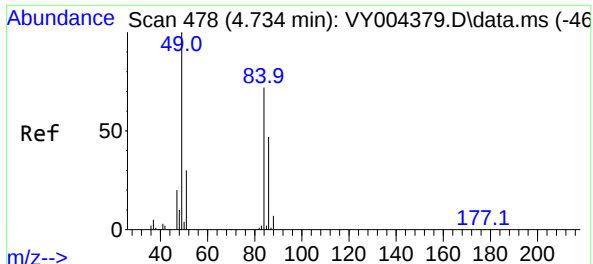

#20

Methylene Chloride

Concen: 1.77 ug/l

RT: 4.728 min Scan# 477

Delta R.T. -0.006 min





Lab File: VY004452.D

Acq: 15 Apr 2021 19:37

Instrument :
MSVOA_Y
ClientSampleId :
SB-06-0-2.0

Tgt Ion: 84 Resp: 44

Ion	Ratio	Lower	Upper
84	100		
49	112.1	111.2	166.8
51	0.0	33.4	50.2#
86	0.0	52.7	79.1#

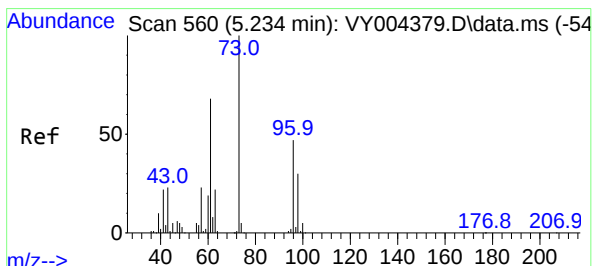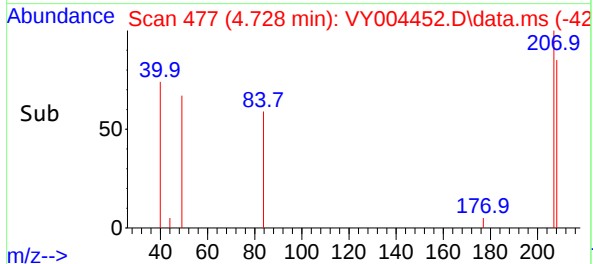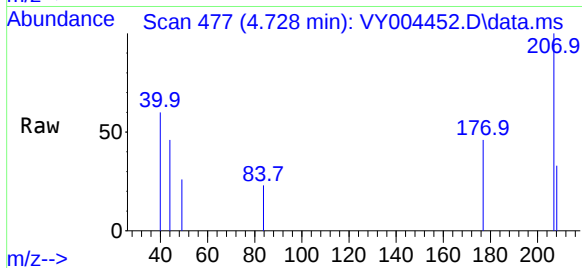

#21

trans-1,2-Dichloroethene

Concen: 2.04 ug/l

RT: 5.149 min Scan# 546




Delta R.T. -0.085 min


Lab File: VY004452.D

Acq: 15 Apr 2021 19:37

Tgt Ion: 96 Resp: 52

Ion	Ratio	Lower	Upper
96	100		
61	0.0	116.5	174.7#
98	0.0	52.0	78.0#


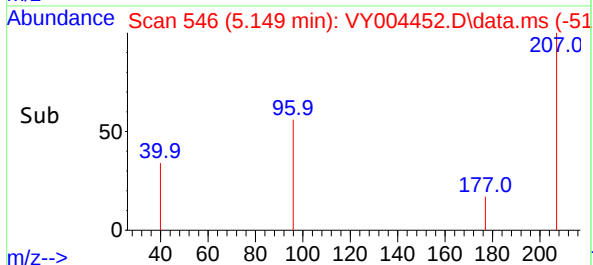
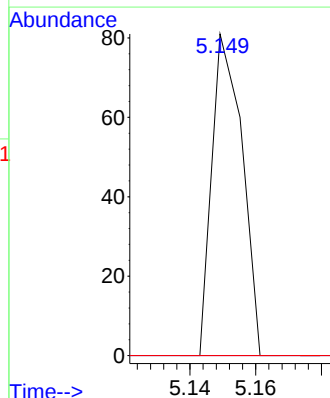
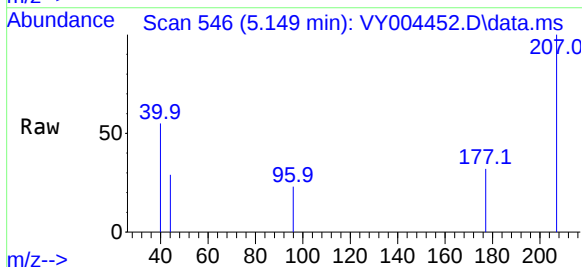




#27
 cis-1,2-Dichloroethene
 Concen: 1.75 ug/l
 RT: 6.996 min Scan# 849
 Delta R.T. -0.006 min
 Lab File: VY004452.D
 Acq: 15 Apr 2021 19:37




Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-06-0-2.0


Tgt Ion: 96 Resp: 50
 Ion Ratio Lower Upper
 96 100
 61 0.0 0.0 303.2
 98 0.0 0.0 130.0

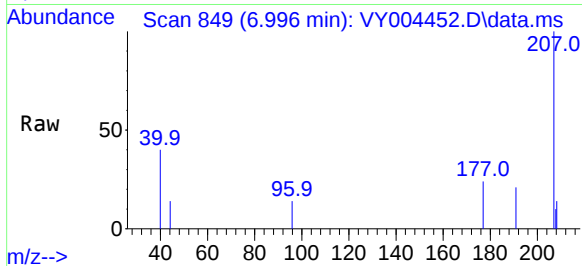

#33
 1,2-Dichloroethane-d4
 Concen: 63.01 ug/l
 RT: 8.142 min Scan# 1037
 Delta R.T. -0.012 min
 Lab File: VY004452.D
 Acq: 15 Apr 2021 19:37

Tgt Ion: 65 Resp: 1625
 Ion Ratio Lower Upper
 65 100
 67 55.3 0.0 106.4


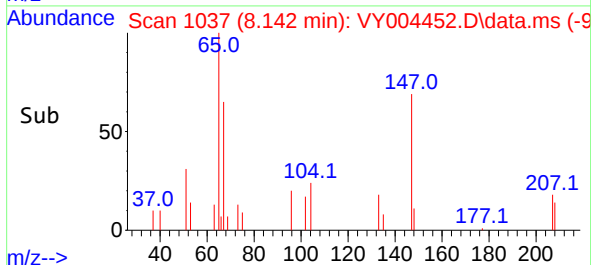
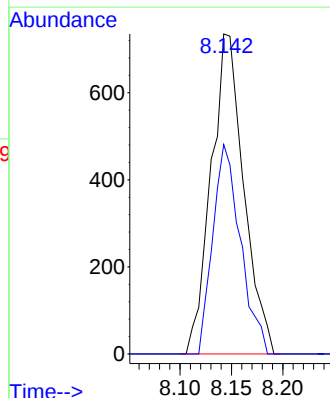
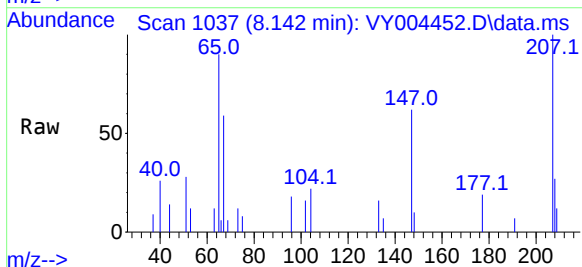


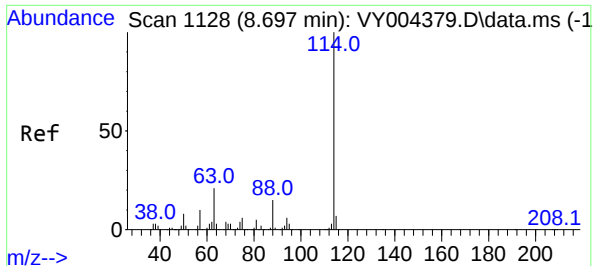

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.691 min Scan# 1127
Delta R.T. -0.006 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37




Instrument :
MSVOA_Y
ClientSampleId :
SB-06-0-2.0


Tgt Ion:	114	Resp:	4085
Ion	Ratio	Lower	Upper
114	100		
63	16.8	0.0	42.4
88	15.4	0.0	30.8

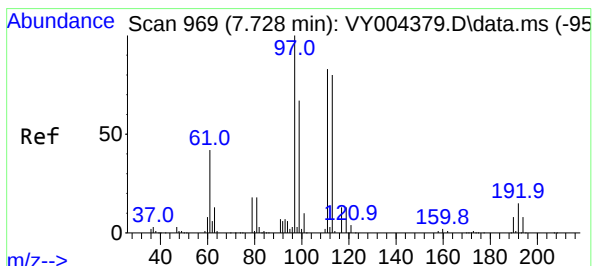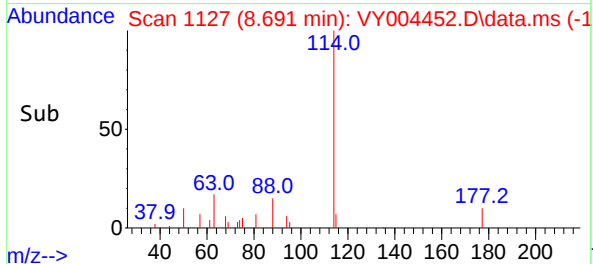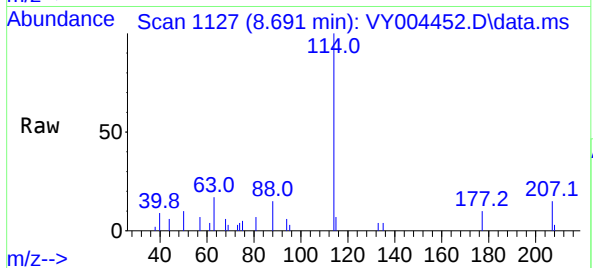

#35
Dibromofluoromethane
Concen: 31.19 ug/l
RT: 7.728 min Scan# 969
Delta R.T. 0.000 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37

Tgt Ion:	113	Resp:	707
Ion	Ratio	Lower	Upper
113	100		
111	109.8	82.6	123.8
192	16.7	16.1	24.1


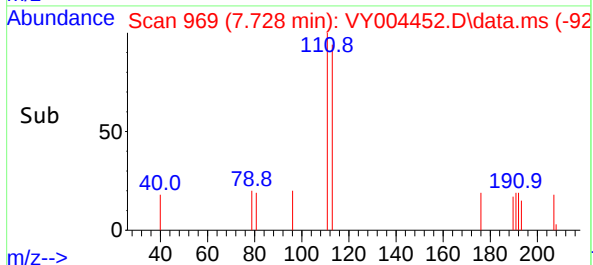
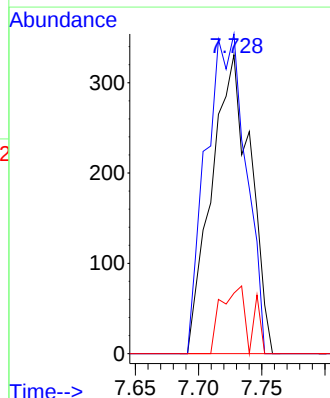
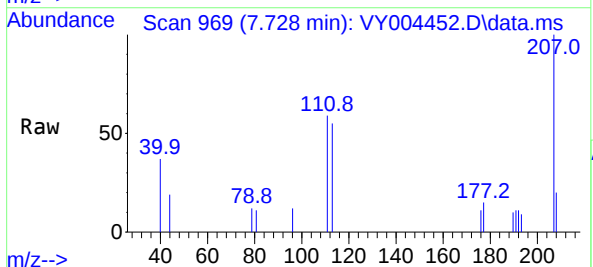


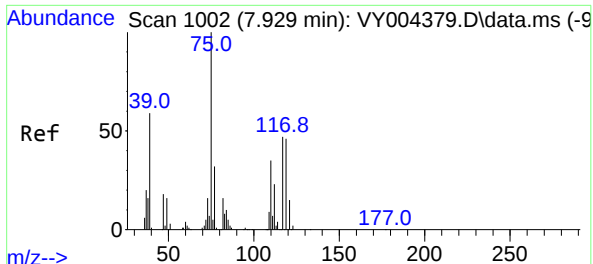

#36
1,1-Dichloropropene
Concen: 1.72 ug/l
RT: 7.911 min Scan# 999
Delta R.T. -0.018 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37




Instrument :
MSVOA_Y
ClientSampleId :
SB-06-0-2.0


Tgt Ion: 75	Resp:	70
Ion	Ratio	Lower Upper
75	100	
110	0.0	17.3 51.7#
77	0.0	24.3 36.5#

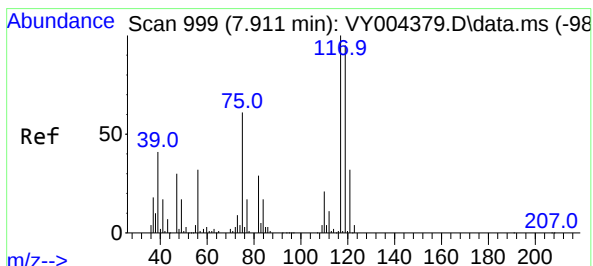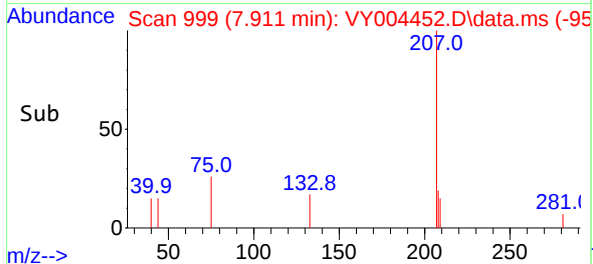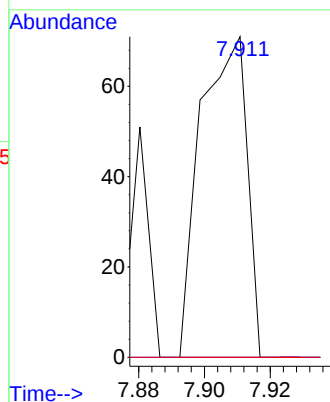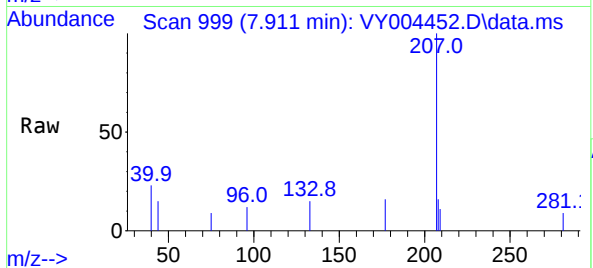

#38
Carbon Tetrachloride
Concen: 6.13 ug/l
RT: 7.807 min Scan# 982
Delta R.T. -0.103 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37

Tgt Ion: 117	Resp:	215
Ion	Ratio	Lower Upper
117	100	
119	0.0	75.8 113.8#
121	0.0	25.3 37.9#


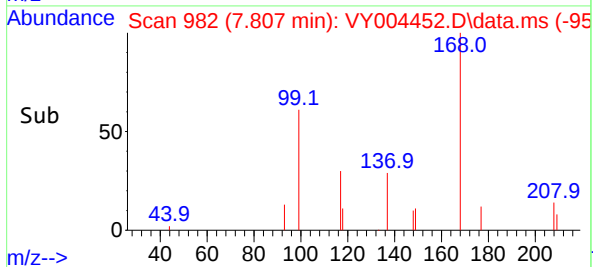

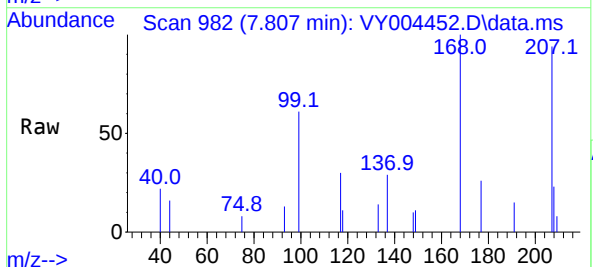


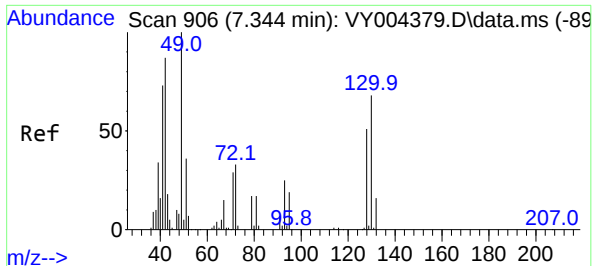

#41
Methacrylonitrile
Concen: 1.26 ug/l
RT: 7.258 min Scan# 892
Delta R.T. -0.085 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37




Instrument :
MSVOA_Y
ClientSampleId :
SB-06-0-2.0


Tgt Ion: 41	Resp: 20
Ion Ratio	Lower Upper
41 100	
39 0.0	0.0 0.0
67 0.0	0.0 0.0
52 0.0	0.0 0.0

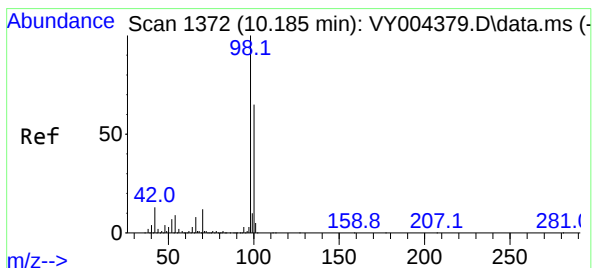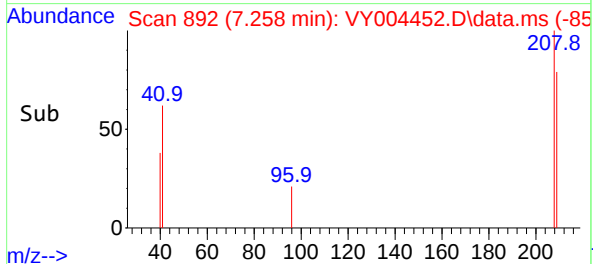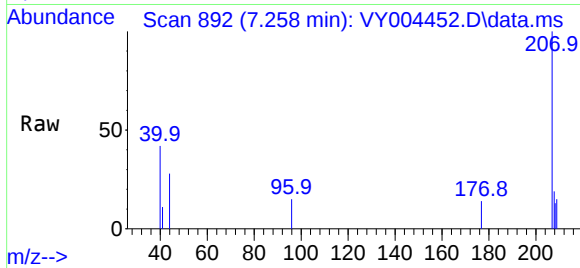

#50
Toluene-d8
Concen: 48.79 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. 0.000 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37

Tgt Ion: 98	Resp:	4705	
Ion	Ratio	Lower	Upper
98	100		
100	66.0	51.8	77.6


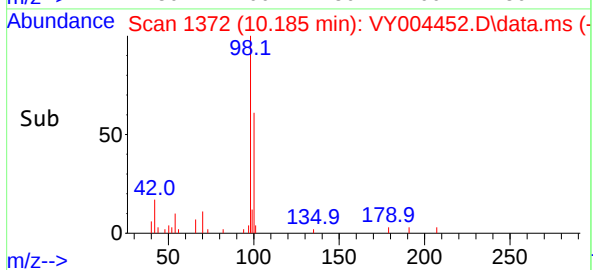

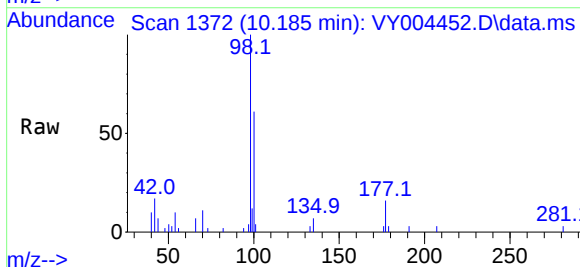




#51
4-Methyl-2-Pentanone
Concen: 2.00 ug/l
RT: 10.069 min Scan# 1353
Delta R.T. -0.006 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37




Instrument :
MSVOA_Y
ClientSampleId :
SB-06-0-2.0


Tgt Ion: 43 Resp: 51
Ion Ratio Lower Upper
43 100
58 0.0 29.2 43.8#

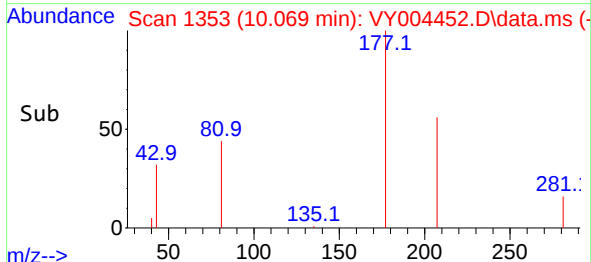

#52
Toluene
Concen: 3.75 ug/l
RT: 10.246 min Scan# 1382
Delta R.T. -0.006 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37

Tgt Ion: 92 Resp: 277
Ion Ratio Lower Upper
92 100
91 143.7 137.8 206.6







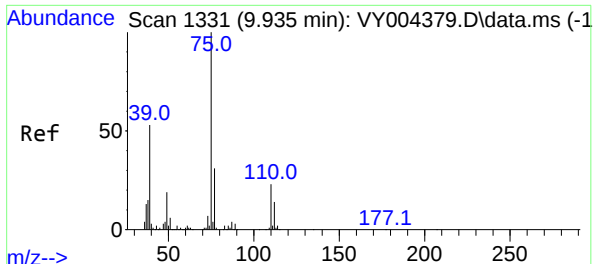

#54
cis-1,3-Dichloropropene
Concen: 1.01 ug/l
RT: 9.886 min Scan# 1323
Delta R.T. -0.049 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37




Instrument :
MSVOA_Y
ClientSampleId :
SB-06-0-2.0


Tgt Ion: 75	Resp:	49
Ion	Ratio	Lower Upper
75	100	
77	0.0	24.6 37.0#
39	0.0	42.1 63.1#

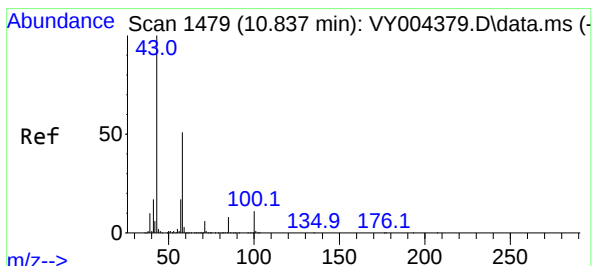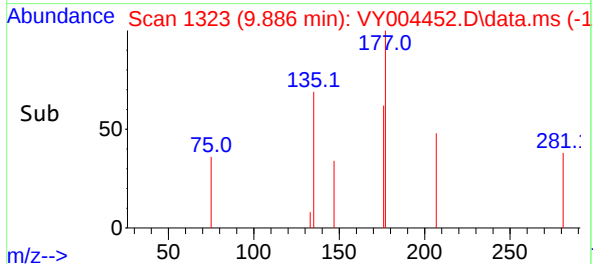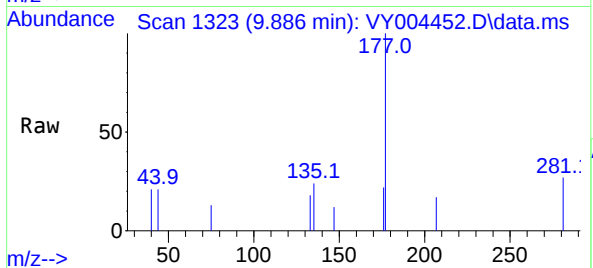

#59
2-Hexanone
Concen: 1.17 ug/l
RT: 10.740 min Scan# 1463
Delta R.T. -0.097 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37

Tgt Ion: 43	Resp:	20
Ion	Ratio	Lower Upper
43	100	
58	0.0	25.4 76.4#


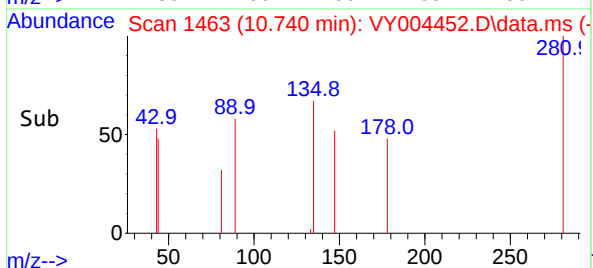
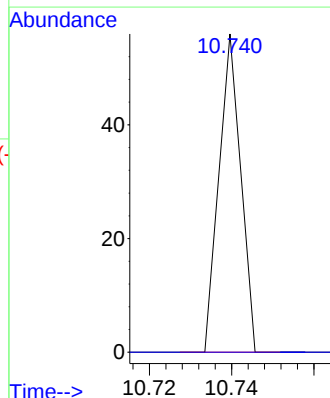
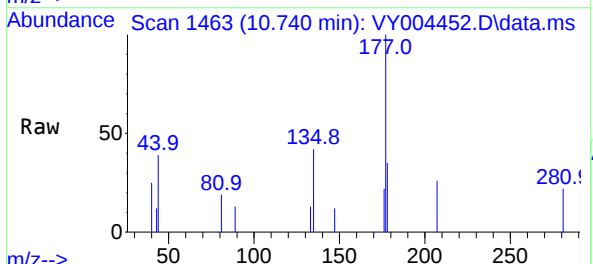




#62
4-Bromofluorobenzene
Concen: 50.91 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37




Instrument :
MSVOA_Y
ClientSampleId :
SB-06-0-2.0


Tgt Ion:	95	Resp:	1666
Ion	Ratio	Lower	Upper
95	100		
174	72.7	0.0	162.4
176	85.1	0.0	156.0

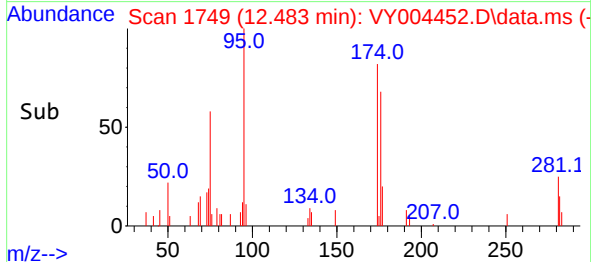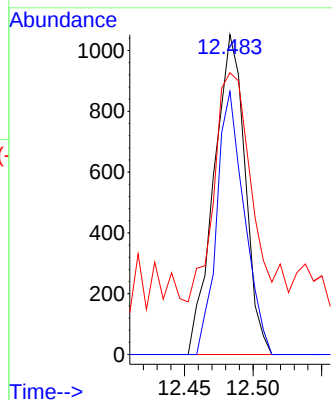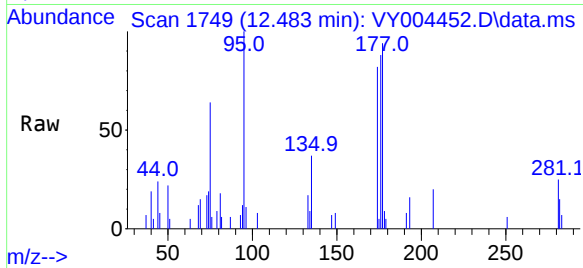

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.489 min Scan# 1586
Delta R.T. -0.006 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37

Tgt Ion:	117	Resp:	3822
Ion	Ratio	Lower	Upper
117	100		
82	50.0	44.9	67.3
119	25.5	25.4	38.0


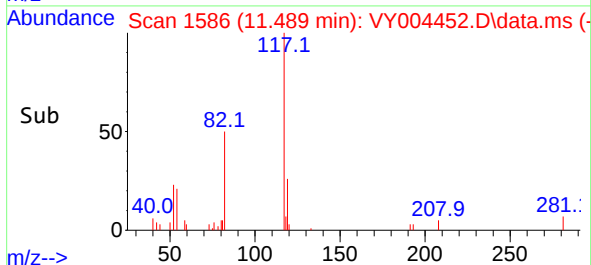
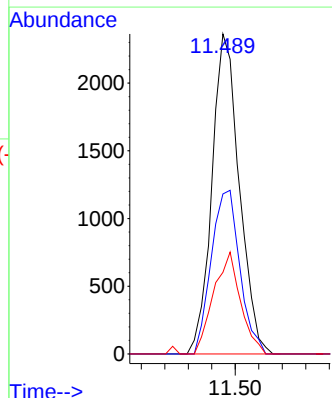
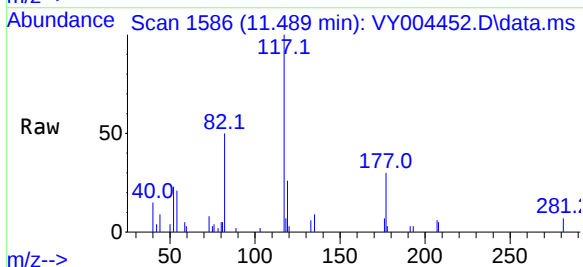




#67
Ethyl Benzene
Concen: 4.28 ug/l
RT: 11.587 min Scan# 1602
Delta R.T. -0.012 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37




Instrument :
MSVOA_Y
ClientSampleId :
SB-06-0-2.0


Tgt Ion: 91 Resp: 624
Ion Ratio Lower Upper
91 100
106 15.1 25.1 37.7#

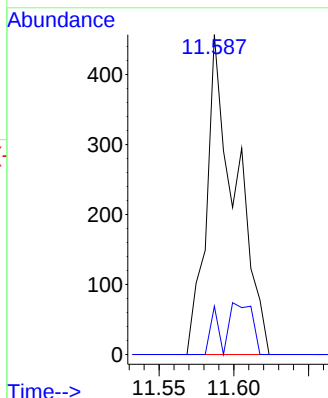

#68
m/p-Xylenes
Concen: 4.41 ug/l
RT: 11.715 min Scan# 1623
Delta R.T. 0.006 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37

Tgt Ion:106 Resp: 239
Ion Ratio Lower Upper
106 100
91 209.6 163.2 244.8

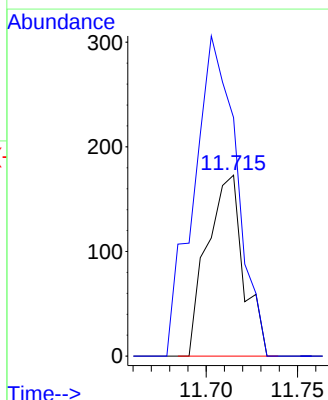







#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37

Instrument :
MSVOA_Y
ClientSampleId :
SB-06-0-2.0

Tgt Ion:152 Resp: 1363




Ion	Ratio	Lower	Upper
152	100		
115	87.2	29.6	88.8
150	166.9	0.0	348.4

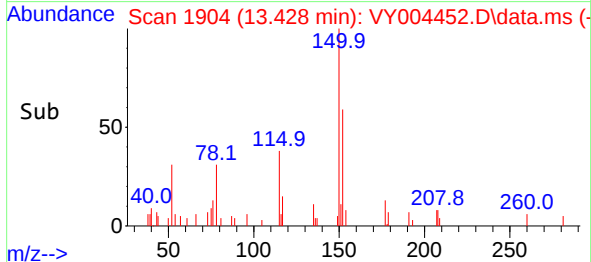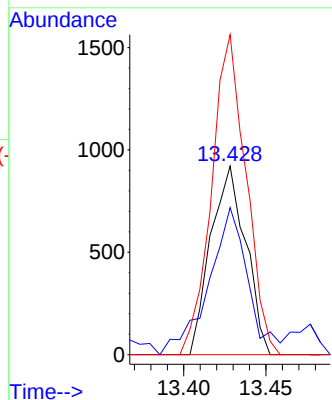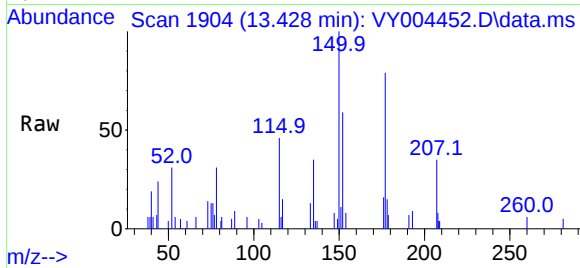


#73
Isopropylbenzene
Concen: 1.49 ug/l
RT: 12.325 min Scan# 1723
Delta R.T. -0.006 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37

Tgt Ion:105 Resp: 157

Ion	Ratio	Lower	Upper
105	100		
120	0.0	13.2	39.5#


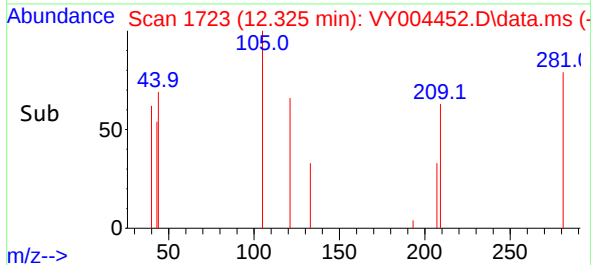
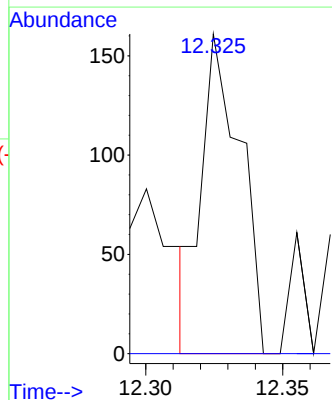
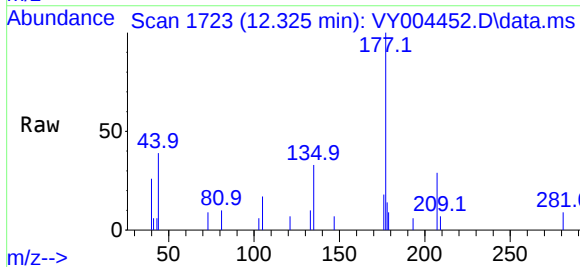




#74
N-amy1 acetate
Concen: 1.58 ug/l
RT: 12.123 min Scan# 1690
Delta R.T. -0.024 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37




Instrument :
MSVOA_Y
ClientSampleId :
SB-06-0-2.0


Tgt Ion: 43	Resp: 56
Ion Ratio	Lower Upper
43 100	
70 0.0	30.4 45.6#
55 0.0	17.4 26.0#
61 0.0	18.2 27.2#

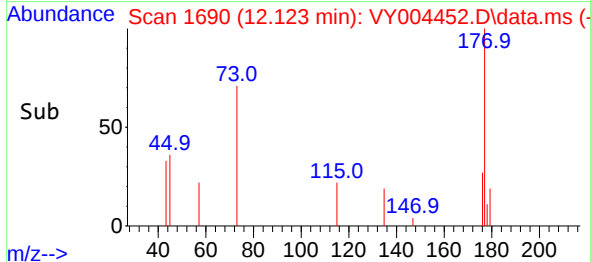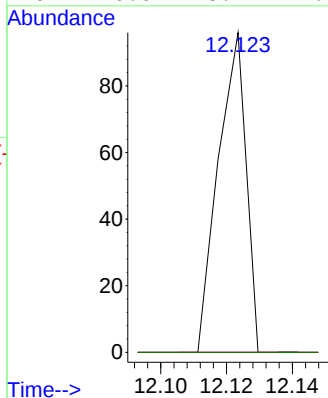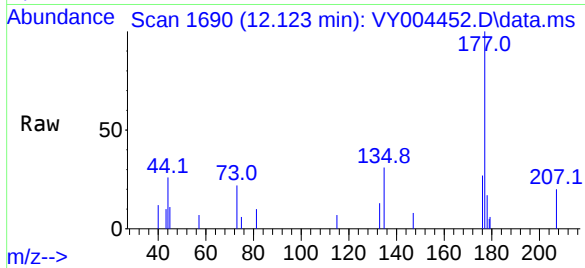

#76
1,2,3-Trichloropropane
Concen: 15.04 ug/l
RT: 12.636 min Scan# 1774
Delta R.T. 0.000 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37

Tgt Ion: 75	Resp: 220
Ion Ratio	Lower Upper
75 100	
77 0.0	0.0 0.0


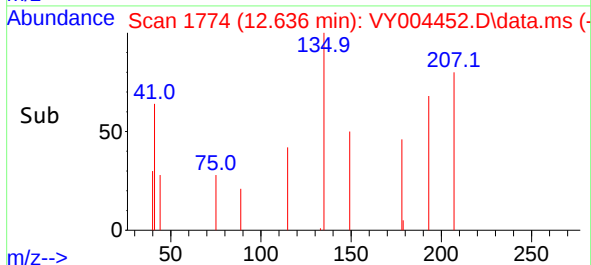
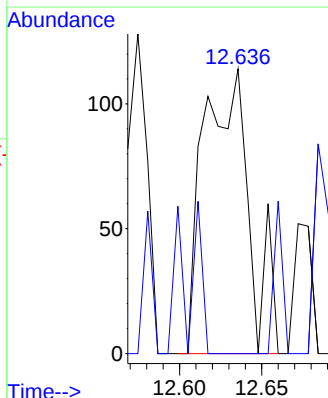
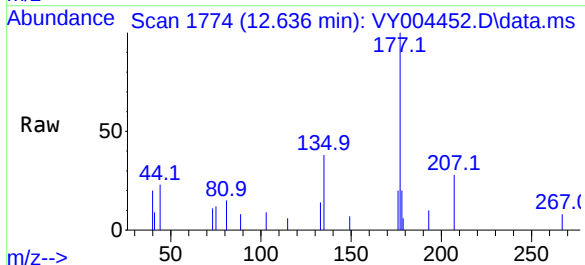




#78
n-propylbenzene
Concen: 2.43 ug/l
RT: 12.666 min Scan# 1779
Delta R.T. -0.006 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37




Instrument :
MSVOA_Y
ClientSampled :
SB-06-0-2.0


Tgt Ion: 91 Resp: 302
Ion Ratio Lower Upper
91 100
120 0.0 11.5 34.4#

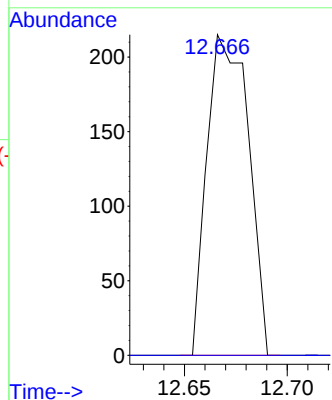

#79
2-Chlorotoluene
Concen: 4.44 ug/l
RT: 12.666 min Scan# 1779
Delta R.T. -0.091 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37

Tgt Ion: 91 Resp: 302
Ion Ratio Lower Upper
91 100
126 0.0 16.7 50.1#



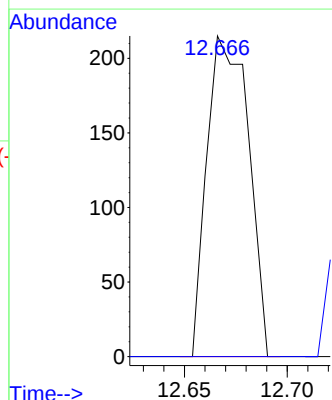





#80
1,3,5-Trimethylbenzene
Concen: 1.87 ug/l
RT: 12.812 min Scan# 1803
Delta R.T. -0.006 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37




Instrument :
MSVOA_Y
ClientSampleId :
SB-06-0-2.0


Tgt Ion:105 Resp: 160
Ion Ratio Lower Upper
105 100
120 0.0 24.6 74.0#

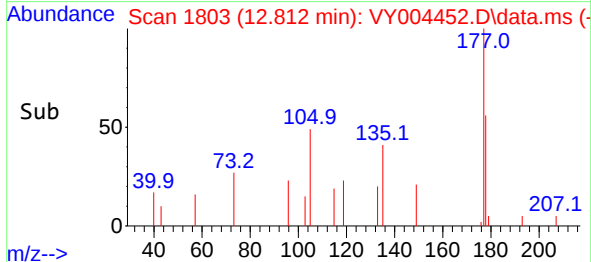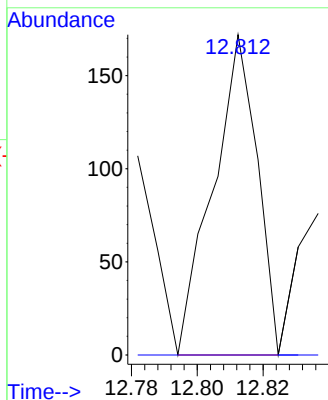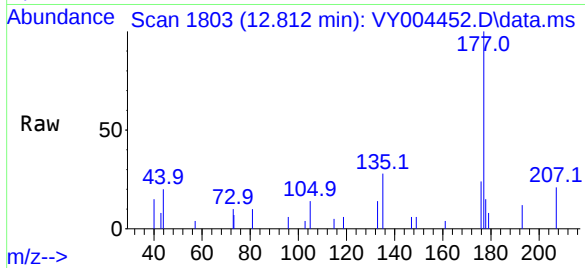

#81
trans-1,4-Dichloro-2-butene
Concen: 11.37 ug/l
RT: 12.361 min Scan# 1729
Delta R.T. -0.024 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37

Tgt Ion: 75 Resp: 93
Ion Ratio Lower Upper
75 100
53 0.0 75.0 112.6#
89 0.0 36.1 54.1#


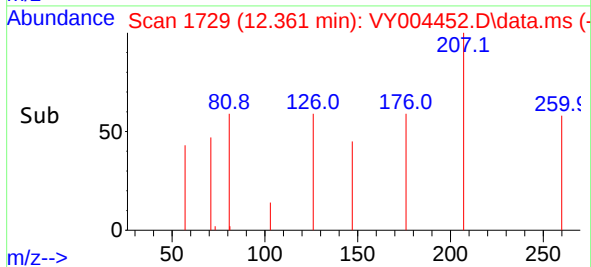
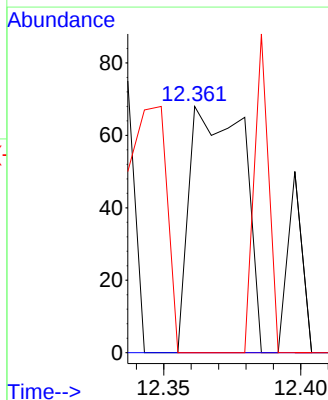
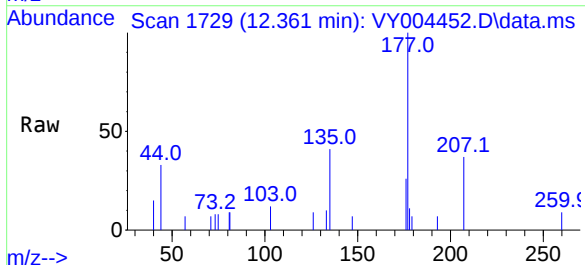




#82
4-Chlorotoluene
Concen: 4.20 ug/l
RT: 12.666 min Scan# 1779
Delta R.T. -0.189 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37




Instrument :
MSVOA_Y
ClientSampleId :
SB-06-0-2.0


Tgt Ion: 91 Resp: 302
Ion Ratio Lower Upper
91 100
126 0.0 16.9 50.7#

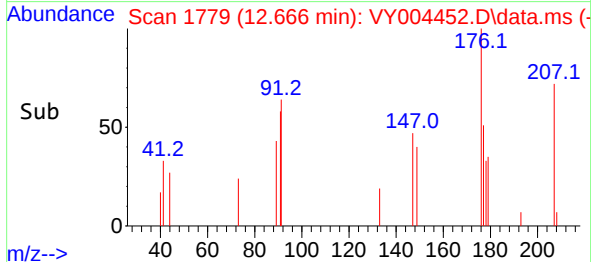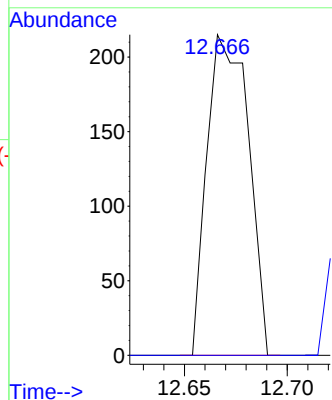

#84
1,2,4-Trimethylbenzene
Concen: 9.78 ug/l
RT: 13.117 min Scan# 1853
Delta R.T. -0.006 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37

Tgt Ion: 105 Resp: 845
Ion Ratio Lower Upper
105 100
120 28.8 22.4 67.3


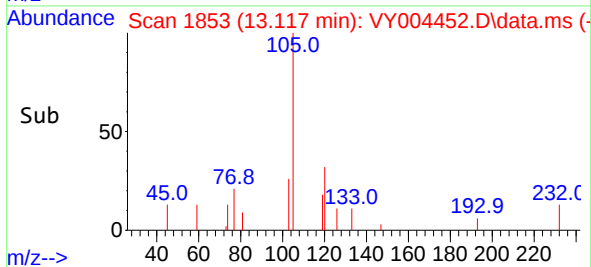
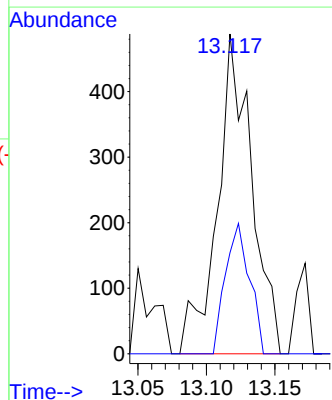
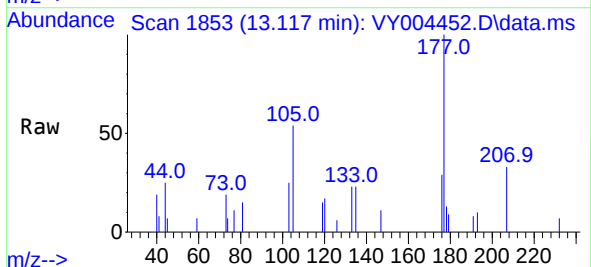




#85
sec-Butylbenzene
Concen: 3.35 ug/l
RT: 13.257 min Scan# 1876
Delta R.T. 0.000 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37




Instrument :
MSVOA_Y
ClientSampleId :
SB-06-0-2.0


Tgt Ion:105 Resp: 342
Ion Ratio Lower Upper
105 100
134 0.0 10.1 30.3#

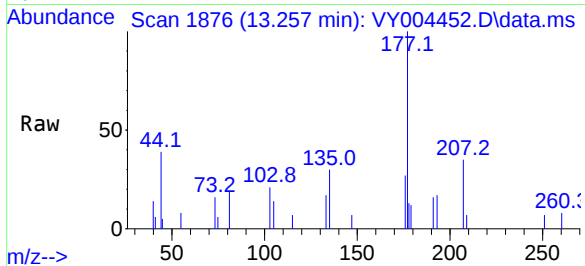

#89
n-Butylbenzene
Concen: 1.32 ug/l
RT: 13.702 min Scan# 1949
Delta R.T. 0.000 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37

Tgt Ion: 91 Resp: 117
Ion Ratio Lower Upper
91 100
92 0.0 26.6 79.8#
134 27.4 12.7 38.1


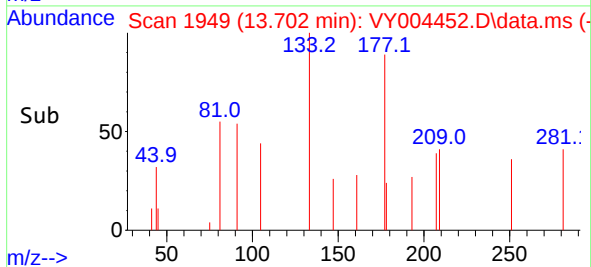

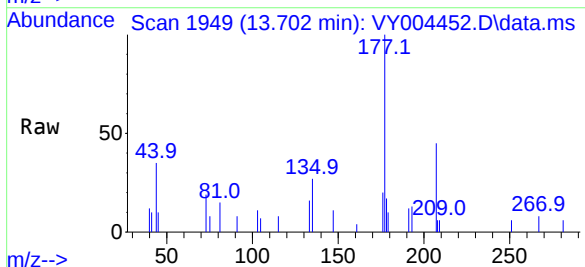




#90
Hexachloroethane
Concen: 11.14 ug/l
RT: 13.983 min Scan# 1995
Delta R.T. 0.018 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37




Instrument :
MSVOA_Y
ClientSampleId :
SB-06-0-2.0


Tgt Ion:117 Resp: 139
Ion Ratio Lower Upper
117 100
201 0.0 36.6 109.9#

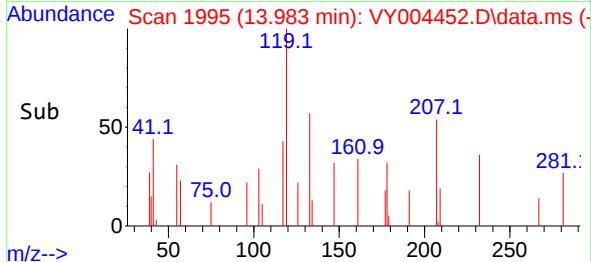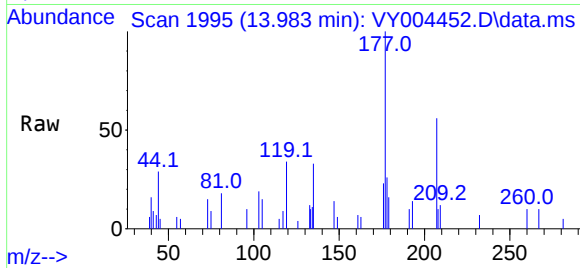

#92
1,2-Dibromo-3-Chloropropane
Concen: 19.86 ug/l
RT: 14.336 min Scan# 2053
Delta R.T. -0.024 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37

Tgt Ion: 75 Resp: 71
Ion Ratio Lower Upper
75 100
155 0.0 40.6 121.8#
157 0.0 53.0 159.0#


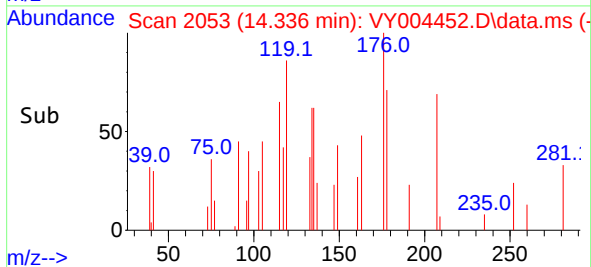

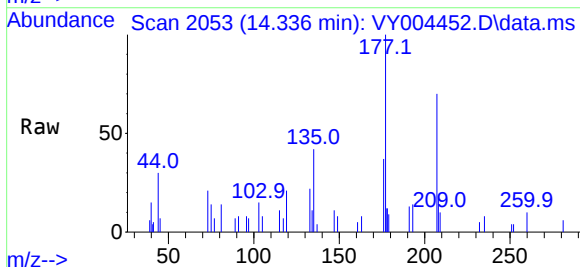




#95
Naphthalene
Concen: 9.08 ug/l
RT: 15.233 min Scan# 2200
Delta R.T. -0.006 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37

Instrument :
MSVOA_Y
ClientSampleId :
SB-06-0-2.0

Tgt Ion:128 Resp: 511
Ion Ratio Lower Upper
128 100
127 7.8 10.2 15.2#
129 4.7 8.8 13.2#

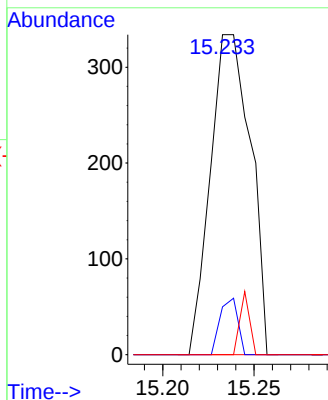

#96
1,2,3-Trichlorobenzene
Concen: 1.05 ug/l
RT: 15.690 min Scan# 2275
Delta R.T. 0.262 min
Lab File: VY004452.D
Acq: 15 Apr 2021 19:37

Tgt Ion:180 Resp: 24
Ion Ratio Lower Upper
180 100
182 0.0 47.6 142.8#
145 0.0 16.3 48.8#

