


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv041620\
 Data File : VY002354.D
 Acq On : 16 Apr 2020 09:51
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y040820S.M
 Title : SW846 8260
 Last Update : Wed Apr 08 15:15:02 2020

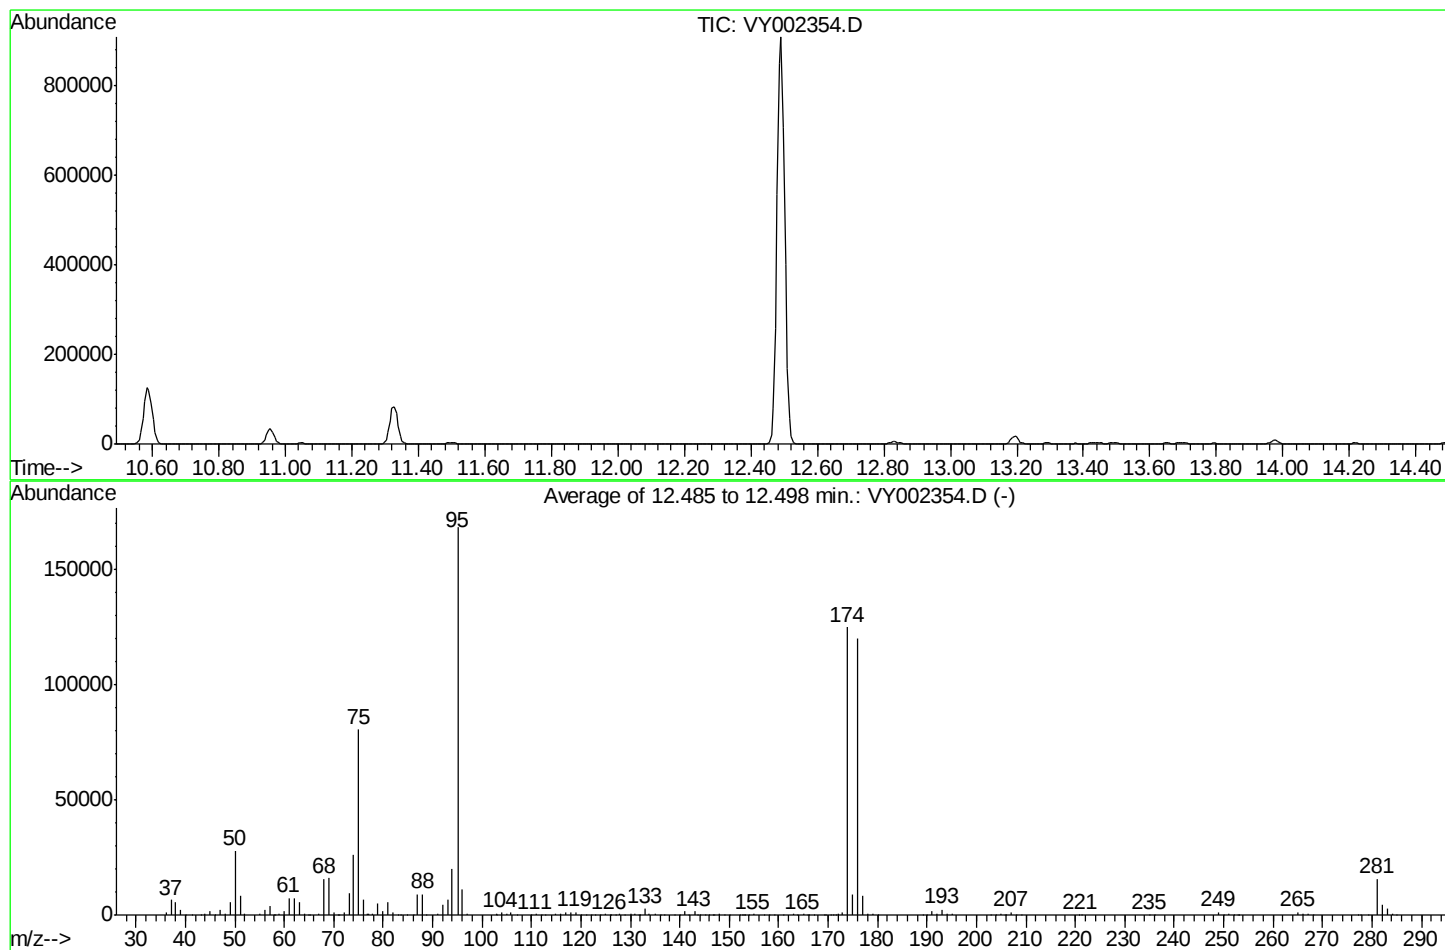

AutoFind: Scans 1763, 1764, 1765; Background Corrected with Scan 1754

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	27829	PASS
75	95	30	60	47.7	80336	PASS
95	95	100	100	100.0	168320	PASS
96	95	5	9	6.7	11341	PASS
173	174	0.00	2	0.8	1030	PASS
174	95	50	100	74.2	124874	PASS
175	174	5	9	6.9	8678	PASS
176	174	95	101	96.2	120104	PASS
177	176	5	9	7.2	8609	PASS