

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041621\
 Data File : VY004481.D
 Acq On : 16 Apr 2021 19:38
 Operator : SY/MD
 Sample : M2048-16
 Misc : 5.09G/5ML/MSVOA_Y/SOIL
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-06-0-2.0

Quant Time: Apr 17 00:58:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041221S.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 13 03:38:02 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.801	168	50128	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	88268	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.495	117	80658	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	36119	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	31664	56.85	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	113.70%
35) Dibromofluoromethane	7.728	113	27519	56.18	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	112.36%
50) Toluene-d8	10.185	98	107543	51.61	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	103.22%
62) 4-Bromofluorobenzene	12.483	95	35162	49.73	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	99.46%
Target Compounds						Qvalue
16) Acetone	3.966	43	3471	10.97	ug/l	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041621\
Data File : VY004481.D
Acq On : 16 Apr 2021 19:38
Operator : SY/MD
Sample : M2048-16
Misc : 5.09G/5ML/MSVOA_Y/SOIL
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SB-06-0-2.0


Quant Time: Apr 17 00:58:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041221S.M
Quant Title : SW846 8260
QLast Update : Tue Apr 13 03:38:02 2021
Response via : Initial Calibration

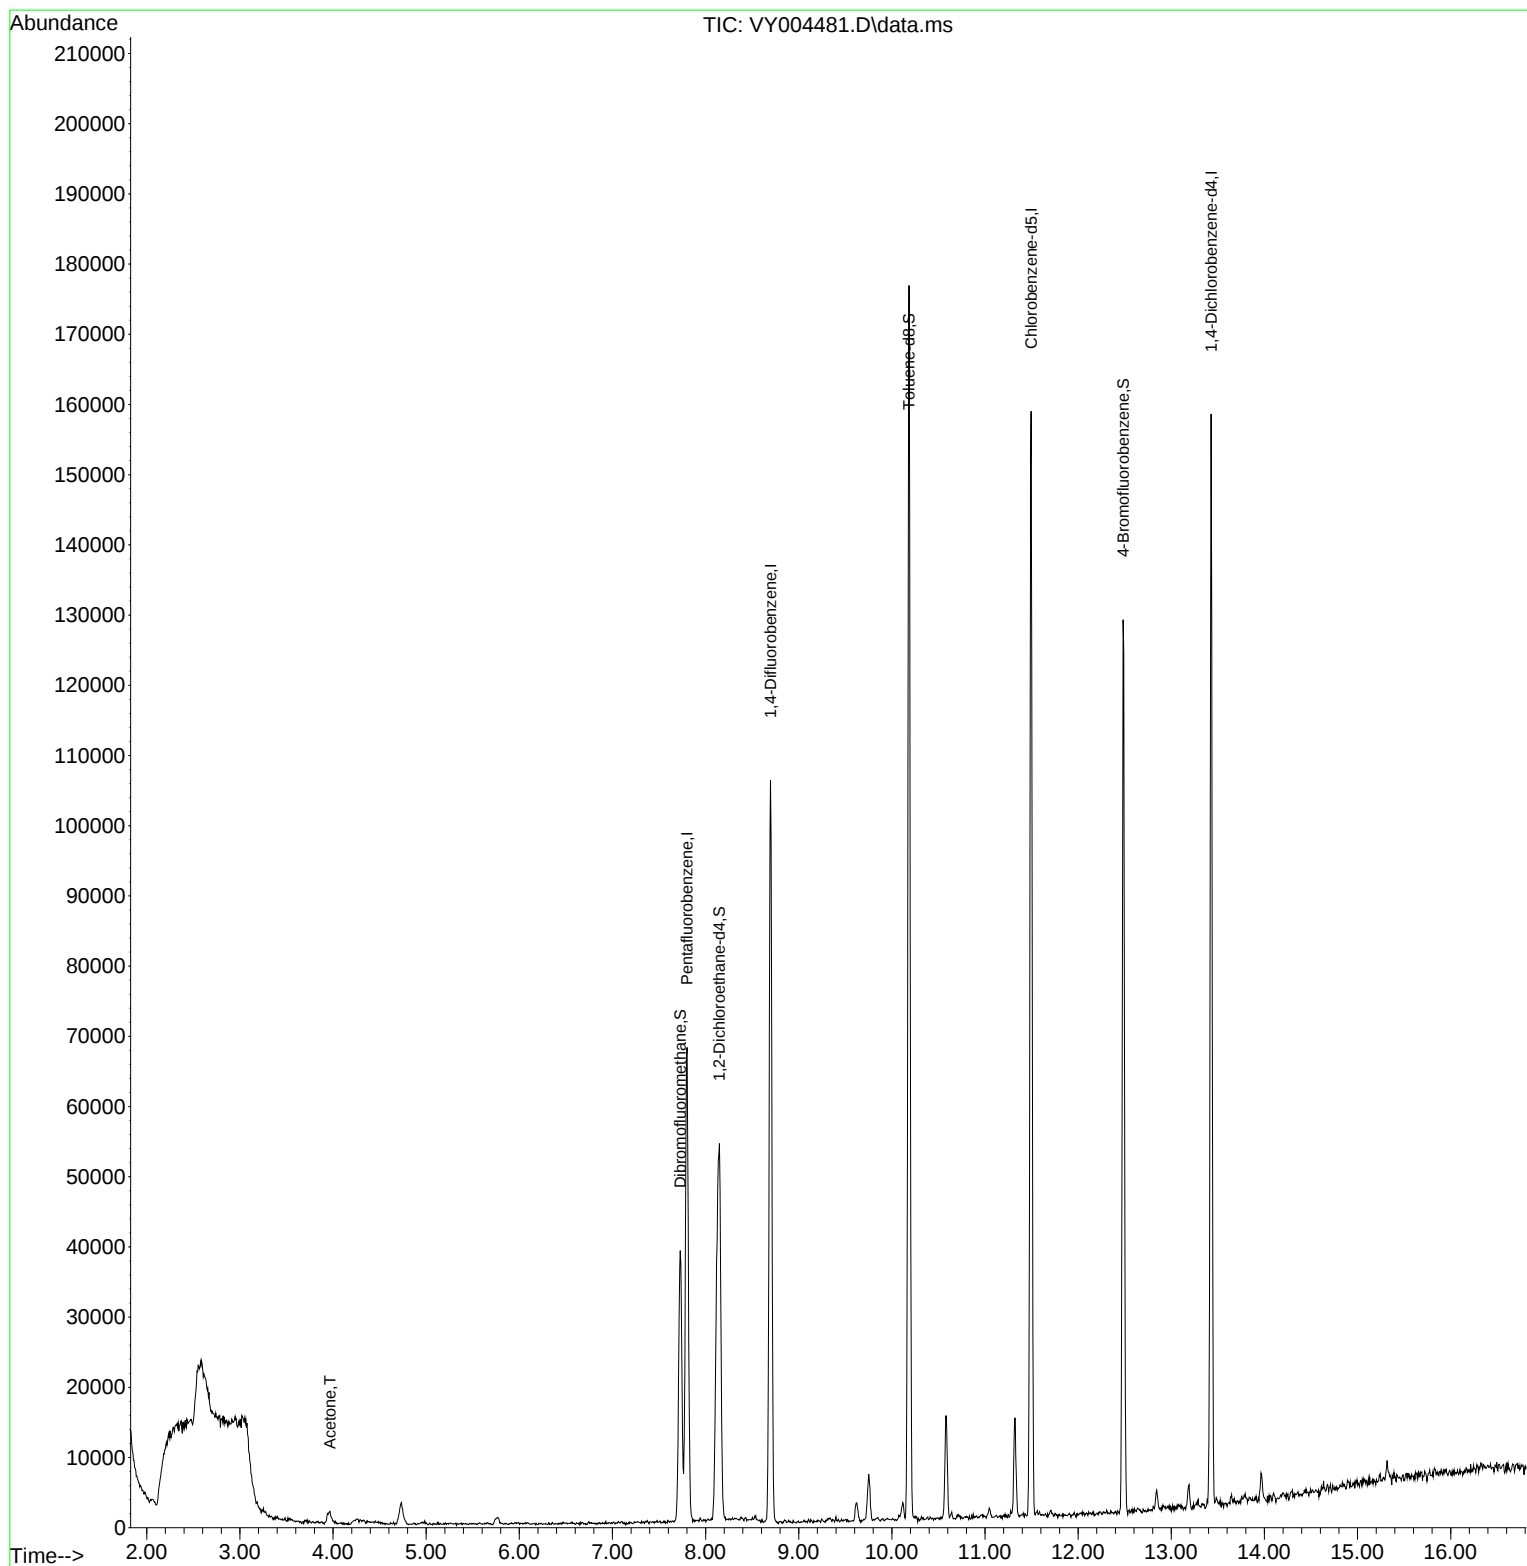



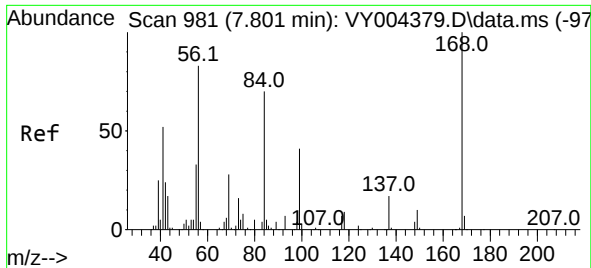


#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.801 min Scan# 981
Delta R.T. 0.000 min
Lab File: VY004481.D
Acq: 16 Apr 2021 19:38


Instrument :
MSVOA_Y
ClientSampleId :
SB-06-0-2.0

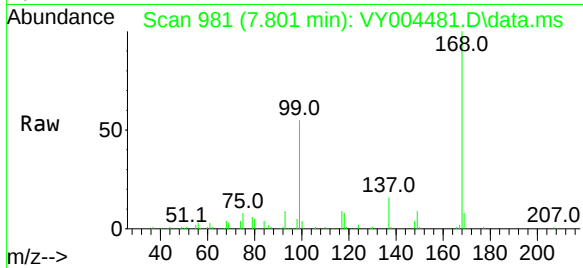



Tgt Ion:168 Resp: 50128
Ion Ratio Lower Upper
168 100
99 54.6 45.5 68.3

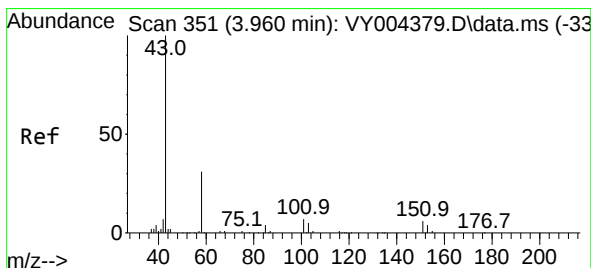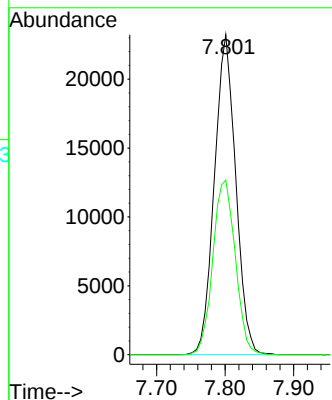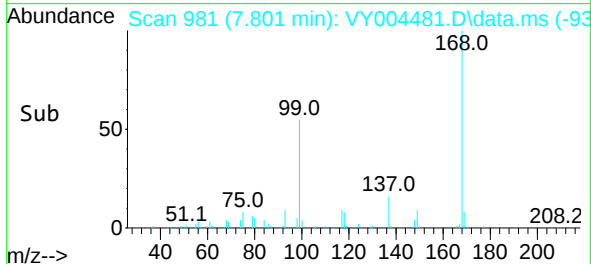


#16
Acetone
Concen: 10.97 ug/l
RT: 3.966 min Scan# 352
Delta R.T. 0.006 min
Lab File: VY004481.D
Acq: 16 Apr 2021 19:38

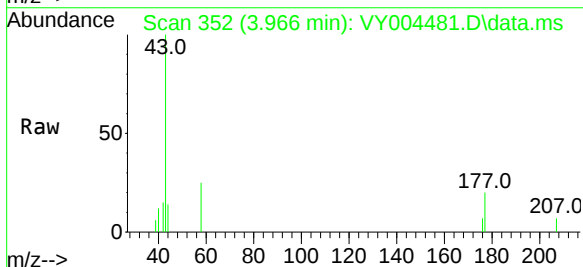

Tgt Ion: 43 Resp: 3471
Ion Ratio Lower Upper
43 100
58 25.5 24.6 37.0



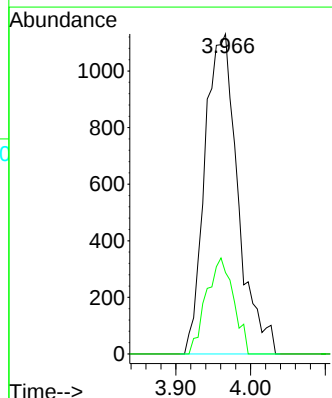
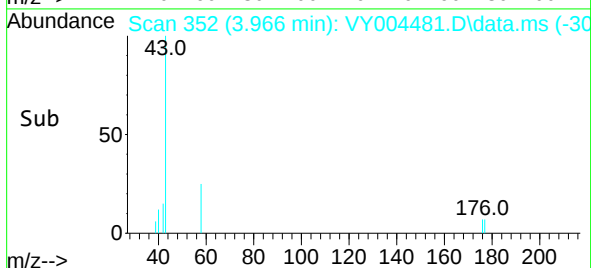


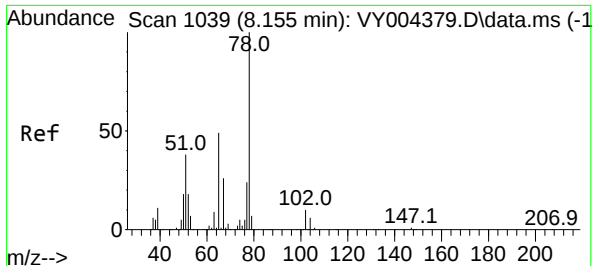

#33
1,2-Dichloroethane-d4
Concen: 56.85 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. -0.006 min
Lab File: VY004481.D
Acq: 16 Apr 2021 19:38




Instrument :
MSVOA_Y
ClientSampleId :
SB-06-0-2.0


Tgt Ion: 65 Resp: 31664
Ion Ratio Lower Upper
65 100
67 54.4 0.0 106.4

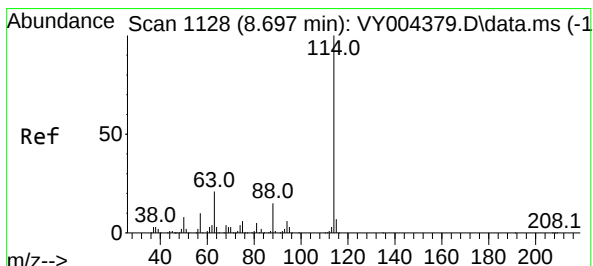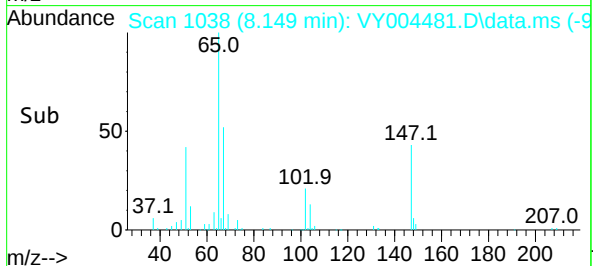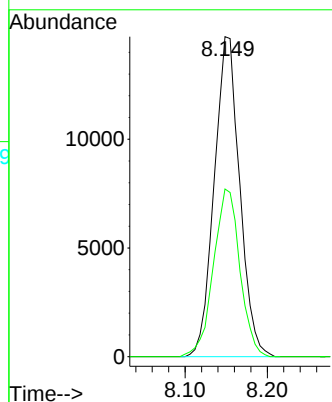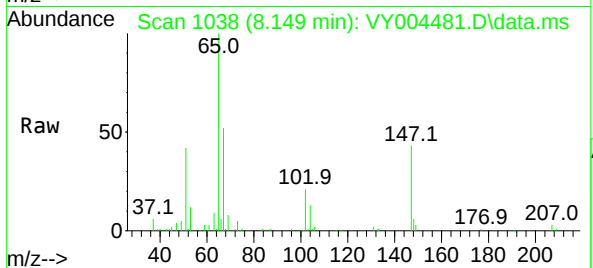

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. 0.000 min
Lab File: VY004481.D
Acq: 16 Apr 2021 19:38


Tgt Ion: 114 Resp: 88268
Ion Ratio Lower Upper
114 100
63 20.1 0.0 42.4
88 14.7 0.0 30.8

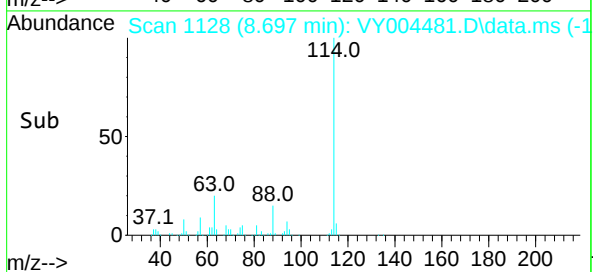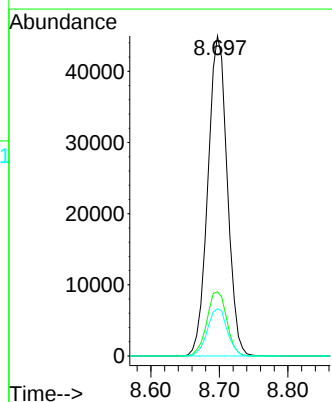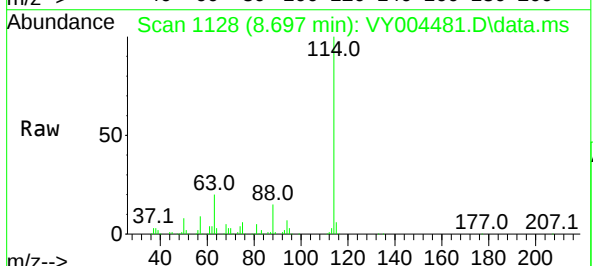



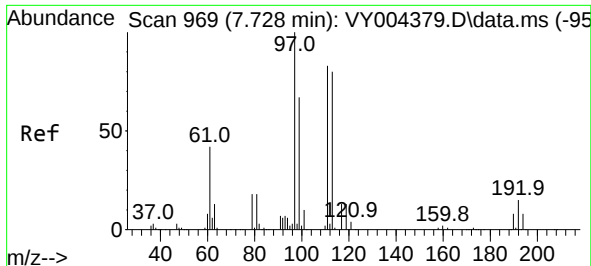


#35
Dibromofluoromethane
Concen: 56.18 ug/l
RT: 7.728 min Scan# 969
Delta R.T. 0.000 min
Lab File: VY004481.D
Acq: 16 Apr 2021 19:38

Instrument :
MSVOA_Y
ClientSampleId :
SB-06-0-2.0



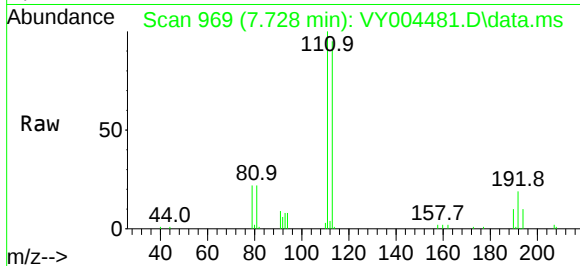



Tgt Ion	Ratio	Lower	Upper
113	100		
111	104.2	82.6	123.8
192	19.6	16.1	24.1

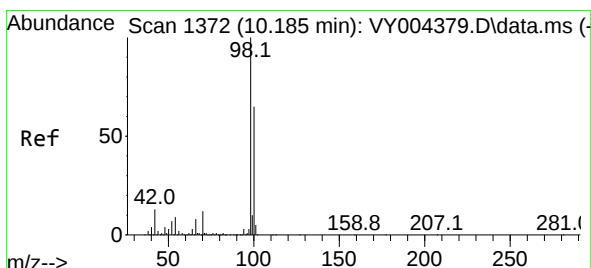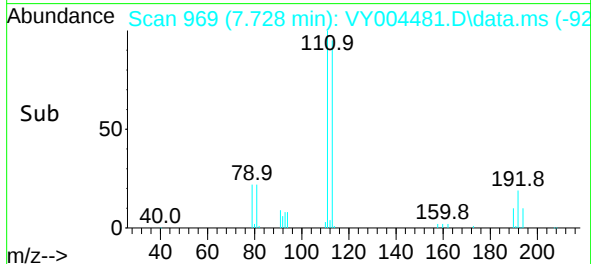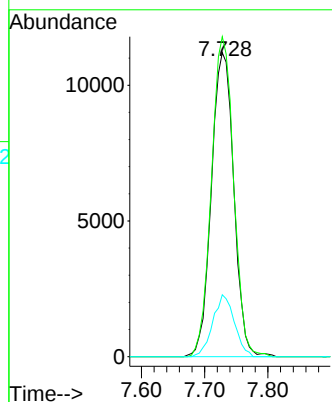

#50
Toluene-d8
Concen: 51.61 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. 0.000 min
Lab File: VY004481.D
Acq: 16 Apr 2021 19:38

Tgt Ion	Ratio	Lower	Upper
98	100		
100	64.4	51.8	77.6


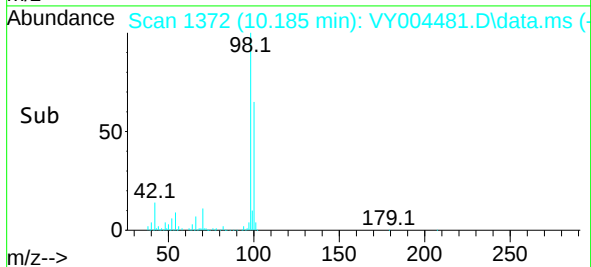
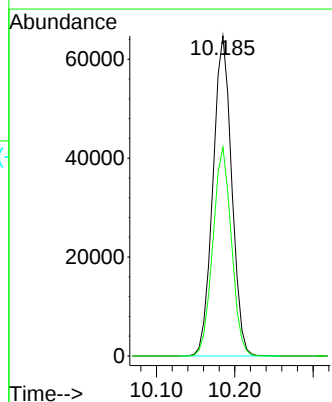
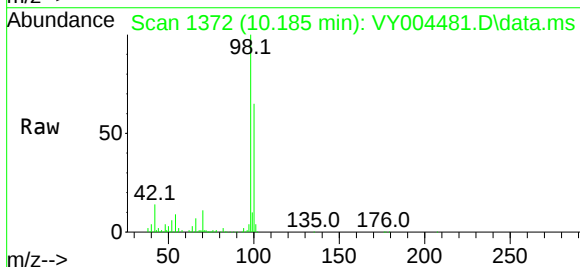


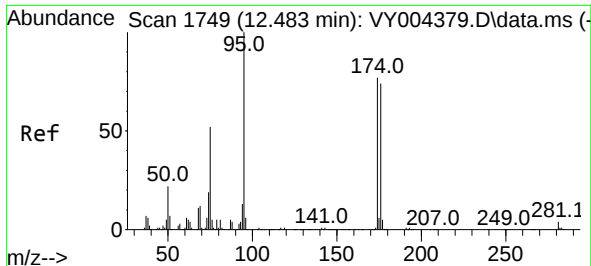

#62
4-Bromofluorobenzene
Concen: 49.73 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY004481.D
Acq: 16 Apr 2021 19:38




Instrument :
MSVOA_Y
ClientSampleId :
SB-06-0-2.0


Tgt Ion: 95 Resp: 35162
Ion Ratio Lower Upper
95 100
174 83.1 0.0 162.4
176 80.7 0.0 156.0

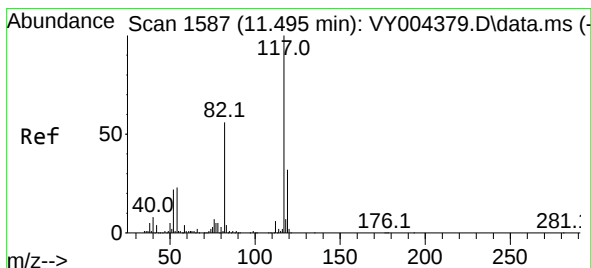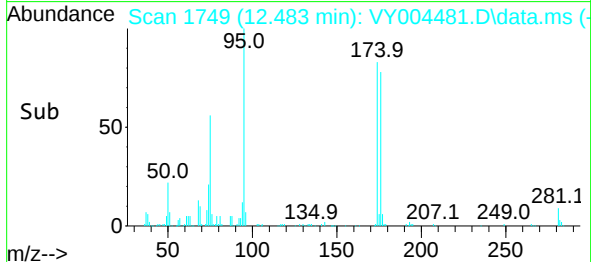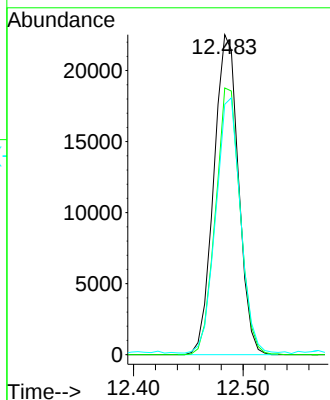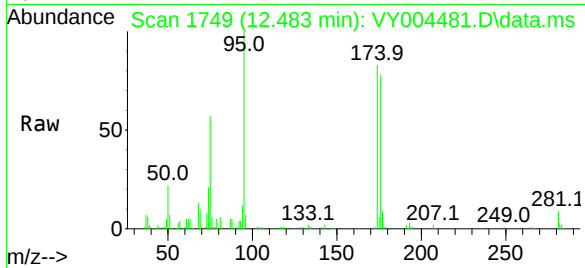

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.495 min Scan# 1587
Delta R.T. 0.000 min
Lab File: VY004481.D
Acq: 16 Apr 2021 19:38

Tgt Ion: 117 Resp: 80658
Ion Ratio Lower Upper
117 100
82 56.5 44.9 67.3
119 32.9 25.4 38.0

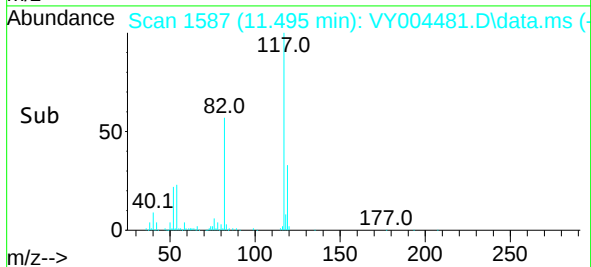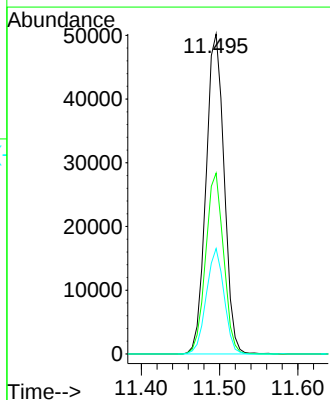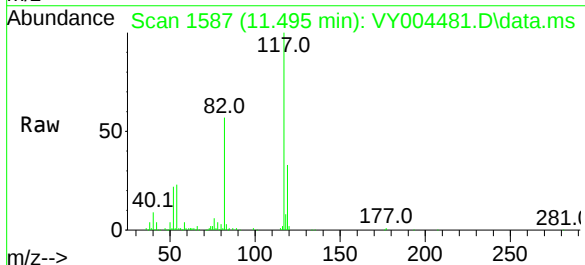

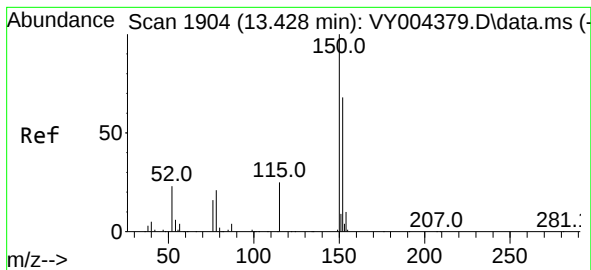

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.00 ug/l
 RT: 13.428 min Scan# 1904
 Delta R.T. 0.000 min
 Lab File: VY004481.D
 Acq: 16 Apr 2021 19:38

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-06-0-2.0

Tgt Ion:152 Resp: 36119
 Ion Ratio Lower Upper
 152 100
 115 59.7 29.6 88.8
 150 156.1 0.0 348.4

