
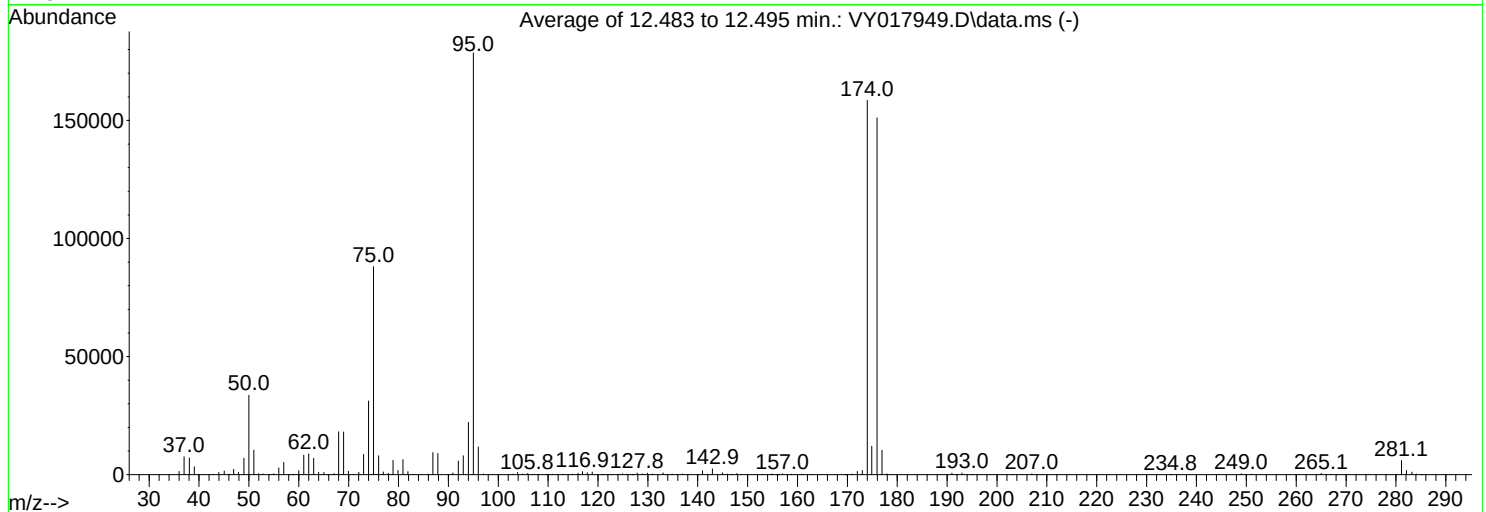


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041724\
Data File : VY017949.D
Acq On : 17 Apr 2024 08:30
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041624S.M
Title : SW846 8260
Last Update : Wed Apr 17 06:24:42 2024

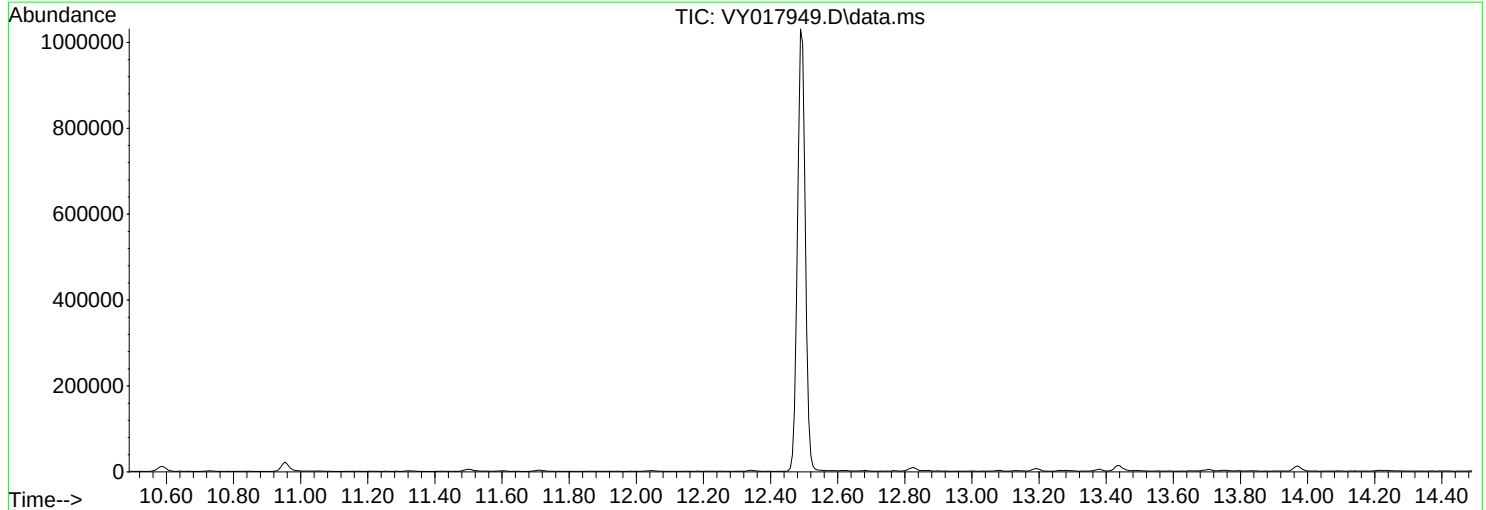

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	33576	PASS
75	95	30	60	49.3	88061	PASS
95	95	100	100	100.0	178624	PASS
96	95	5	9	6.6	11734	PASS
173	174	0.00	2	1.1	1741	PASS
174	95	50	100	88.7	158475	PASS
175	174	5	9	7.6	12023	PASS
176	174	95	101	95.4	151115	PASS
177	176	5	9	6.8	10288	PASS