

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041921\
 Data File : VY004504.D
 Acq On : 19 Apr 2021 17:34
 Operator : SY/MD
 Sample : M2075-28
 Misc : 6.3G/5ML/MSVOA_Y/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-8-D

Quant Time: Apr 20 01:50:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041221S.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 13 03:38:02 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.801	168	136413	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	241070	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.495	117	230075	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	106051	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.148	65	89630	59.14	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 118.28%	
35) Dibromofluoromethane	7.728	113	73641	55.05	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 110.10%	
50) Toluene-d8	10.185	98	299468	52.63	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 105.26%	
62) 4-Bromofluorobenzene	12.483	95	103653	53.68	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 107.36%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041921\
Data File : VY004504.D
Acq On : 19 Apr 2021 17:34
Operator : SY/MD
Sample : M2075-28
Misc : 6.3G/5ML/MSVOA_Y/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TP-8-D

Quant Time: Apr 20 01:50:16 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041221S.M
Quant Title : SW846 8260
QLast Update : Tue Apr 13 03:38:02 2021
Response via : Initial Calibration




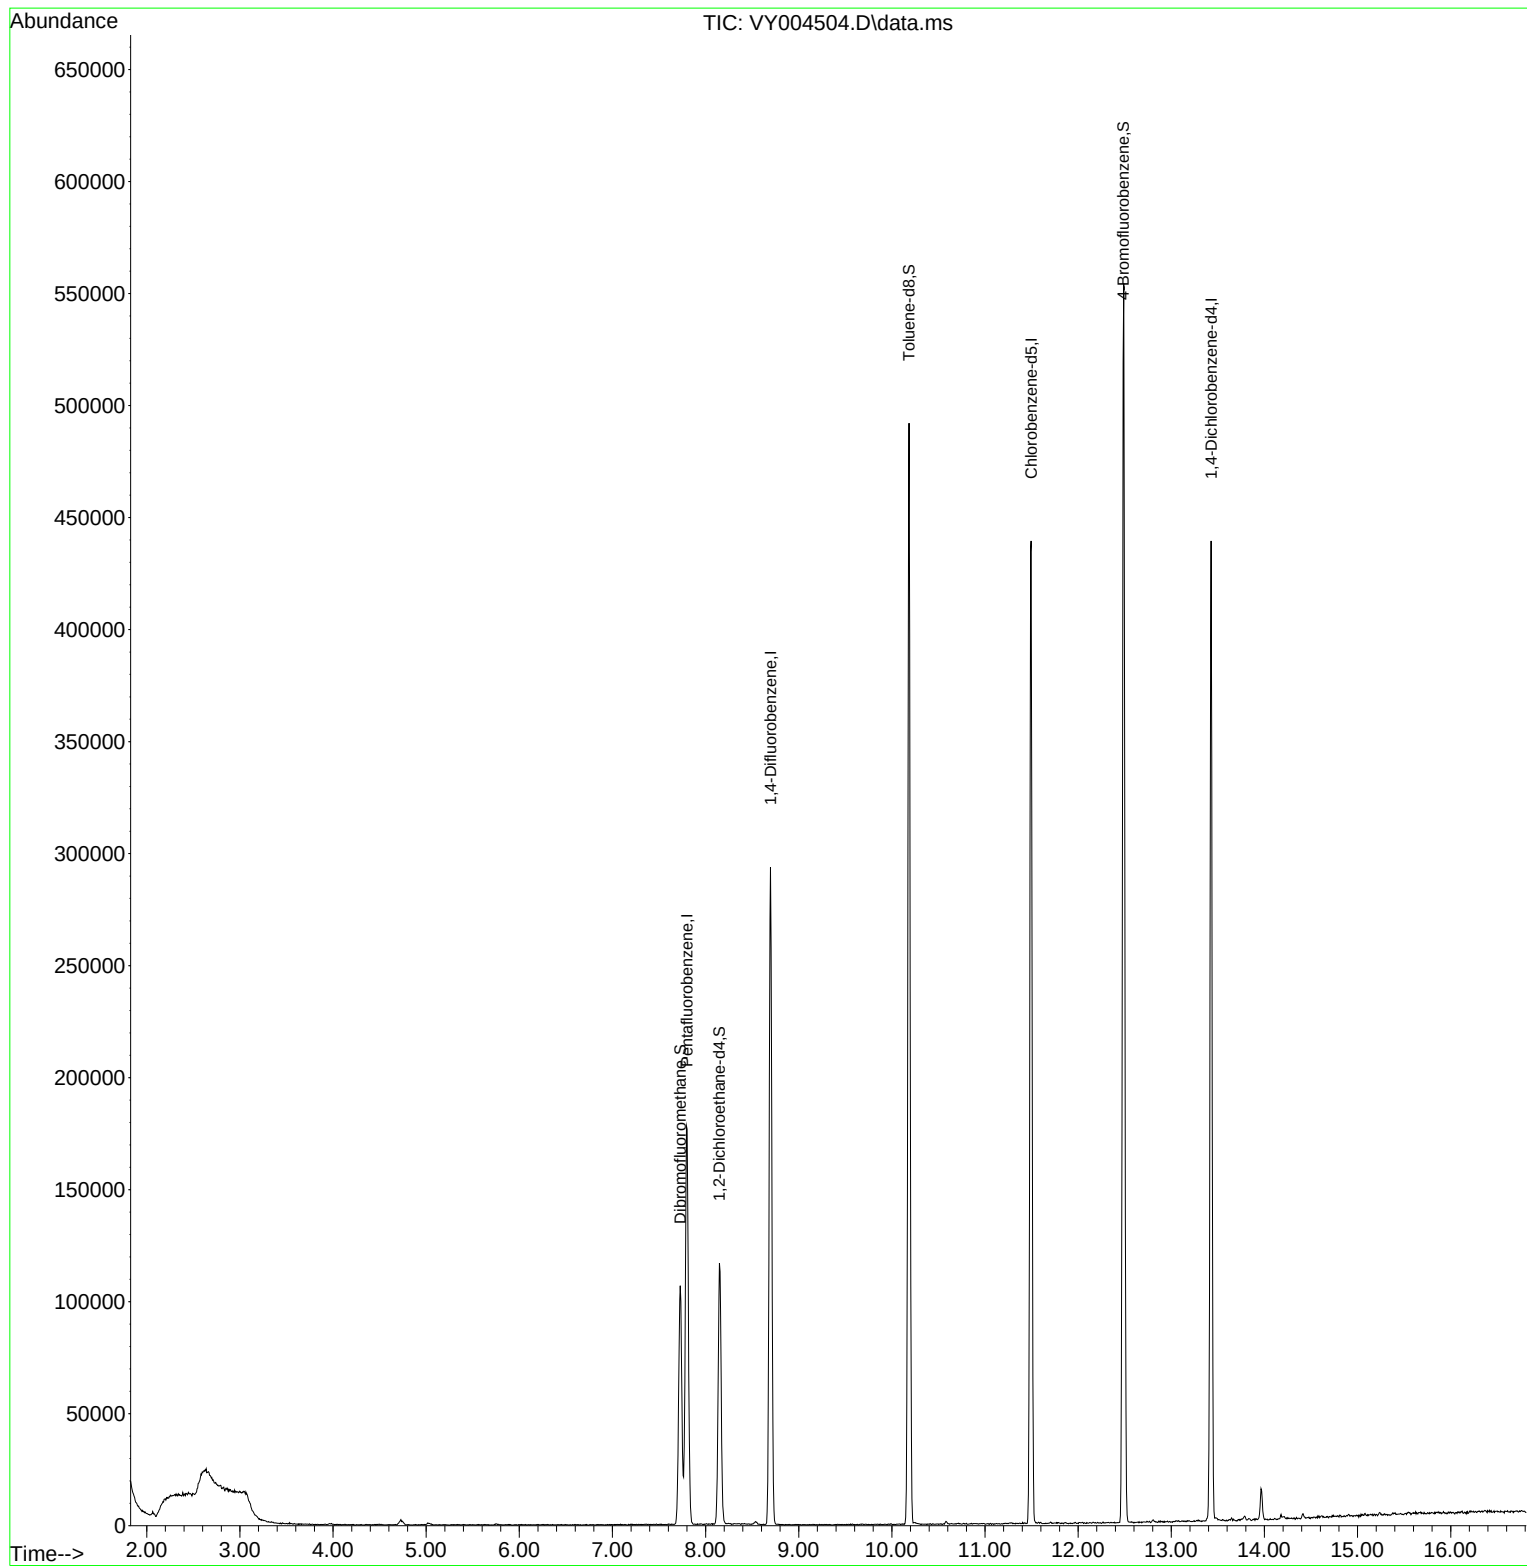


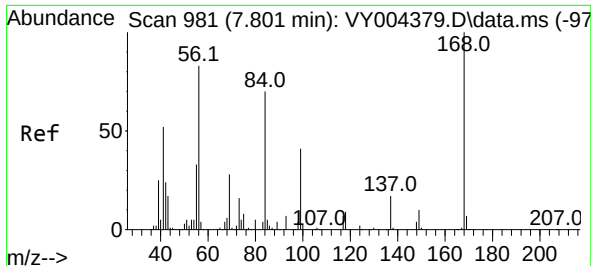

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.801 min Scan# 981
Delta R.T. -0.000 min
Lab File: VY004504.D
Acq: 19 Apr 2021 17:34




Instrument :
MSVOA_Y
ClientSampleId :
TP-8-D


Tgt Ion:168 Resp: 136413
Ion Ratio Lower Upper
168 100
99 55.0 45.5 68.3

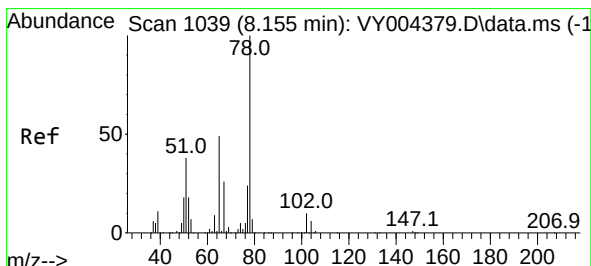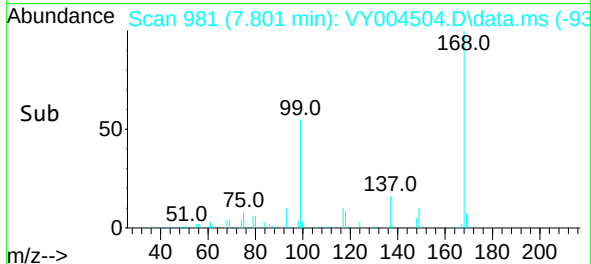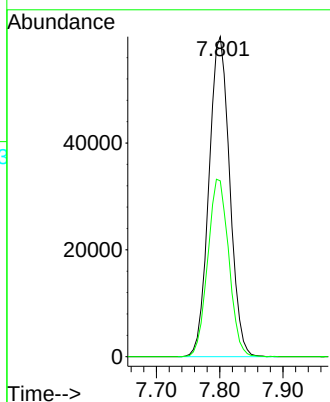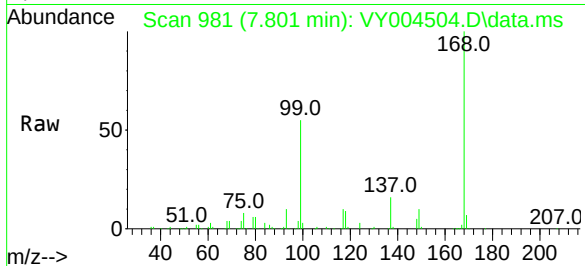

#33
1,2-Dichloroethane-d4
Concen: 59.14 ug/l
RT: 8.148 min Scan# 1038
Delta R.T. -0.006 min
Lab File: VY004504.D
Acq: 19 Apr 2021 17:34

Tgt Ion: 65 Resp: 89630
Ion Ratio Lower Upper
65 100
67 53.0 0.0 106.4


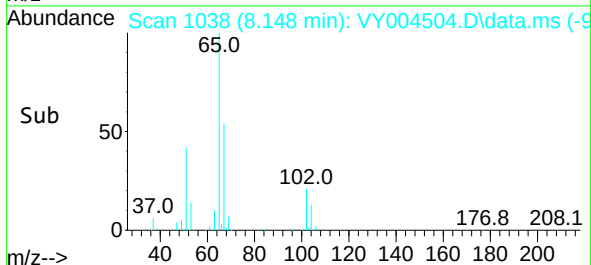
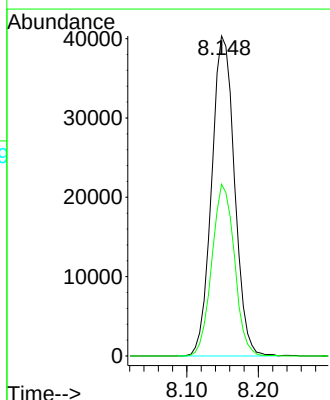
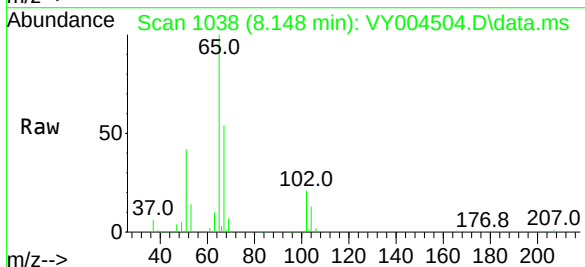


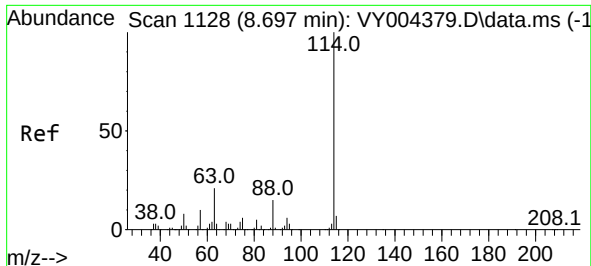

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. 0.000 min
Lab File: VY004504.D
Acq: 19 Apr 2021 17:34




Instrument :
MSVOA_Y
ClientSampled :
TP-8-D


Tgt Ion:114 Resp: 241070
Ion Ratio Lower Upper
114 100
63 21.5 0.0 42.4
88 15.6 0.0 30.8

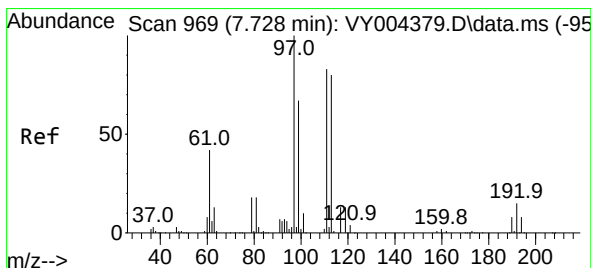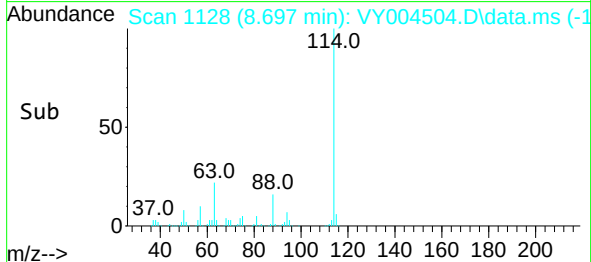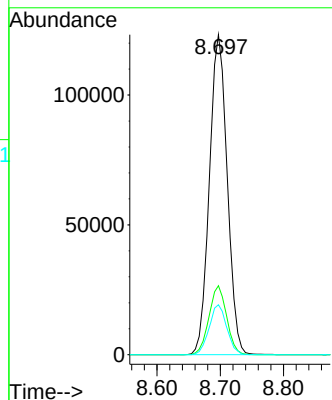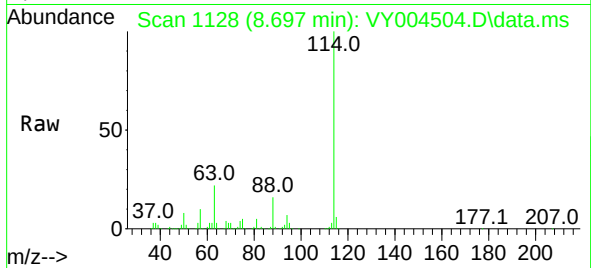

#35
Dibromofluoromethane
Concen: 55.05 ug/l
RT: 7.728 min Scan# 969
Delta R.T. 0.000 min
Lab File: VY004504.D
Acq: 19 Apr 2021 17:34

Tgt Ion:113 Resp: 73641
Ion Ratio Lower Upper
113 100
111 103.5 82.6 123.8
192 19.5 16.1 24.1


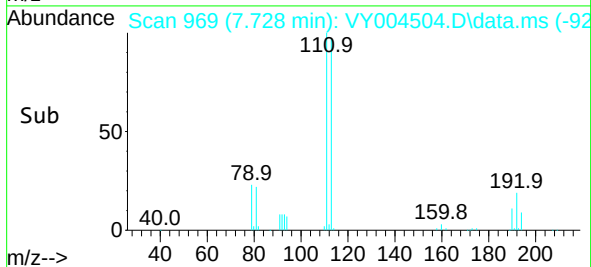
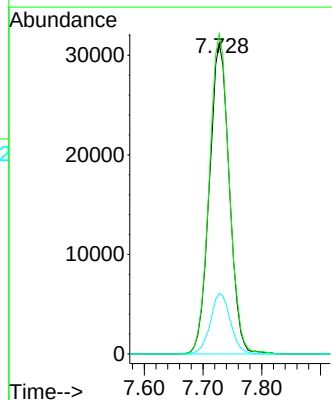
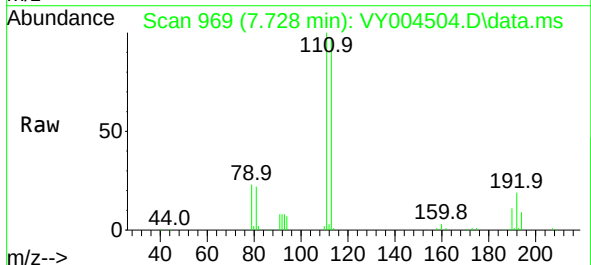


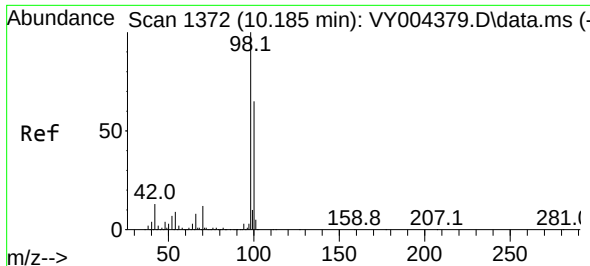

#50
Toluene-d8
Concen: 52.63 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. 0.000 min
Lab File: VY004504.D
Acq: 19 Apr 2021 17:34




Instrument :
MSVOA_Y
ClientSampled :
TP-8-D


Tgt Ion: 98 Resp: 299468
Ion Ratio Lower Upper
98 100
100 64.9 51.8 77.6

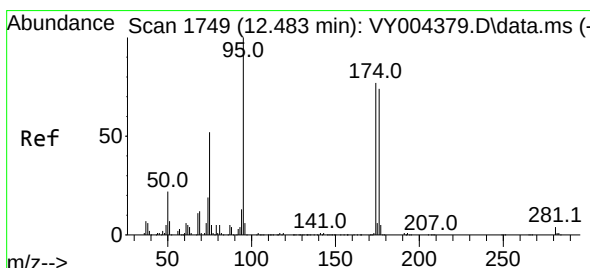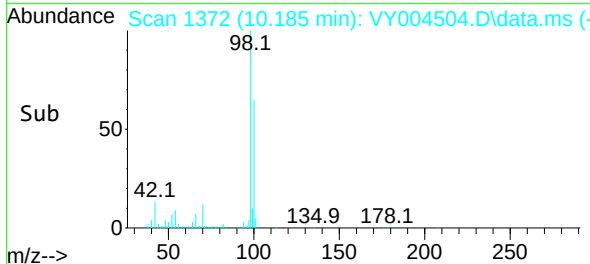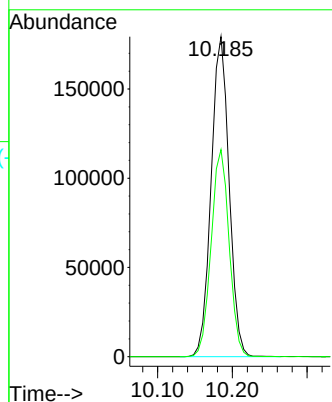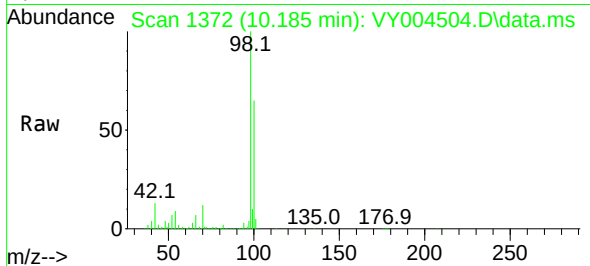

#62
4-Bromofluorobenzene
Concen: 53.68 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY004504.D
Acq: 19 Apr 2021 17:34

Tgt Ion: 95 Resp: 103653
Ion Ratio Lower Upper
95 100
174 83.1 0.0 162.4
176 81.1 0.0 156.0


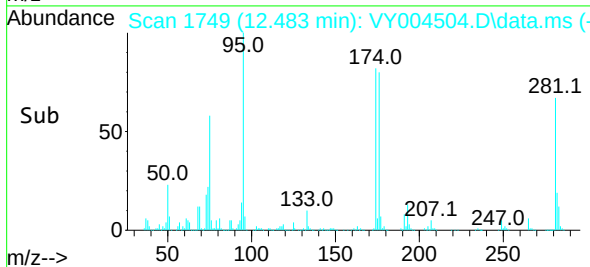
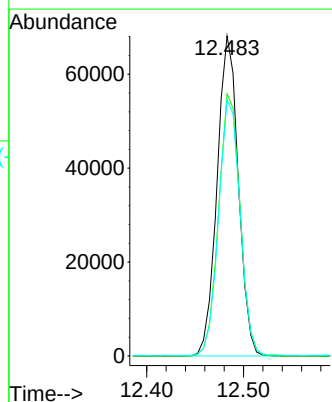
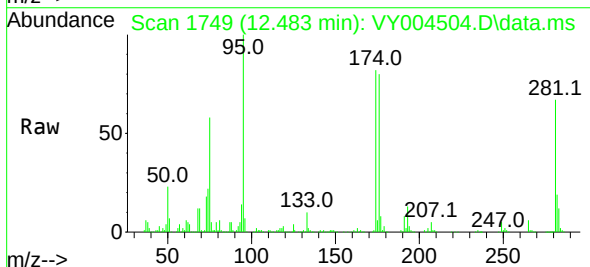


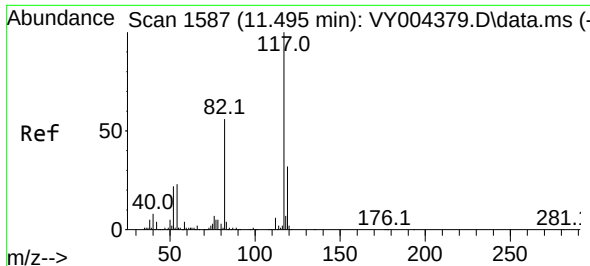

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.495 min Scan# 1587
Delta R.T. 0.000 min
Lab File: VY004504.D
Acq: 19 Apr 2021 17:34

Instrument :
MSVOA_Y
ClientSampled :
TP-8-D

Tgt Ion:	117	Resp:	230075
Ion	Ratio	Lower	Upper
117	100		
82	53.5	44.9	67.3
119	31.4	25.4	38.0

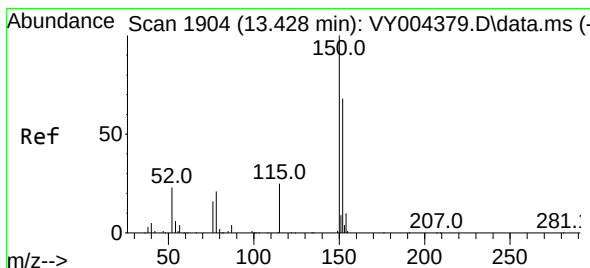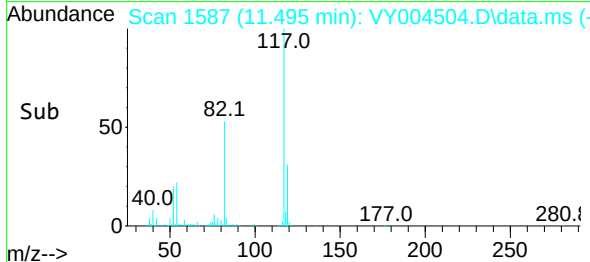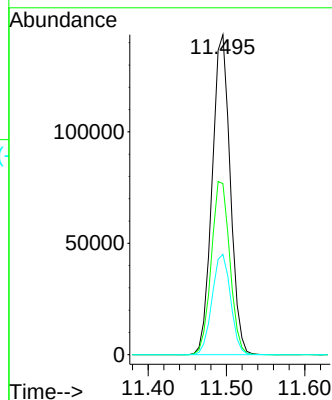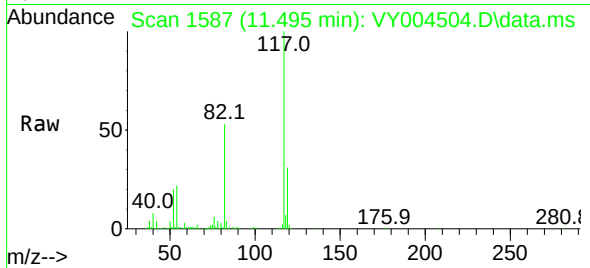

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY004504.D
Acq: 19 Apr 2021 17:34

Tgt Ion:	152	Resp:	106051
Ion	Ratio	Lower	Upper
152	100		
115	58.1	29.6	88.8
150	155.7	0.0	348.4

