
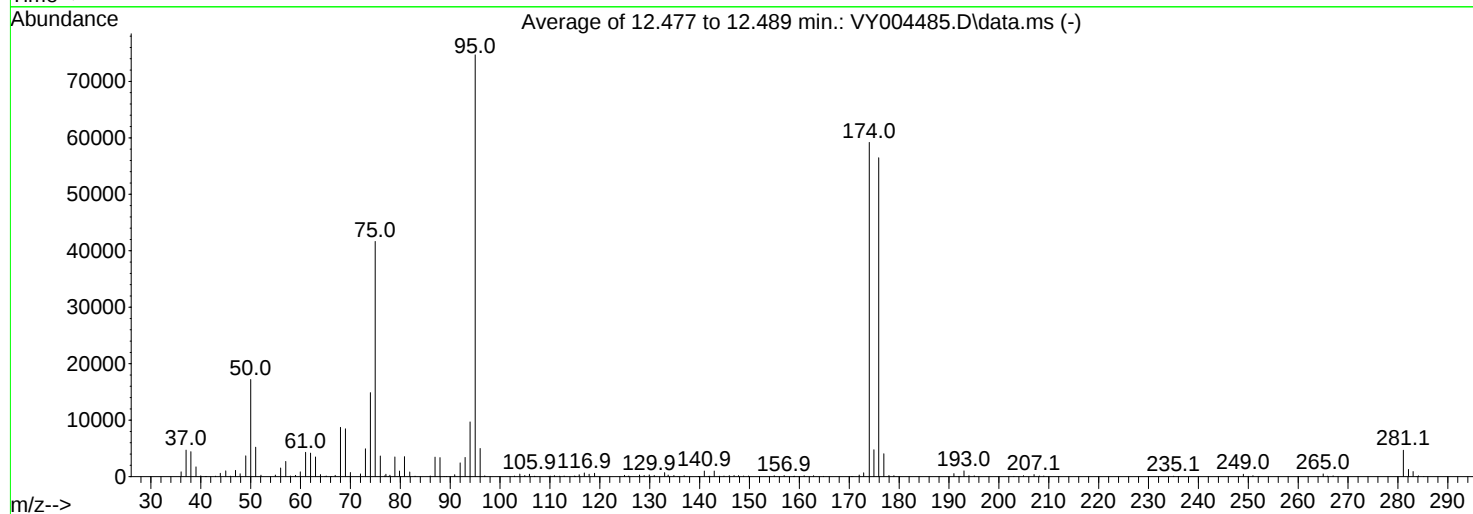


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041921\
Data File : VY004485.D
Acq On : 19 Apr 2021 09:20
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041221S.M
Title : SW846 8260
Last Update : Tue Apr 13 03:38:02 2021

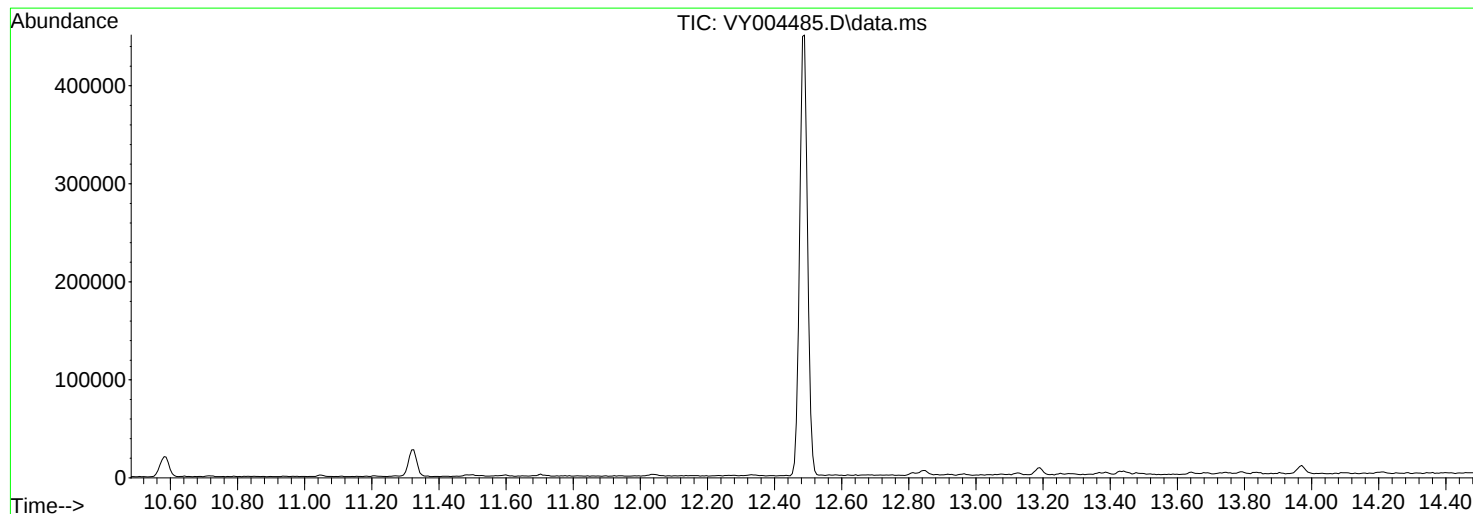

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.0	17192	PASS
75	95	30	60	55.8	41645	PASS
95	95	100	100	100.0	74699	PASS
96	95	5	9	6.7	5000	PASS
173	174	0.00	2	1.2	685	PASS
174	95	50	100	79.2	59195	PASS
175	174	5	9	8.0	4761	PASS
176	174	95	101	95.4	56468	PASS
177	176	5	9	7.2	4054	PASS