

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041922\
 Data File : VY008405.D
 Acq On : 19 Apr 2022 18:51
 Operator : KP/MD
 Sample : N2468-05
 Misc : 5.02g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 WC-15-1-7-GR

Quant Time: Apr 20 06:31:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y040822S.M
 Quant Title : SW846 8260
 QLast Update : Fri Apr 08 16:02:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	99688	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	162596	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	153864	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	58396	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	50586	54.022	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 108.040%			
35) Dibromofluoromethane	7.722	113	54550	58.086	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 116.180%			
50) Toluene-d8	10.179	98	205740	64.024	ug/l	0.00
Spiked Amount 50.000	Range 49 - 140		Recovery = 128.040%			
62) 4-Bromofluorobenzene	12.483	95	63320	52.388	ug/l	0.00
Spiked Amount 50.000	Range 25 - 144		Recovery = 104.780%			
Target Compounds						
					Qvalue	
3) Chloromethane	2.107	50	711	Below Cal	#	80
5) Bromomethane	2.656	94	161	Below Cal	#	53
16) Acetone	3.930	43	1514	6.722	ug/l #	47
17) Carbon Disulfide	4.186	76	26268	10.127	ug/l	99
18) Methyl Acetate	4.533	43	1701	Below Cal	#	56
20) Methylene Chloride	4.710	84	4509	Below Cal		90
25) 2-Butanone	7.021	43	7352	20.876	ug/l #	87
31) Cyclohexane	7.783	56	9246	5.460	ug/l #	55
36) 1,1-Dichloropropene	7.783	75	7838	5.227	ug/l #	53
37) Ethyl Acetate	7.021	43	7352	9.508	ug/l #	72
38) Carbon Tetrachloride	7.789	117	10008	6.203	ug/l #	15
39) Methylcyclohexane	9.179	83	22405	11.612	ug/l	90
40) Benzene	8.161	78	19246	4.310	ug/l	97
48) Methyl methacrylate	9.240	41	1054	1.728	ug/l #	50
51) 4-Methyl-2-Pentanone	10.081	43	1051	1.418	ug/l	95
52) Toluene	10.246	92	52770	17.935	ug/l	96
55) 1,1,2-Trichloroethane	10.618	97	4773	4.634	ug/l #	18
56) Ethyl methacrylate	10.520	69	2299	1.821	ug/l #	20
59) 2-Hexanone	10.801	43	7859	15.413	ug/l #	32
68) m/p-Xylenes	11.697	106	2894	1.282	ug/l	88
73) Isopropylbenzene	12.331	105	4858	1.119	ug/l	99
74) N-amyl acetate	12.123	43	14155	15.017	ug/l #	68
75) 1,1,2,2-Tetrachloroethane	12.556	83	2094	2.279	ug/l #	45
76) 1,2,3-Trichloropropane	12.483	75	34576	53.536	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.812	105	6708	1.884	ug/l	96
81) trans-1,4-Dichloro-2-b...	12.483	75	34576	119.785	ug/l #	9
84) 1,2,4-Trimethylbenzene	13.123	105	19751	5.606	ug/l	99
85) sec-Butylbenzene	13.257	105	6904	1.458	ug/l	90
90) Hexachloroethane	13.971	117	755	1.022	ug/l #	6
95) Naphthalene	15.239	128	5112	2.152	ug/l #	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041922\
Data File : VY008405.D
Acq On : 19 Apr 2022 18:51
Operator : KP/MD
Sample : N2468-05
Misc : 5.02g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
WC-15-1-7-GR

Quant Time: Apr 20 06:31:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y040822S.M
Quant Title : SW846 8260
QLast Update : Fri Apr 08 16:02:50 2022
Response via : Initial Calibration




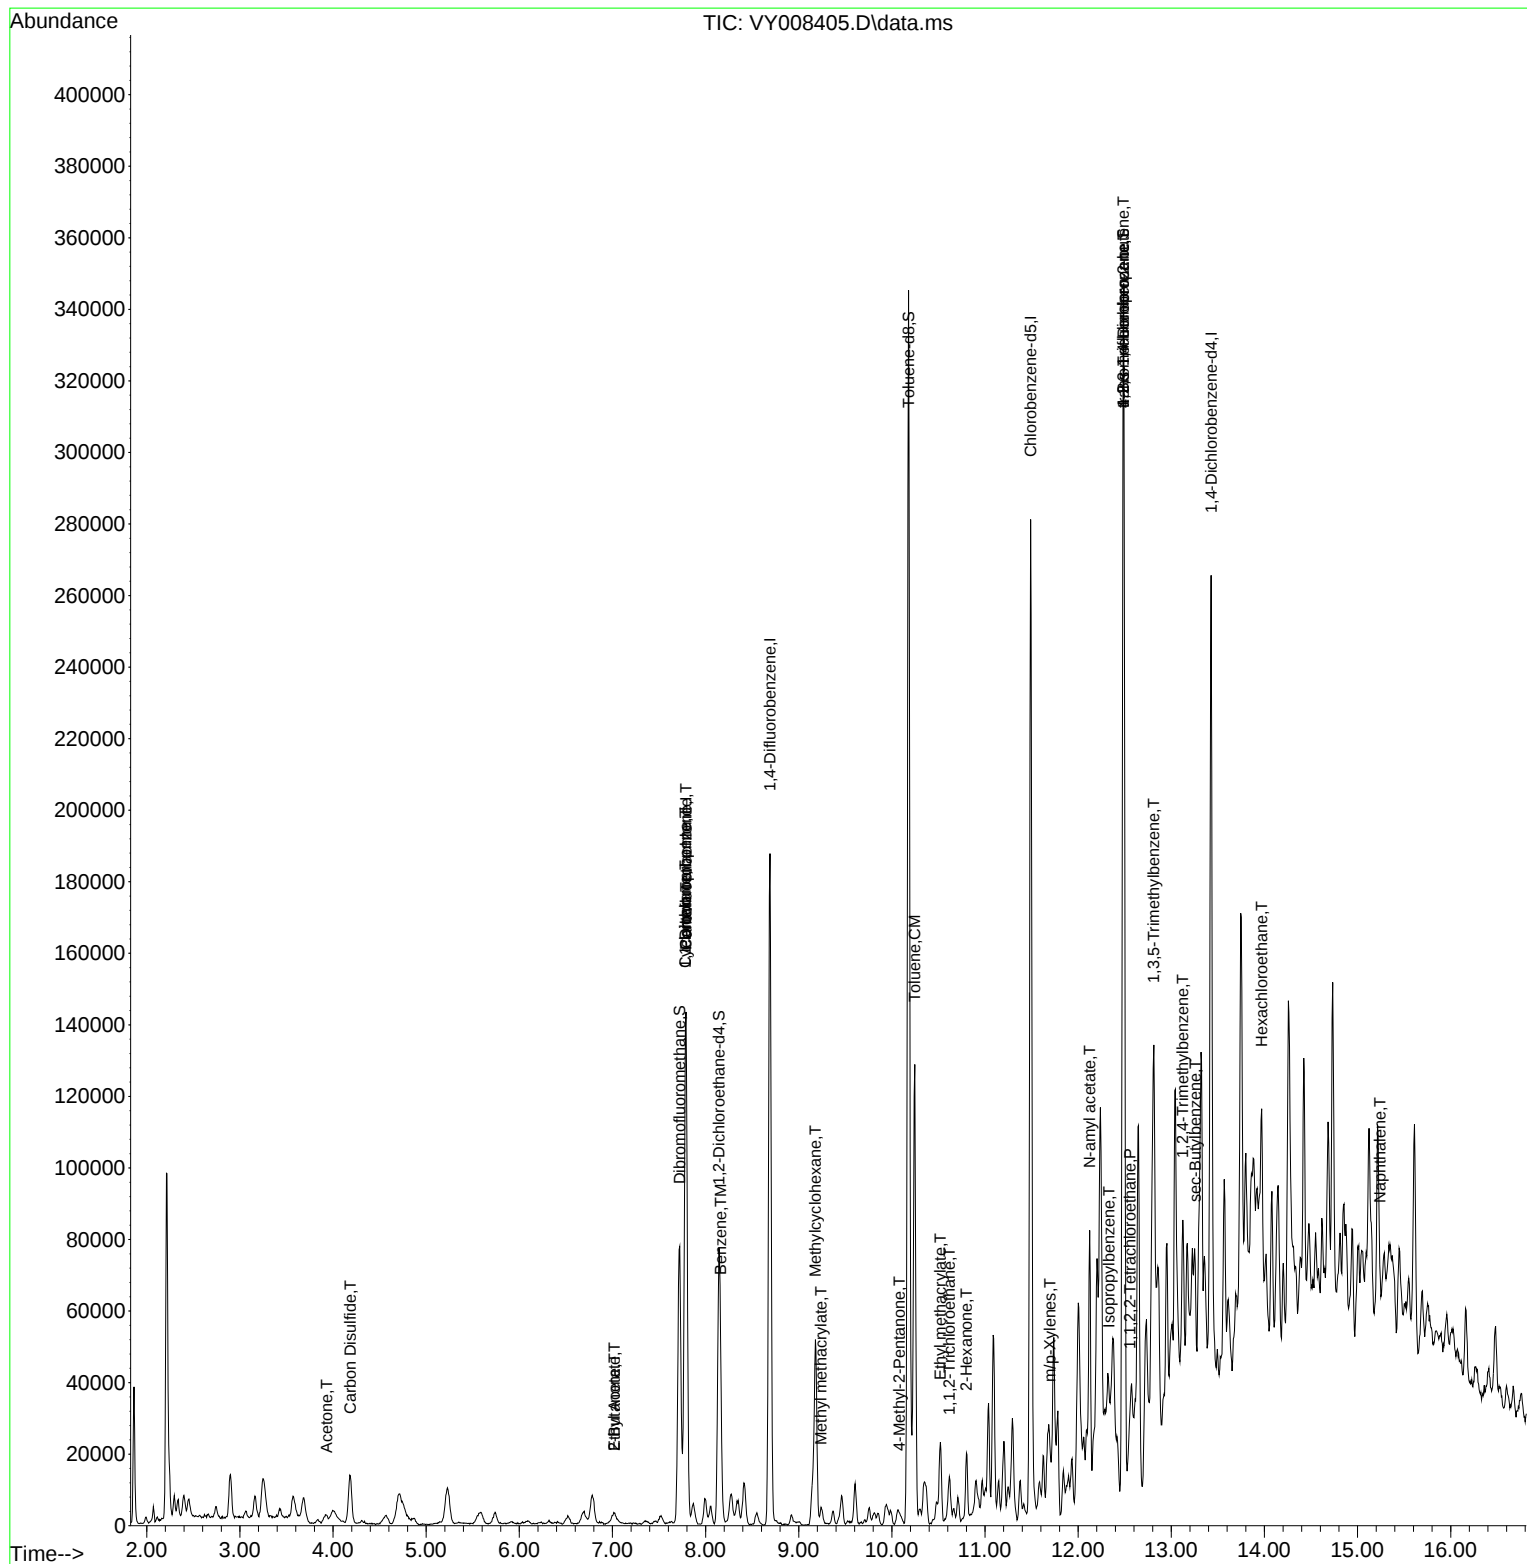




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51




Instrument :
MSVOA_Y
ClientSampleId :
WC-15-1-7-GR


Tgt Ion:168 Resp: 99688
Ion Ratio Lower Upper
168 100
99 54.4 46.9 70.3

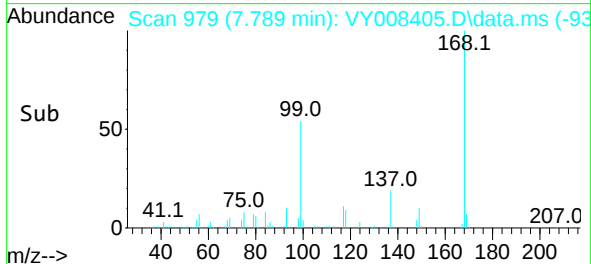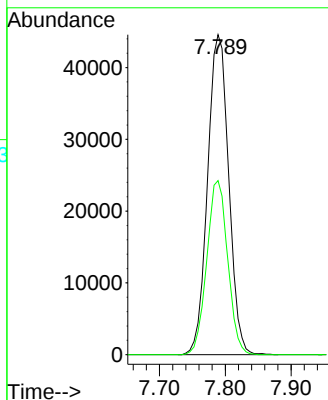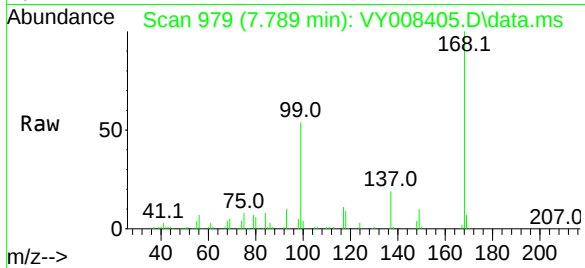

#3
Chloromethane
Concen: Below Cal
RT: 2.107 min Scan# 47
Delta R.T. -0.006 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51

Tgt Ion: 50 Resp: 711
Ion Ratio Lower Upper
50 100
52 41.8 24.6 37.0#


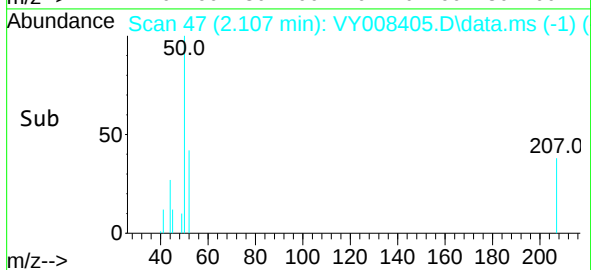
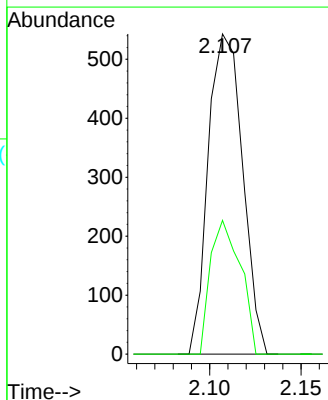
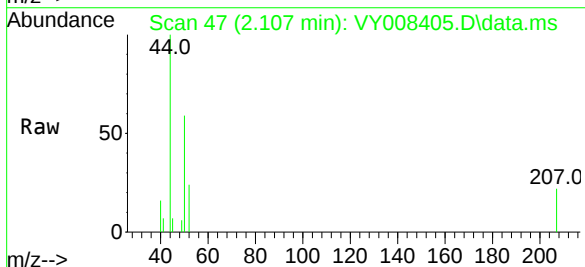




#5
Bromomethane
Concen: Below Cal
RT: 2.656 min Scan# 11
Delta R.T. 0.007 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51




Instrument :
MSVOA_Y
ClientSampleId :
WC-15-1-7-GR


Tgt Ion: 94 Resp: 161
Ion Ratio Lower Upper
94 100
96 137.0 73.5 110.3#

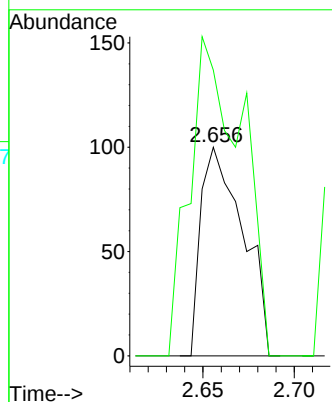

#16
Acetone
Concen: 6.722 ug/l
RT: 3.930 min Scan# 346
Delta R.T. -0.012 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51

Tgt Ion: 43 Resp: 1514
Ion Ratio Lower Upper
43 100
58 0.0 22.0 33.0#


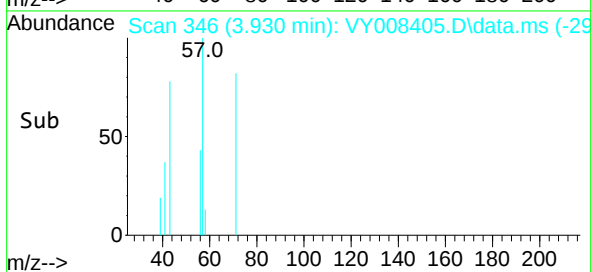
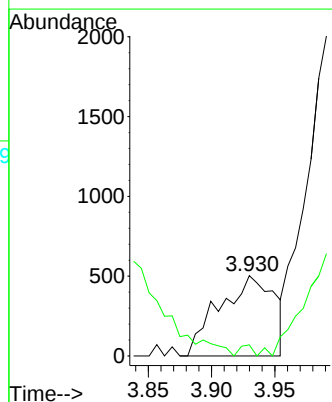





#17
Carbon Disulfide
Concen: 10.127 ug/l
RT: 4.186 min Scan# 311
Delta R.T. -0.006 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51




Instrument :
MSVOA_Y
ClientSampleId :
WC-15-1-7-GR


Tgt Ion: 76 Resp: 26268
Ion Ratio Lower Upper
76 100
78 8.9 7.4 11.0

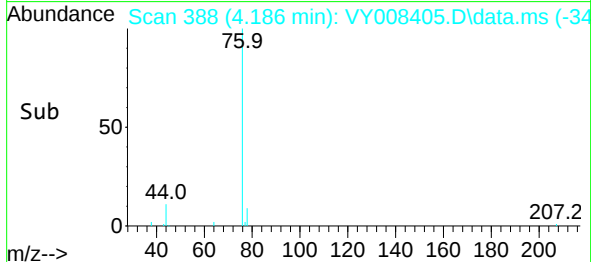

#18
Methyl Acetate
Concen: Below Cal
RT: 4.533 min Scan# 445
Delta R.T. 0.055 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51

Tgt Ion: 43 Resp: 1701
Ion Ratio Lower Upper
43 100
74 0.0 16.6 24.8#

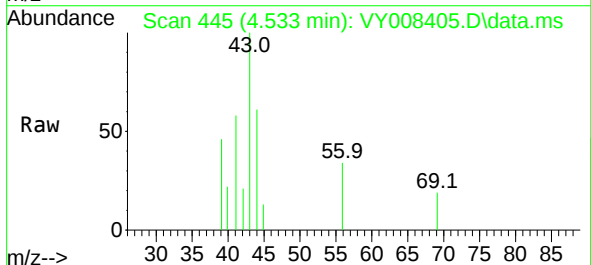







#20
Methylene Chloride
Concen: Below Cal
RT: 4.710 min Scan# 41
Delta R.T. 0.000 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51

Instrument :
MSVOA_Y
ClientSampleId :
WC-15-1-7-GR

Tgt Ion: 84 Resp: 4509




Ion	Ratio	Lower	Upper
84	100		
49	126.4	114.4	171.6
51	40.6	35.3	52.9
86	62.2	53.7	80.5

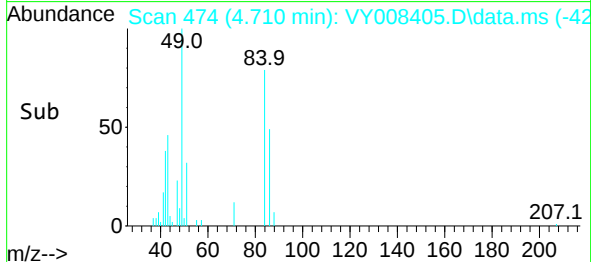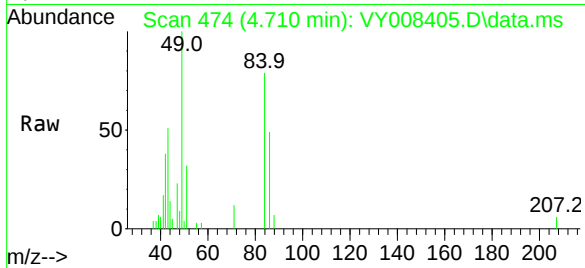


#25
2-Butanone
Concen: 20.876 ug/l
RT: 7.021 min Scan# 853
Delta R.T. 0.037 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51

Tgt Ion: 43 Resp: 7352

Ion	Ratio	Lower	Upper
43	100		
72	28.3	17.7	26.5




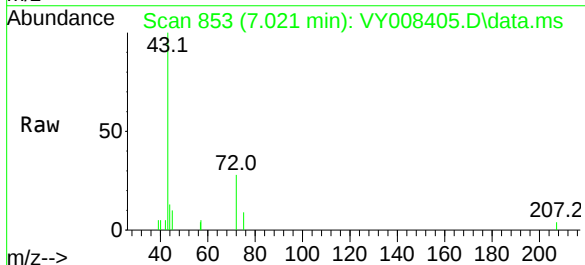




#31
Cyclohexane
Concen: 5.460 ug/l
RT: 7.783 min Scan# 91
Delta R.T. 0.001 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51




Instrument :
MSVOA_Y
ClientSampleId :
WC-15-1-7-GR


Tgt Ion: 56 Resp: 9246
Ion Ratio Lower Upper
56 100
69 66.3 26.7 40.1#
84 120.7 67.2 100.8#

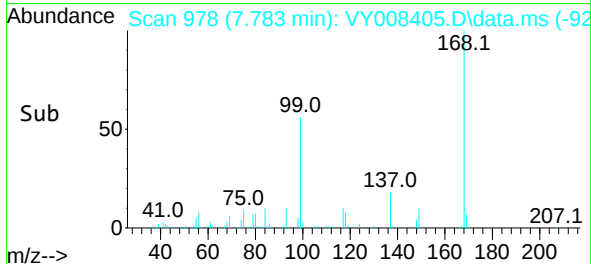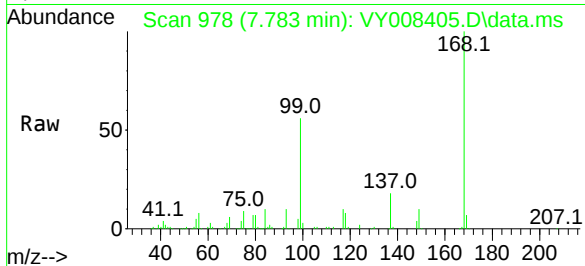

#33
1,2-Dichloroethane-d4
Concen: 54.022 ug/l
RT: 8.142 min Scan# 1037
Delta R.T. 0.000 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51

Tgt Ion: 65 Resp: 50586
Ion Ratio Lower Upper
65 100
67 53.8 0.0 99.4




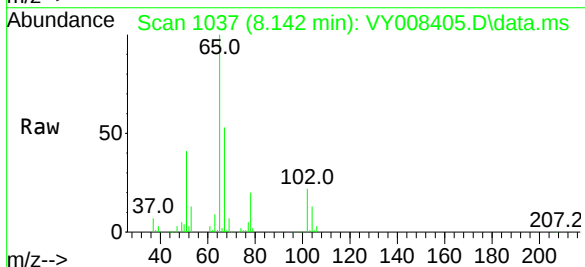




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.691 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51




Instrument :
MSVOA_Y
ClientSampleId :
WC-15-1-7-GR


Tgt Ion:114 Resp: 162596
Ion Ratio Lower Upper
114 100
63 18.8 0.0 43.2
88 14.3 0.0 31.8

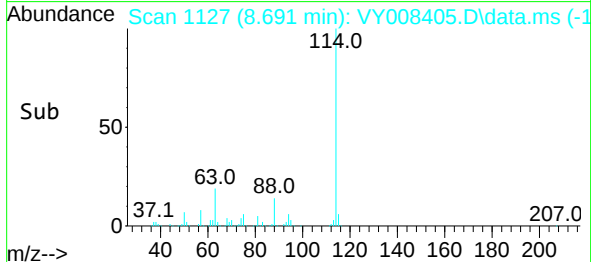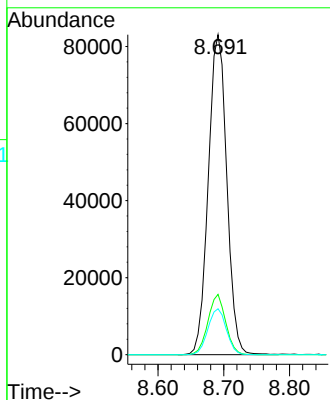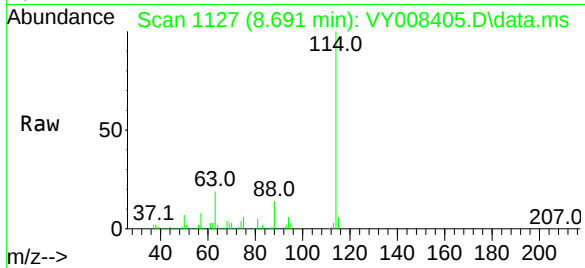

#35
Dibromofluoromethane
Concen: 58.086 ug/l
RT: 7.722 min Scan# 968
Delta R.T. 0.007 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51

Tgt Ion:113 Resp: 54550
Ion Ratio Lower Upper
113 100
111 102.7 82.6 124.0
192 18.6 17.6 26.4


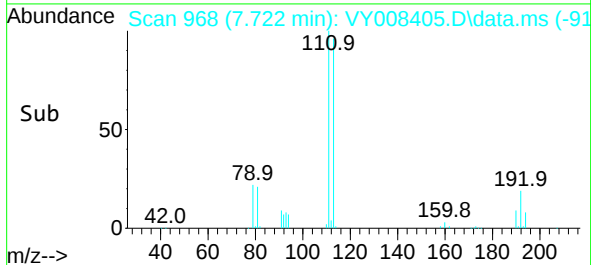
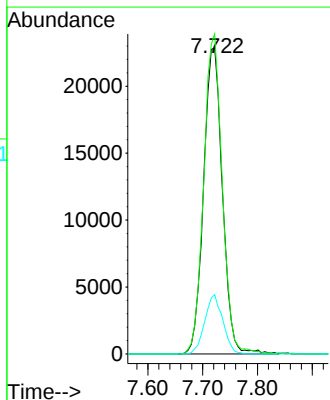
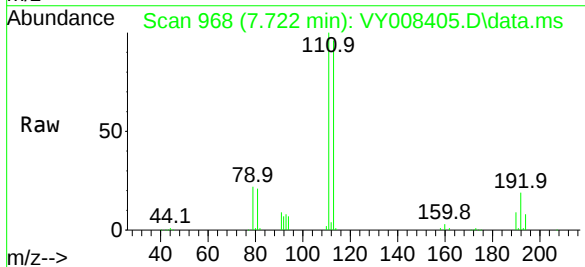


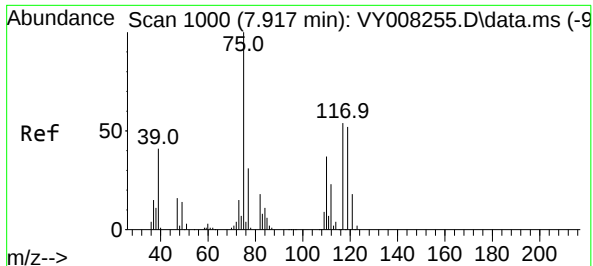

#36
1,1-Dichloropropene
Concen: 5.227 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.134 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51




Instrument :
MSVOA_Y
ClientSampleId :
WC-15-1-7-GR


Tgt Ion: 75 Resp: 7838
Ion Ratio Lower Upper
75 100
110 9.5 17.1 51.2#
77 2.3 24.4 36.6#

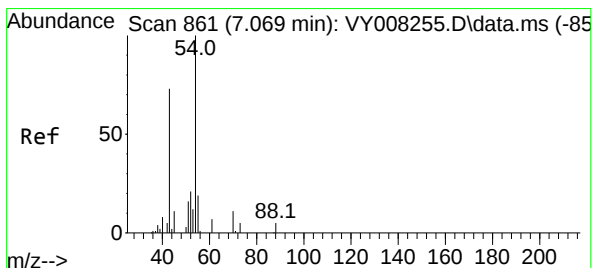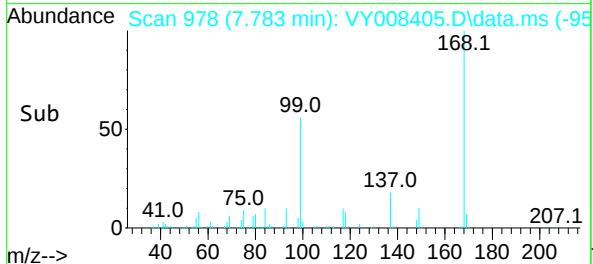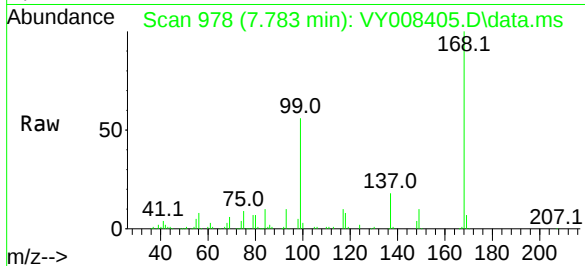

#37
Ethyl Acetate
Concen: 9.508 ug/l
RT: 7.021 min Scan# 853
Delta R.T. -0.048 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51

Tgt Ion: 43 Resp: 7352
Ion Ratio Lower Upper
43 100
61 0.0 9.7 14.5#
70 0.0 7.1 10.7#


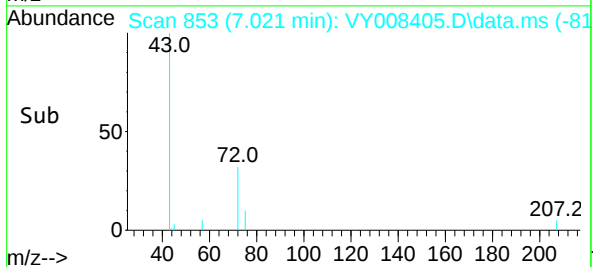

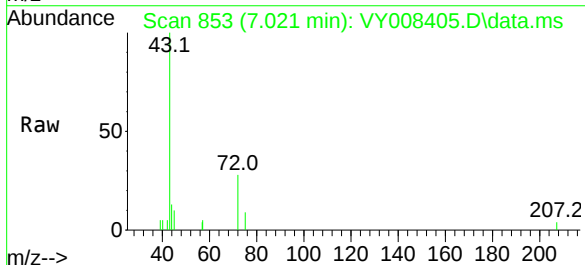




#38
Carbon Tetrachloride
Concen: 6.203 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.109 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51




Instrument :
MSVOA_Y
ClientSampleId :
WC-15-1-7-GR


Tgt Ion:117 Resp: 10008
Ion Ratio Lower Upper
117 100
119 4.5 77.9 116.9#
121 0.0 24.8 37.2#

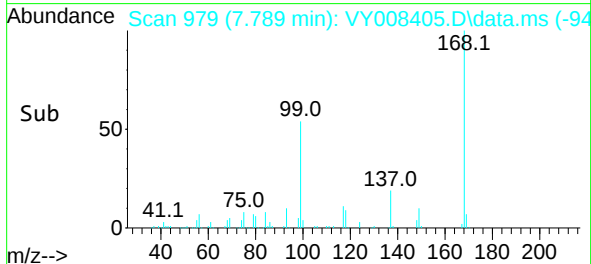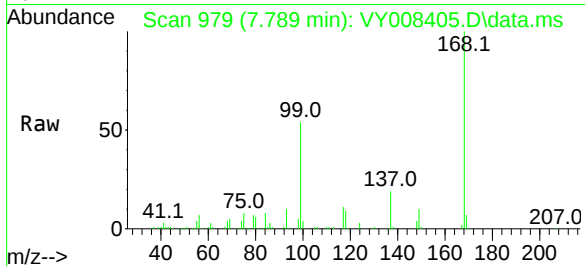

#39
Methylcyclohexane
Concen: 11.612 ug/l
RT: 9.179 min Scan# 1207
Delta R.T. -0.006 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51

Tgt Ion: 83 Resp: 22405
Ion Ratio Lower Upper
83 100
55 70.0 66.5 99.7
98 48.3 37.9 56.9




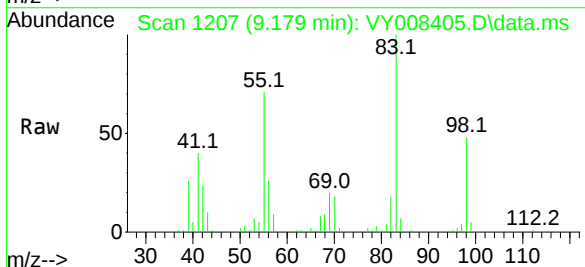


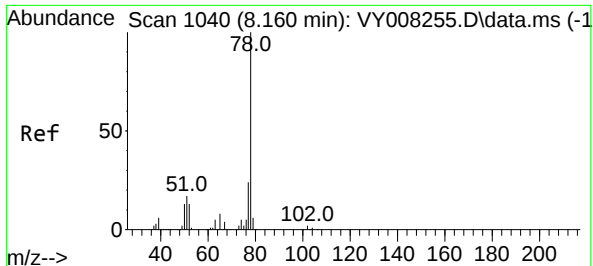

#40
Benzene
Concen: 4.310 ug/l
RT: 8.161 min Scan# 110
Delta R.T. 0.001 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51




Instrument :
MSVOA_Y
ClientSampleId :
WC-15-1-7-GR


Tgt Ion: 78 Resp: 19246
Ion Ratio Lower Upper
78 100
77 24.0 20.4 30.6

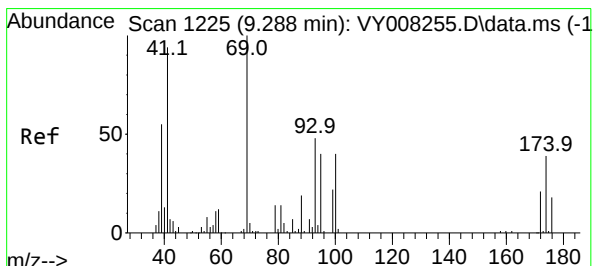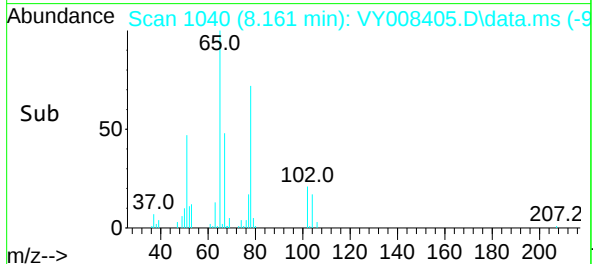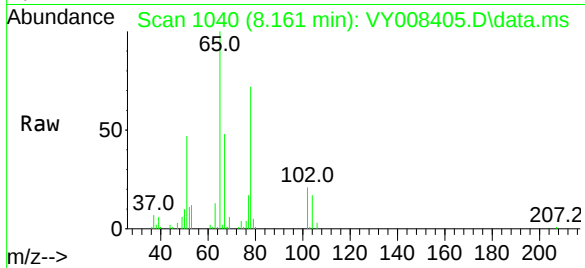

#48
Methyl methacrylate
Concen: 1.728 ug/l
RT: 9.240 min Scan# 1217
Delta R.T. -0.048 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51

Tgt Ion: 41 Resp: 1054
Ion Ratio Lower Upper
41 100
69 0.0 58.2 87.2#
39 54.8 47.4 71.0


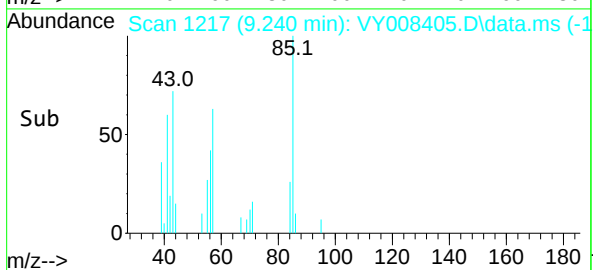

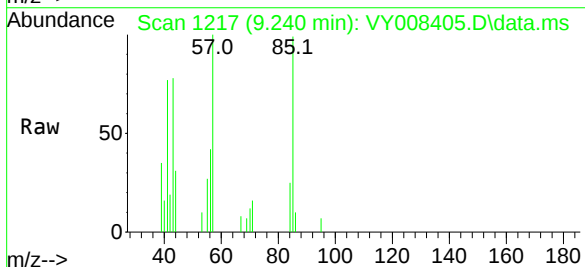




#50
Toluene-d8
Concen: 64.024 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. 0.001 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51




Instrument :
MSVOA_Y
ClientSampleId :
WC-15-1-7-GR


Tgt Ion: 98 Resp: 205740
Ion Ratio Lower Upper
98 100
100 64.5 50.2 75.2

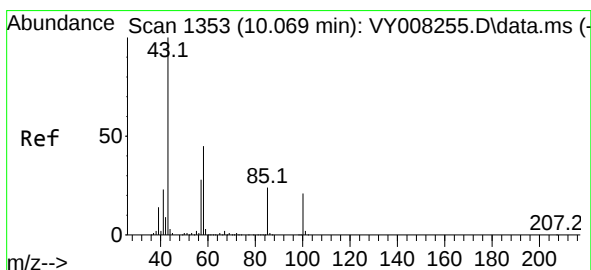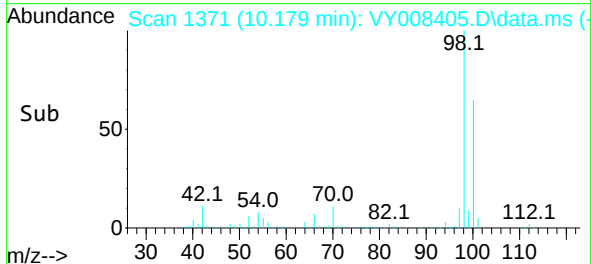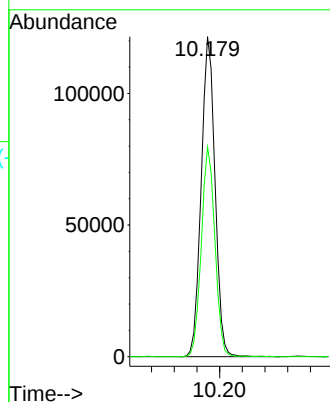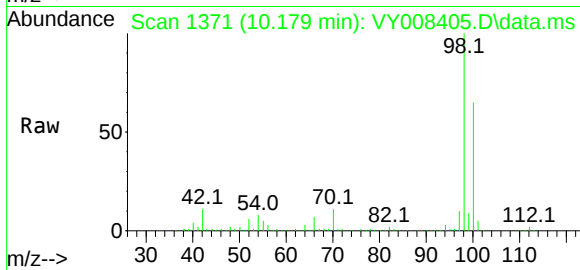

#51
4-Methyl-2-Pentanone
Concen: 1.418 ug/l
RT: 10.081 min Scan# 1355
Delta R.T. 0.012 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51

Tgt Ion: 43 Resp: 1051
Ion Ratio Lower Upper
43 100
58 32.4 28.1 42.1



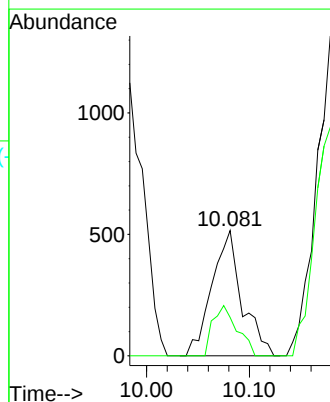
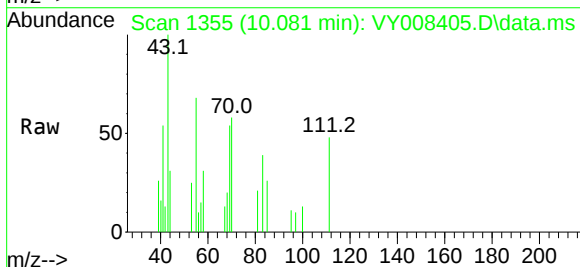


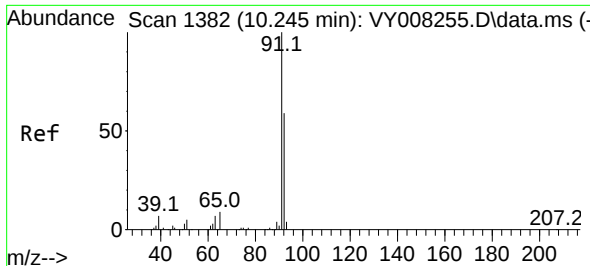

#52
Toluene
Concen: 17.935 ug/l
RT: 10.246 min Scan# 11
Delta R.T. 0.001 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51




Instrument :
MSVOA_Y
ClientSampleId :
WC-15-1-7-GR


Tgt Ion: 92 Resp: 52770
Ion Ratio Lower Upper
92 100
91 172.8 142.6 213.8

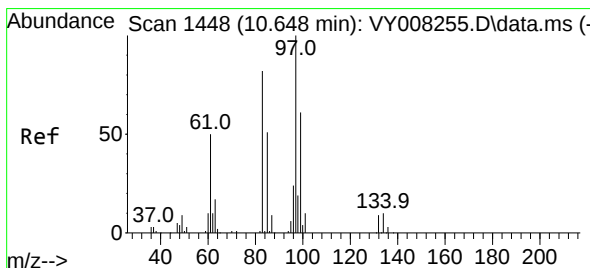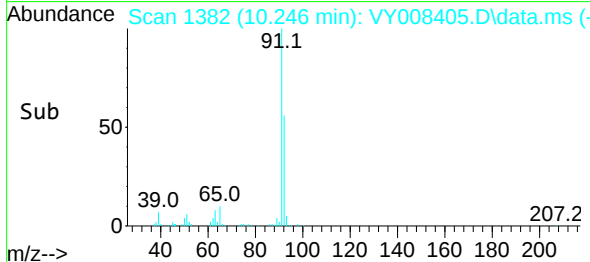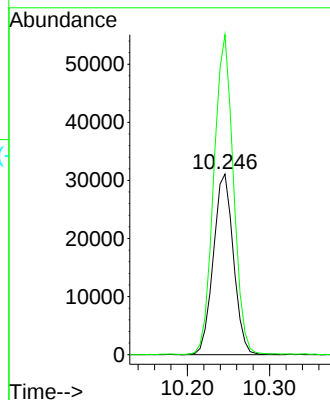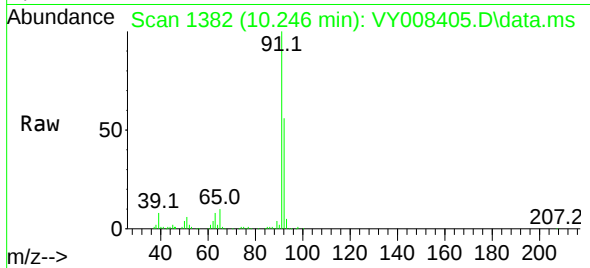

#55
1,1,2-Trichloroethane
Concen: 4.634 ug/l
RT: 10.618 min Scan# 1443
Delta R.T. -0.030 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51

Tgt Ion: 97 Resp: 4773
Ion Ratio Lower Upper
97 100
83 7.3 69.8 104.8#
85 0.0 44.3 66.5#
99 0.0 49.8 74.6#


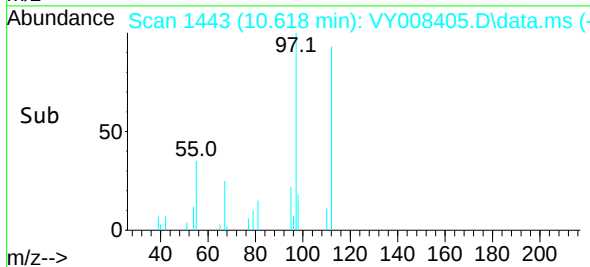
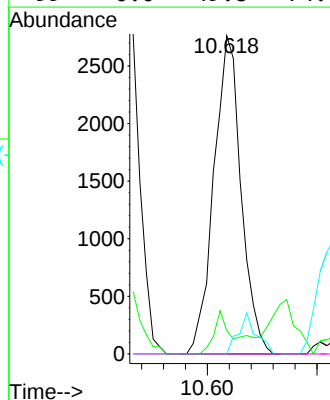
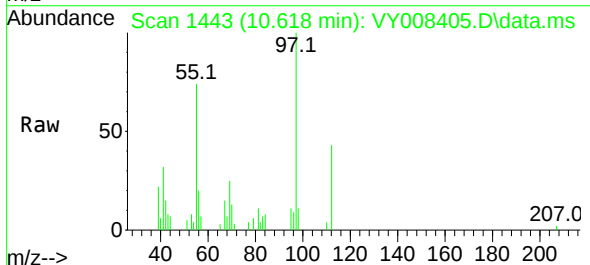


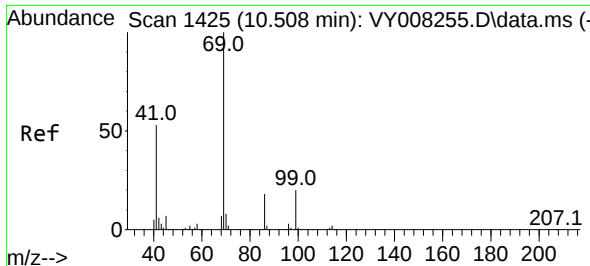

#56
Ethyl methacrylate
Concen: 1.821 ug/l
RT: 10.520 min Scan# 1427
Delta R.T. 0.012 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51




Instrument :
MSVOA_Y
ClientSampleId :
WC-15-1-7-GR


Tgt Ion: 69 Resp: 2299
Ion Ratio Lower Upper
69 100
41 149.5 63.4 95.0#
39 96.2 35.8 53.8#

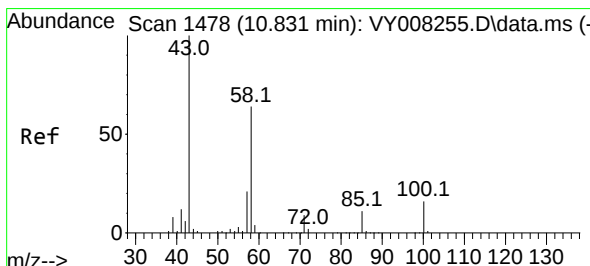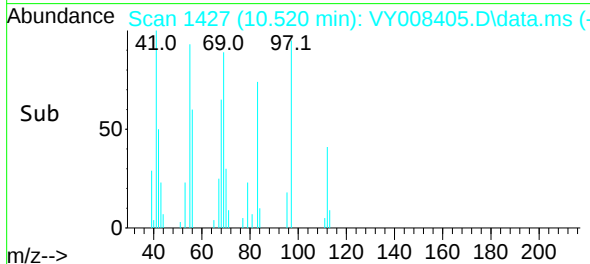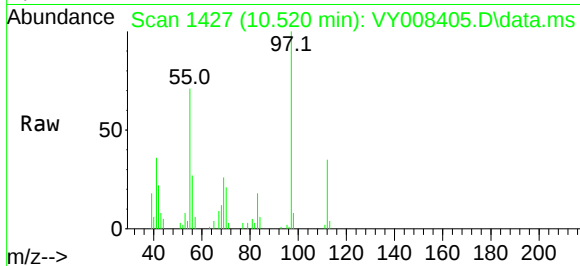

#59
2-Hexanone
Concen: 15.413 ug/l
RT: 10.801 min Scan# 1473
Delta R.T. -0.030 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51

Tgt Ion: 43 Resp: 7859
Ion Ratio Lower Upper
43 100
58 2.3 24.4 73.4#


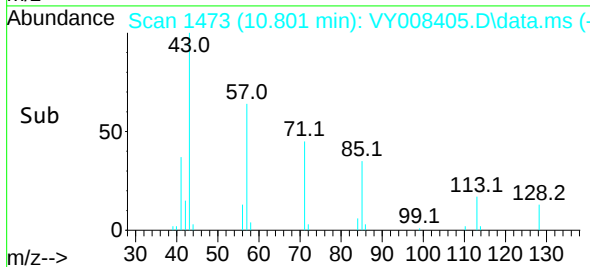

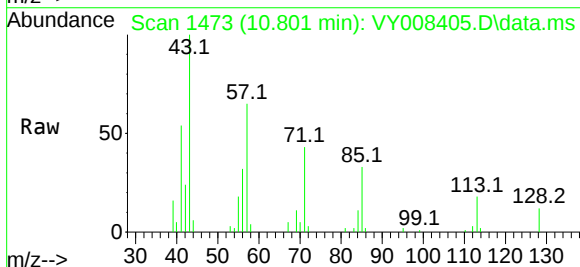




#62
4-Bromofluorobenzene
Concen: 52.388 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51




Instrument :
MSVOA_Y
ClientSampleId :
WC-15-1-7-GR


Tgt Ion: 95 Resp: 63320
Ion Ratio Lower Upper
95 100
174 82.8 0.0 177.0
176 81.0 0.0 175.8

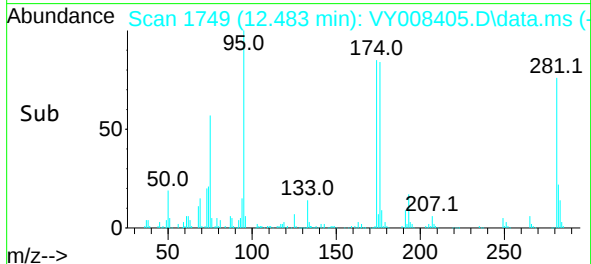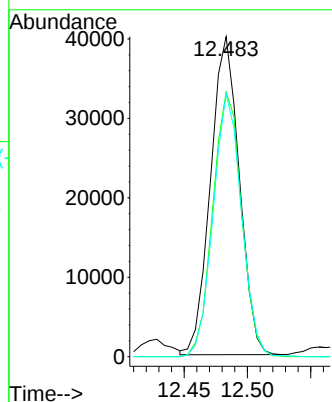

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 1586
Delta R.T. 0.000 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51

Tgt Ion: 117 Resp: 153864
Ion Ratio Lower Upper
117 100
82 51.9 43.0 64.4
119 32.1 25.4 38.0



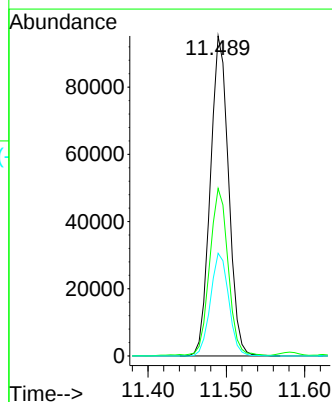



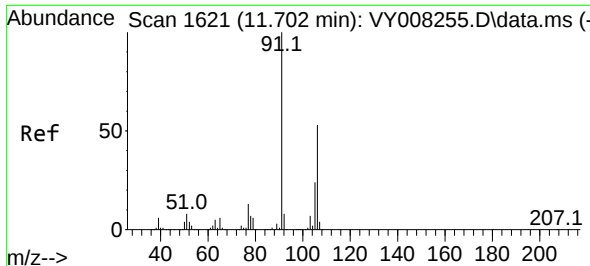

#68
m/p-Xylenes
Concen: 1.282 ug/l
RT: 11.697 min Scan# 1
Delta R.T. -0.005 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51




Instrument :
MSVOA_Y
ClientSampleId :
WC-15-1-7-GR


Tgt Ion:106 Resp: 2894
Ion Ratio Lower Upper
106 100
91 226.3 166.6 249.8

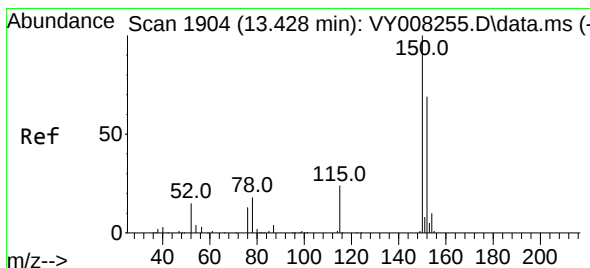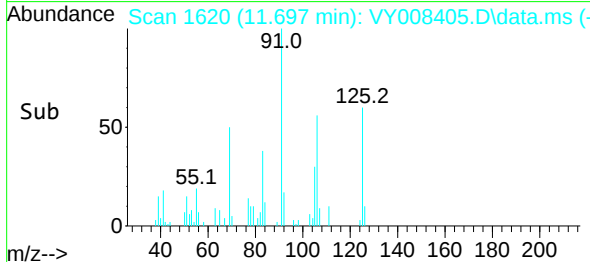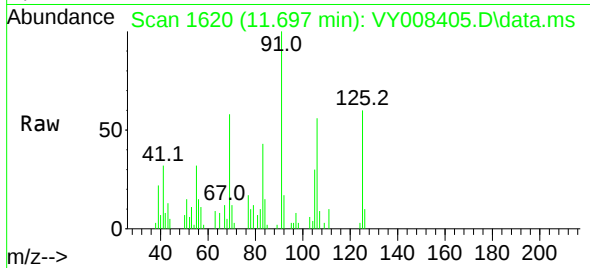

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51

Tgt Ion:152 Resp: 58396
Ion Ratio Lower Upper
152 100
115 56.5 28.2 84.7
150 152.6 0.0 347.6


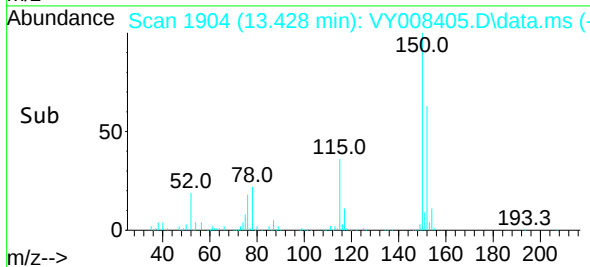

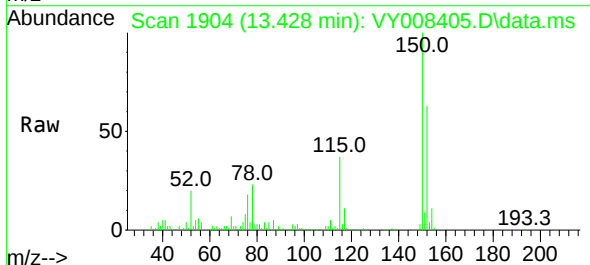




#73
Isopropylbenzene
Concen: 1.119 ug/l
RT: 12.331 min Scan# 11
Delta R.T. 0.001 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51




Instrument :
MSVOA_Y
ClientSampleId :
WC-15-1-7-GR


Tgt Ion:105 Resp: 4858
Ion Ratio Lower Upper
105 100
120 26.3 13.4 40.2

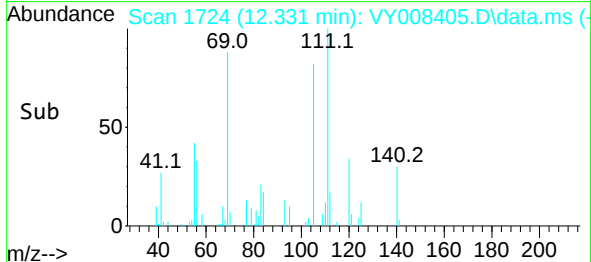

#74
N-ethyl acetate
Concen: 15.017 ug/l
RT: 12.123 min Scan# 1690
Delta R.T. -0.025 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51

Tgt Ion: 43 Resp: 14155
Ion Ratio Lower Upper
43 100
70 11.1 28.7 43.1#
55 21.1 17.3 25.9
61 0.2 17.0 25.6#




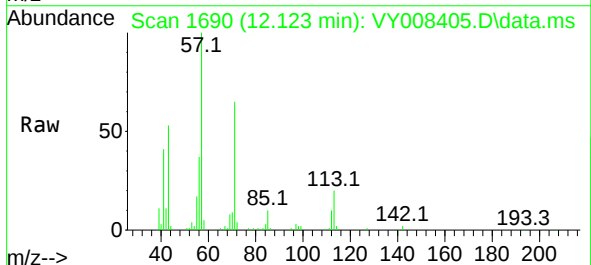




#75
1,1,2,2-Tetrachloroethane
Concen: 2.279 ug/l
RT: 12.556 min Scan# 1761
Delta R.T. -0.030 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51




Instrument :
MSVOA_Y
ClientSampleId :
WC-15-1-7-GR


Tgt Ion: 83 Resp: 2094
Ion Ratio Lower Upper
83 100
131 0.0 5.6 16.8#
85 111.7 32.3 96.8#

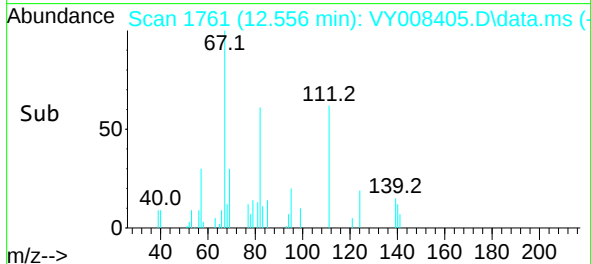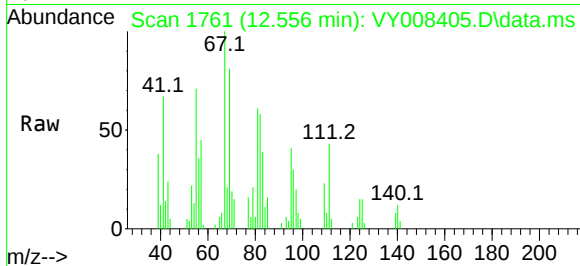

#76
1,2,3-Trichloropropane
Concen: 53.536 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.152 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51

Tgt Ion: 75 Resp: 34576
Ion Ratio Lower Upper
75 100
77 1.8 0.0 0.0#




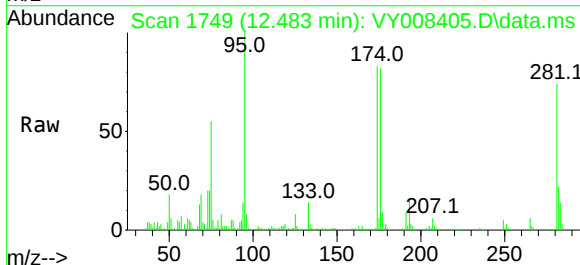




#80
 1,3,5-Trimethylbenzene
 Concen: 1.884 ug/l
 RT: 12.812 min Scan# 1749
 Delta R.T. 0.000 min
 Lab File: VY008405.D
 Acq: 19 Apr 2022 18:51




Instrument :
 MSVOA_Y
 ClientSampleId :
 WC-15-1-7-GR


Tgt Ion:105 Resp: 6708
 Ion Ratio Lower Upper
 105 100
 120 51.7 24.4 73.4

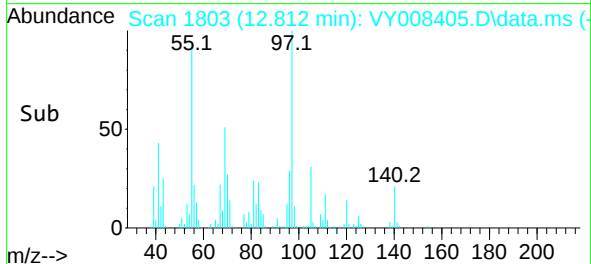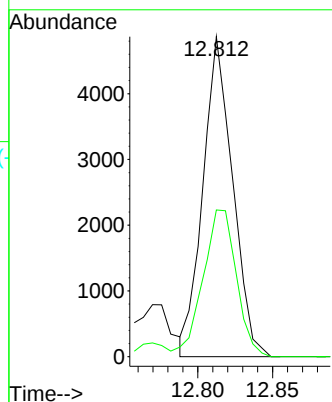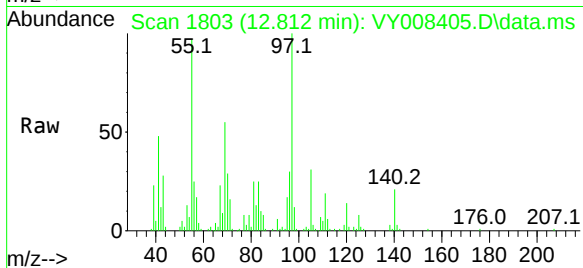

#81
 trans-1,4-Dichloro-2-butene
 Concen: 119.785 ug/l
 RT: 12.483 min Scan# 1749
 Delta R.T. 0.104 min
 Lab File: VY008405.D
 Acq: 19 Apr 2022 18:51

Tgt Ion: 75 Resp: 34576
 Ion Ratio Lower Upper
 75 100
 53 1.9 85.3 127.9#
 89 1.6 37.0 55.4#

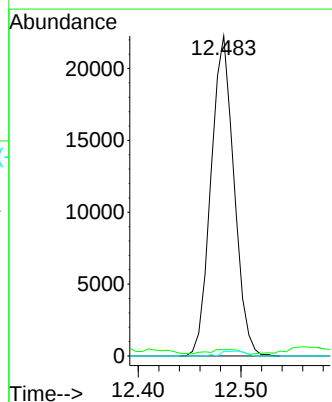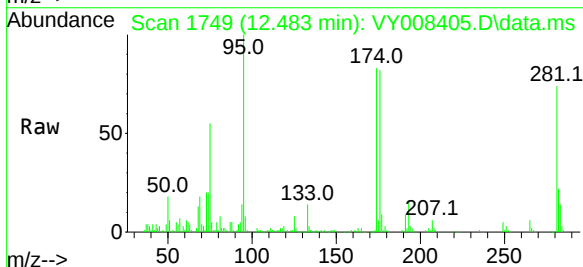



#84

1,2,4-Trimethylbenzene

Concen: 5.606 ug/l

RT: 13.123 min Scan# 1854

Delta R.T. 0.000 min

Lab File: VY008405.D

Acq: 19 Apr 2022 18:51

Instrument :

MSVOA_Y

ClientSampleId :





WC-15-1-7-GR

Tgt Ion:105 Resp: 19751

Ion Ratio Lower Upper

105 100

120 45.0 22.3 66.9

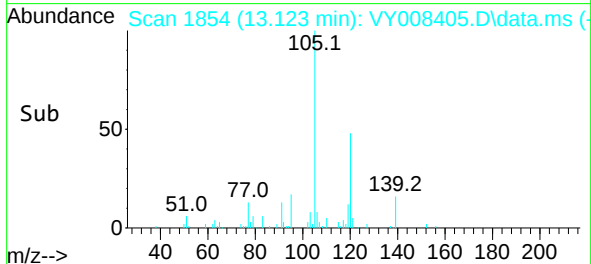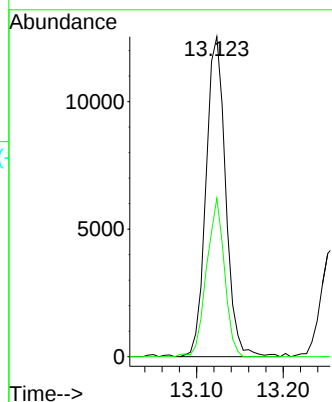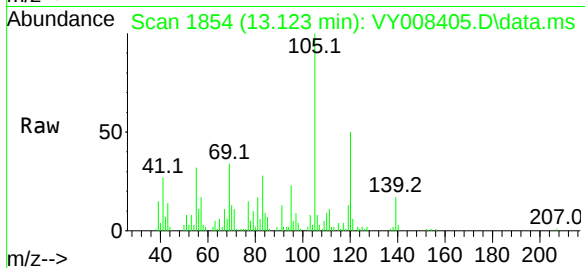

#85

sec-Butylbenzene

Concen: 1.458 ug/l

RT: 13.257 min Scan# 1876

Delta R.T. 0.006 min

Lab File: VY008405.D




Acq: 19 Apr 2022 18:51


Tgt Ion:105 Resp: 6904

Ion Ratio Lower Upper

105 100

134 15.6 10.2 30.4




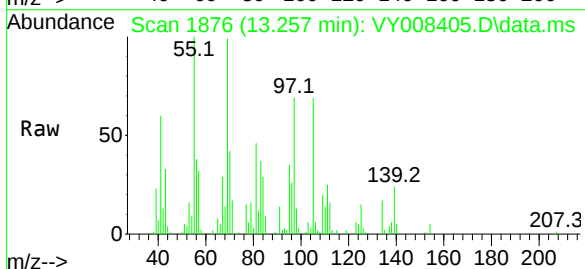




#90
Hexachloroethane
Concen: 1.022 ug/l
RT: 13.971 min Scan# 1993
Delta R.T. 0.007 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51

Instrument :
MSVOA_Y
ClientSampleId :
WC-15-1-7-GR

Tgt Ion:117 Resp: 755
Ion Ratio Lower Upper
117 100
201 0.0 43.0 128.8#

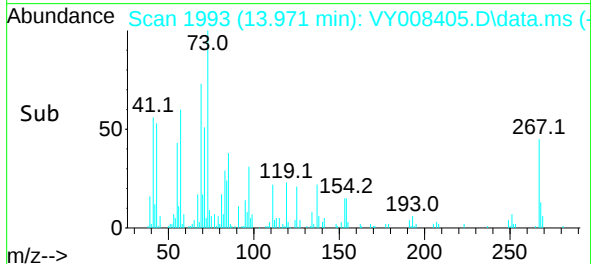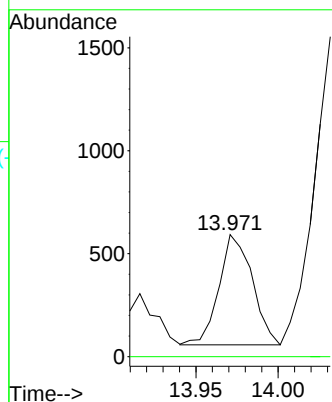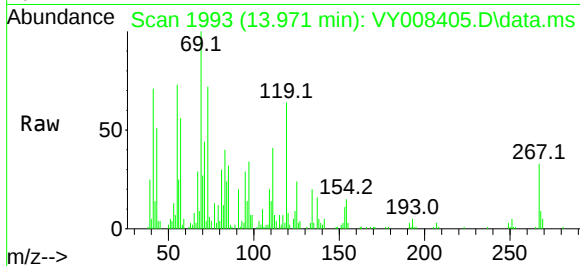

#95
Naphthalene
Concen: 2.152 ug/l
RT: 15.239 min Scan# 2201
Delta R.T. 0.001 min
Lab File: VY008405.D
Acq: 19 Apr 2022 18:51

Tgt Ion:128 Resp: 5112
Ion Ratio Lower Upper
128 100
127 32.2 11.0 16.4#
129 12.2 8.4 12.6

