


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\vy042020\  
 Data File : VY002417.D  
 Acq On : 20 Apr 2020 11:41  
 Operator : SY/MD  
 Sample : BFB  
 Misc : 5.00G/5ML/MSVOA\_Y/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_Y\METHODS\82Y042020S.M  
 Title : SW846 8260  
 Last Update : Mon Apr 20 12:59:30 2020

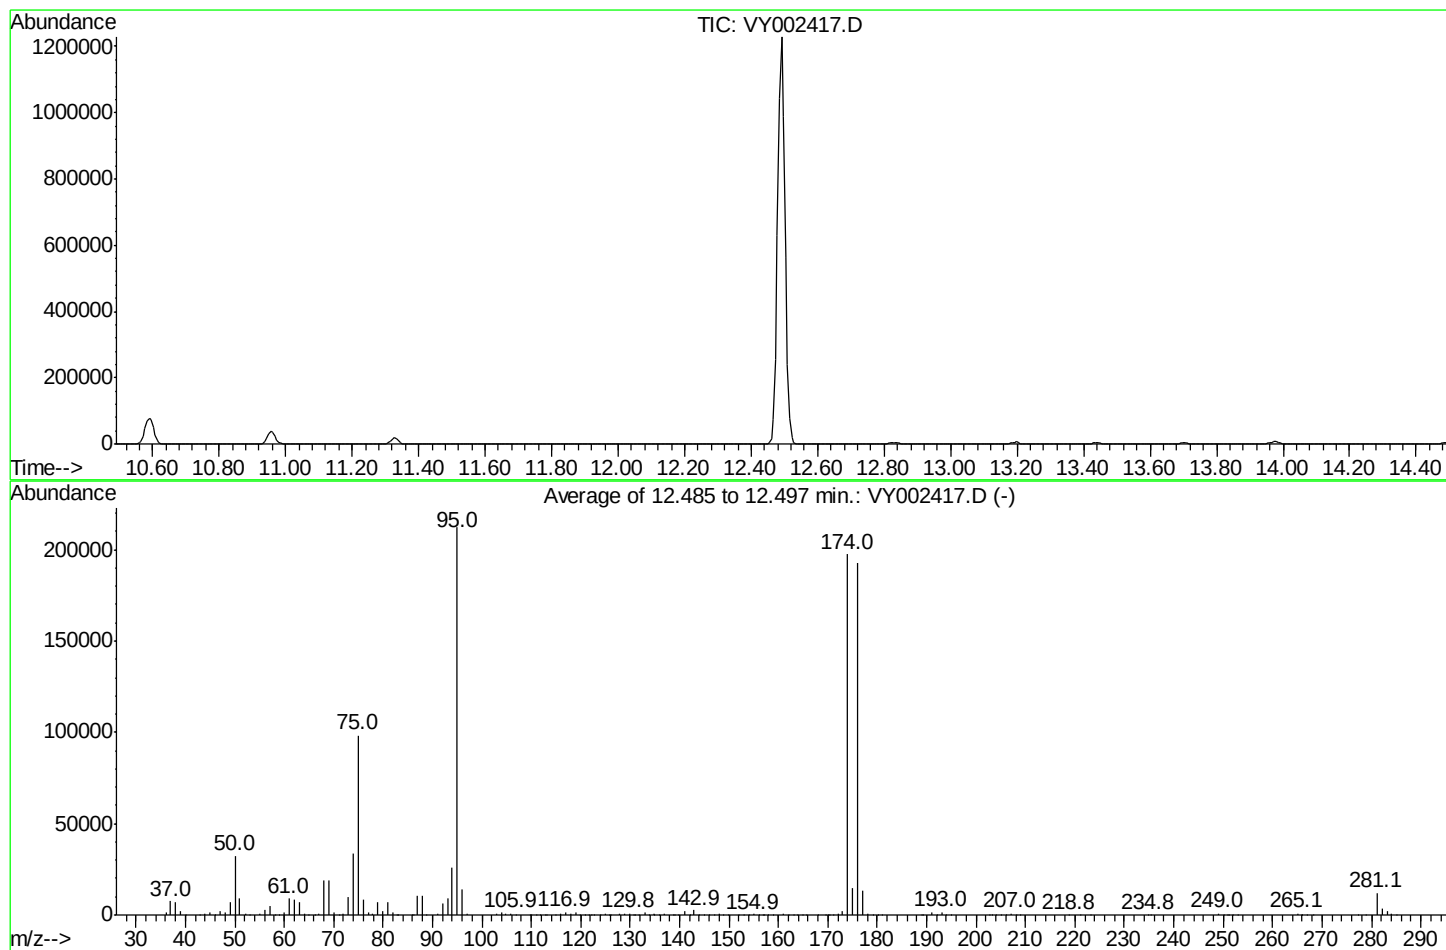

AutoFind: Scans 1763, 1764, 1765; Background Corrected with Scan 1754

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 15.3      | 32370   | PASS             |
| 75          | 95           | 30           | 60           | 46.3      | 98202   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 212224  | PASS             |
| 96          | 95           | 5            | 9            | 6.7       | 14113   | PASS             |
| 173         | 174          | 0.00         | 2            | 1.0       | 1976    | PASS             |
| 174         | 95           | 50           | 100          | 93.0      | 197418  | PASS             |
| 175         | 174          | 5            | 9            | 7.4       | 14663   | PASS             |
| 176         | 174          | 95           | 101          | 97.5      | 192490  | PASS             |
| 177         | 176          | 5            | 9            | 6.9       | 13326   | PASS             |