


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv042120\
 Data File : VY002426.D
 Acq On : 21 Apr 2020 10:27
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y042020S.M
 Title : SW846 8260
 Last Update : Mon Apr 20 15:14:11 2020

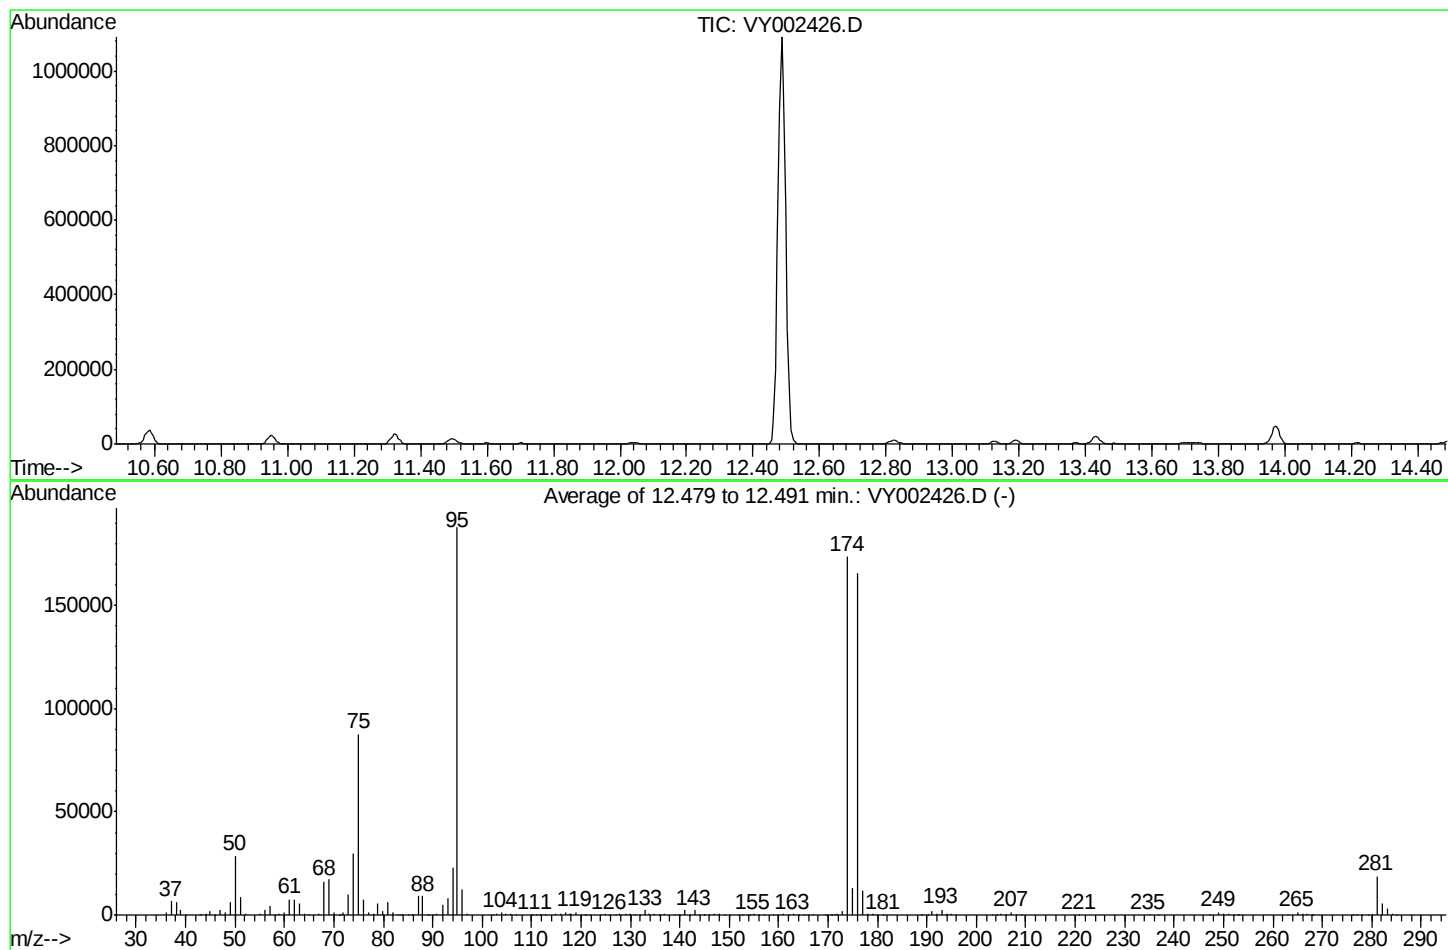

AutoFind: Scans 1762, 1763, 1764; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	28688	PASS
75	95	30	60	46.6	87554	PASS
95	95	100	100	100.0	187840	PASS
96	95	5	9	6.7	12607	PASS
173	174	0.00	2	1.0	1738	PASS
174	95	50	100	92.4	173482	PASS
175	174	5	9	7.5	13076	PASS
176	174	95	101	95.5	165589	PASS
177	176	5	9	7.0	11524	PASS