

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042121\
 Data File : VY004544.D
 Acq On : 21 Apr 2021 10:30
 Operator : SY/MD
 Sample : VY0421SBL01
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :

Quant Time: Apr 22 11:04:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042121W.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 22 08:25:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.795	168	139427	50.00	ug/l	0.20
34) 1,4-Difluorobenzene	8.697	114	251361	50.00	ug/l	0.18
63) Chlorobenzene-d5	11.496	117	229273	50.00	ug/l	0.15
72) 1,4-Dichlorobenzene-d4	13.428	152	103366	50.00	ug/l	0.14
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	90198	52.95	ug/l	0.20
Spiked Amount 50.000			Recovery	=	105.90%	
35) Dibromofluoromethane	7.722	113	75578	48.01	ug/l	0.21
Spiked Amount 50.000			Recovery	=	96.02%	
50) Toluene-d8	10.185	98	304839	49.66	ug/l	0.16
Spiked Amount 50.000			Recovery	=	99.32%	
62) 4-Bromofluorobenzene	12.483	95	100229	47.68	ug/l	0.14
Spiked Amount 50.000			Recovery	=	95.36%	
Target Compounds						Qvalue
3) Chloromethane	2.119	50	1780	0.79	ug/l	98
4) Vinyl Chloride	2.198	62	5772	2.89	ug/l #	43
5) Bromomethane	2.674	94	411	0.36	ug/l	98
10) Methyl Iodide	4.101	142	453	0.21	ug/l #	88
11) Tert butyl alcohol	4.966	59	639	2.96	ug/l #	73
13) Acrolein	3.729	56	74	0.31	ug/l #	15
15) Acrylonitrile	5.167	53	309	0.42	ug/l #	78
16) Acetone	3.960	43	1261	1.98	ug/l #	88
20) Methylene Chloride	4.735	84	4529	2.39	ug/l #	89
25) 2-Butanone	7.009	43	334	0.37	ug/l #	46
29) Tetrahydrofuran	7.350	42	287	0.46	ug/l #	88
31) Cyclohexane	7.789	56	3663	1.32	ug/l #	39
36) 1,1-Dichloropropene	7.795	75	11657	4.99	ug/l #	49
38) Carbon Tetrachloride	7.795	117	14317	6.44	ug/l #	15
43) Isopropyl Acetate	8.118	43	1824	0.47	ug/l #	22
51) 4-Methyl-2-Pentanone	10.075	43	2037	0.93	ug/l	88
56) Ethyl methacrylate	10.648	69	20	3.16	ug/l #	1
59) 2-Hexanone	10.922	43	240	16.77	ug/l #	23
66) 1,1,1,2-Tetrachloroethane	11.313	131	454	0.27	ug/l #	1
70) Styrene	12.050	104	462	3.06	ug/l	98
76) 1,2,3-Trichloropropane	12.483	75	56849	25.70	ug/l #	100
79) 2-Chlorotoluene	12.483	91	540	1.03	ug/l	94
81) trans-1,4-Dichloro-2-b...	12.483	75	56763	75.44	ug/l #	12
87) 1,3-Dichlorobenzene	13.373	146	765	0.24	ug/l	95
88) 1,4-Dichlorobenzene	13.373	146	765	0.22	ug/l	96
89) n-Butylbenzene	13.696	91	1128	0.22	ug/l	89
92) 1,2-Dibromo-3-Chloropr...	14.215	75	104	0.24	ug/l #	1
93) 1,2,4-Trichlorobenzene	15.007	180	791	2.39	ug/l	98
94) Hexachlorobutadiene	15.111	225	227	0.23	ug/l #	70
95) Naphthalene	15.239	128	2441	2.34	ug/l	99
96) 1,2,3-Trichlorobenzene	15.422	180	796	1.78	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042121\
Data File : VY004544.D
Acq On : 21 Apr 2021 10:30
Operator : SY/MD
Sample : VY0421SBL01
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :

Quant Time: Apr 22 11:04:02 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042121W.M
Quant Title : SW846 8260
QLast Update : Thu Apr 22 08:25:55 2021
Response via : Initial Calibration




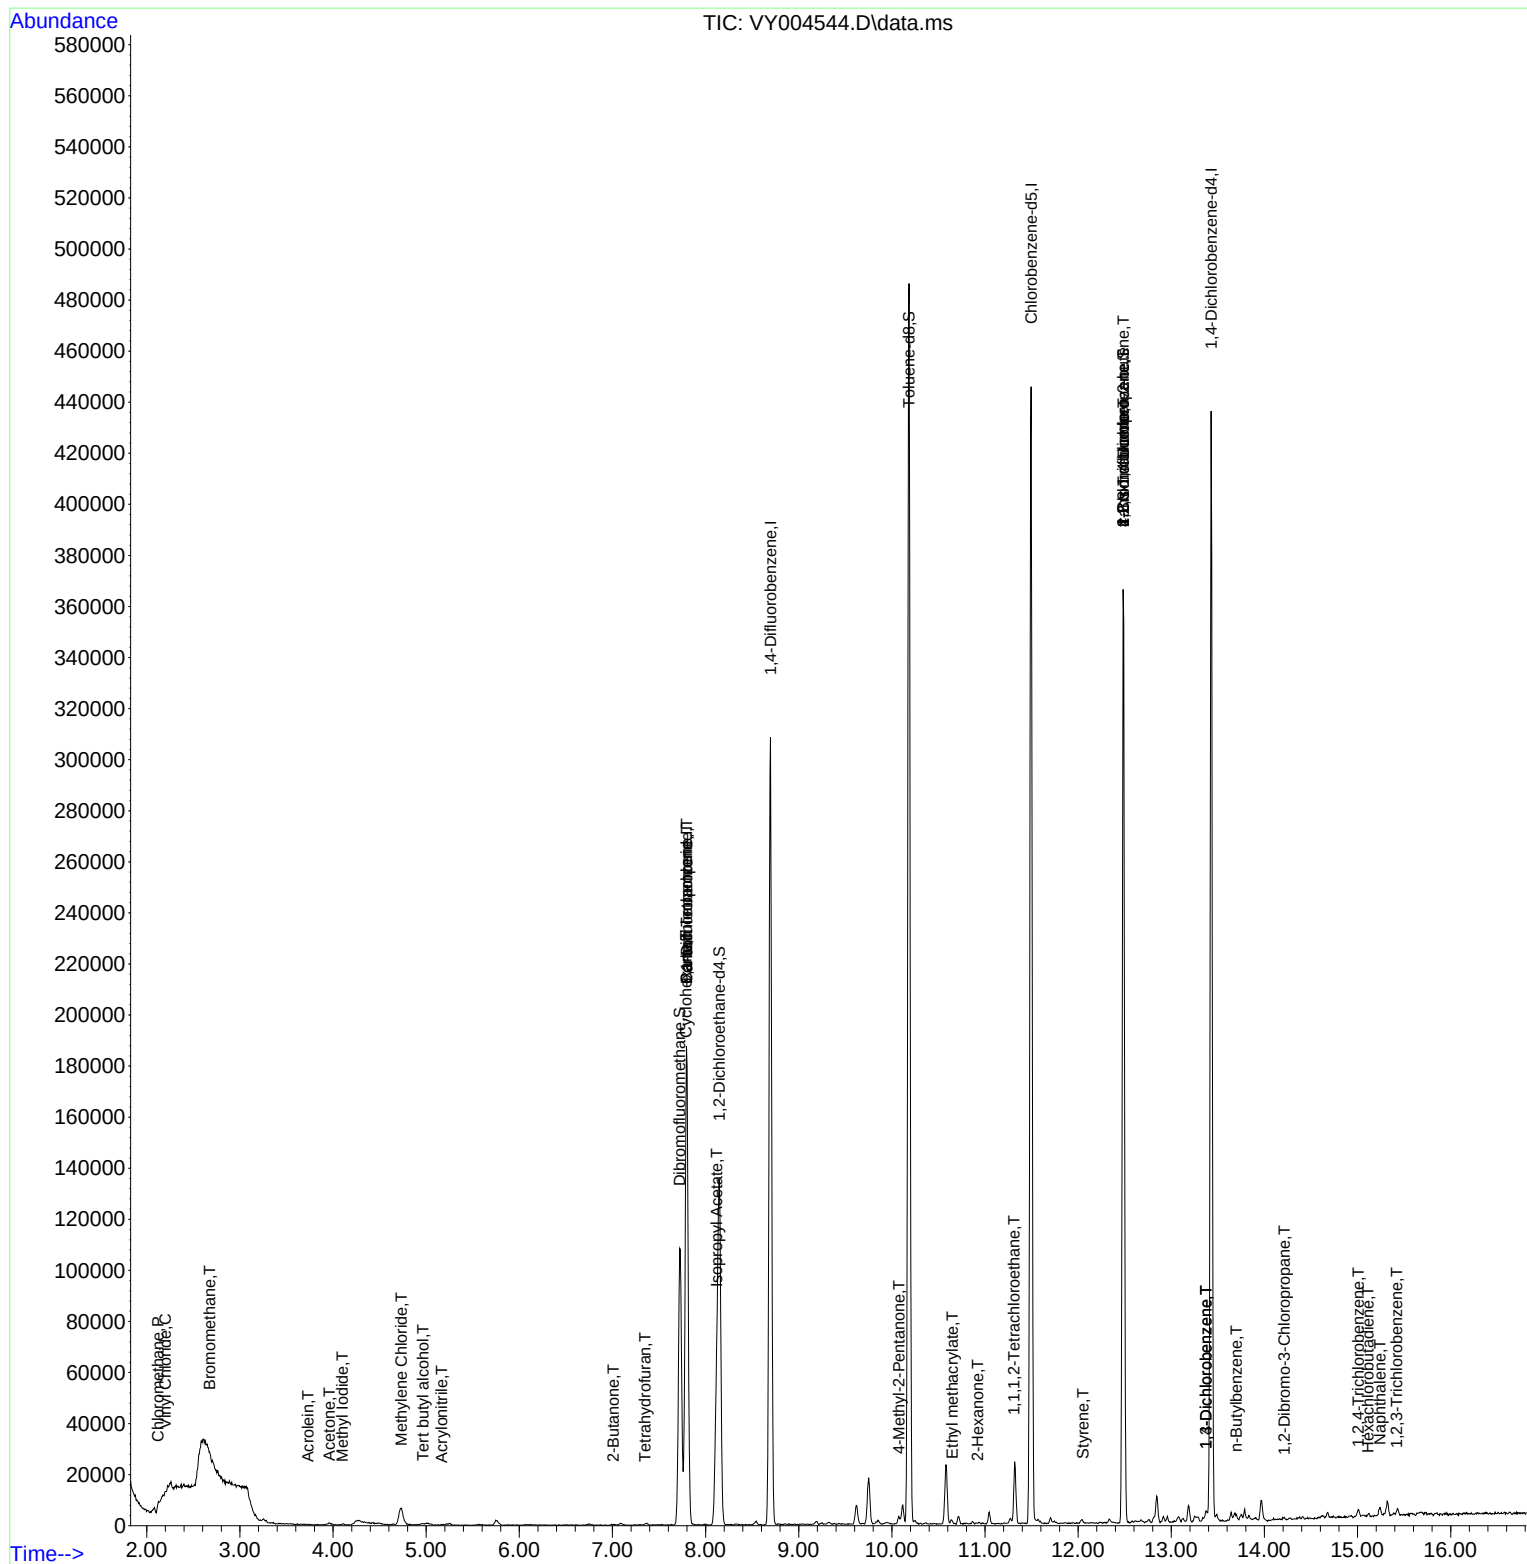




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.795 min Scan# 980
Delta R.T. 0.204 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:168 Resp: 139427
Ion Ratio Lower Upper
168 100
99 56.2 42.6 63.8

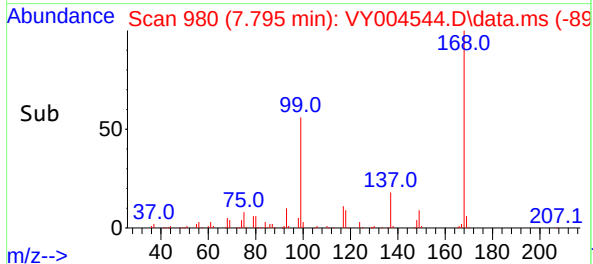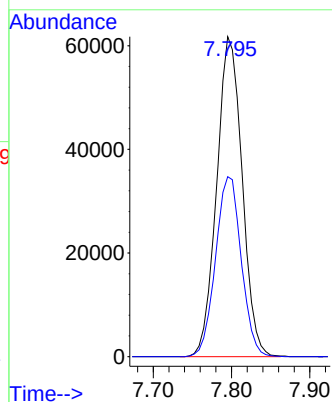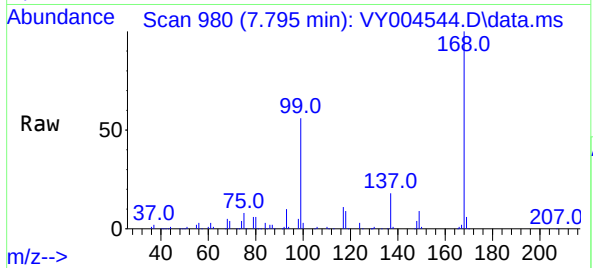

#3
Chloromethane
Concen: 0.79 ug/l
RT: 2.119 min Scan# 49
Delta R.T. 0.085 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30

Tgt Ion: 50 Resp: 1780
Ion Ratio Lower Upper
50 100
52 31.3 25.8 38.8


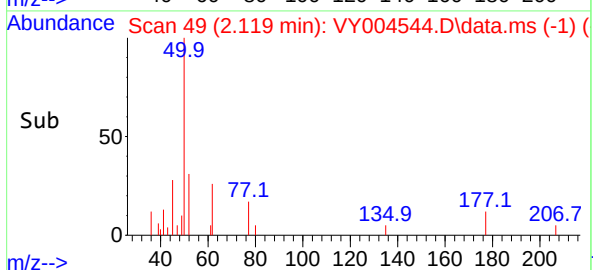






#4
 Vinyl Chloride
 Concen: 2.89 ug/l
 RT: 2.198 min Scan# 62
 Delta R.T. 0.035 min
 Lab File: VY004544.D
 Acq: 21 Apr 2021 10:30




Instrument :
 MSVOA_Y
 ClientSampled :


Tgt Ion: 62 Resp: 5772
 Ion Ratio Lower Upper
 62 100
 64 0.0 25.1 37.7#

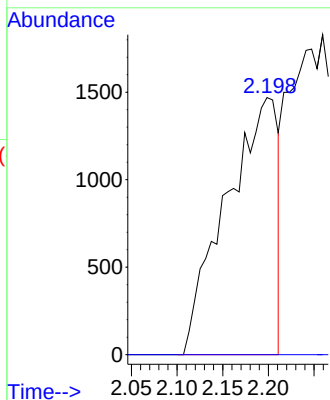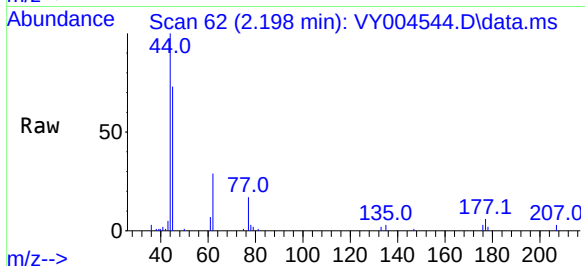

#5
 Bromomethane
 Concen: 0.36 ug/l
 RT: 2.674 min Scan# 140
 Delta R.T. 0.171 min
 Lab File: VY004544.D
 Acq: 21 Apr 2021 10:30

Tgt Ion: 94 Resp: 411
 Ion Ratio Lower Upper
 94 100
 96 93.3 73.0 109.4



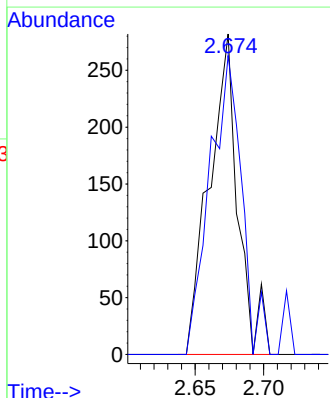
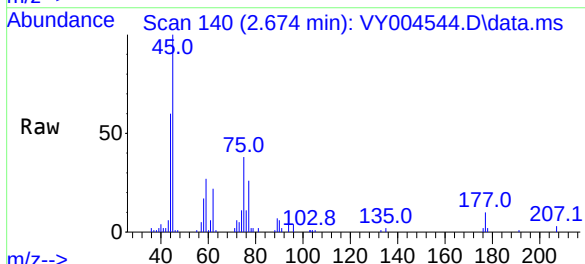




#10
Methyl Iodide
Concen: 0.21 ug/l
RT: 4.101 min Scan# 374
Delta R.T. 0.214 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30




Instrument :
MSVOA_Y
ClientSampled :


Tgt Ion:142 Resp: 453
Ion Ratio Lower Upper
142 100
127 42.6 31.7 47.5
141 0.0 10.9 16.3#

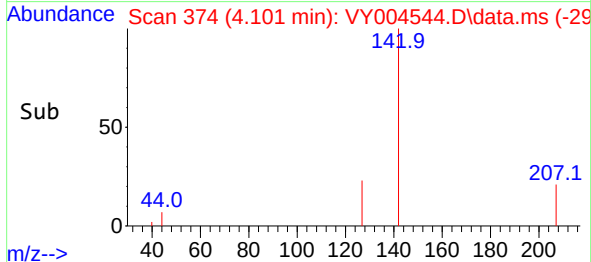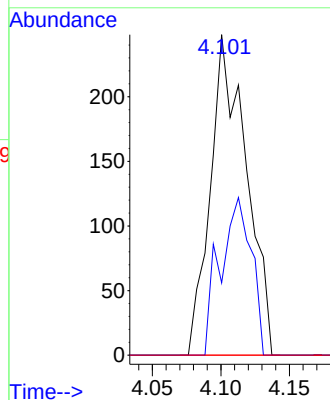

#11
Tert butyl alcohol
Concen: 2.96 ug/l
RT: 4.966 min Scan# 516
Delta R.T. 0.261 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30

Tgt Ion: 59 Resp: 639
Ion Ratio Lower Upper
59 100
57 0.0 8.0 12.0#


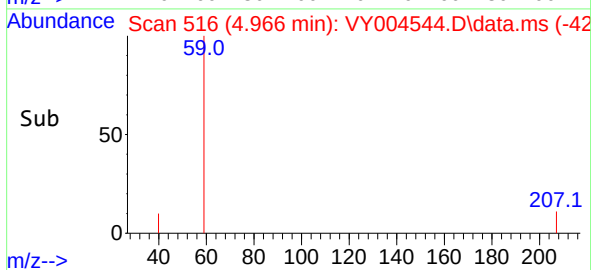
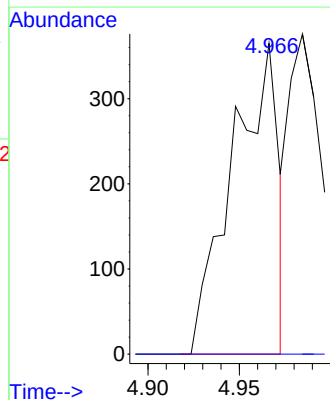





#13
Acrolein
Concen: 0.31 ug/l
RT: 3.729 min Scan# 313
Delta R.T. 0.182 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30




Instrument :
MSVOA_Y
ClientSampled :


Tgt Ion: 56 Resp: 74
Ion Ratio Lower Upper
56 100
55 0.0 56.0 84.0#

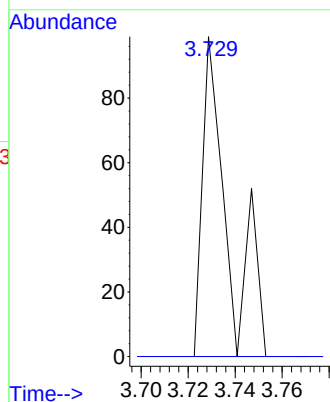

#15
Acrylonitrile
Concen: 0.42 ug/l
RT: 5.167 min Scan# 549
Delta R.T. 0.271 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30

Tgt Ion: 53 Resp: 309
Ion Ratio Lower Upper
53 100
52 76.7 66.1 99.1
51 0.0 27.9 41.9#



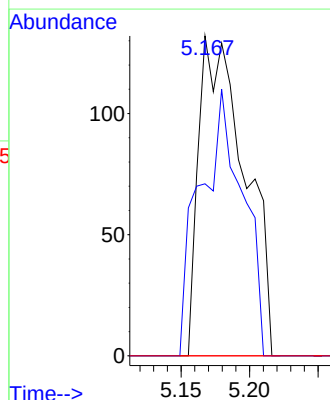





#16
Acetone
Concen: 1.98 ug/l
RT: 3.960 min Scan# 351
Delta R.T. 0.207 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30




Instrument :
MSVOA_Y
ClientSampled :


Tgt Ion: 43 Resp: 1261
Ion Ratio Lower Upper
43 100
58 26.9 27.0 40.6#

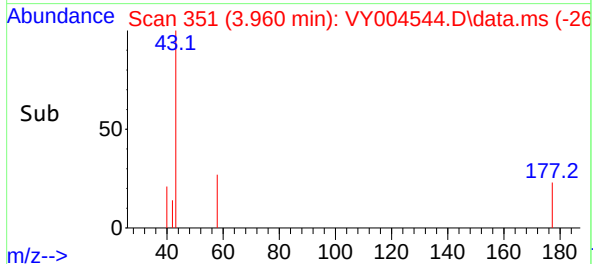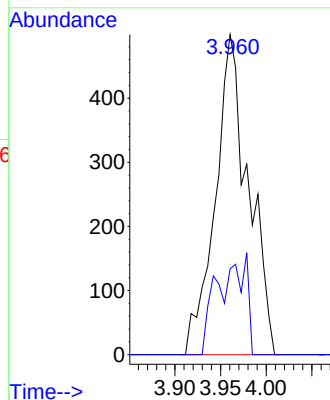

#20
Methylene Chloride
Concen: 2.39 ug/l
RT: 4.735 min Scan# 478
Delta R.T. 0.266 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30

Tgt Ion: 84 Resp: 4529
Ion Ratio Lower Upper
84 100
49 135.1 94.6 141.8
51 45.9 29.9 44.9#
86 66.3 51.4 77.2


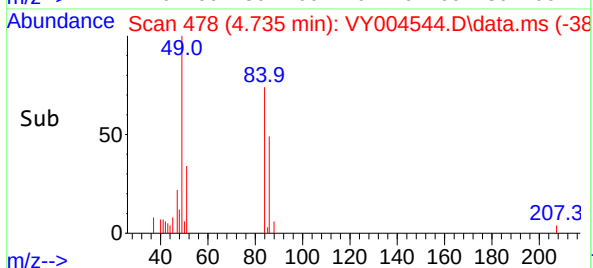
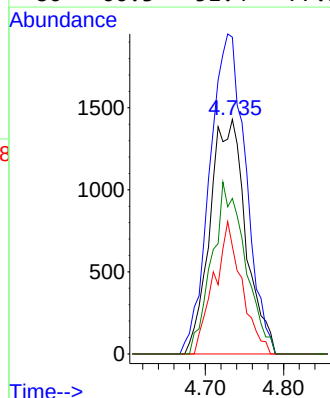
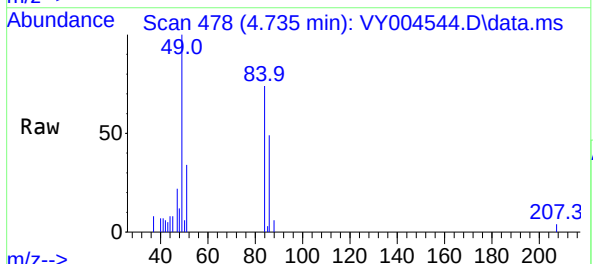




#25
2-Butanone
Concen: 0.37 ug/l
RT: 7.009 min Scan# 851
Delta R.T. 0.263 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30




Instrument :
MSVOA_Y
ClientSampled :


Tgt Ion: 43 Resp: 334
Ion Ratio Lower Upper
43 100
72 0.0 23.1 34.7#

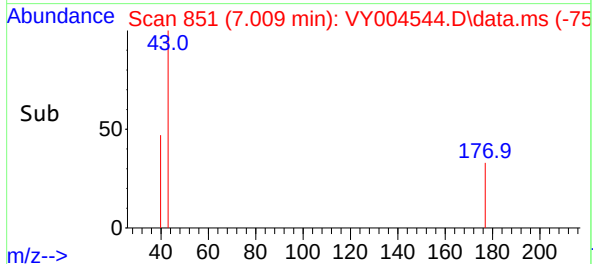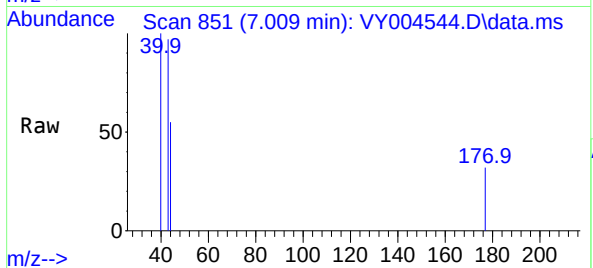

#29
Tetrahydrofuran
Concen: 0.46 ug/l
RT: 7.350 min Scan# 907
Delta R.T. 0.223 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30


Tgt Ion: 42 Resp: 287
Ion Ratio Lower Upper
42 100
72 60.3 36.6 55.0#
71 43.6 34.3 51.5

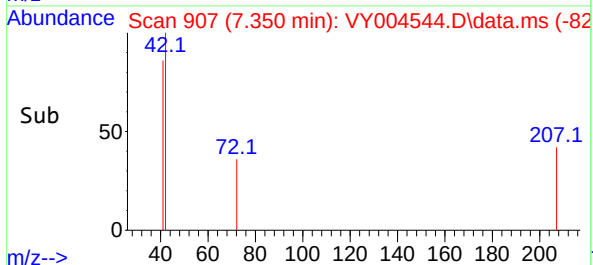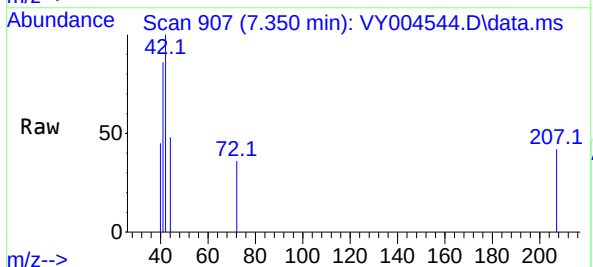






#31
Cyclohexane
Concen: 1.32 ug/l
RT: 7.789 min Scan# 979
Delta R.T. 0.211 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30


Instrument :
MSVOA_Y
ClientSampled :





Tgt Ion: 56 Resp: 3663
Ion Ratio Lower Upper
56 100
69 133.6 26.6 39.8#
84 103.6 70.4 105.6

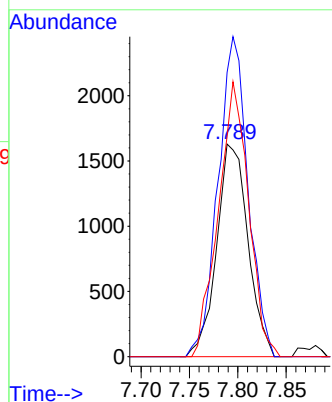


#33
1,2-Dichloroethane-d4
Concen: 52.95 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. 0.196 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30



Tgt Ion: 65 Resp: 90198
Ion Ratio Lower Upper
65 100
67 52.6 0.0 107.2









#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. 0.178 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30

Instrument :
MSVOA_Y
ClientSampled :




Tgt Ion:114 Resp: 251361
Ion Ratio Lower Upper
114 100
63 20.2 0.0 38.6
88 14.6 0.0 30.6

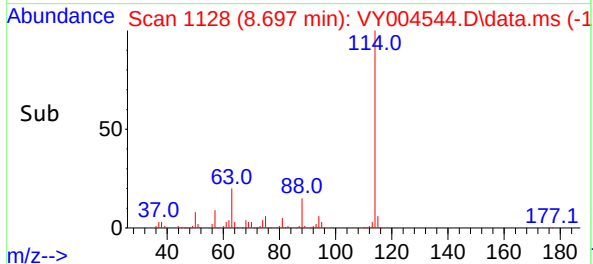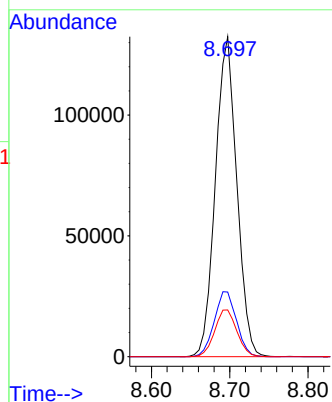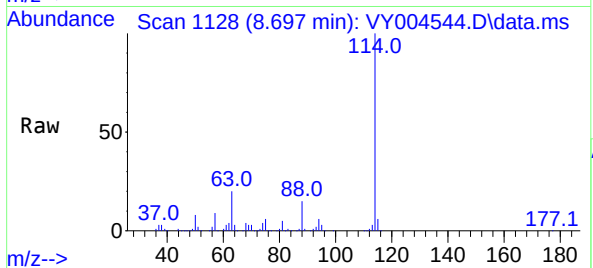


#35

Dibromofluoromethane
Concen: 48.01 ug/l
RT: 7.722 min Scan# 968
Delta R.T. 0.209 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30

Tgt Ion:113 Resp: 75578
Ion Ratio Lower Upper
113 100
111 102.5 82.2 123.2
192 19.5 15.4 23.0


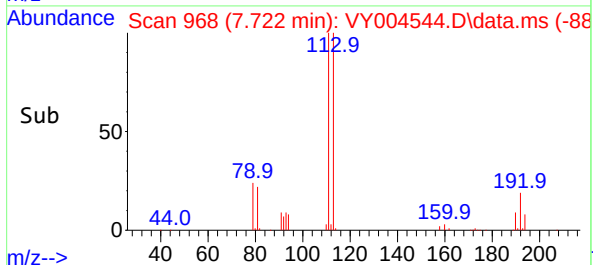

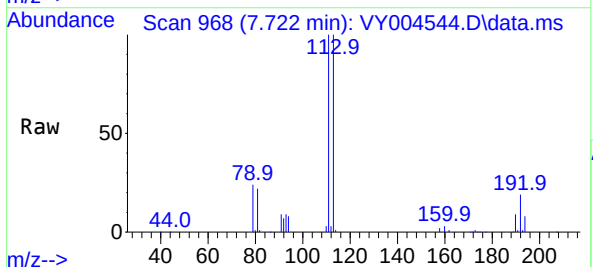




#36
1,1-Dichloropropene
Concen: 4.99 ug/l
RT: 7.795 min Scan# 980
Delta R.T. 0.078 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30




Instrument :
MSVOA_Y
ClientSampled :


Tgt Ion:	75	Resp:	11657
Ion	Ratio	Lower	Upper
75	100		
110	8.8	18.2	54.6#
77	0.0	24.9	37.3#

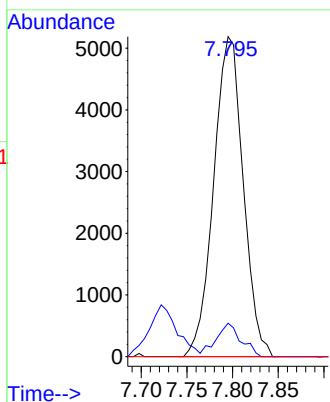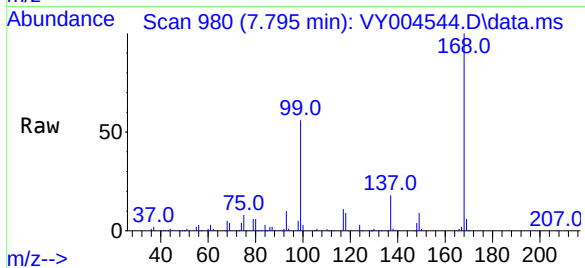

#38
Carbon Tetrachloride
Concen: 6.44 ug/l
RT: 7.795 min Scan# 980
Delta R.T. 0.097 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30

Tgt Ion:	117	Resp:	14317
Ion	Ratio	Lower	Upper
117	100		
119	3.9	76.0	114.0#
121	0.0	24.5	36.7#


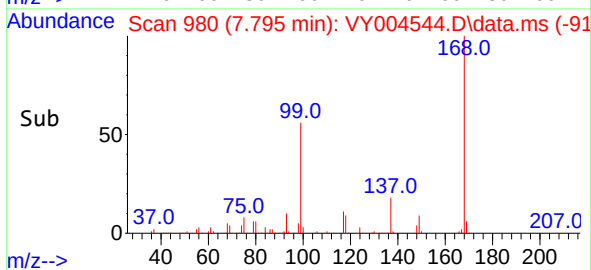
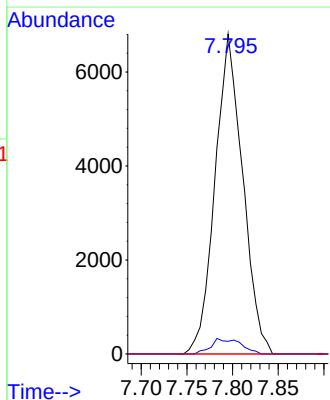
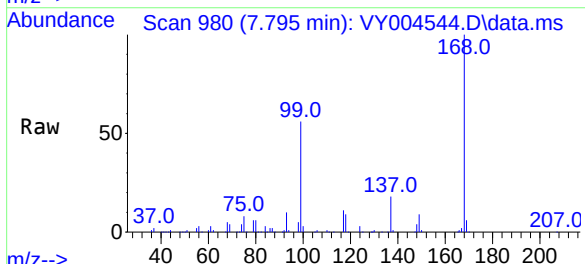




#43
Isopropyl Acetate
Concen: 0.47 ug/l
RT: 8.118 min Scan# 1033
Delta R.T. 0.025 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30




Instrument :
MSVOA_Y
ClientSampled :


Tgt Ion: 43 Resp: 1824
Ion Ratio Lower Upper
43 100
61 0.0 22.5 33.7#
87 65.4 11.1 16.7#

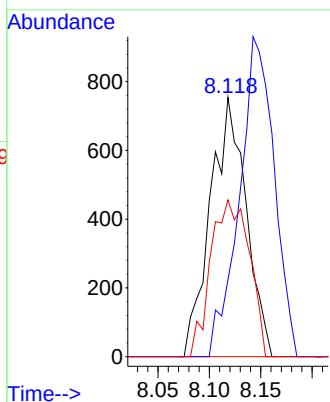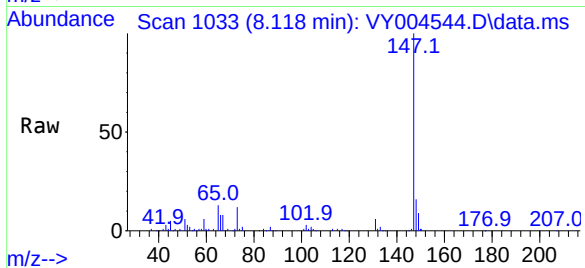

#50
Toluene-d8
Concen: 49.66 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. 0.156 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30

Tgt Ion: 98 Resp: 304839
Ion Ratio Lower Upper
98 100
100 64.6 50.5 75.7


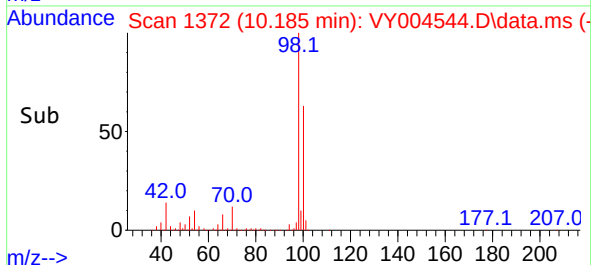
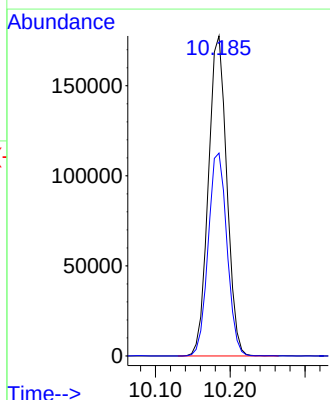
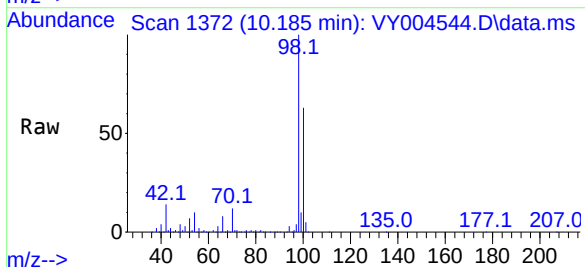




#51
4-Methyl-2-Pentanone
Concen: 0.93 ug/l
RT: 10.075 min Scan# 1354
Delta R.T. 0.153 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 43 Resp: 2037
Ion Ratio Lower Upper
43 100
58 33.2 32.5 48.7

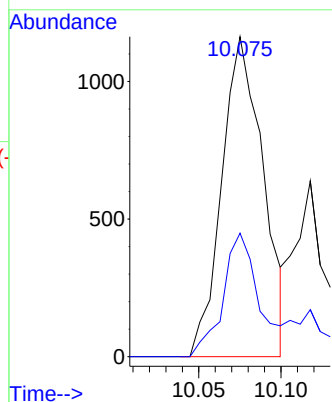

#56
Ethyl methacrylate
Concen: 3.16 ug/l
RT: 10.648 min Scan# 1448
Delta R.T. 0.278 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30

Tgt Ion: 69 Resp: 20
Ion Ratio Lower Upper
69 100
41 1825.0 49.6 74.4#
39 620.0 28.0 42.0#


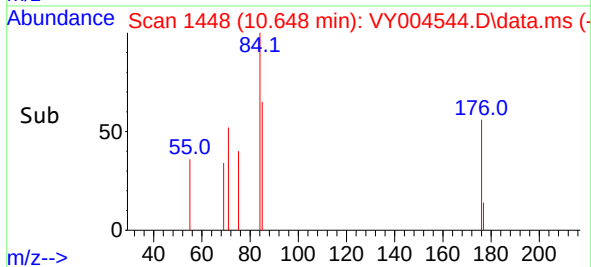

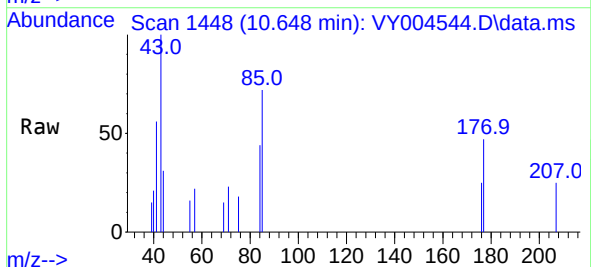




#59
2-Hexanone
Concen: 16.77 ug/l
RT: 10.922 min Scan# 1493
Delta R.T. 0.228 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30




Instrument :
MSVOA_Y
ClientSampled :


Tgt Ion: 43 Resp: 240
Ion Ratio Lower Upper
43 100
58 0.0 28.1 84.3#

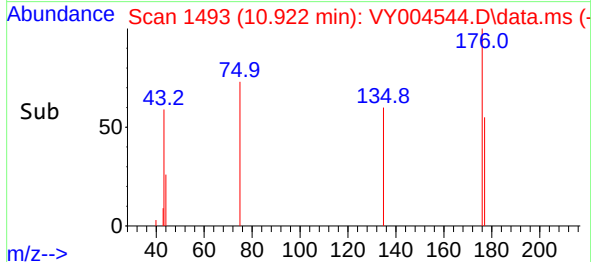

#62
4-Bromofluorobenzene
Concen: 47.68 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.137 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30


Tgt Ion: 95 Resp: 100229
Ion Ratio Lower Upper
95 100
174 83.4 0.0 169.0
176 80.9 0.0 162.4

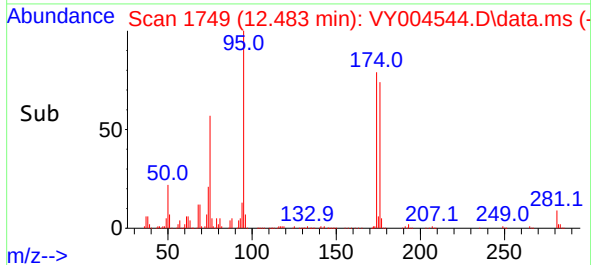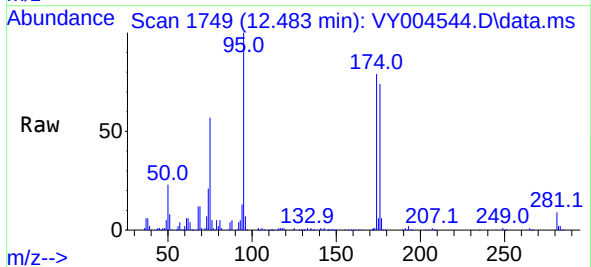



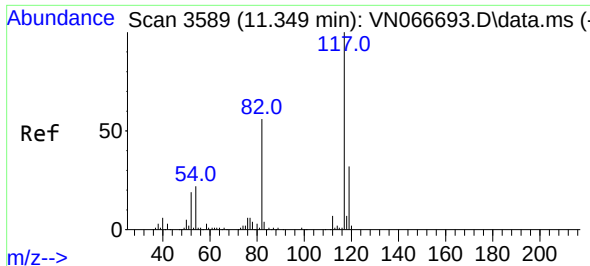


#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.496 min Scan# 1587
Delta R.T. 0.147 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30

Instrument :
MSVOA_Y
ClientSampled :



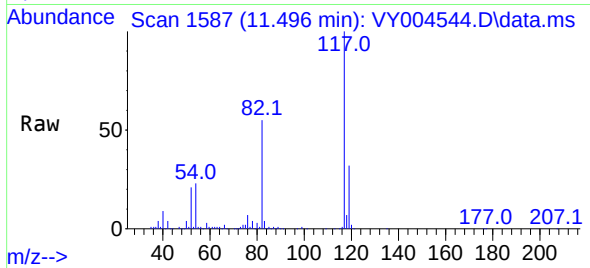



Tgt Ion:117 Resp: 229273
Ion Ratio Lower Upper
117 100
82 55.2 43.7 65.5
119 31.7 26.1 39.1

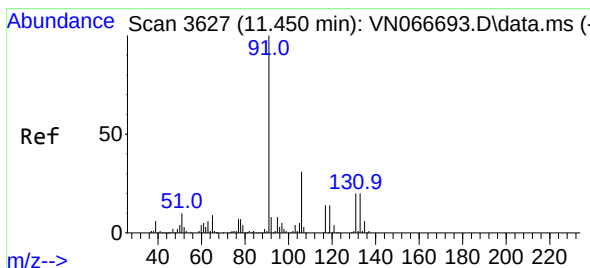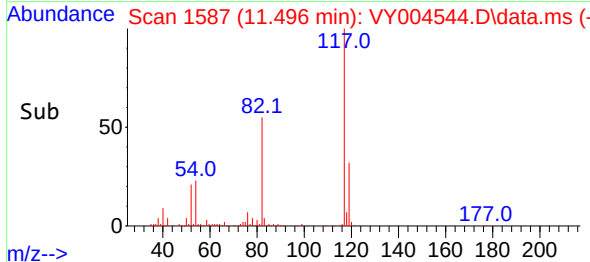

#66
1,1,1,2-Tetrachloroethane
Concen: 0.27 ug/l
RT: 11.313 min Scan# 1557
Delta R.T. -0.137 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30

Tgt Ion:131 Resp: 454
Ion Ratio Lower Upper
131 100
133 408.1 48.0 144.0#
119 0.0 34.1 102.2#


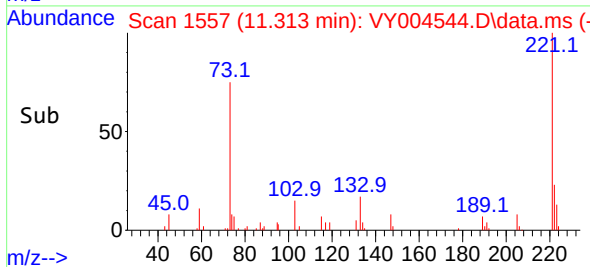

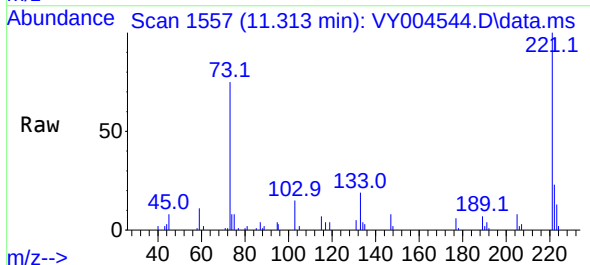




#70
Styrene
Concen: 3.06 ug/l
RT: 12.050 min Scan# 1678
Delta R.T. 0.141 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:	104	Resp:	462
Ion	Ratio	Lower	Upper
104	100		
78	47.2	39.0	58.4
103	57.1	44.5	66.7

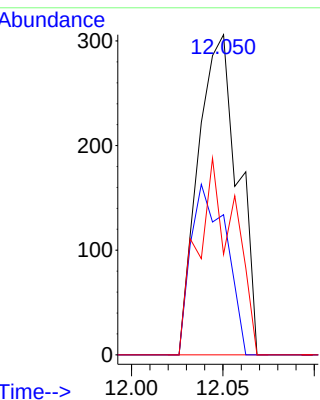

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.140 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30

Tgt Ion:	152	Resp:	103366
Ion	Ratio	Lower	Upper
152	100		
115	58.8	28.5	85.6
150	156.8	0.0	347.6


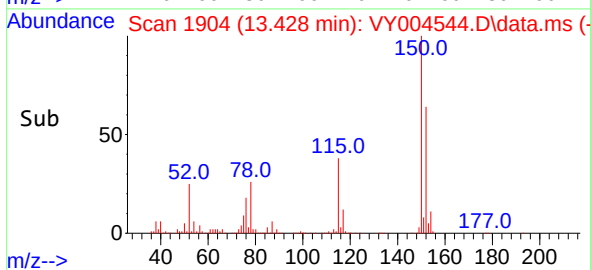
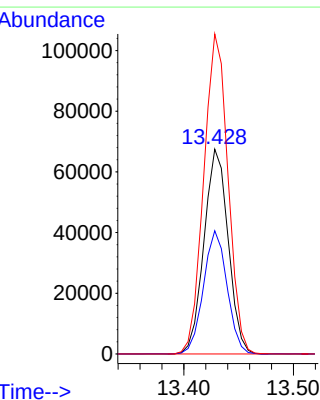





#76
1,2,3-Trichloropropane
Concen: 25.70 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.013 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30




Instrument :
MSVOA_Y
ClientSampled :


Tgt Ion: 75 Resp: 56849
Ion Ratio Lower Upper
75 100
77 1.3 0.0 0.0#



#79
2-Chlorotoluene
Concen: 1.03 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.134 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30

Tgt Ion: 91 Resp: 540
Ion Ratio Lower Upper
91 100
126 38.3 17.4 52.3



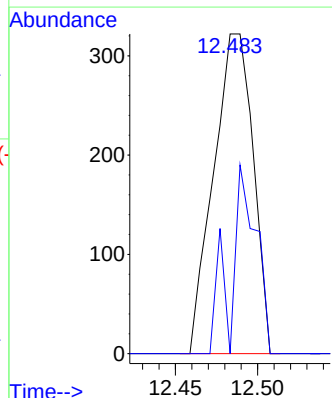





#81
trans-1,4-Dichloro-2-butene
Concen: 75.44 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.239 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 75 Resp: 56763
Ion Ratio Lower Upper
75 100
53 0.0 74.6 111.8#
89 0.0 35.8 53.8#

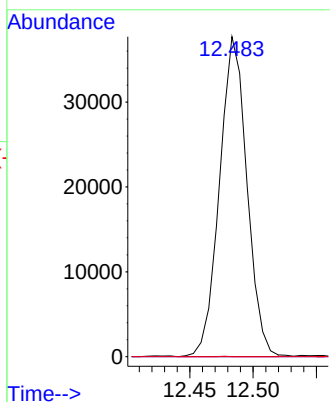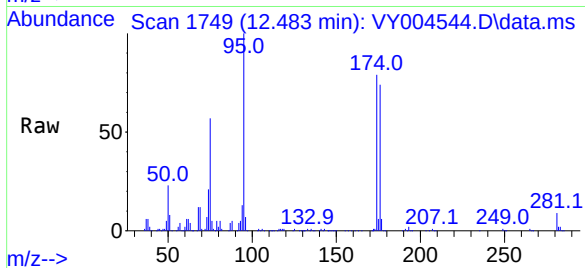

#87
1,3-Dichlorobenzene
Concen: 0.24 ug/l
RT: 13.373 min Scan# 1895
Delta R.T. 0.147 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30

Tgt Ion:146 Resp: 765
Ion Ratio Lower Upper
146 100
111 37.0 19.5 58.5
148 59.5 32.3 96.9


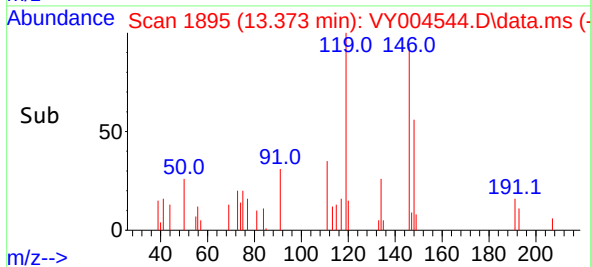
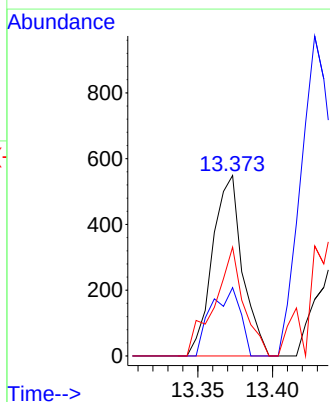
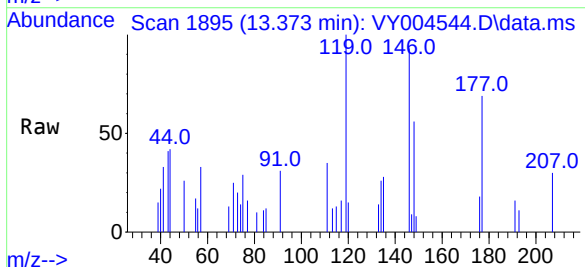




#88
1,4-Dichlorobenzene
Concen: 0.22 ug/l
RT: 13.373 min Scan# 1895
Delta R.T. 0.067 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30




Instrument :
MSVOA_Y
ClientSampled :


Tgt Ion:	146	Resp:	765
Ion	Ratio	Lower	Upper
146	100		
111	37.0	19.0	57.0
148	59.5	31.8	95.3

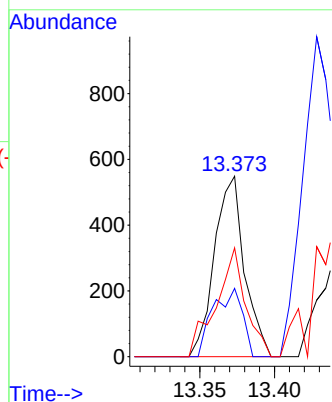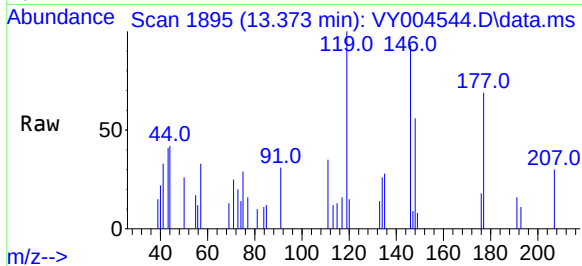

#89
n-Butylbenzene
Concen: 0.22 ug/l
RT: 13.696 min Scan# 1948
Delta R.T. 0.138 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30

Tgt Ion:	91	Resp:	1128
Ion	Ratio	Lower	Upper
91	100		
92	59.6	26.1	78.3
134	32.6	13.0	38.9


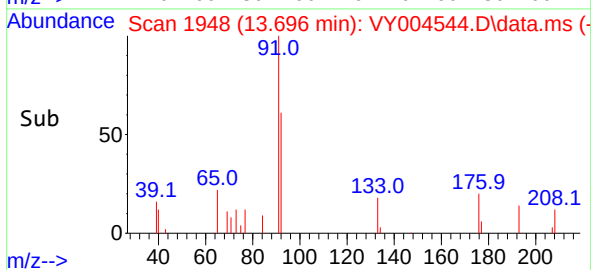

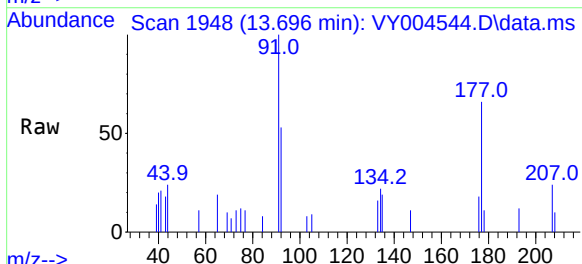




#92
1,2-Dibromo-3-Chloropropane
Concen: 0.24 ug/l
RT: 14.215 min Scan# 2033
Delta R.T. -0.001 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 75 Resp: 104
Ion Ratio Lower Upper
75 100
155 0.0 44.1 132.4#
157 0.0 56.0 168.2#

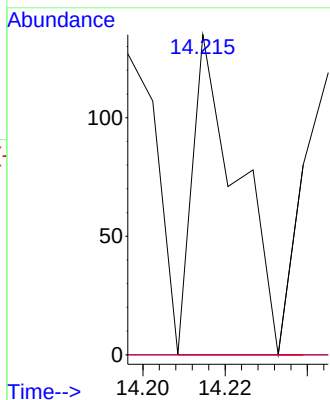

#93
1,2,4-Trichlorobenzene
Concen: 2.39 ug/l
RT: 15.007 min Scan# 2163
Delta R.T. 0.156 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30

Tgt Ion:180 Resp: 791
Ion Ratio Lower Upper
180 100
182 92.7 47.3 142.0
145 32.9 15.6 46.8


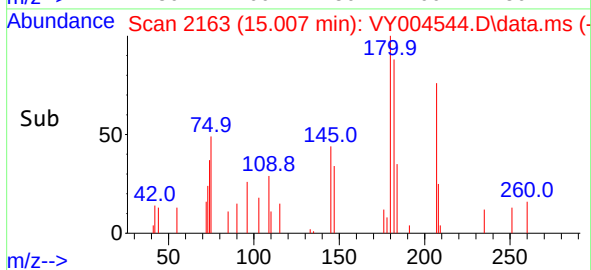
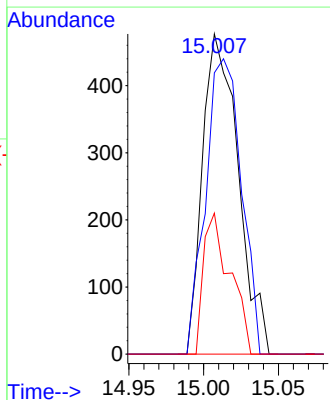





#94
Hexachlorobutadiene
Concen: 0.23 ug/l
RT: 15.111 min Scan# 2180
Delta R.T. 0.163 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30




Instrument :
MSVOA_Y
ClientSampled :


Tgt Ion:	225	Resp:	227
Ion	Ratio	Lower	Upper
225	100		
223	71.8	31.9	95.9
227	23.8	31.6	95.0#

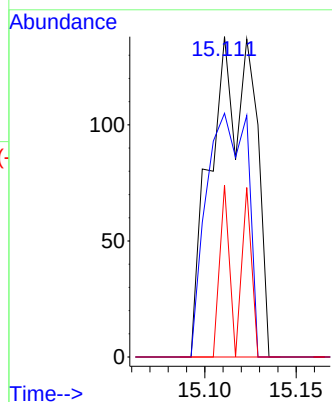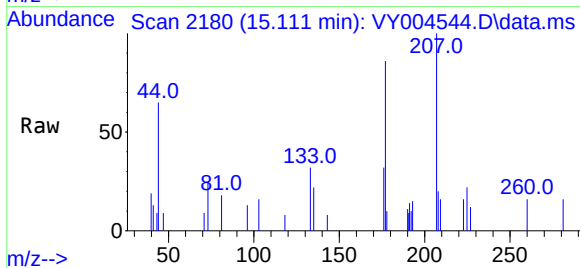

#95
Naphthalene
Concen: 2.34 ug/l
RT: 15.239 min Scan# 2201
Delta R.T. 0.168 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30


Tgt Ion:	128	Resp:	2441
Ion	Ratio	Lower	Upper
128	100		
127	12.9	10.2	15.2
129	10.4	8.6	13.0

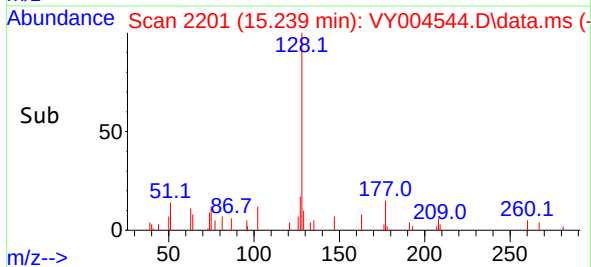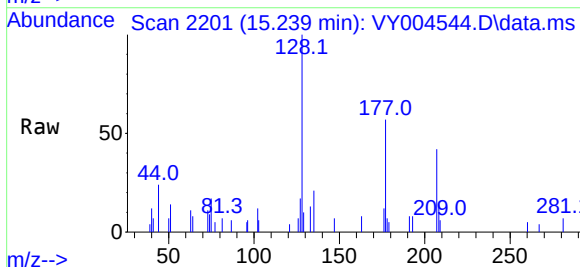



#96
1,2,3-Trichlorobenzene
Concen: 1.78 ug/l
RT: 15.422 min Scan# 2231
Delta R.T. 0.174 min
Lab File: VY004544.D
Acq: 21 Apr 2021 10:30

Instrument :
MSVOA_Y
ClientSampleId :

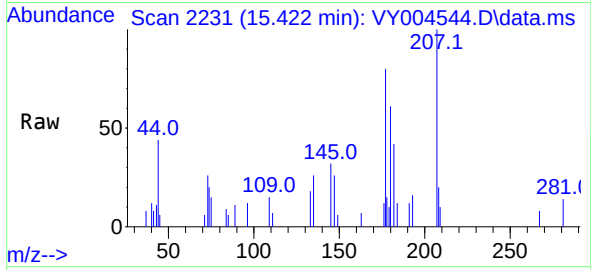

Tgt Ion:	180	Resp:	796
Ion	Ratio	Lower	Upper
180	100		
182	97.5	47.4	142.3
145	32.7	16.5	49.5

