
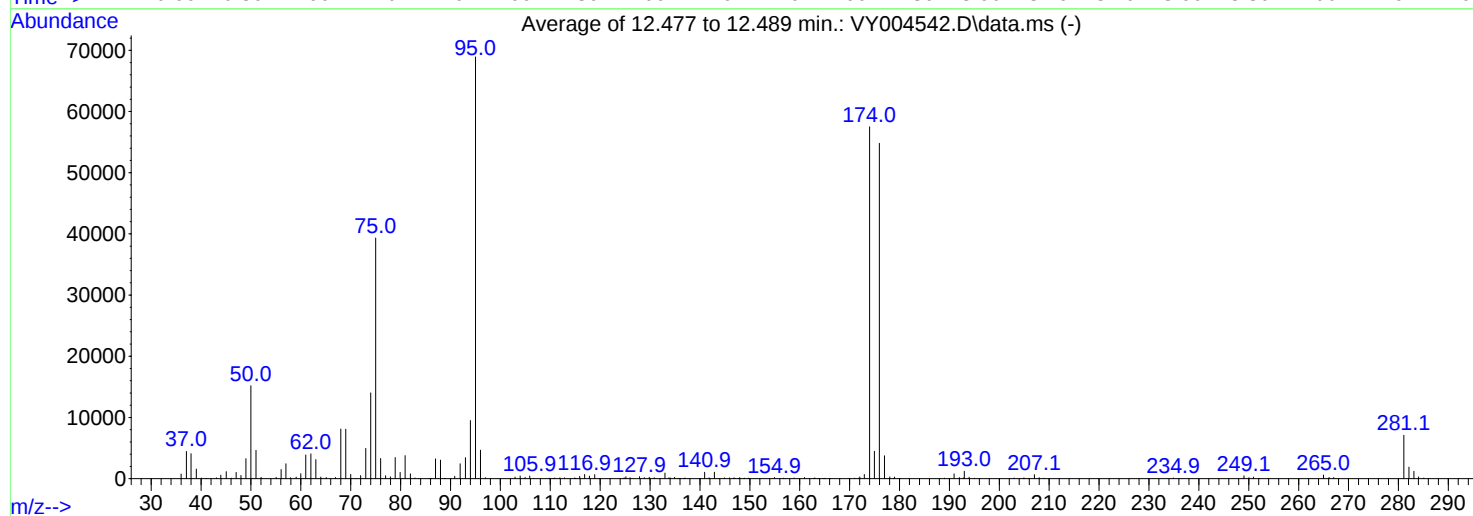


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042121\
 Data File : VY004542.D
 Acq On : 21 Apr 2021 09:10
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041221S.M
 Title : SW846 8260
 Last Update : Tue Apr 13 03:38:02 2021

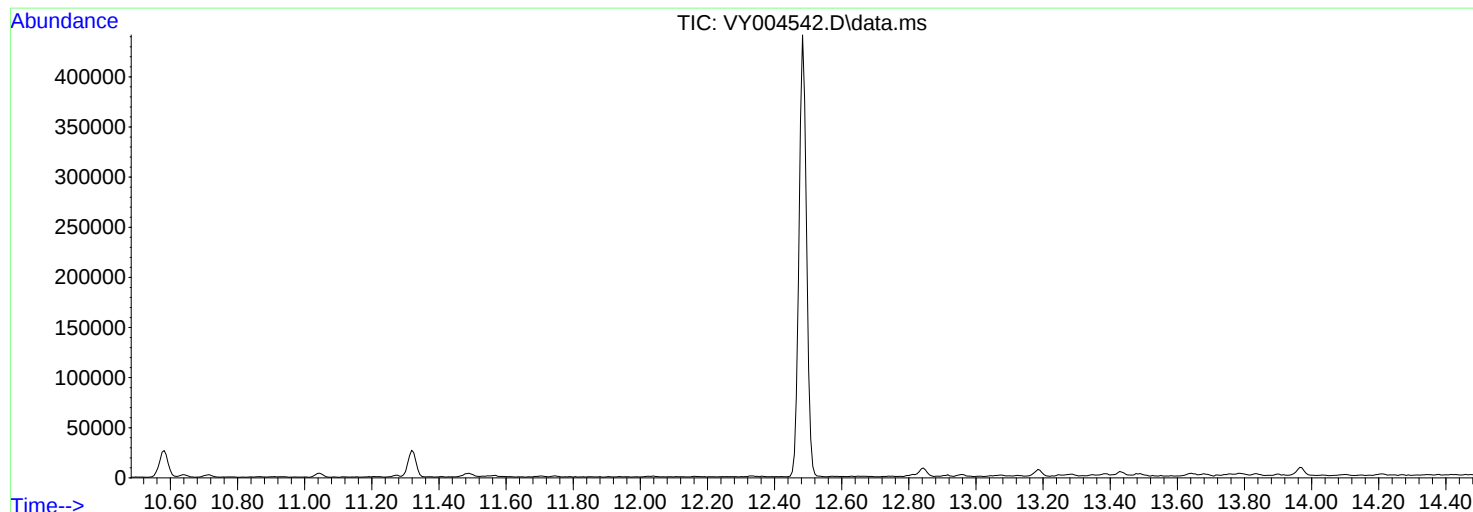

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	15204	PASS
75	95	30	60	57.0	39325	PASS
95	95	100	100	100.0	68933	PASS
96	95	5	9	6.8	4657	PASS
173	174	0.00	2	1.2	691	PASS
174	95	50	100	83.4	57512	PASS
175	174	5	9	7.8	4478	PASS
176	174	95	101	95.3	54807	PASS
177	176	5	9	6.8	3745	PASS