


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042224\
Data File : VY018006.D
Acq On : 22 Apr 2024 12:36
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041624S.M
Title : SW846 8260
Last Update : Wed Apr 17 06:24:42 2024

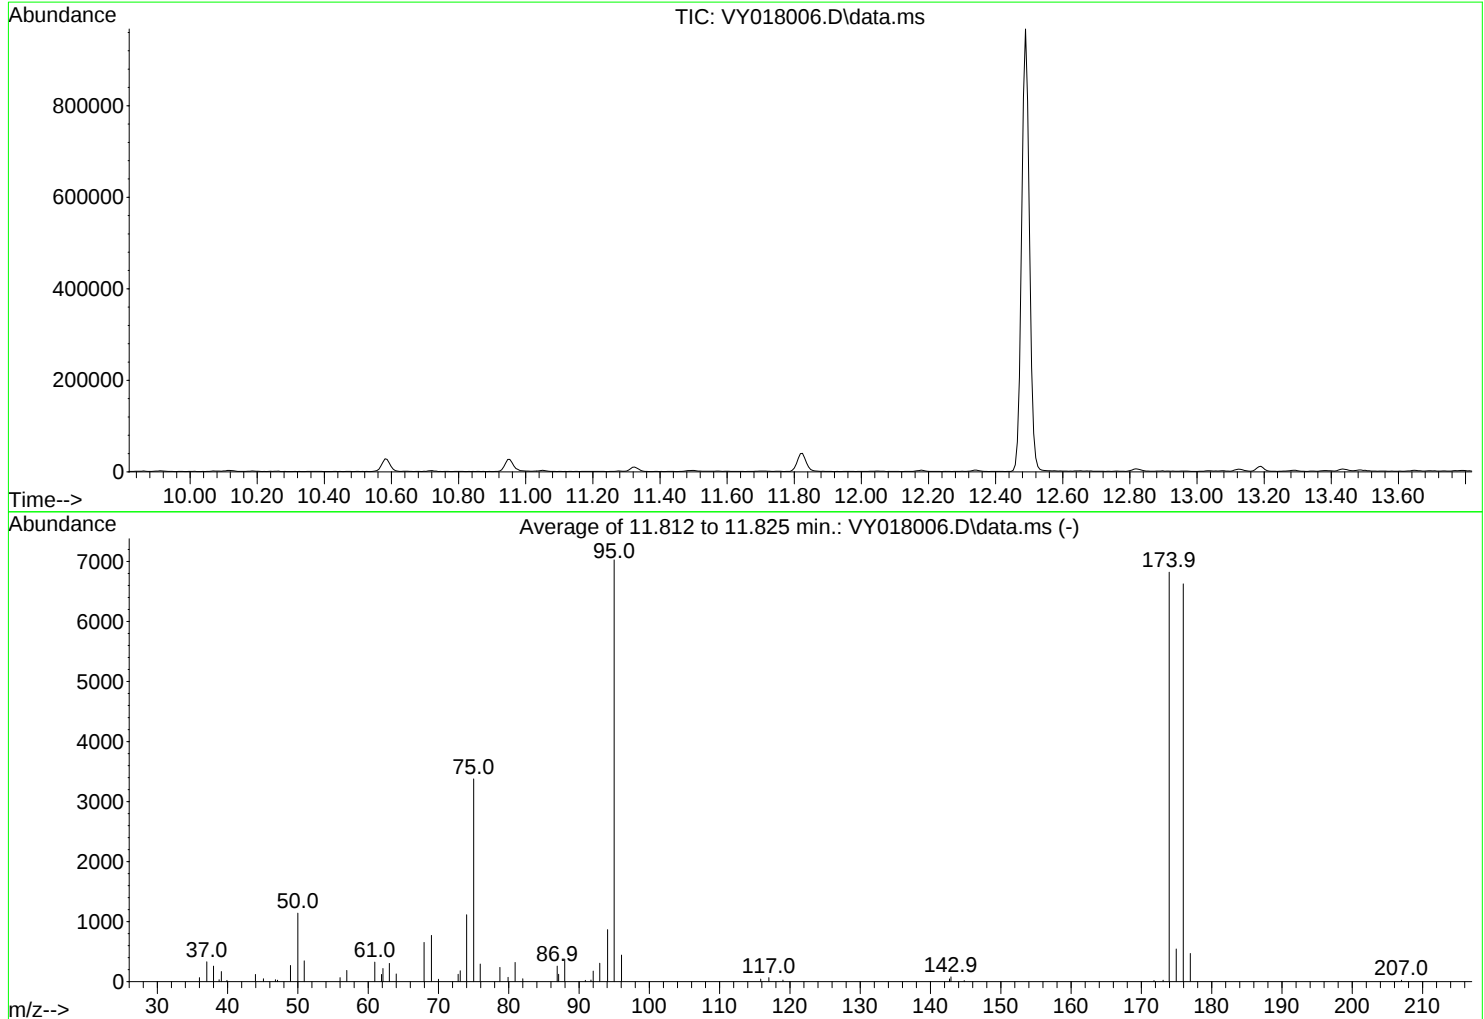

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	1142	PASS
75	95	30	60	48.1	3379	PASS
95	95	100	100	100.0	7028	PASS
96	95	5	9	6.3	443	PASS
173	174	0.00	2	0.3	23	PASS
174	95	50	100	97.1	6821	PASS
175	174	5	9	8.0	543	PASS
176	174	95	101	97.1	6626	PASS
177	176	5	9	7.1	469	PASS