
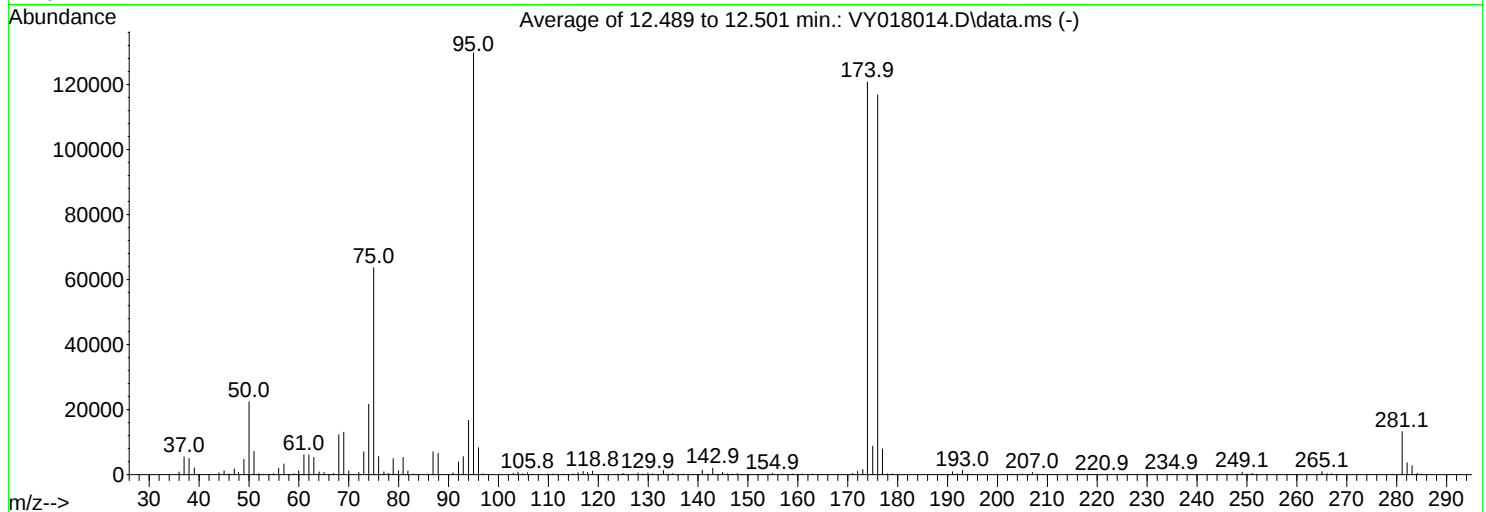


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042324\
Data File : VY018014.D
Acq On : 23 Apr 2024 08:21
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041624S.M
Title : SW846 8260
Last Update : Wed Apr 17 06:24:42 2024

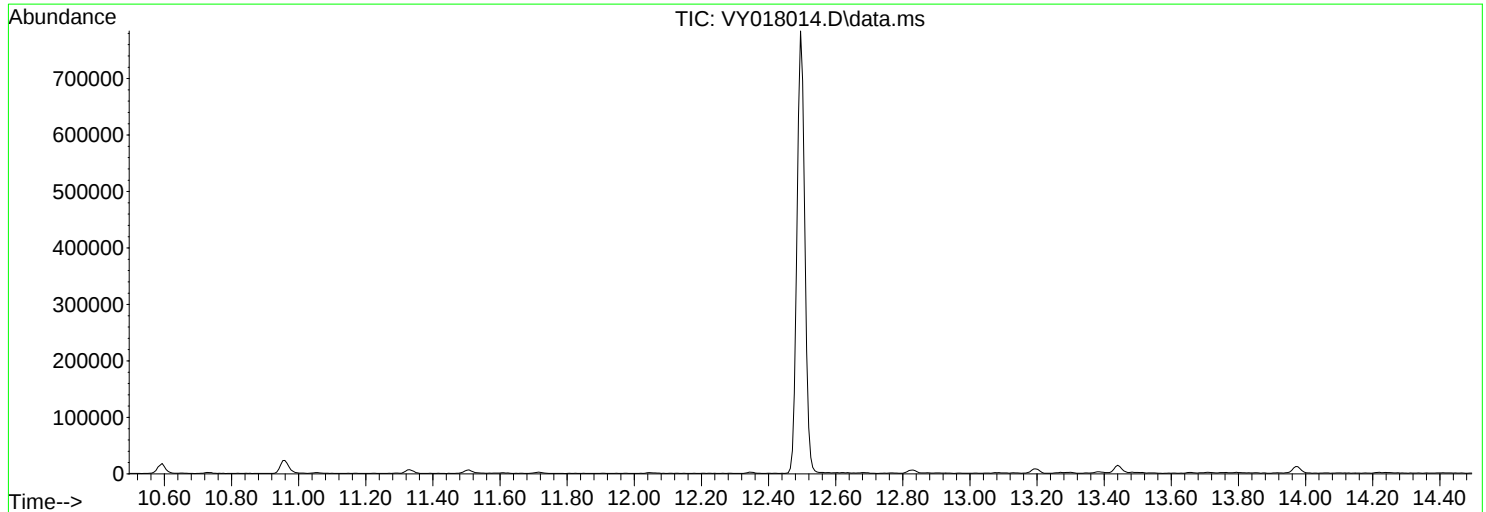

AutoFind: Scans 1750, 1751, 1752; Background Corrected with Scan 1742

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.2	22381	PASS
75	95	30	60	49.1	63656	PASS
95	95	100	100	100.0	129755	PASS
96	95	5	9	6.4	8311	PASS
173	174	0.00	2	1.3	1556	PASS
174	95	50	100	93.1	120811	PASS
175	174	5	9	7.3	8762	PASS
176	174	95	101	96.7	116805	PASS
177	176	5	9	6.8	7905	PASS