

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042623\
 Data File : VY013467.D
 Acq On : 26 Apr 2023 12:46
 Operator : KP/MD
 Sample : 02386-10
 Misc : 3.95g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SPA-3WC-23-04

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 05/01/2023
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 27 01:31:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 25 02:39:58 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	161647	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	261019	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	175554	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.434	152	141531	50.000	ug/l	# 0.01
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	103248	58.266	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 116.540%			
35) Dibromofluoromethane	7.716	113	88185	53.716	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 107.440%			
50) Toluene-d8	10.179	98	485974	83.212	ug/l	0.00
Spiked Amount 50.000	Range 58 - 134		Recovery = 166.420%#			
62) 4-Bromofluorobenzene	12.477	95	279208	141.812	ug/l	0.00
Spiked Amount 50.000	Range 30 - 143		Recovery = 283.620%#			
Target Compounds						
						Qvalue
16) Acetone	3.979	43	116495	166.938	ug/l	92
17) Carbon Disulfide	4.192	76	17591	3.224	ug/l	100
25) 2-Butanone	6.990	43	57090	64.508	ug/l	# 82
27) cis-1,2-Dichloroethene	6.996	96	3204	1.579	ug/l	54
31) Cyclohexane	7.771	56	442253	139.396	ug/l	# 59
39) Methylcyclohexane	9.185	83	1711518	532.844	ug/l	92
40) Benzene	8.161	78	2664711	347.198	ug/l	100
52) Toluene	10.246	92	7124481	1542.586	ug/l	92
65) Chlorobenzene	11.520	112	6931704	1812.571	ug/l	95
67) Ethyl Benzene	11.587	91	22262525m	3315.170	ug/l	
68) m/p-Xylenes	11.691	106	24355948m	9540.613	ug/l	
69) o-Xylene	12.032	106	12036399	4985.314	ug/l	58
73) Isopropylbenzene	12.331	105	3488611	325.889	ug/l	96
78) n-propylbenzene	12.672	91	7726697	585.999	ug/l	97
80) 1,3,5-Trimethylbenzene	12.813	105	13521641	1547.578	ug/l	94
83) tert-Butylbenzene	13.081	119	879697	116.213	ug/l	90
84) 1,2,4-Trimethylbenzene	13.117	105	19885138m	2340.884	ug/l	
85) sec-Butylbenzene	13.258	105	1543118	135.829	ug/l	# 42
86) p-Isopropyltoluene	13.373	119	5308481	581.051	ug/l	# 68
87) 1,3-Dichlorobenzene	13.367	146	1856887m	375.758	ug/l	
88) 1,4-Dichlorobenzene	13.453	146	9038048	1810.546	ug/l	90
91) 1,2-Dichlorobenzene	13.745	146	11726530	2627.795	ug/l	87
93) 1,2,4-Trichlorobenzene	15.007	180	525153	197.383	ug/l	# 88
94) Hexachlorobutadiene	15.111	225	7039	4.546	ug/l	98
96) 1,2,3-Trichlorobenzene	15.422	180	58193	24.540	ug/l	# 73

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Manual Integrations APPROVED


Quant Time: Apr 27 01:31:06 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
Quant Title : SW846 8260
QLast Update : Tue Apr 25 02:39:58 2023
Response via : Initial Calibration





#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46




Instrument :
MSVOA_Y
ClientSampleId :
SPA-3WC-23-04



Tgt Ion:168 Resp: 16164
Ion Ratio Lower Upper
168 100
99 55.6 41.8 62.6




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023

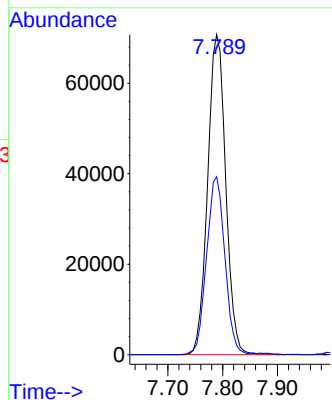

#16
Acetone
Concen: 166.938 ug/l
RT: 3.979 min Scan# 354
Delta R.T. 0.031 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46

Tgt Ion: 43 Resp: 116495
Ion Ratio Lower Upper
43 100
58 27.1 25.4 38.0

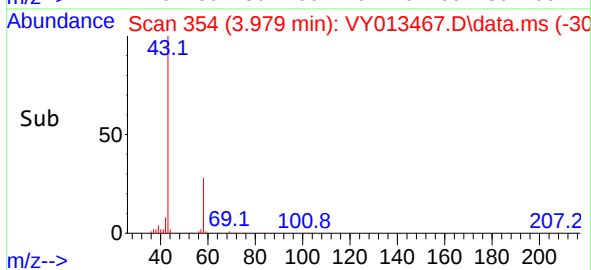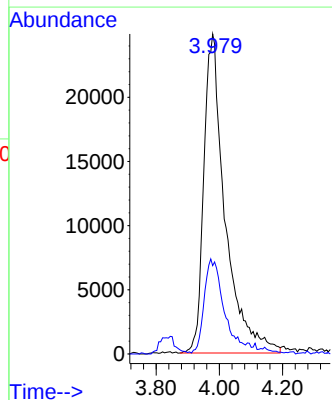







#17
Carbon Disulfide
Concen: 3.224 ug/l
RT: 4.192 min Scan# 389
Delta R.T. 0.000 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46

Instrument :
MSVOA_Y
ClientSampleId :
SPA-3WC-23-04

Tgt Ion: 76 Resp: 1759
Ion Ratio Lower Upper
76 100
78 9.2 7.2 10.8




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023

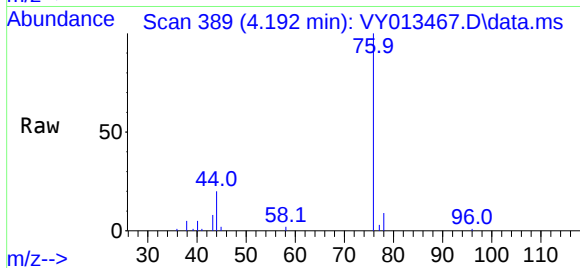

#25
2-Butanone
Concen: 64.508 ug/l
RT: 6.990 min Scan# 848
Delta R.T. 0.006 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46


Tgt Ion: 43 Resp: 57090
Ion Ratio Lower Upper
43 100
72 17.8 21.9 32.9#

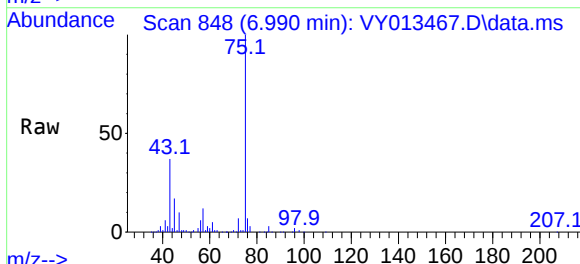



#27
cis-1,2-Dichloroethene
Concen: 1.579 ug/l
RT: 6.996 min Scan# 849
Delta R.T. 0.012 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46




Instrument :
MSVOA_Y
ClientSampleId :
SPA-3WC-23-04

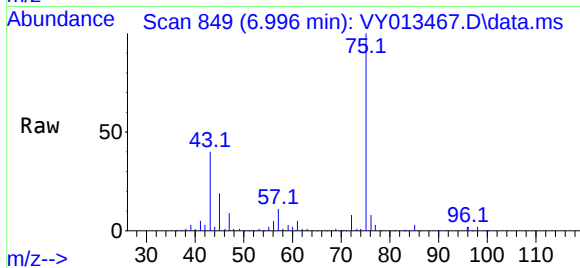

Tgt Ion: 96 Resp: 3204
Ion Ratio Lower Upper
96 100
61 223.7 0.0 285.0
98 62.9 0.0 130.6




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023

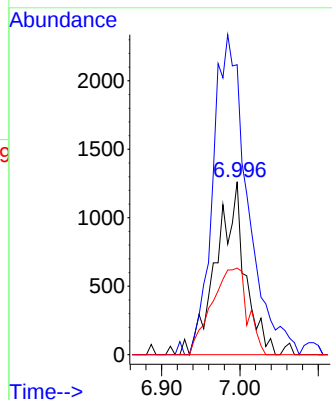

#31
Cyclohexane
Concen: 139.396 ug/l
RT: 7.771 min Scan# 976
Delta R.T. -0.012 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46

Tgt Ion: 56 Resp: 442253
Ion Ratio Lower Upper
56 100
69 15.9 29.2 43.8#
84 50.5 73.0 109.6#

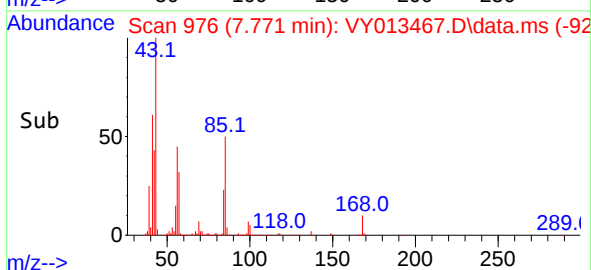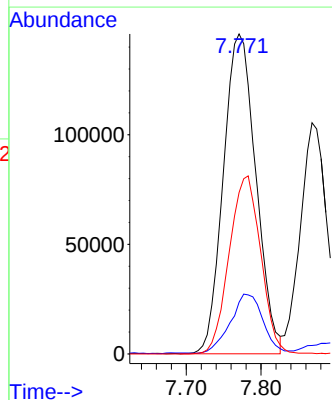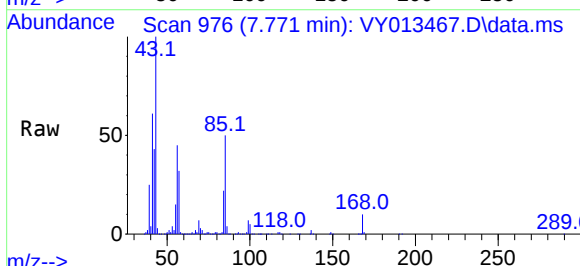

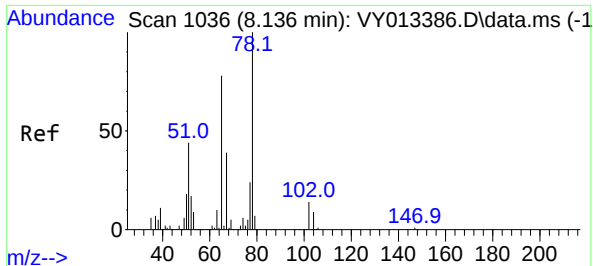

#33

1,2-Dichloroethane-d4

Concen: 58.266 ug/l

RT: 8.143 min Scan# 1036

Delta R.T. 0.007 min

Lab File: VY013467.D

Acq: 26 Apr 2023 12:46

Instrument :

MSVOA_Y

ClientSampleId :

SPA-3WC-23-04

Tgt Ion: 65 Resp: 10324

Ion Ratio Lower Upper

65 100





67 53.1 0.0 103.4

Manual Integrations

APPROVED

Reviewed By :Krupa Patel 05/01/2023

Supervised By :Mahesh Dadoda 05/01/2023

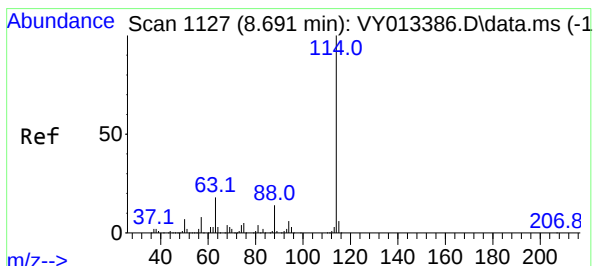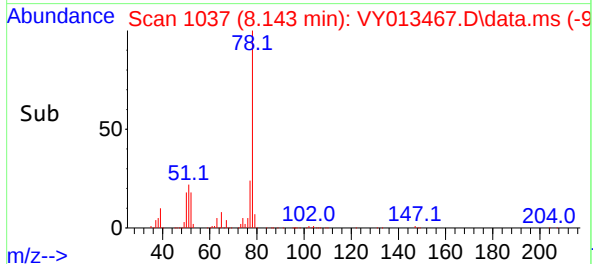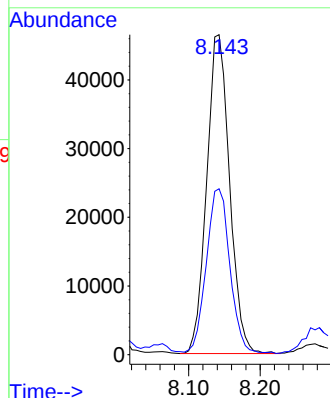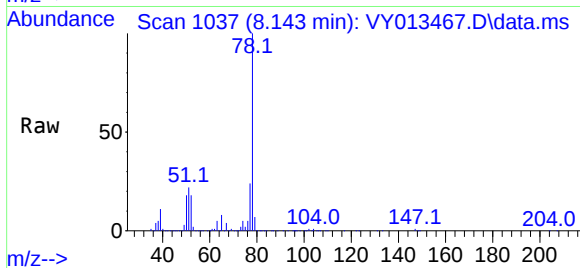

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY013467.D

Acq: 26 Apr 2023 12:46




Tgt Ion:114 Resp: 261019


Ion Ratio Lower Upper

114 100

63 21.0 0.0 36.6


88 15.4 0.0 28.8

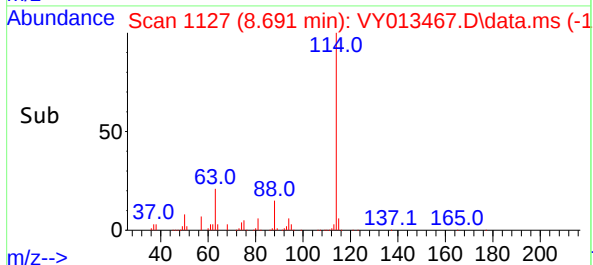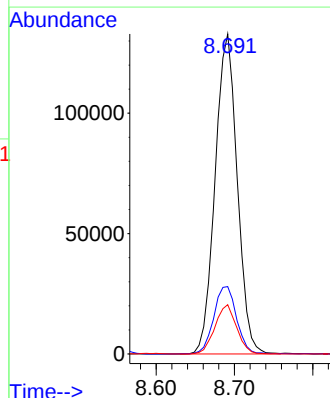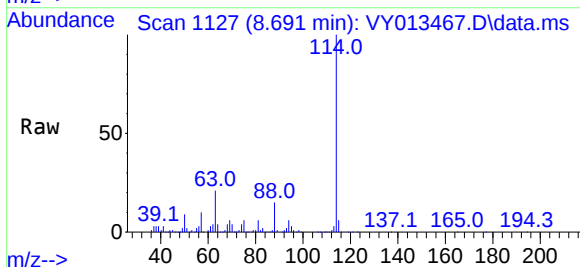



#35
Dibromofluoromethane
Concen: 53.716 ug/l
RT: 7.716 min Scan# 90
Delta R.T. -0.000 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46




Instrument :
MSVOA_Y
ClientSampleId :
SPA-3WC-23-04




Tgt Ion: 113 Resp: 8818
Ion Ratio Lower Upper
113 100
111 103.1 82.2 123.2
192 19.4 16.7 25.1

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023

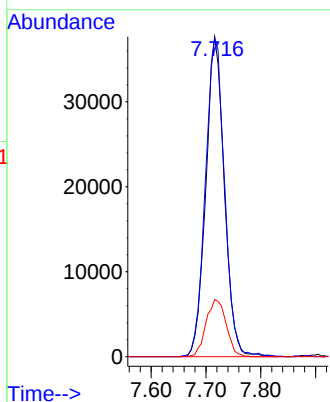


#39
Methylcyclohexane
Concen: 532.844 ug/l
RT: 9.185 min Scan# 1208
Delta R.T. 0.006 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46




Tgt Ion: 83 Resp: 1711518
Ion Ratio Lower Upper
83 100
55 83.5 59.0 88.4
98 45.3 37.0 55.4

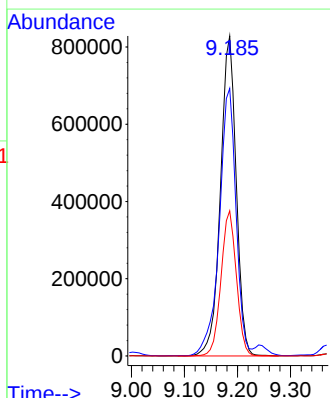



#40
Benzene
Concen: 347.198 ug/l
RT: 8.161 min Scan# 1040
Delta R.T. -0.000 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46




Instrument :
MSVOA_Y
ClientSampleId :
SPA-3WC-23-04



Tgt Ion: 78 Resp: 266471
Ion Ratio Lower Upper
78 100
77 24.1 19.2 28.8




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023



#50
Toluene-d8
Concen: 83.212 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46


Tgt Ion: 98 Resp: 485974
Ion Ratio Lower Upper
98 100
100 36.1 50.5 75.7#

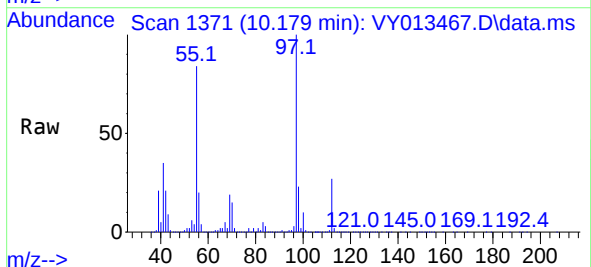



#52
Toluene
Concen: 1542.586 ug/l
RT: 10.246 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46




Instrument :
MSVOA_Y
ClientSampleId :
SPA-3WC-23-04



Tgt Ion: 92 Resp: 712448
Ion Ratio Lower Upper
92 100
91 164.5 140.2 210.4




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023

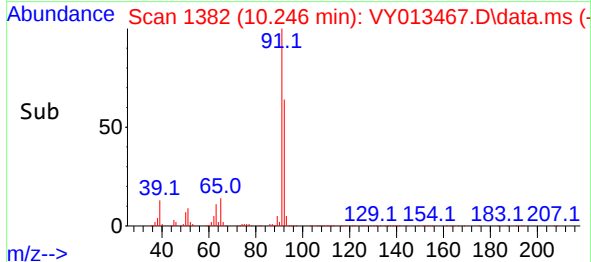

#62
4-Bromofluorobenzene
Concen: 141.812 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.000 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46


Tgt Ion: 95 Resp: 279208
Ion Ratio Lower Upper
95 100
174 18.6 0.0 182.0
176 18.2 0.0 175.4

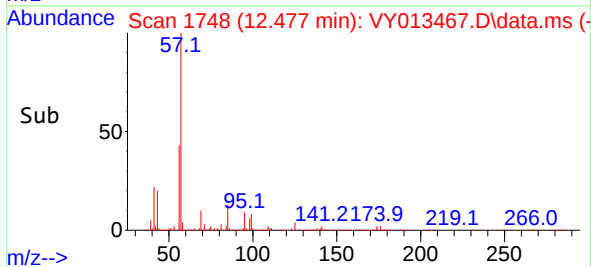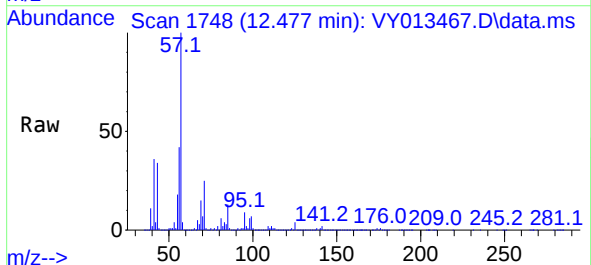



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 11586
Delta R.T. 0.001 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46




Instrument :
MSVOA_Y
ClientSampleId :
SPA-3WC-23-04




Tgt Ion:117 Resp: 175554
Ion Ratio Lower Upper
117 100
82 52.6 43.0 64.6
119 31.6 25.5 38.3

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023




#65
Chlorobenzene
Concen: 1812.571 ug/l
RT: 11.520 min Scan# 1591
Delta R.T. 0.006 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46




Tgt Ion:112 Resp: 6931704
Ion Ratio Lower Upper
112 100
114 34.0 24.9 37.3

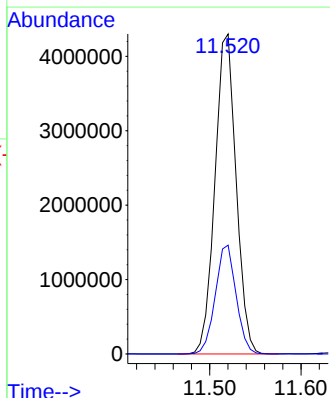



#67
Ethyl Benzene
Concen: 3315.170 ug/l m
RT: 11.587 min Scan# 1602
Delta R.T. -0.006 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46




Instrument :
MSVOA_Y
ClientSampleId :
SPA-3WC-23-04

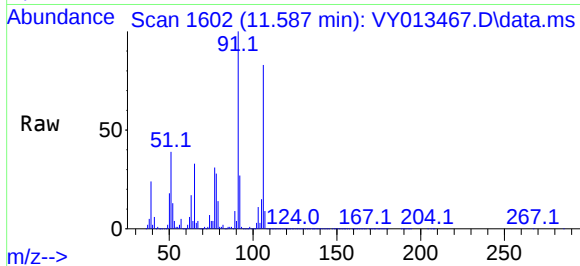


Tgt Ion: 91 Resp:2226252
Ion Ratio Lower Upper
91 100
106 82.6 25.1 37.7

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023

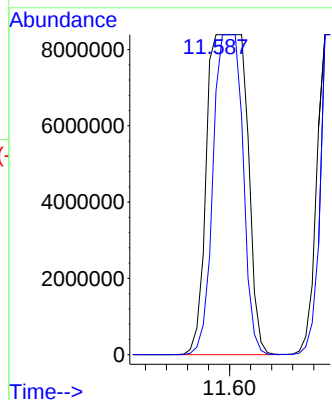


#68
m/p-Xylenes
Concen: 9540.613 ug/l m
RT: 11.691 min Scan# 1619
Delta R.T. -0.012 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46

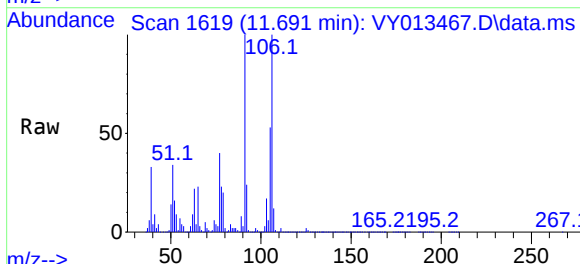

Tgt Ion:106 Resp:24355948
Ion Ratio Lower Upper
106 100
91 0.0 160.9 241.3

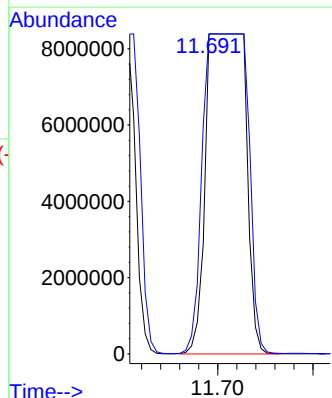







#69
o-Xylene
Concen: 4985.314 ug/l
RT: 12.032 min Scan# 106
Delta R.T. 0.006 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46

Instrument :
MSVOA_Y
ClientSampleId :
SPA-3WC-23-04

Tgt Ion:106 Resp:1203639
Ion Ratio Lower Upper
106 100
91 144.6 105.5 316.4




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023

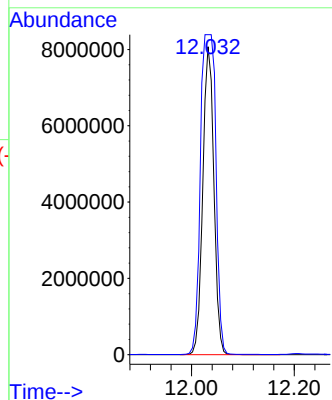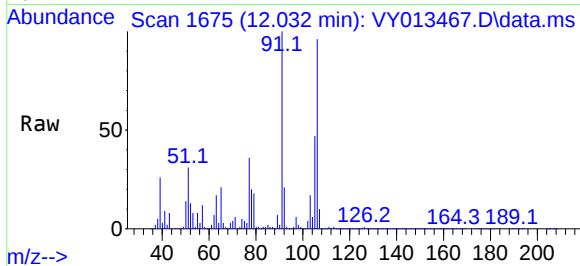

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.434 min Scan# 1905
Delta R.T. 0.012 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46


Tgt Ion:152 Resp: 141531
Ion Ratio Lower Upper
152 100
115 0.0 28.1 84.2#
150 0.0 0.0 352.0

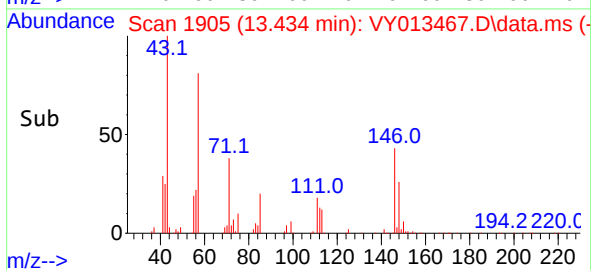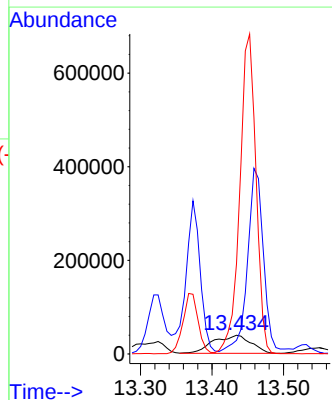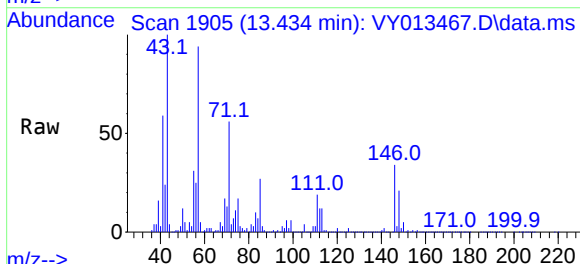



#73
Isopropylbenzene
Concen: 325.889 ug/l
RT: 12.331 min Scan# 1724
Delta R.T. -0.000 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46




Instrument :
MSVOA_Y
ClientSampleId :
SPA-3WC-23-04




Tgt Ion: 105 Resp: 348861
Ion Ratio Lower Upper
105 100
120 25.0 13.7 41.0

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023




#78
n-propylbenzene
Concen: 585.999 ug/l
RT: 12.672 min Scan# 1780
Delta R.T. 0.000 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46




Tgt Ion: 91 Resp: 7726697
Ion Ratio Lower Upper
91 100
120 22.3 11.9 35.9

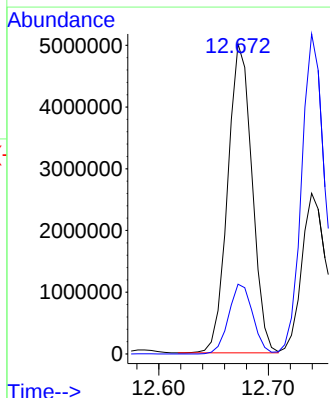



#80
1,3,5-Trimethylbenzene
Concen: 1547.578 ug/l
RT: 12.813 min Scan# 1803
Delta R.T. 0.001 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46




Instrument :
MSVOA_Y
ClientSampleId :
SPA-3WC-23-04




Tgt Ion:105 Resp:1352164
Ion Ratio Lower Upper
105 100
120 53.3 24.7 74.1

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023

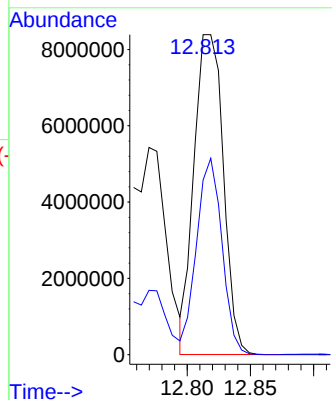


#83
tert-Butylbenzene
Concen: 116.213 ug/l
RT: 13.081 min Scan# 1847
Delta R.T. 0.007 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46




Tgt Ion:119 Resp: 879697
Ion Ratio Lower Upper
119 100
91 74.5 32.2 96.6
134 23.6 13.0 38.9

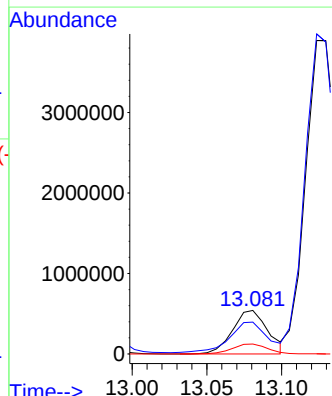



#84
1,2,4-Trimethylbenzene
Concen: 2340.884 ug/l m
RT: 13.117 min Scan# 1853
Delta R.T. 0.000 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46




Instrument :
MSVOA_Y
ClientSampleId :
SPA-3WC-23-04




Tgt Ion:105 Resp:19885138
Ion Ratio Lower Upper
105 100
120 12.6 22.3 66.9

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023

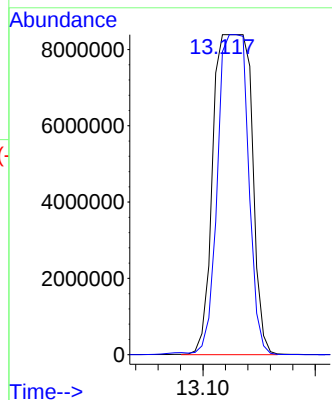


#85
sec-Butylbenzene
Concen: 135.829 ug/l
RT: 13.258 min Scan# 1876
Delta R.T. 0.007 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46




Tgt Ion:105 Resp: 1543118
Ion Ratio Lower Upper
105 100
134 47.6 10.3 30.9

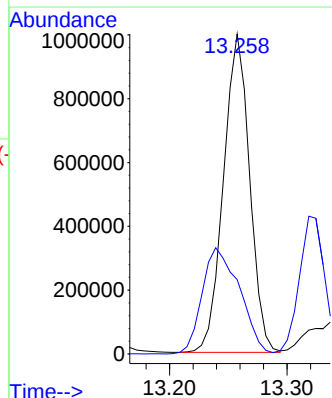



#86
p-Isopropyltoluene
Concen: 581.051 ug/l
RT: 13.373 min Scan# 1895
Delta R.T. 0.006 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46




Instrument :
MSVOA_Y
ClientSampleId :
SPA-3WC-23-04




Tgt Ion:119 Resp: 530848
Ion Ratio Lower Upper
119 100
134 26.2 13.4 40.2
91 57.0 12.1 36.3

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023

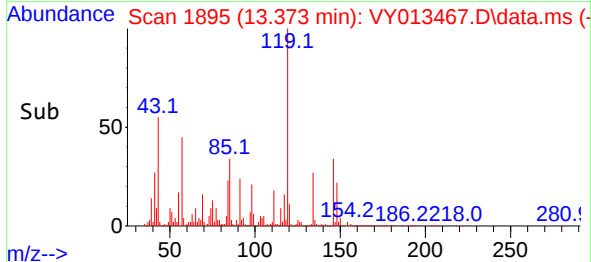


#87
1,3-Dichlorobenzene
Concen: 375.758 ug/l m
RT: 13.367 min Scan# 1894
Delta R.T. 0.000 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46




Tgt Ion:146 Resp: 1856887
Ion Ratio Lower Upper
146 100
111 244.3 19.3 57.9#
148 321.6 31.9 95.7#

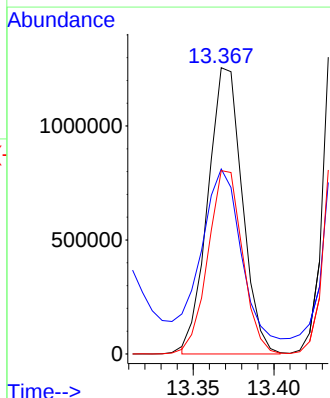



#88
1,4-Dichlorobenzene
Concen: 1810.546 ug/l
RT: 13.453 min Scan# 1908
Delta R.T. 0.007 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46




Instrument :
MSVOA_Y
ClientSampleId :
SPA-3WC-23-04

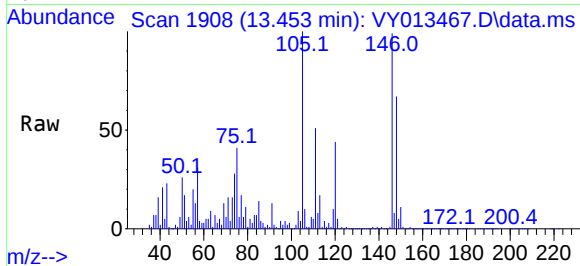


Tgt Ion:146 Resp: 903804
Ion Ratio Lower Upper
146 100
111 50.2 18.9 56.5
148 66.1 31.9 95.5

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023

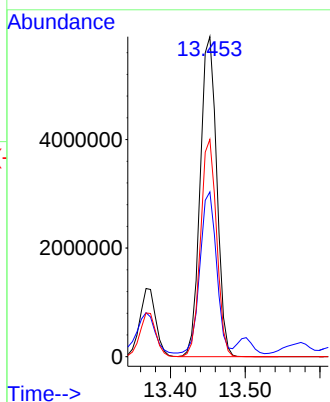


#91
1,2-Dichlorobenzene
Concen: 2627.795 ug/l
RT: 13.745 min Scan# 1956
Delta R.T. 0.006 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46

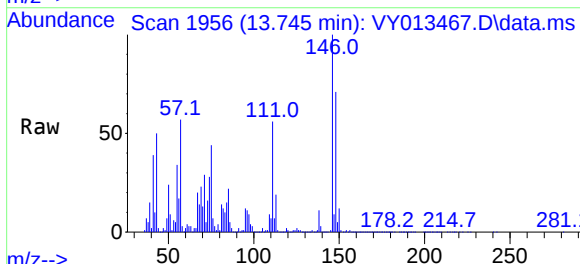


Tgt Ion:146 Resp:11726530
Ion Ratio Lower Upper
146 100
111 54.8 19.8 59.4
148 68.0 31.8 95.4





#93
1,2,4-Trichlorobenzene
Concen: 197.383 ug/l
RT: 15.007 min Scan# 2163
Delta R.T. 0.000 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46




Instrument :
MSVOA_Y
ClientSampleId :
SPA-3WC-23-04




Tgt Ion:180 Resp: 52515
Ion Ratio Lower Upper
180 100
182 96.1 48.5 145.5
145 56.0 15.0 45.0

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023

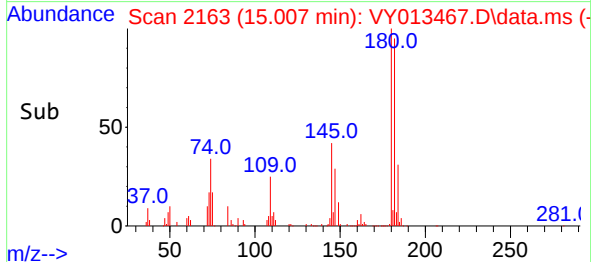


#94
Hexachlorobutadiene
Concen: 4.546 ug/l
RT: 15.111 min Scan# 2180
Delta R.T. -0.000 min
Lab File: VY013467.D
Acq: 26 Apr 2023 12:46



Tgt Ion:225 Resp: 7039
Ion Ratio Lower Upper
225 100
223 64.7 31.4 94.2
227 65.2 32.0 96.0

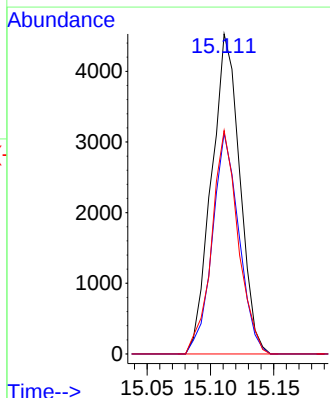



#96
 1,2,3-Trichlorobenzene
 Concen: 24.540 ug/l
 RT: 15.422 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VY013467.D
 Acq: 26 Apr 2023 12:46

Instrument :
 MSVOA_Y
 ClientSampleId :
 SPA-3WC-23-04

Tgt Ion:180	Resp:	5819
Ion Ratio	Lower	Upper
180	100	
182	92.1	47.1 141.3
145	87.3	15.9 47.7

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 05/01/2023
 Supervised By :Mahesh Dadoda 05/01/2023

