
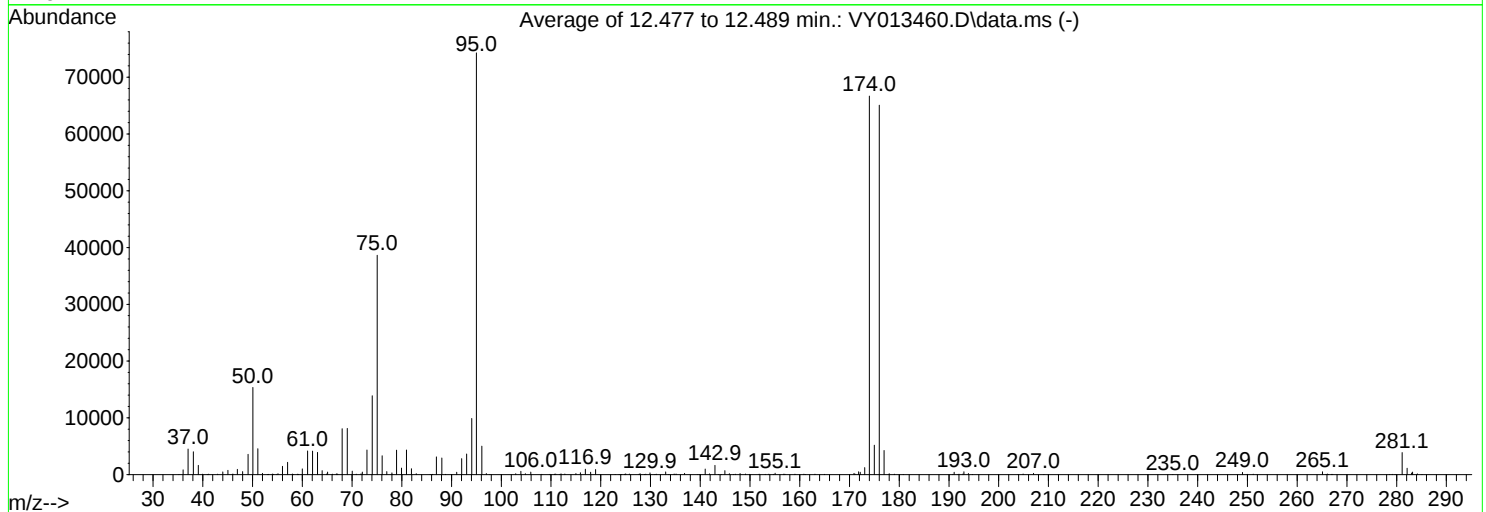


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042623\
Data File : VY013460.D
Acq On : 26 Apr 2023 09:12
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
Title : SW846 8260
Last Update : Tue Apr 25 02:39:58 2023

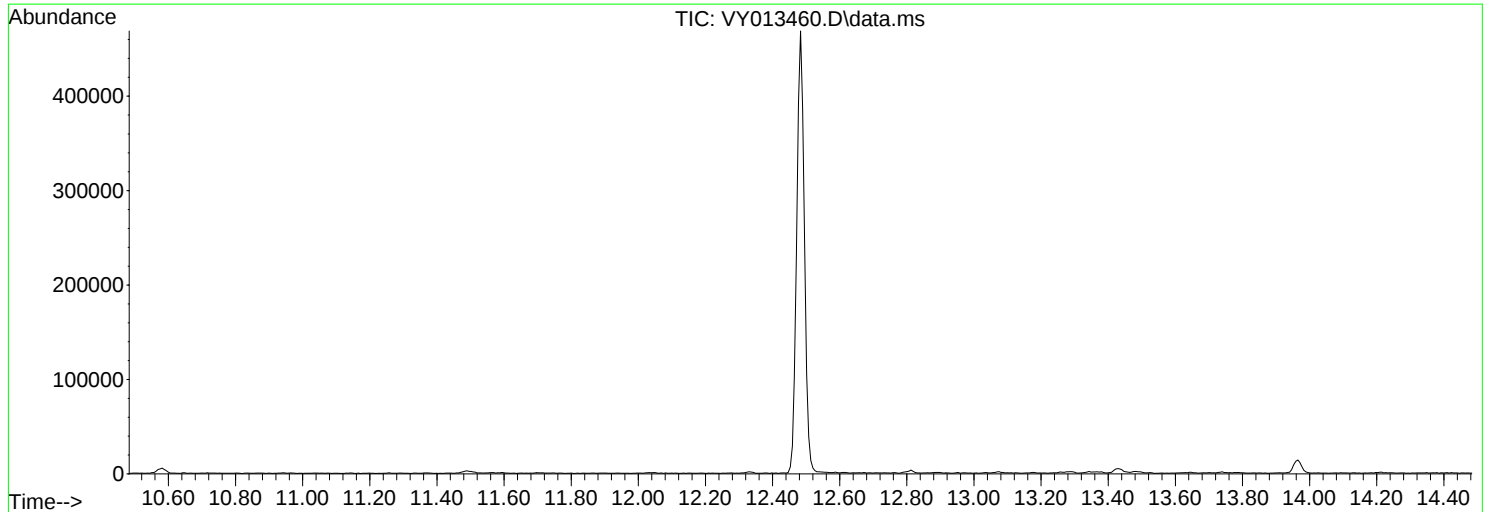

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	15353	PASS
75	95	30	60	52.0	38637	PASS
95	95	100	100	100.0	74293	PASS
96	95	5	9	6.8	5025	PASS
173	174	0.00	2	1.9	1244	PASS
174	95	50	100	89.8	66685	PASS
175	174	5	9	7.8	5190	PASS
176	174	95	101	97.6	65085	PASS
177	176	5	9	6.5	4251	PASS