

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042723\
 Data File : VY013498.D
 Acq On : 27 Apr 2023 17:40
 Operator : KP/MD
 Sample : 02470-07
 Misc : 5.02g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-08-8.5-9.0

Quant Time: Apr 28 01:32:48 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 25 02:39:58 2023
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.783	168	224361	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	395564	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	381022	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	169573	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.137	65	164863	67.031	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 134.060%	
35) Dibromofluoromethane	7.710	113	139461	56.055	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 112.120%	
50) Toluene-d8	10.179	98	488030	55.141	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 110.280%	
62) 4-Bromofluorobenzene	12.477	95	154753	51.866	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	= 103.740%	
Target Compounds						
					Qvalue	
13) Acrolein	3.747	56	20	Below Cal	#	16
20) Methylene Chloride	4.710	84	23452	Below Cal	#	84
31) Cyclohexane	7.783	56	5403	1.227	ug/l #	17
36) 1,1-Dichloropropene	7.783	75	18449	4.468	ug/l #	49
38) Carbon Tetrachloride	7.777	117	23068	5.330	ug/l #	14
76) 1,2,3-Trichloropropane	12.477	75	83484	36.505	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.477	75	83484	74.674	ug/l #	13


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042723\
Data File : VY013498.D
Acq On : 27 Apr 2023 17:40
Operator : KP/MD
Sample : 02470-07
Misc : 5.02g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SB-08-8.5-9.0

Quant Time: Apr 28 01:32:48 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
Quant Title : SW846 8260
QLast Update : Tue Apr 25 02:39:58 2023
Response via : Initial Calibration




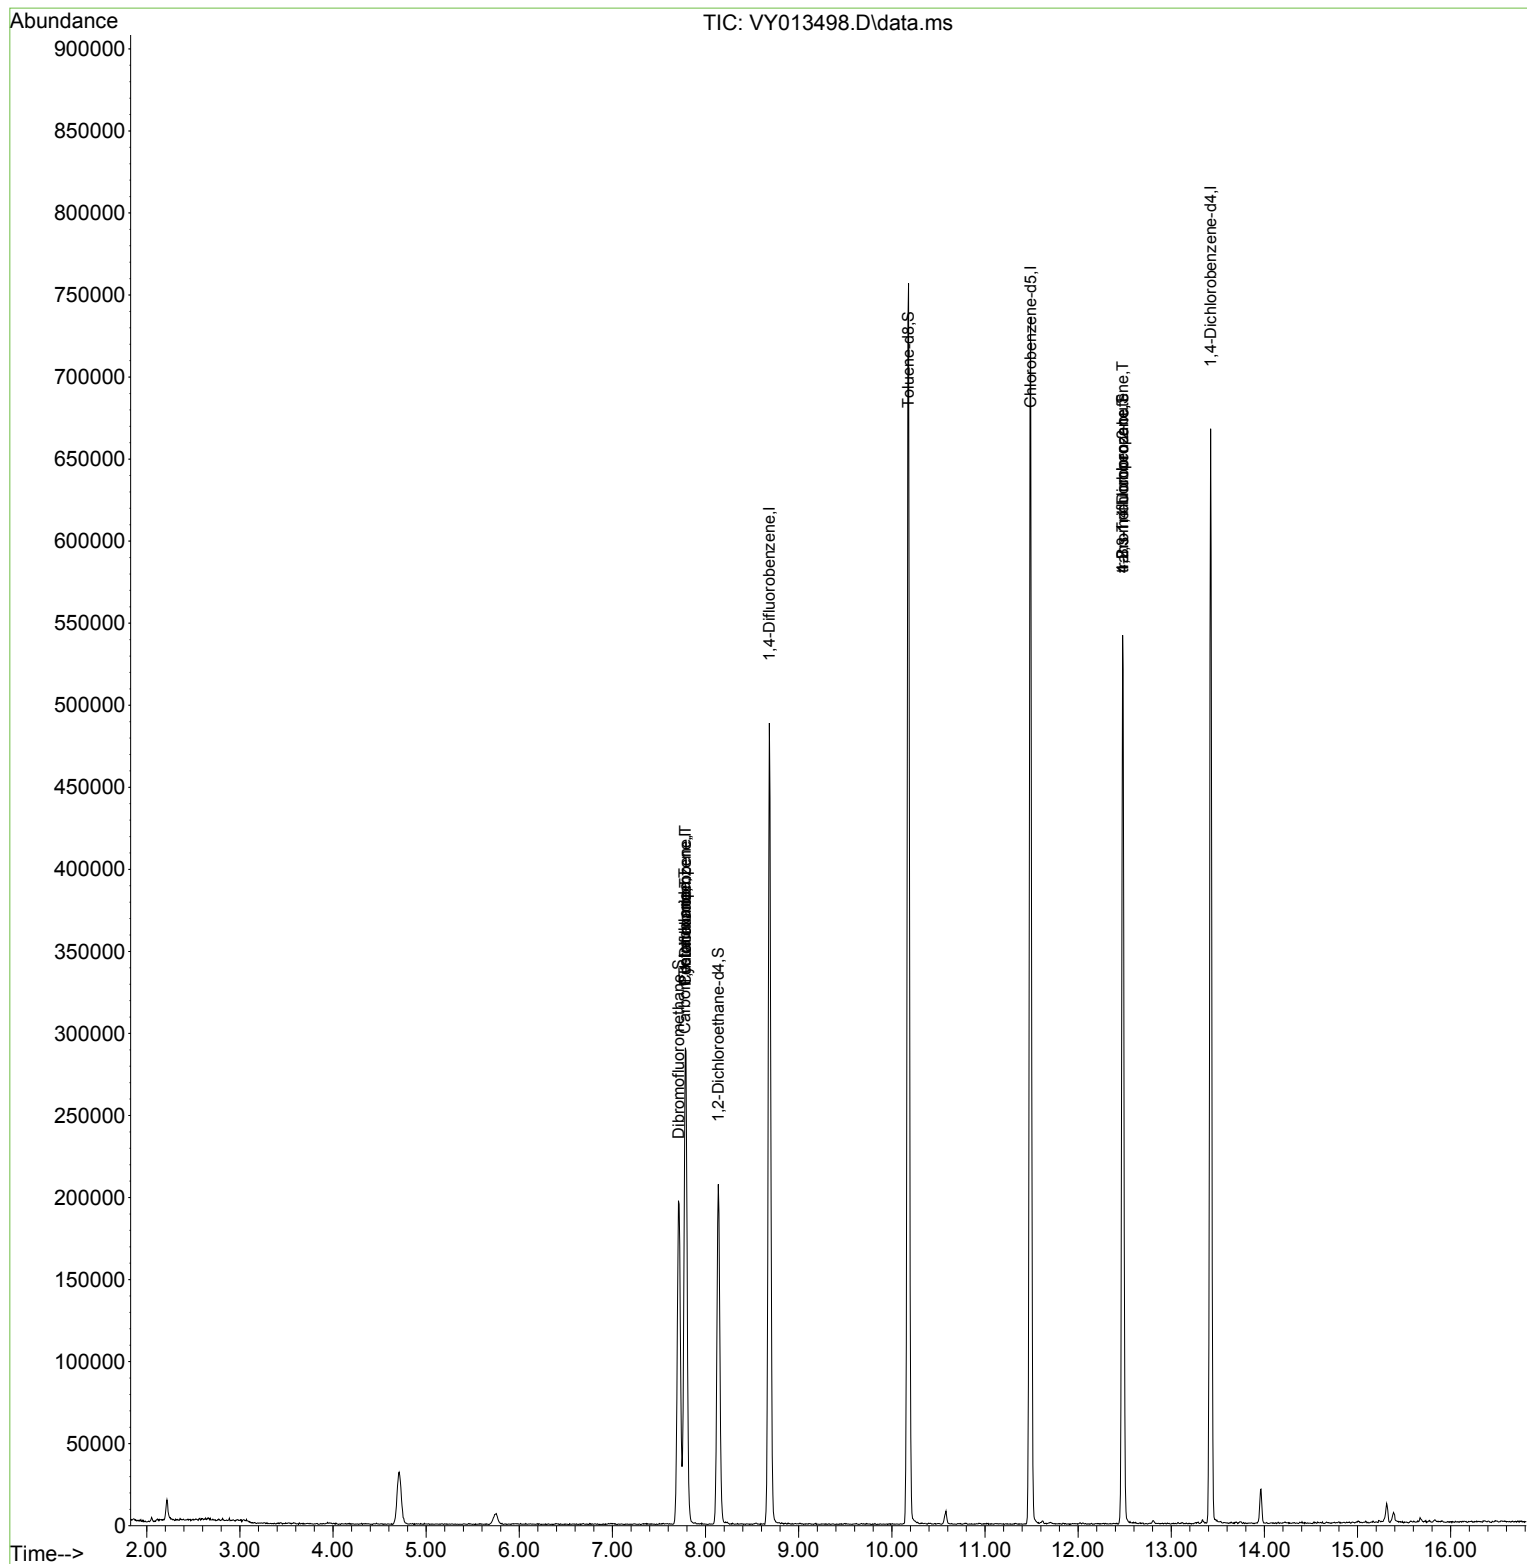


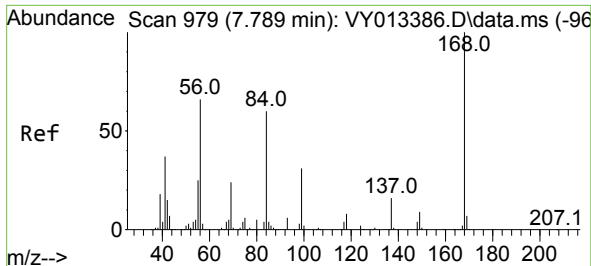

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY013498.D
Acq: 27 Apr 2023 17:40




Instrument :
MSVOA_Y
ClientSampleId :
SB-08-8.5-9.0


Tgt Ion:168 Resp: 224361
Ion Ratio Lower Upper
168 100
99 51.8 41.8 62.6

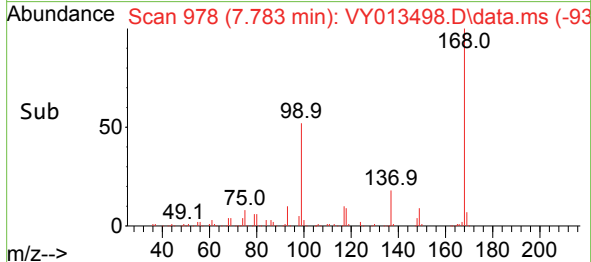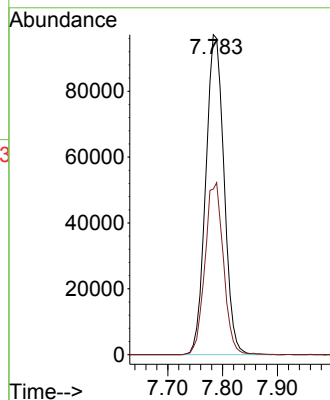

#13
Acrolein
Concen: Below Cal
RT: 3.747 min Scan# 316
Delta R.T. 0.018 min
Lab File: VY013498.D
Acq: 27 Apr 2023 17:40

Tgt Ion: 56 Resp: 20
Ion Ratio Lower Upper
56 100
55 0.0 54.1 81.1#


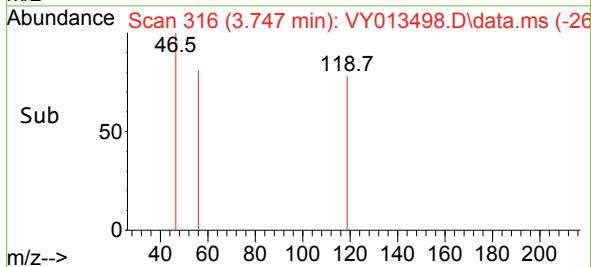
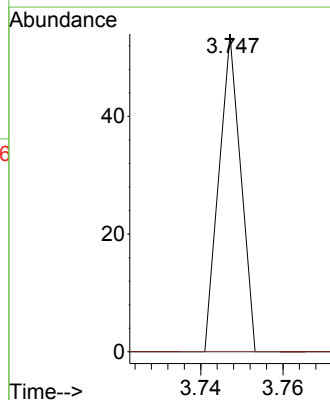
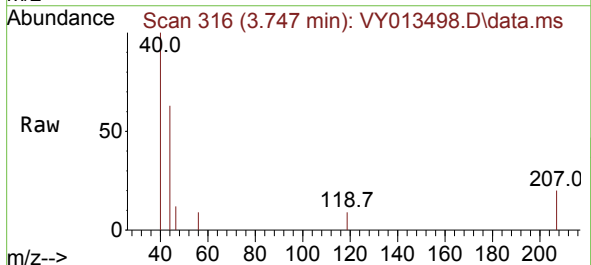


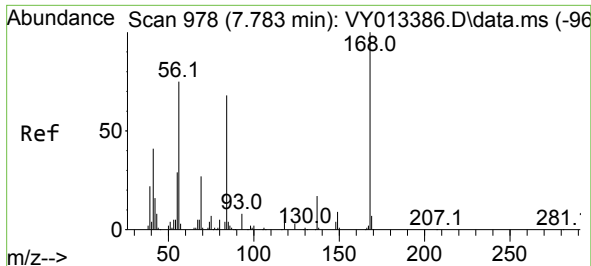

#31
Cyclohexane
Concen: 1.227 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY013498.D
Acq: 27 Apr 2023 17:40




Instrument :
MSVOA_Y
ClientSampleId :
SB-08-8.5-9.0


Tgt Ion: 56 Resp: 5403
Ion Ratio Lower Upper
56 100
69 159.0 29.2 43.8#
84 122.8 73.0 109.6#

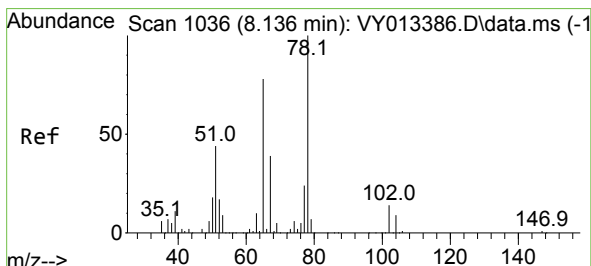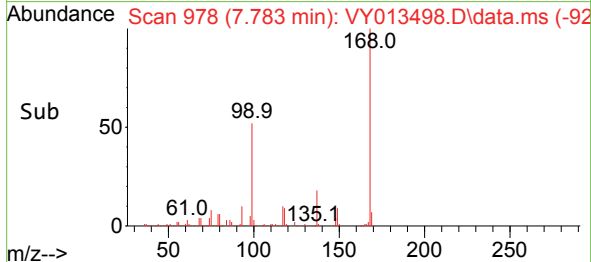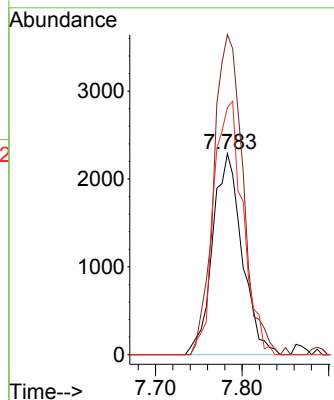

#33
1,2-Dichloroethane-d4
Concen: 67.031 ug/l
RT: 8.137 min Scan# 1036
Delta R.T. 0.001 min
Lab File: VY013498.D
Acq: 27 Apr 2023 17:40

Tgt Ion: 65 Resp: 164863
Ion Ratio Lower Upper
65 100
67 51.8 0.0 103.4


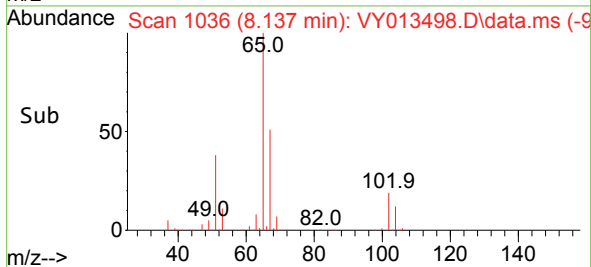
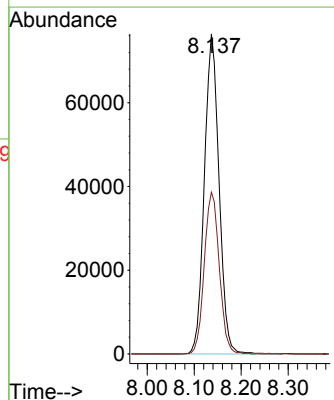
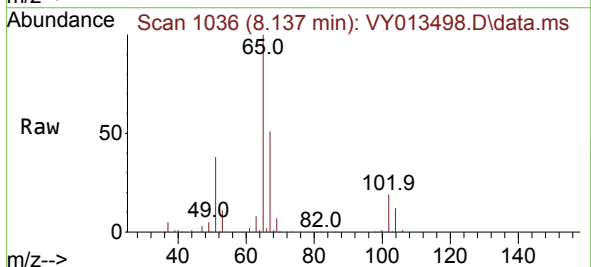


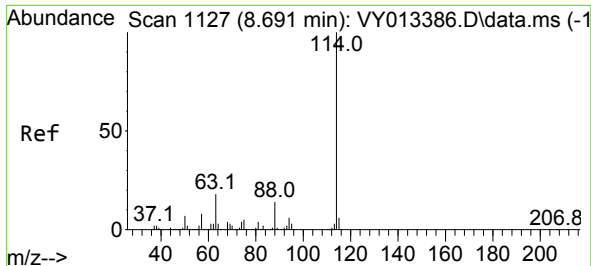

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.685 min Scan# 1126
Delta R.T. -0.006 min
Lab File: VY013498.D
Acq: 27 Apr 2023 17:40




Instrument :
MSVOA_Y
ClientSampleId :
SB-08-8.5-9.0


Tgt Ion:114 Resp: 395564
Ion Ratio Lower Upper
114 100
63 19.5 0.0 36.6
88 14.4 0.0 28.8

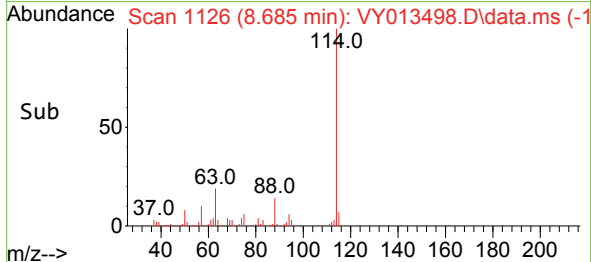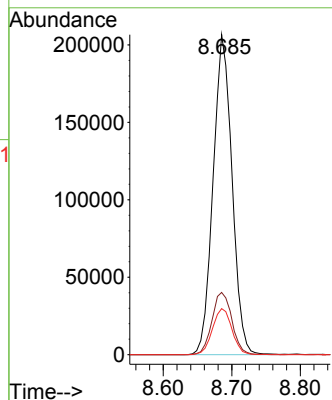

#35
Dibromofluoromethane
Concen: 56.055 ug/l
RT: 7.710 min Scan# 966
Delta R.T. -0.006 min
Lab File: VY013498.D
Acq: 27 Apr 2023 17:40

Tgt Ion:113 Resp: 139461
Ion Ratio Lower Upper
113 100
111 103.3 82.2 123.2
192 20.6 16.7 25.1


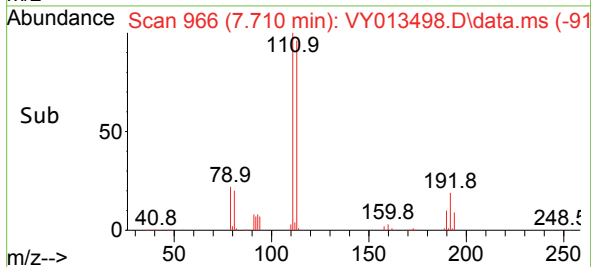
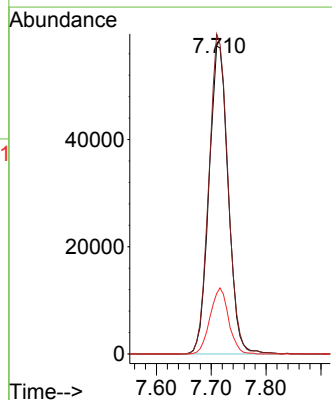
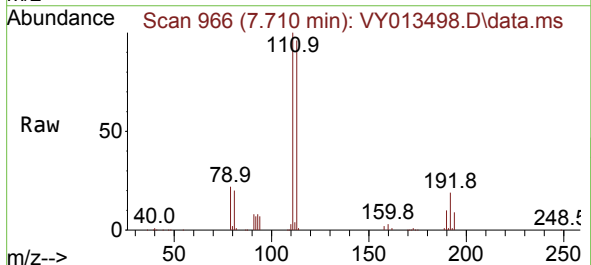


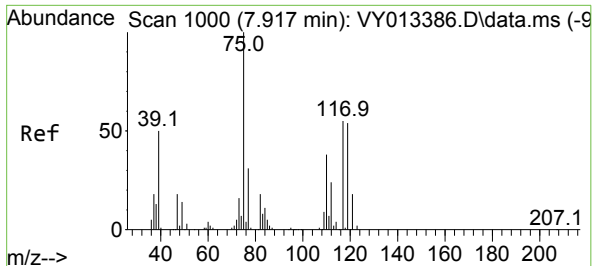

#36
1,1-Dichloropropene
Concen: 4.468 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.134 min
Lab File: VY013498.D
Acq: 27 Apr 2023 17:40




Instrument :
MSVOA_Y
ClientSampleId :
SB-08-8.5-9.0


Tgt Ion: 75 Resp: 18449
Ion Ratio Lower Upper
75 100
110 9.6 18.7 56.1#
77 0.0 24.6 37.0#

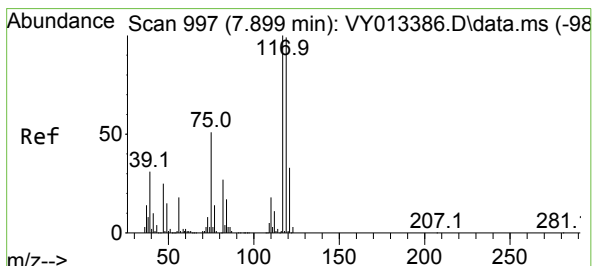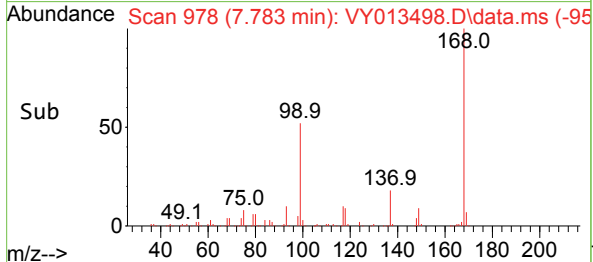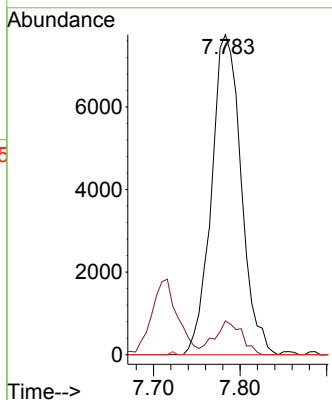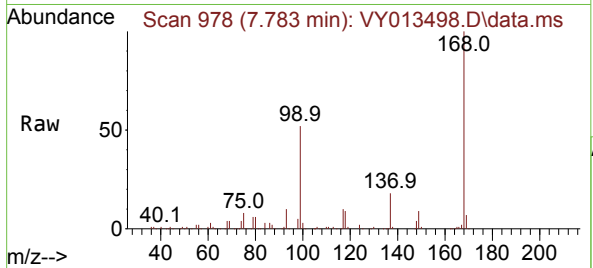

#38
Carbon Tetrachloride
Concen: 5.330 ug/l
RT: 7.777 min Scan# 977
Delta R.T. -0.122 min
Lab File: VY013498.D
Acq: 27 Apr 2023 17:40

Tgt Ion: 117 Resp: 23068
Ion Ratio Lower Upper
117 100
119 3.6 79.0 118.6#
121 0.0 26.6 40.0#


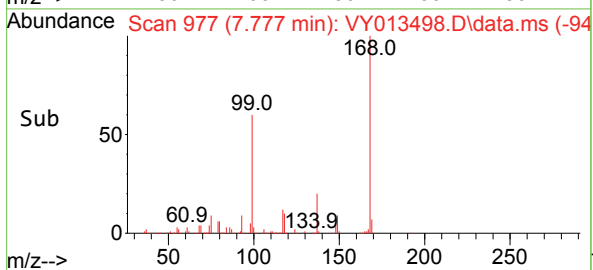
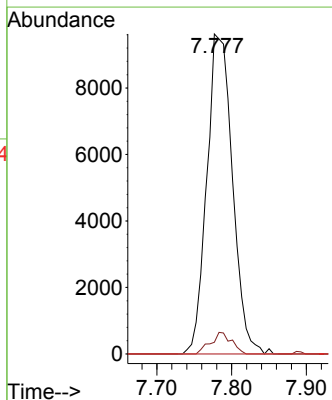
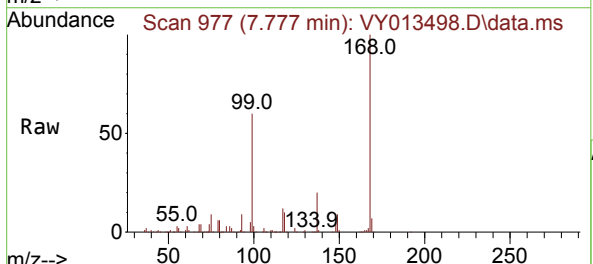


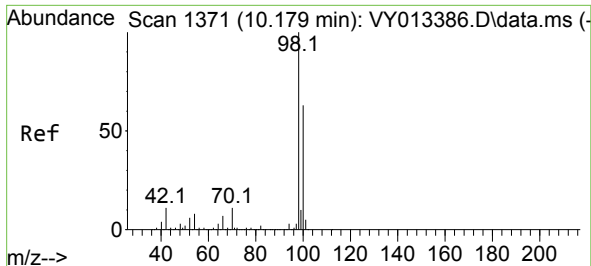

#50
Toluene-d8
Concen: 55.141 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY013498.D
Acq: 27 Apr 2023 17:40




Instrument :
MSVOA_Y
ClientSampleId :
SB-08-8.5-9.0


Tgt Ion: 98 Resp: 488030
Ion Ratio Lower Upper
98 100
100 62.6 50.5 75.7

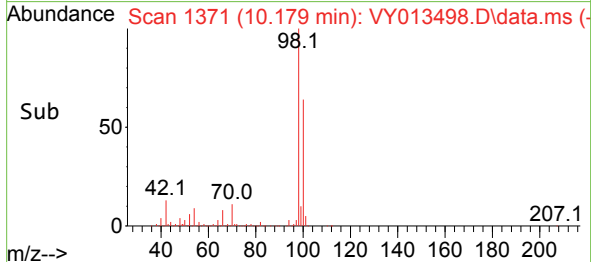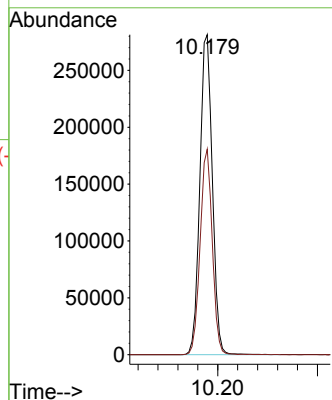

#62
4-Bromofluorobenzene
Concen: 51.866 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.000 min
Lab File: VY013498.D
Acq: 27 Apr 2023 17:40

Tgt Ion: 95 Resp: 154753
Ion Ratio Lower Upper
95 100
174 89.5 0.0 182.0
176 85.7 0.0 175.4


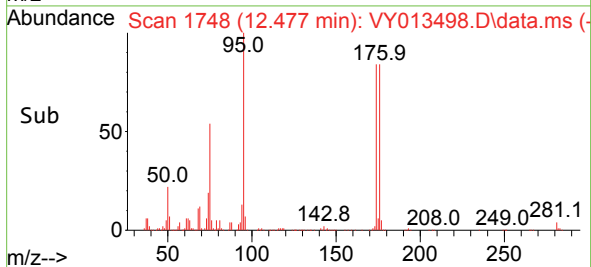
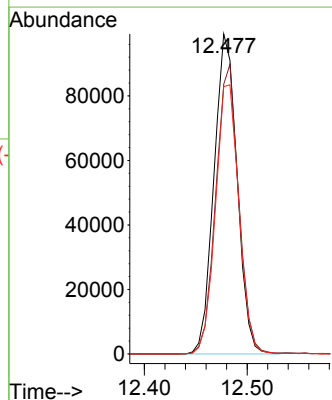
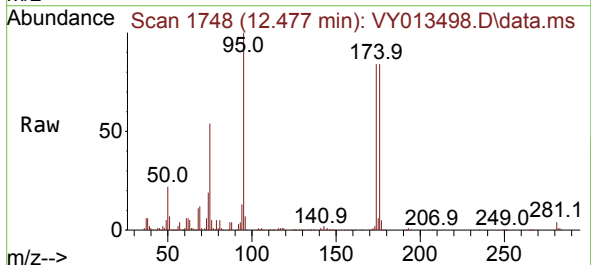




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 117
Delta R.T. 0.001 min
Lab File: VY013498.D
Acq: 27 Apr 2023 17:40




Instrument :
MSVOA_Y
ClientSampleId :
SB-08-8.5-9.0


Tgt Ion:117 Resp: 381022
Ion Ratio Lower Upper
117 100
82 53.8 43.0 64.6
119 31.1 25.5 38.3

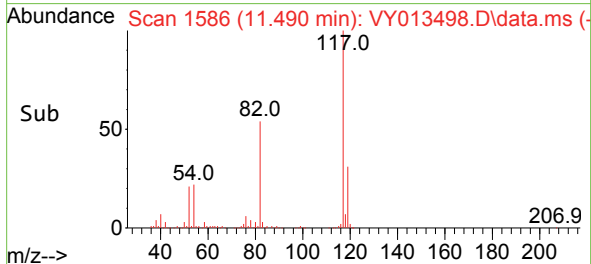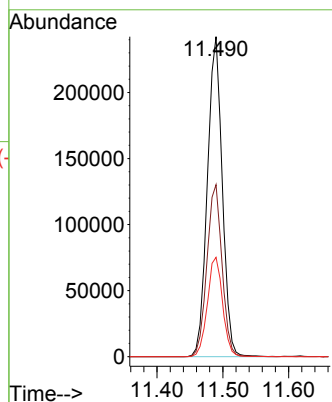

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. 0.000 min
Lab File: VY013498.D
Acq: 27 Apr 2023 17:40

Tgt Ion:152 Resp: 169573
Ion Ratio Lower Upper
152 100
115 56.1 28.1 84.2
150 154.7 0.0 352.0


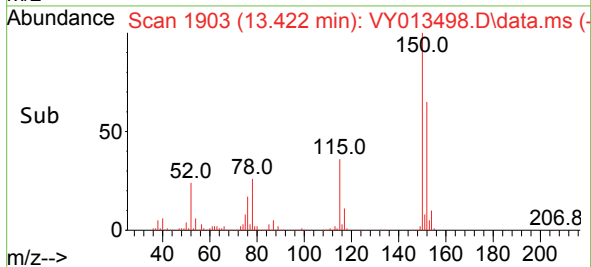
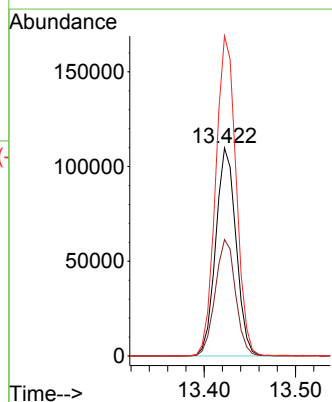
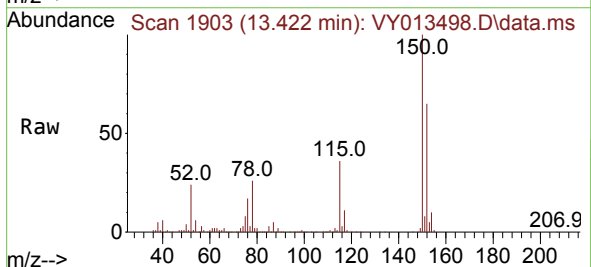


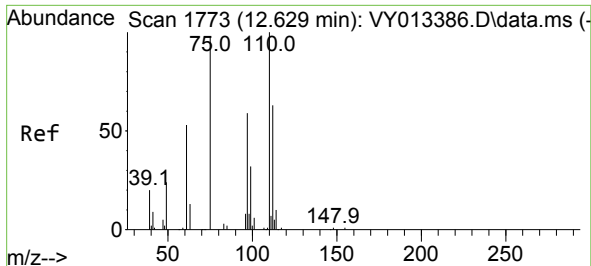

#76
1,2,3-Trichloropropane
Concen: 36.505 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.152 min
Lab File: VY013498.D
Acq: 27 Apr 2023 17:40

Instrument :
MSVOA_Y
ClientSampleId :
SB-08-8.5-9.0

Tgt Ion: 75 Resp: 83484
Ion Ratio Lower Upper
75 100
77 1.3 0.0 0.0#

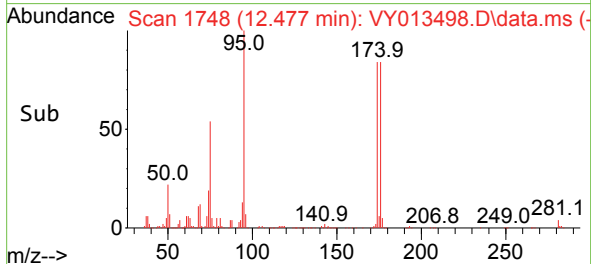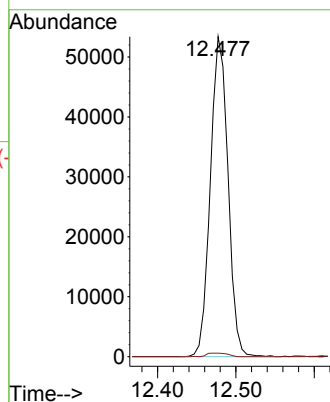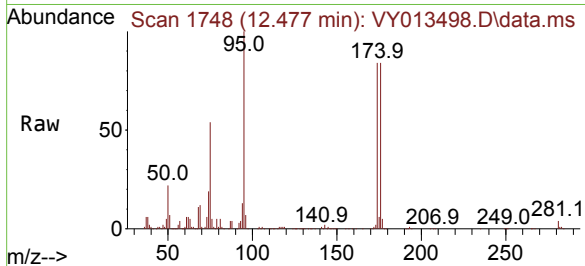

#81
trans-1,4-Dichloro-2-butene
Concen: 74.674 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.098 min
Lab File: VY013498.D
Acq: 27 Apr 2023 17:40

Tgt Ion: 75 Resp: 83484
Ion Ratio Lower Upper
75 100
53 0.4 73.2 109.8#
89 0.2 38.0 57.0#

