

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042723\
 Data File : VY013490.D
 Acq On : 27 Apr 2023 14:32
 Operator : KP/MD
 Sample : VY0427SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0427SBL01

Quant Time: Apr 27 16:14:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 25 02:39:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	262881	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	433384	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	390354	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	179244	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	173508	60.209	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	120.420%
35) Dibromofluoromethane	7.710	113	150914	55.365	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	110.740%
50) Toluene-d8	10.179	98	491114	50.647	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	101.300%
62) 4-Bromofluorobenzene	12.477	95	162727	49.779	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	99.560%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042723\
Data File : VY013490.D
Acq On : 27 Apr 2023 14:32
Operator : KP/MD
Sample : VY0427SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0427SBL01

Quant Time: Apr 27 16:14:01 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
Quant Title : SW846 8260
QLast Update : Tue Apr 25 02:39:58 2023
Response via : Initial Calibration




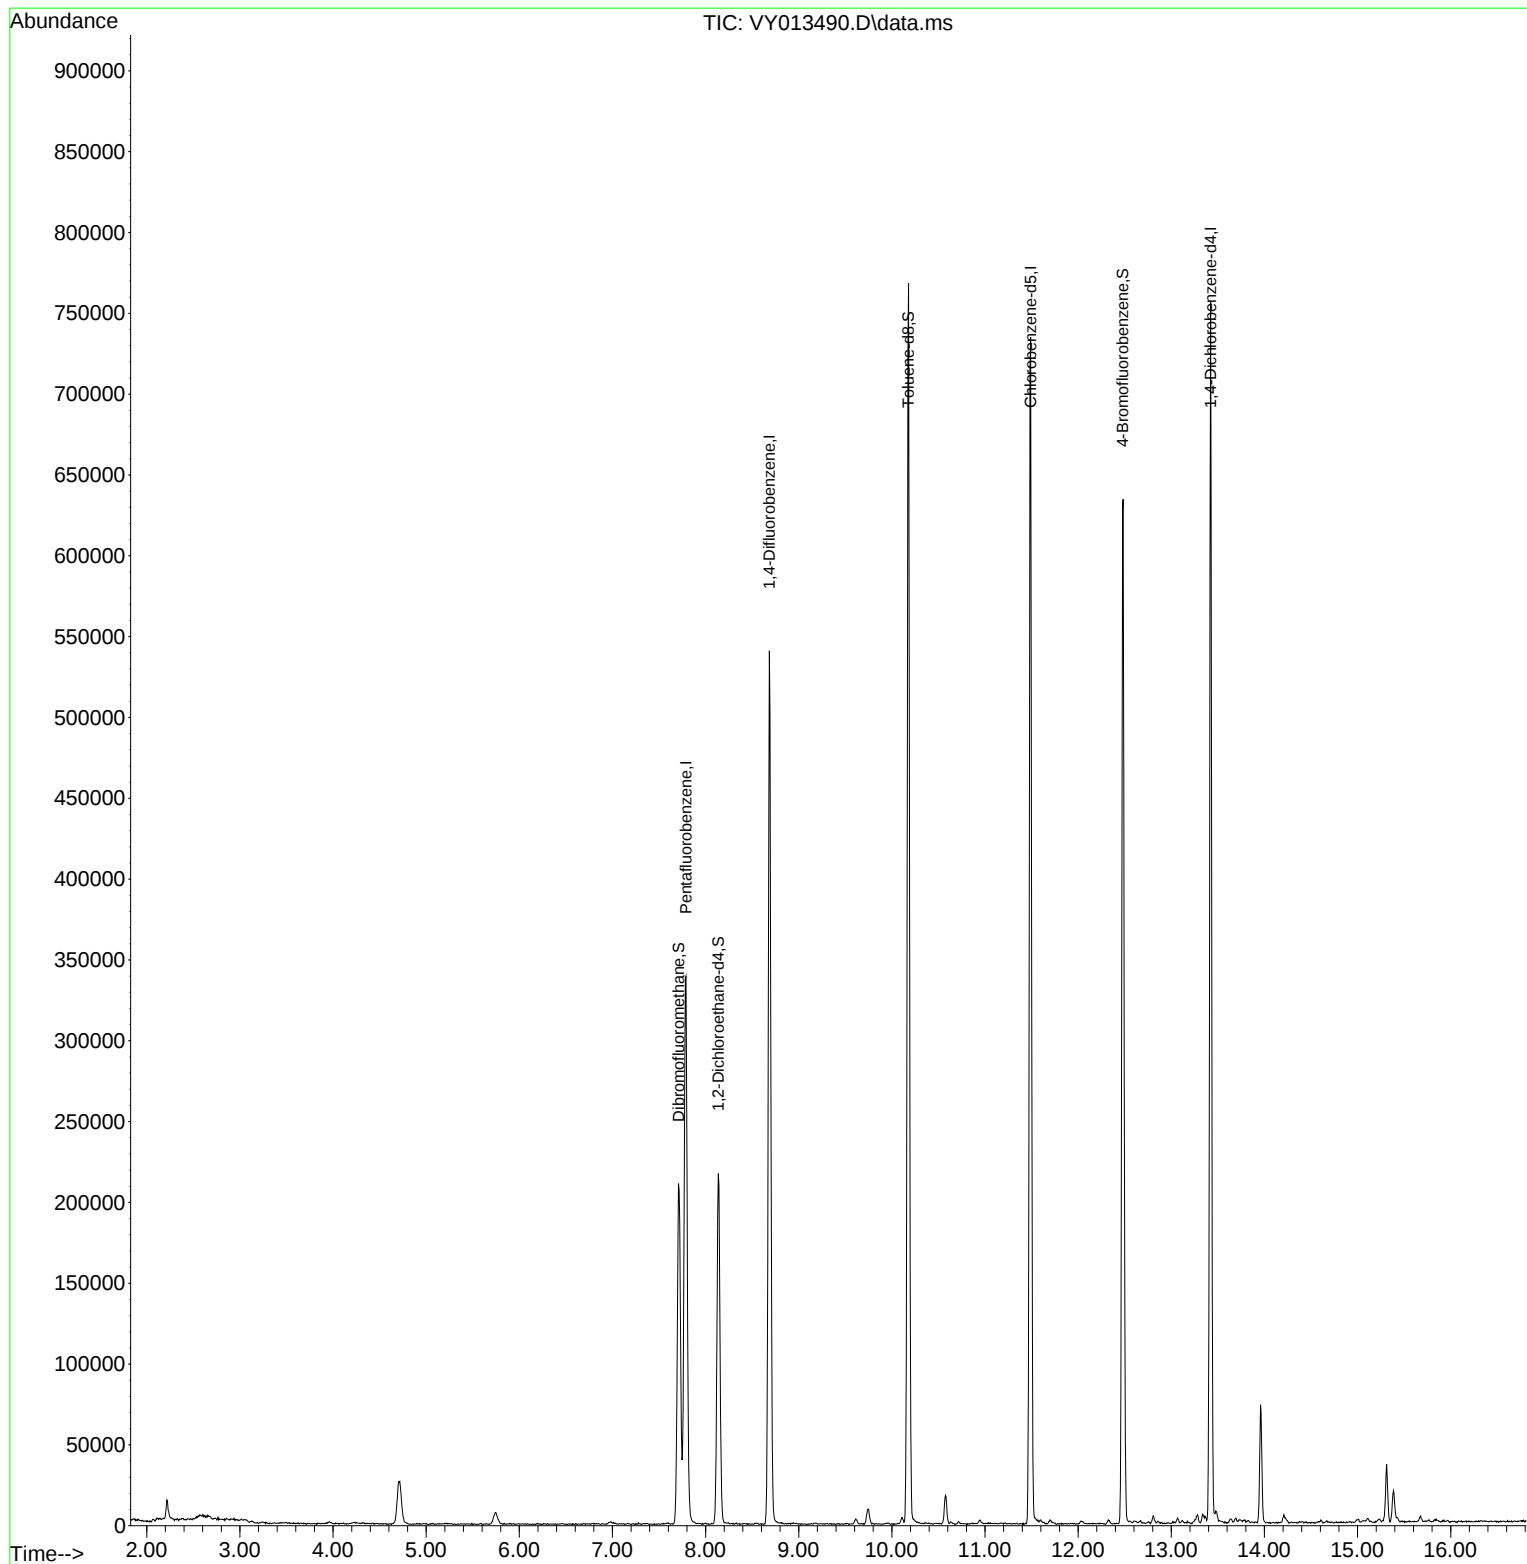




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY013490.D
Acq: 27 Apr 2023 14:32




Instrument :
MSVOA_Y
ClientSampleId :
VY0427SBL01

Tgt Ion:168 Resp: 262881
Ion Ratio Lower Upper
168 100
99 52.0 41.8 62.6

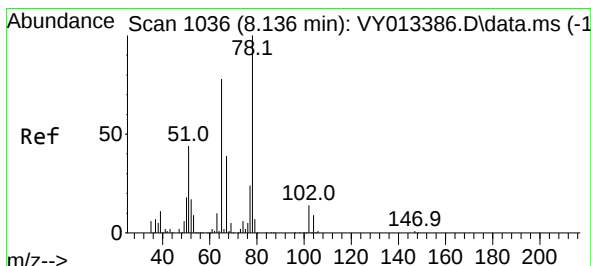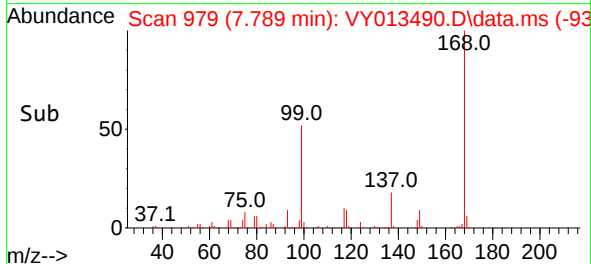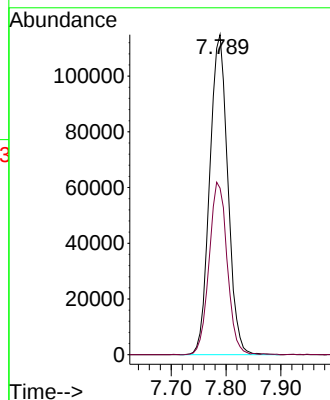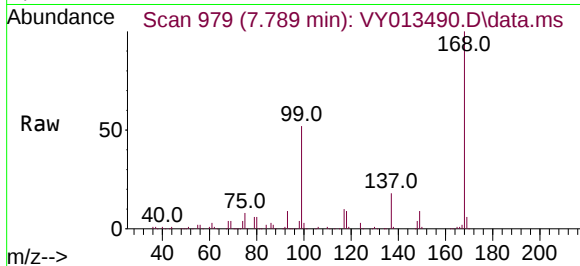

#33
1,2-Dichloroethane-d4
Concen: 60.209 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. 0.000 min
Lab File: VY013490.D
Acq: 27 Apr 2023 14:32

Tgt Ion: 65 Resp: 173508
Ion Ratio Lower Upper
65 100
67 52.7 0.0 103.4

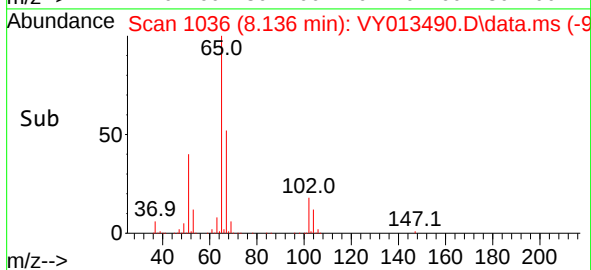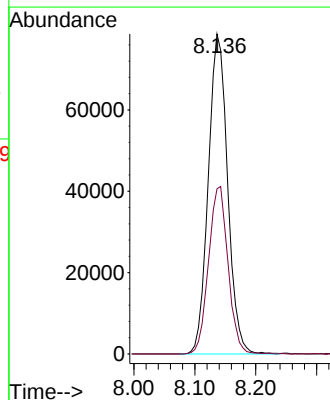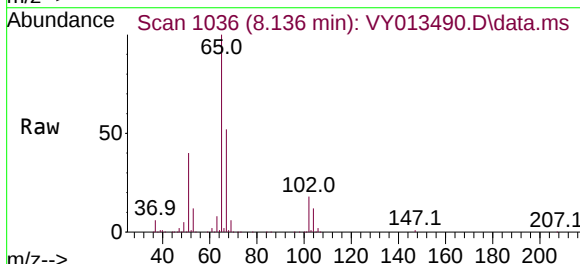



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.006 min

Lab File: VY013490.D

Acq: 27 Apr 2023 14:32

Instrument :

MSVOA_Y

ClientSampleId :

VY0427SBL01





Tgt Ion:114 Resp: 433384

Ion Ratio Lower Upper

114 100

63 20.8 0.0 36.6

88 14.8 0.0 28.8

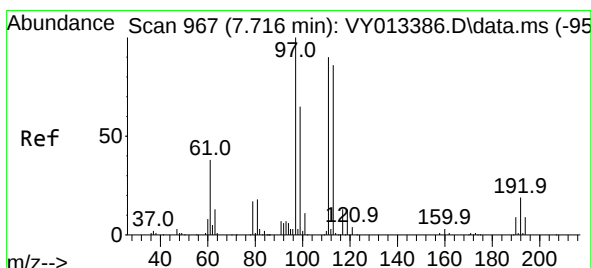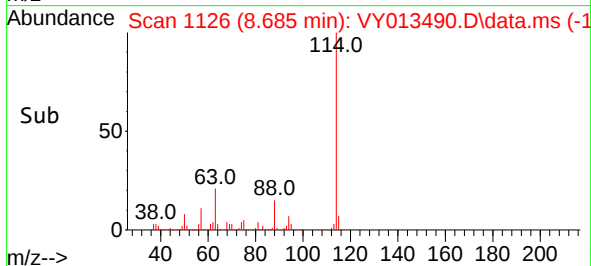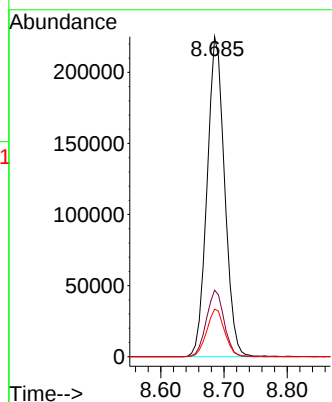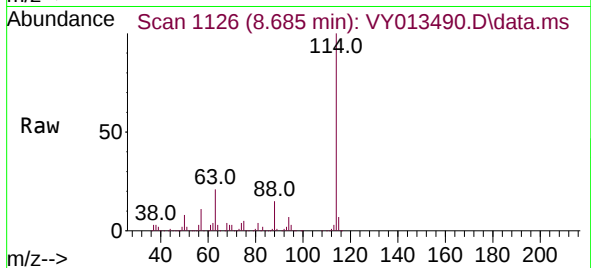

#35

Dibromofluoromethane

Concen: 55.365 ug/l

RT: 7.710 min Scan# 966

Delta R.T. -0.006 min

Lab File: VY013490.D

Acq: 27 Apr 2023 14:32




Tgt Ion:113 Resp: 150914


Ion Ratio Lower Upper

113 100

111 101.7 82.2 123.2

192 20.4 16.7 25.1

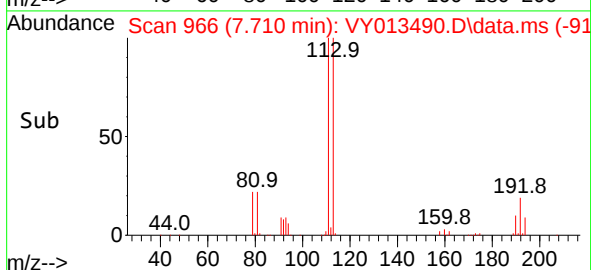
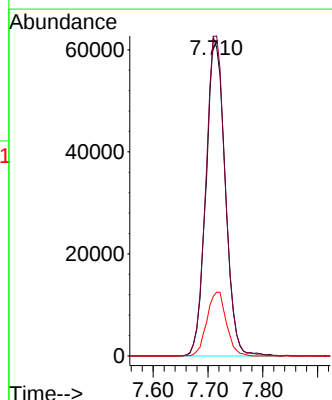
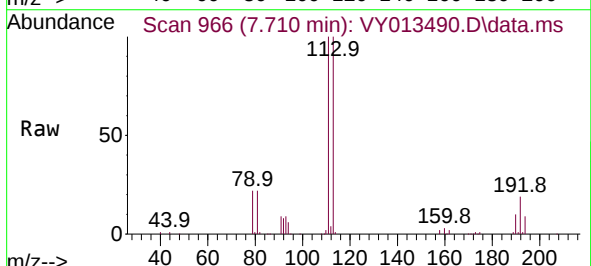


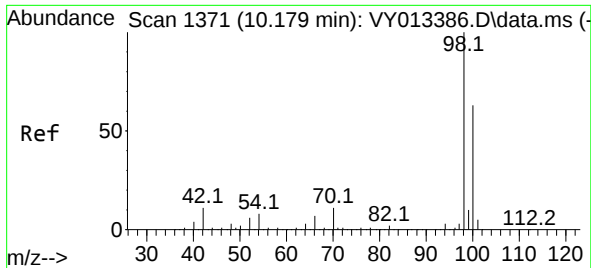

#50
Toluene-d8
Concen: 50.647 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY013490.D
Acq: 27 Apr 2023 14:32




Instrument :
MSVOA_Y
ClientSampleId :
VY0427SBL01


Tgt Ion: 98 Resp: 491114
Ion Ratio Lower Upper
98 100
100 62.6 50.5 75.7

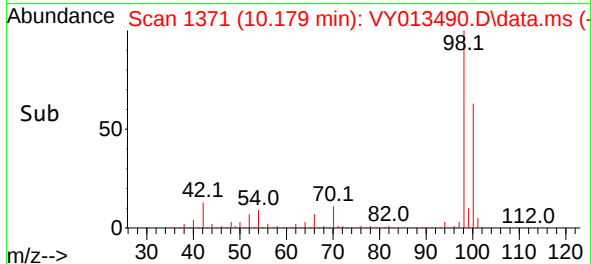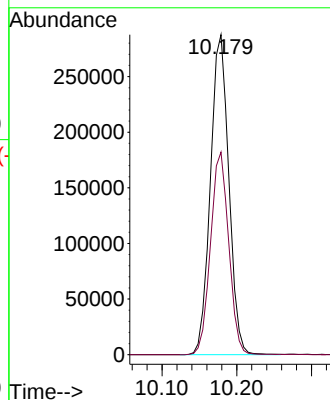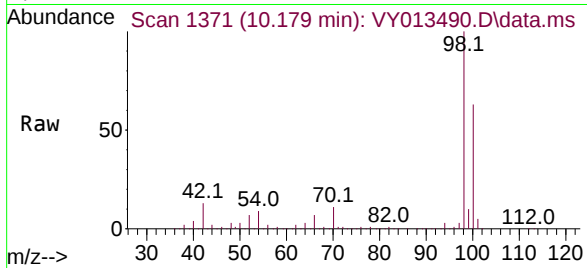

#62
4-Bromofluorobenzene
Concen: 49.779 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.000 min
Lab File: VY013490.D
Acq: 27 Apr 2023 14:32

Tgt Ion: 95 Resp: 162727
Ion Ratio Lower Upper
95 100
174 87.7 0.0 182.0
176 83.4 0.0 175.4


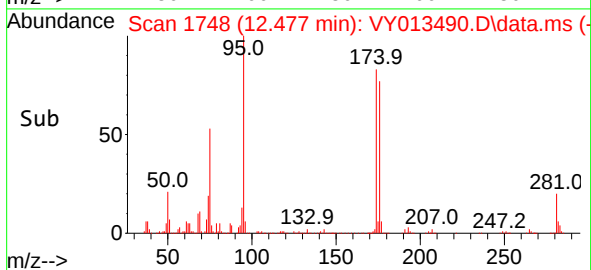
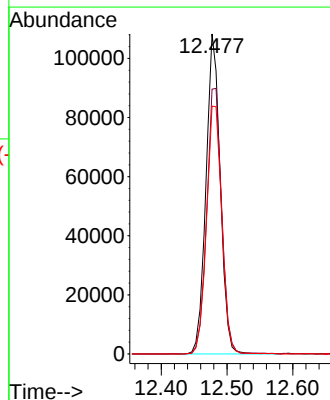
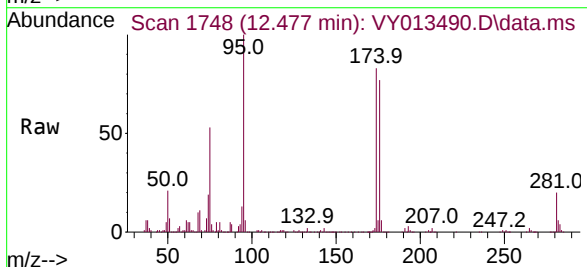


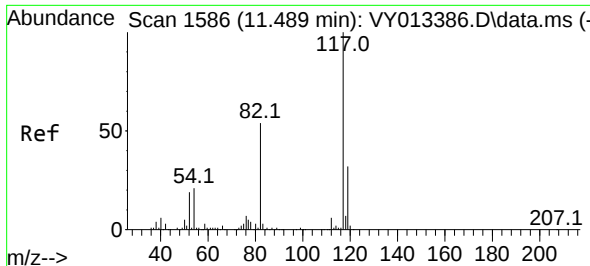

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 117
Delta R.T. 0.001 min
Lab File: VY013490.D
Acq: 27 Apr 2023 14:32

Instrument :
MSVOA_Y
ClientSampleId :
VY0427SBL01

Tgt Ion:117 Resp: 390354
Ion Ratio Lower Upper
117 100
82 54.6 43.0 64.6
119 31.8 25.5 38.3

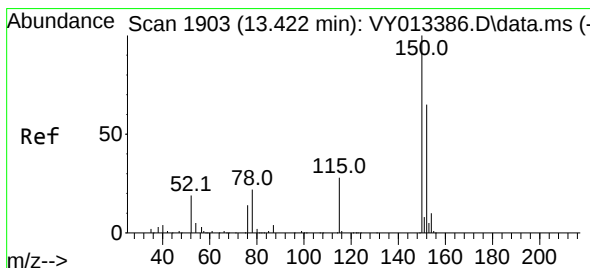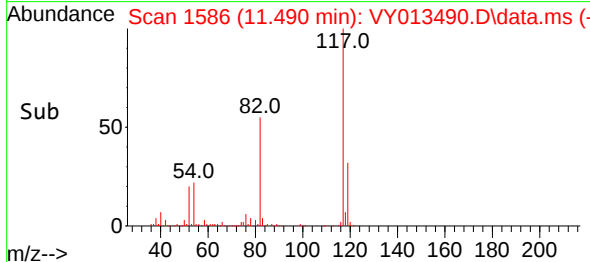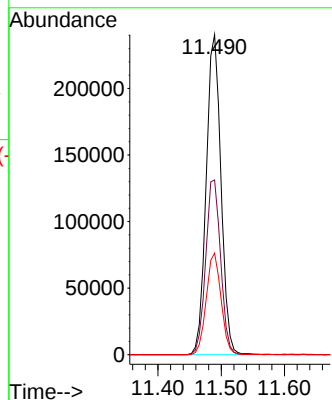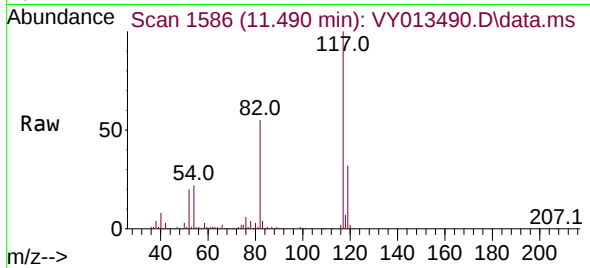

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. 0.000 min
Lab File: VY013490.D
Acq: 27 Apr 2023 14:32

Tgt Ion:152 Resp: 179244
Ion Ratio Lower Upper
152 100
115 57.2 28.1 84.2
150 156.8 0.0 352.0

