
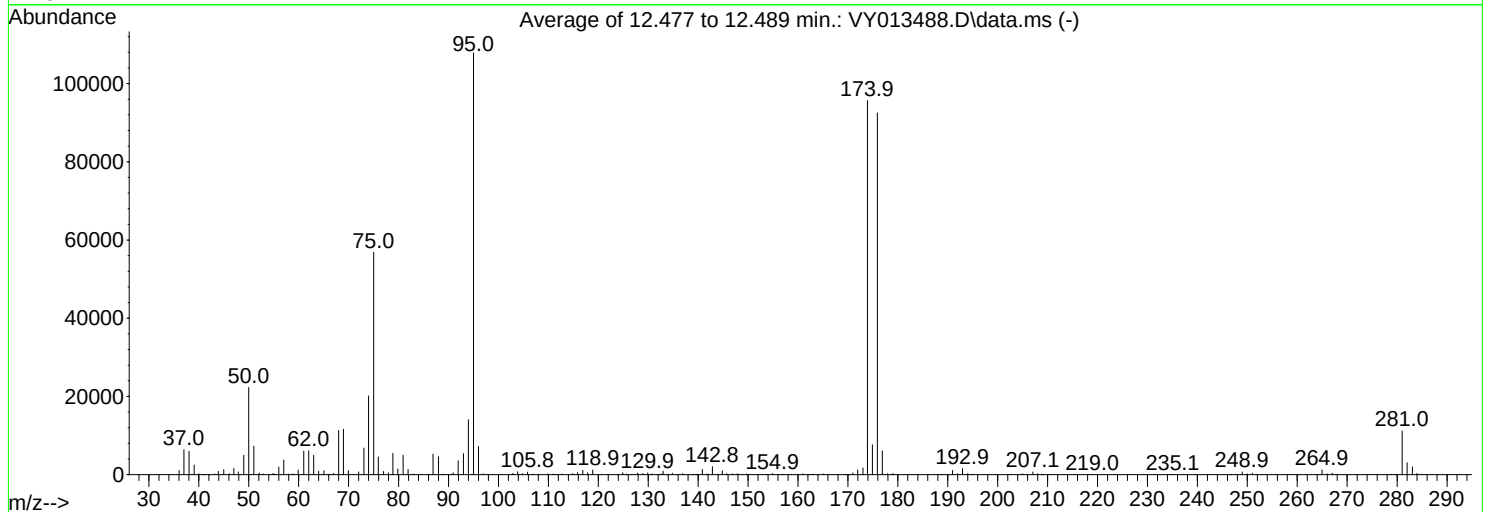


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042723\
Data File : VY013488.D
Acq On : 27 Apr 2023 13:05
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
Title : SW846 8260
Last Update : Tue Apr 25 02:39:58 2023

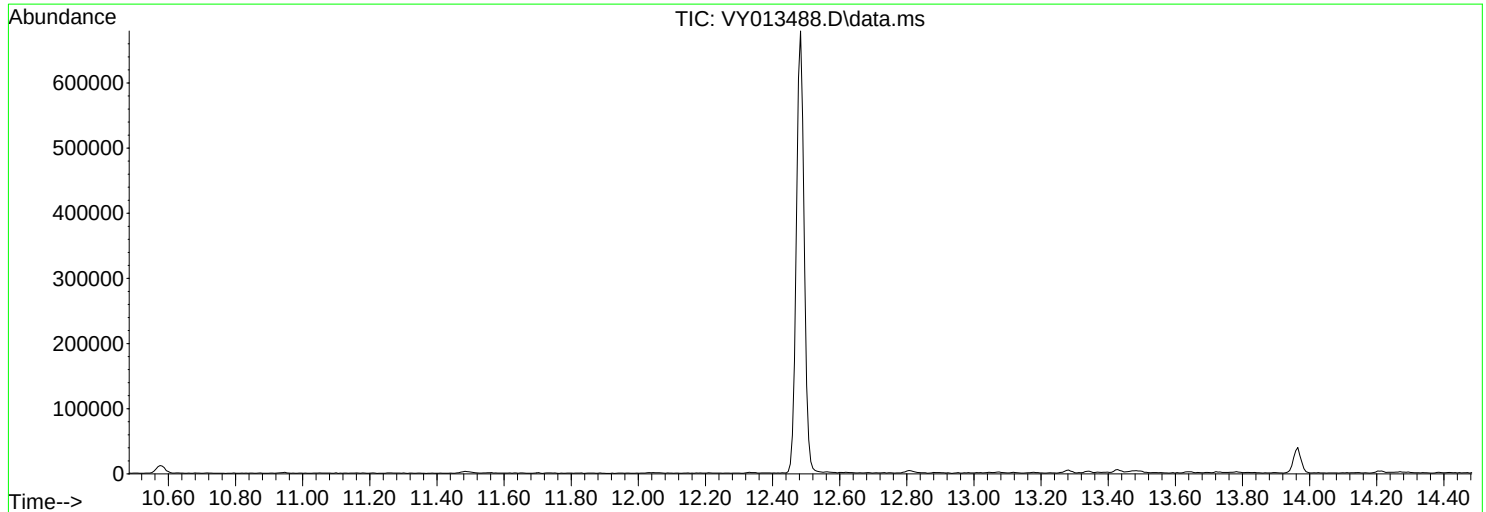

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1739

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.7	22285	PASS
75	95	30	60	52.7	56813	PASS
95	95	100	100	100.0	107856	PASS
96	95	5	9	6.7	7187	PASS
173	174	0.00	2	1.8	1705	PASS
174	95	50	100	88.7	95675	PASS
175	174	5	9	8.0	7632	PASS
176	174	95	101	96.6	92459	PASS
177	176	5	9	6.6	6088	PASS