


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv042820\
 Data File : VY002484.D
 Acq On : 28 Apr 2020 09:48
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y042320S.M
 Title : SW846 8260
 Last Update : Thu Apr 23 14:11:26 2020

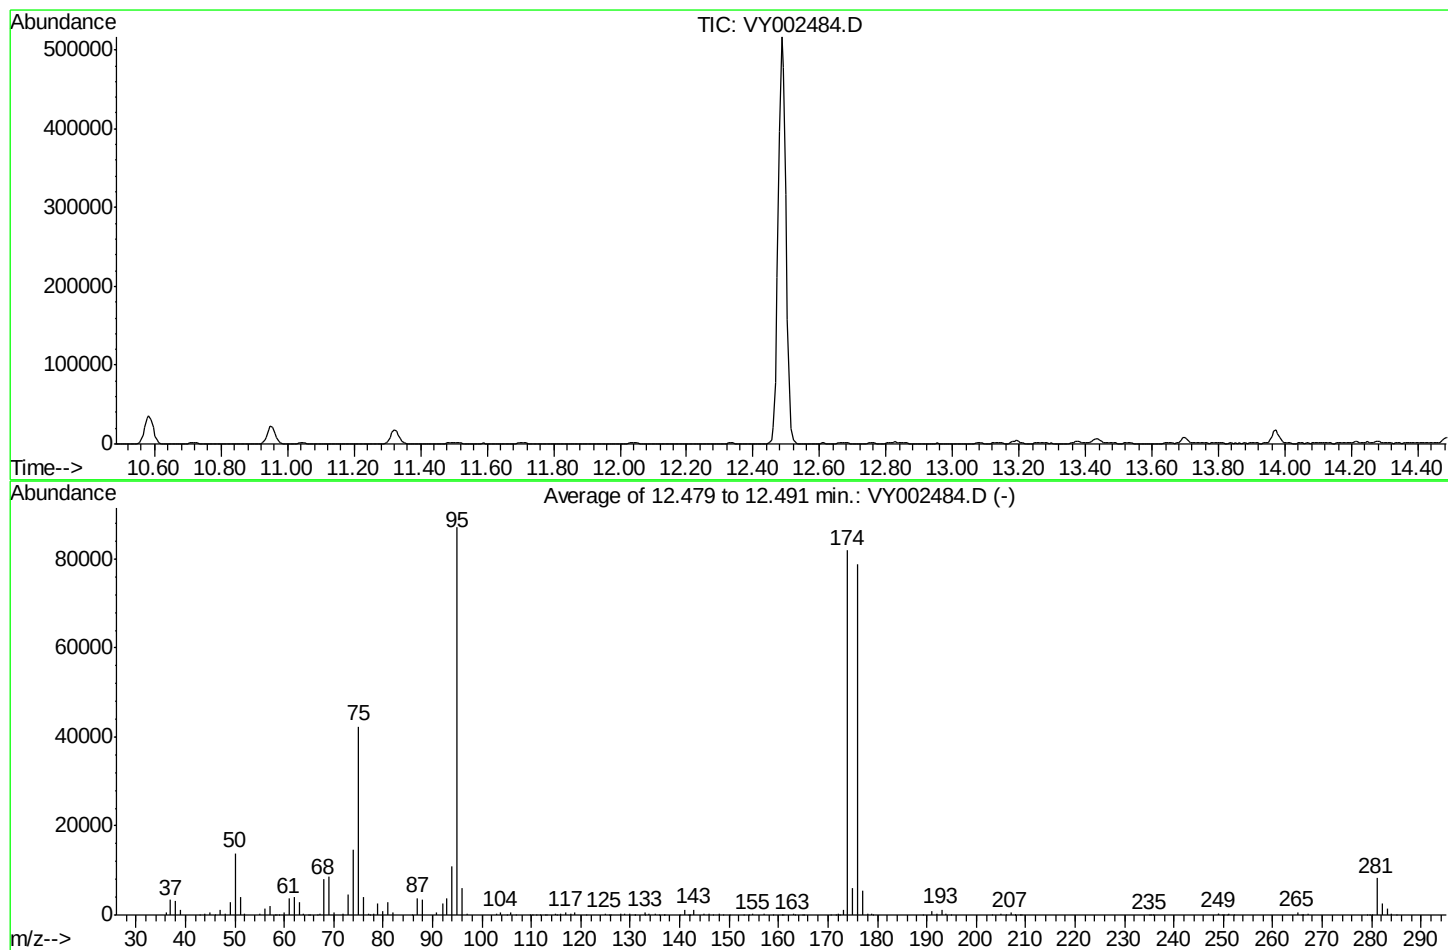

AutoFind: Scans 1762, 1763, 1764; Background Corrected with Scan 1754

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	13845	PASS
75	95	30	60	48.6	42346	PASS
95	95	100	100	100.0	87112	PASS
96	95	5	9	6.8	5962	PASS
173	174	0.00	2	1.3	1091	PASS
174	95	50	100	94.0	81880	PASS
175	174	5	9	7.3	6002	PASS
176	174	95	101	96.2	78765	PASS
177	176	5	9	7.1	5554	PASS