
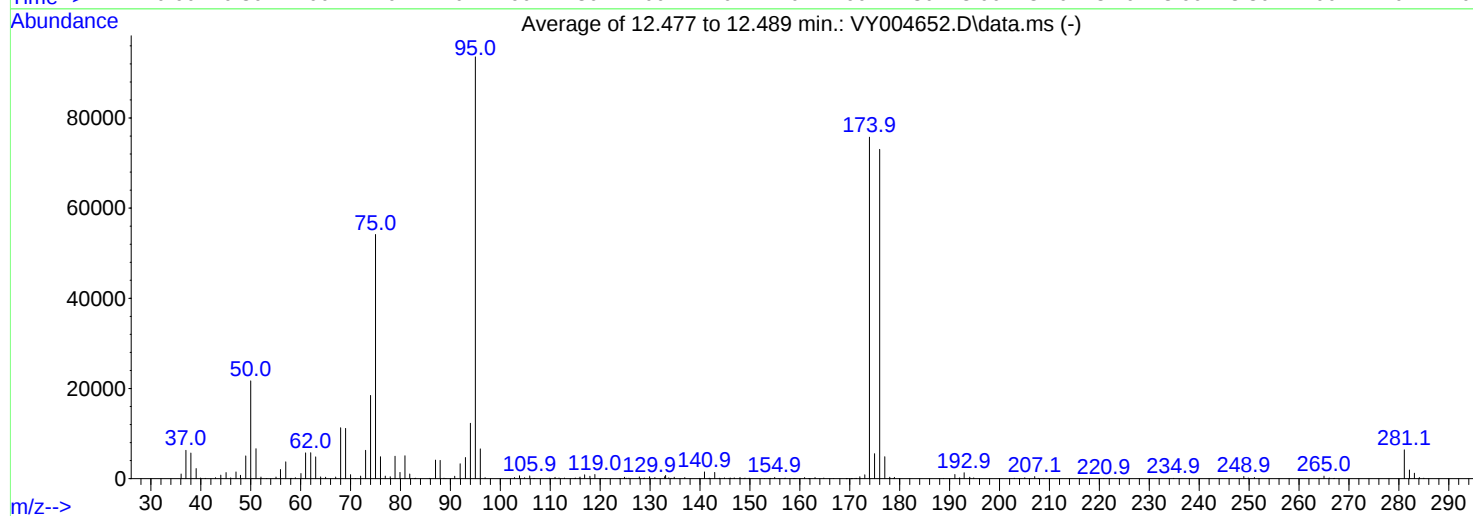


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042921\
 Data File : VY004652.D
 Acq On : 29 Apr 2021 09:55
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041221S.M
 Title : SW846 8260
 Last Update : Tue Apr 13 03:38:02 2021

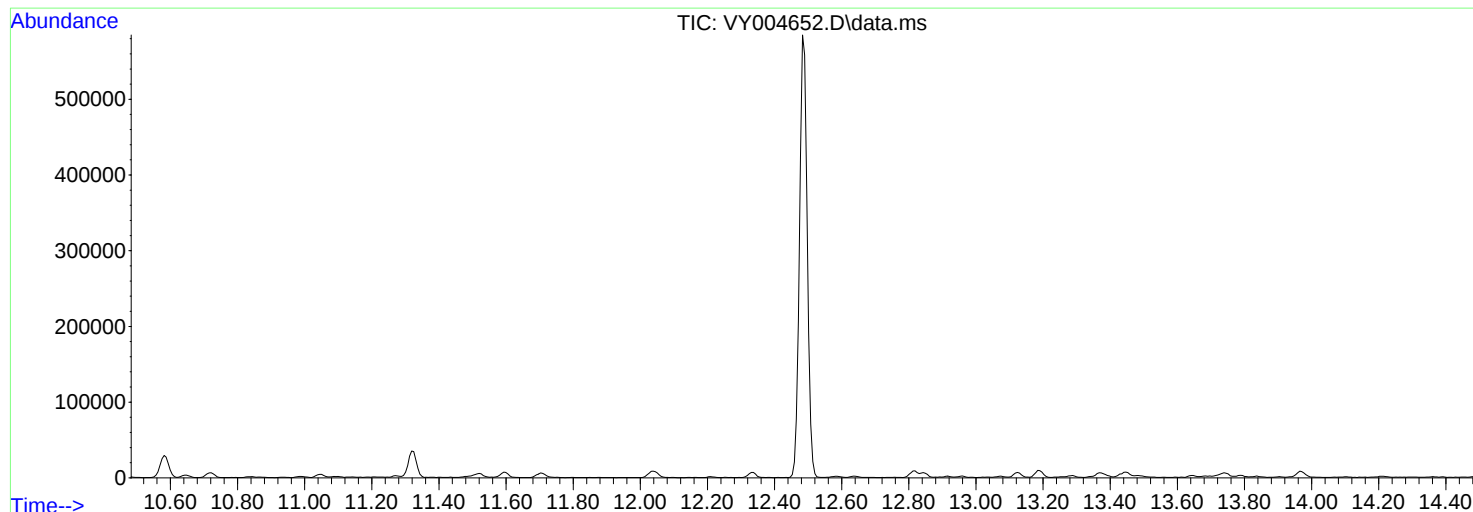

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	21699	PASS
75	95	30	60	57.9	54171	PASS
95	95	100	100	100.0	93563	PASS
96	95	5	9	7.1	6621	PASS
173	174	0.00	2	1.1	867	PASS
174	95	50	100	81.0	75749	PASS
175	174	5	9	7.3	5527	PASS
176	174	95	101	96.4	73029	PASS
177	176	5	9	6.7	4872	PASS