

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042924\
 Data File : VY018076.D
 Acq On : 29 Apr 2024 18:18
 Operator : SY/MD
 Sample : P2294-02
 Misc : 5.15g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :

Quant Time: Apr 30 01:02:45 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041624S.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 17 06:24:42 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.782	168	289350	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	521517	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	467939	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	182391	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	129743	51.815	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 103.640%	
35) Dibromofluoromethane	7.709	113	168612	52.406	ug/l	-0.01
Spiked Amount	50.000	Range	54 - 147	Recovery	= 104.820%	
50) Toluene-d8	10.178	98	592269	48.512	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 97.020%	
62) 4-Bromofluorobenzene	12.477	95	159839	42.274	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	= 84.540%	
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	4.948	59	49	Below Cal	#	88
16) Acetone	3.942	43	1699	3.434	ug/l	91
20) Methylene Chloride	4.704	84	38832	11.585	ug/l	93
36) 1,1-Dichloropropene	7.782	75	18572	3.969	ug/l #	47
38) Carbon Tetrachloride	7.782	117	24870	5.261	ug/l #	17
76) 1,2,3-Trichloropropane	12.477	75	74781	43.692	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.477	75	74781	90.086	ug/l #	16


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042924\
Data File : VY018076.D
Acq On : 29 Apr 2024 18:18
Operator : SY/MD
Sample : P2294-02
Misc : 5.15g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :


Quant Time: Apr 30 01:02:45 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041624S.M
Quant Title : SW846 8260
QLast Update : Wed Apr 17 06:24:42 2024
Response via : Initial Calibration

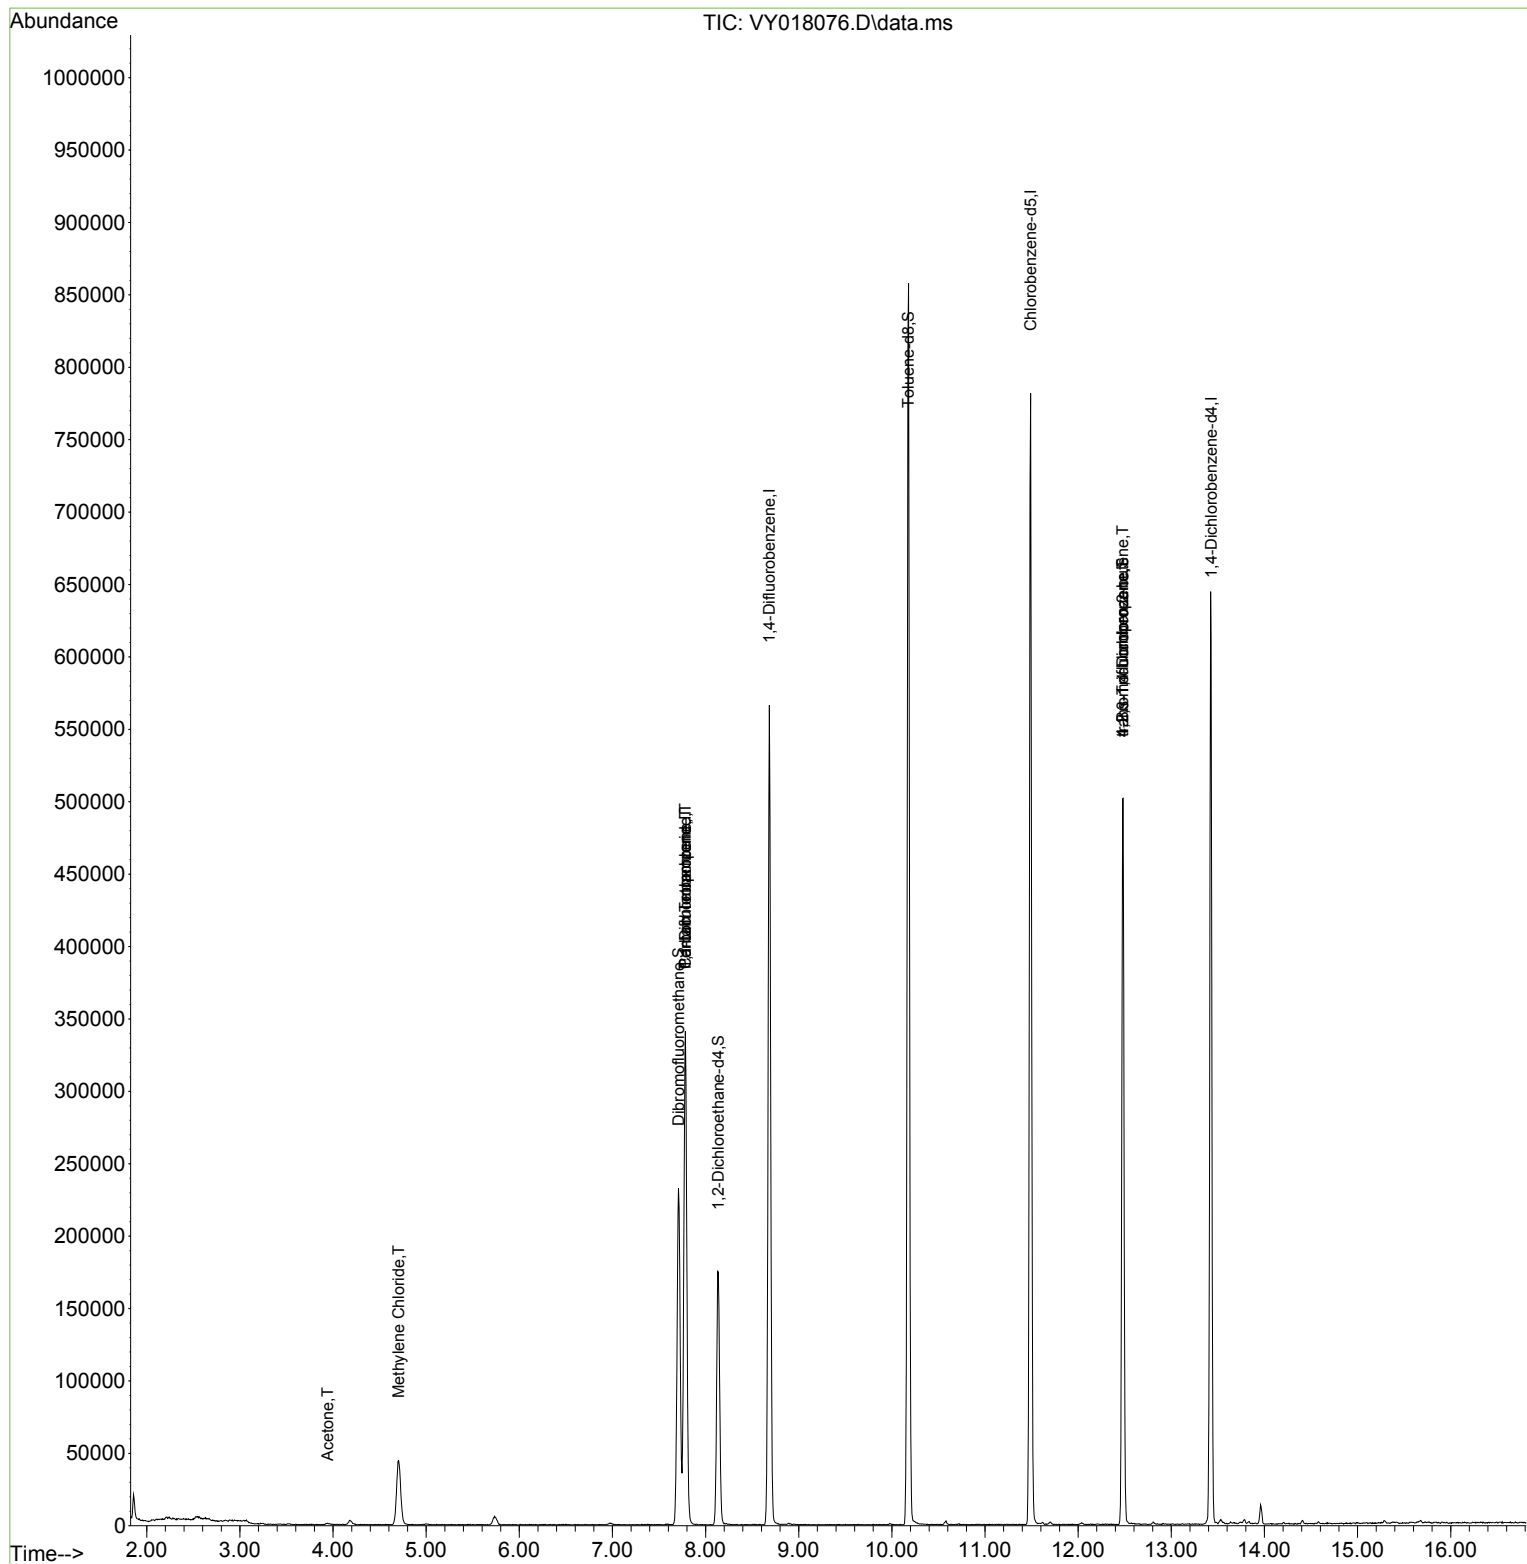



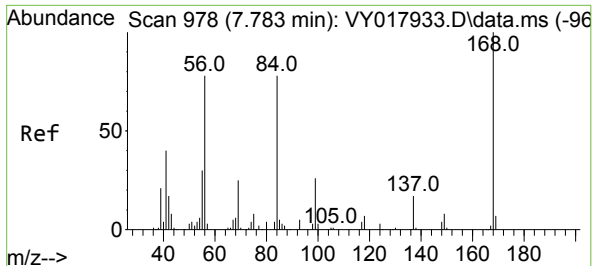


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.782 min Scan# 91
Delta R.T. -0.007 min
Lab File: VY018076.D
Acq: 29 Apr 2024 18:18

Instrument :
MSVOA_Y
ClientSampleId :



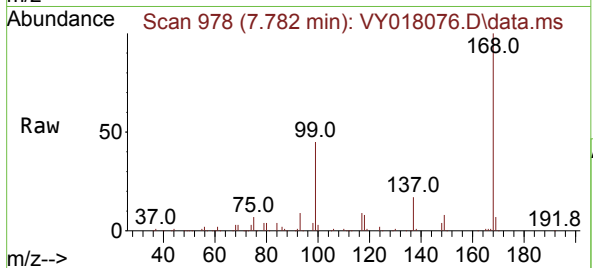



Tgt Ion:168 Resp: 289350
Ion Ratio Lower Upper
168 100
99 44.6 39.1 58.7

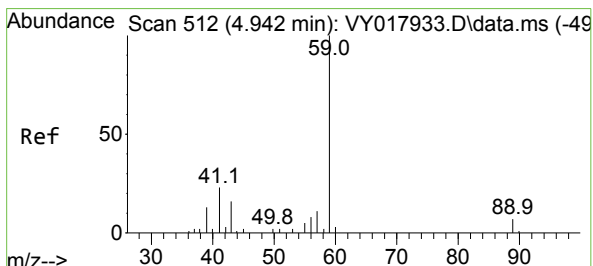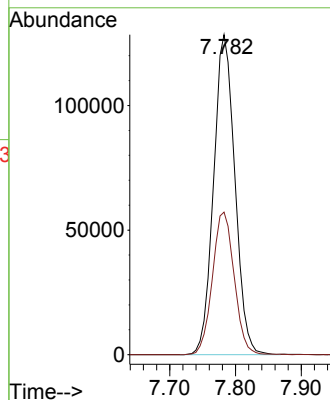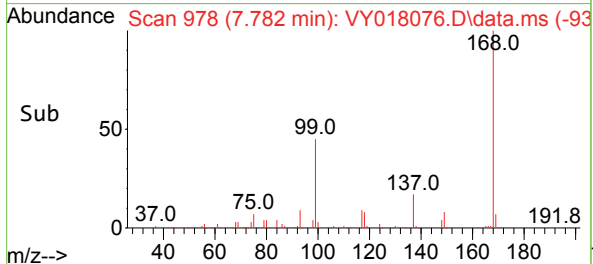

#11
Tert butyl alcohol
Concen: Below Cal
RT: 4.948 min Scan# 513
Delta R.T. -0.006 min
Lab File: VY018076.D
Acq: 29 Apr 2024 18:18

Tgt Ion: 59 Resp: 49
Ion Ratio Lower Upper
59 100
57 0.0 3.0 4.6#

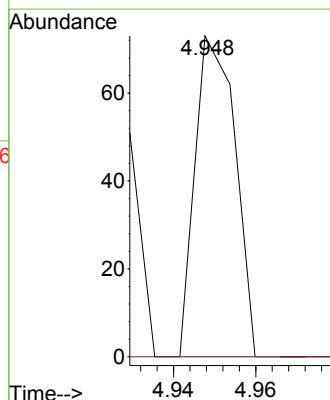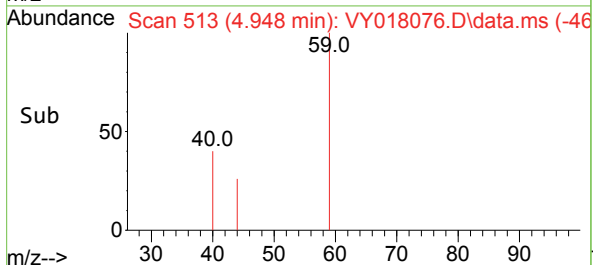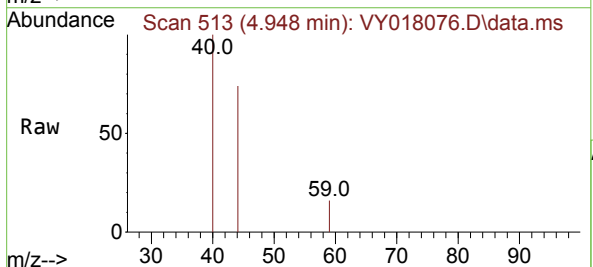



#16

Acetone

Concen: 3.434 ug/l

RT: 3.942 min Scan# 346

Delta R.T. -0.006 min

Lab File: VY018076.D

Acq: 29 Apr 2024 18:18

Instrument :

MSVOA_Y





ClientSampleId :

Tgt Ion: 43 Resp: 1699

Ion Ratio Lower Upper

43 100

58 34.0 31.7 47.5

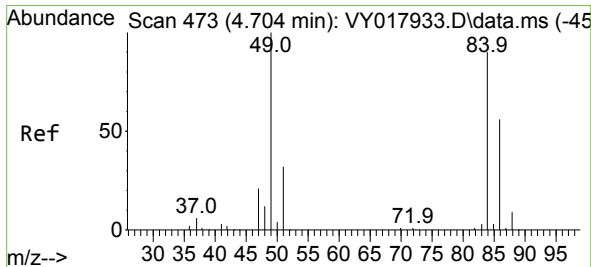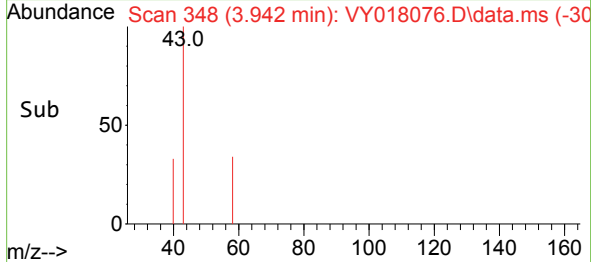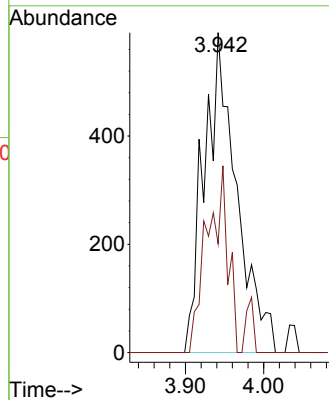

#20

Methylene Chloride

Concen: 11.585 ug/l

RT: 4.704 min Scan# 473

Delta R.T. -0.012 min

Lab File: VY018076.D

Acq: 29 Apr 2024 18:18

Tgt Ion: 84 Resp: 38832




Ion Ratio Lower Upper


84 100

49 95.0 84.4 126.6

51 30.0 26.0 39.0

86 60.4 49.5 74.3


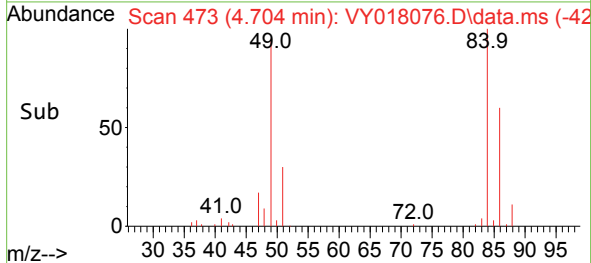
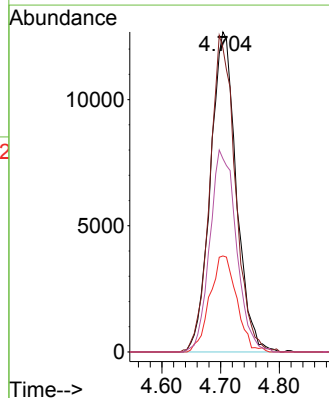
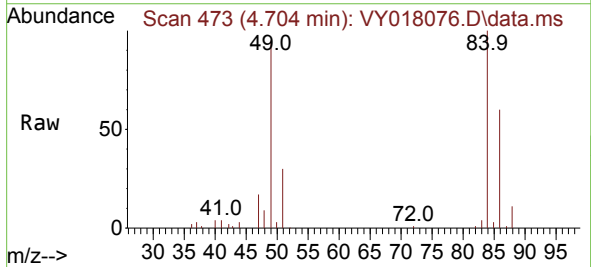


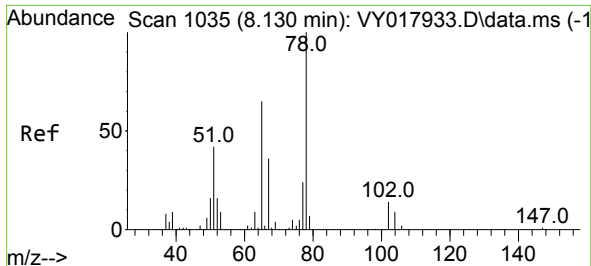

#33
1,2-Dichloroethane-d4
Concen: 51.815 ug/l
RT: 8.136 min Scan# 1035
Delta R.T. -0.006 min
Lab File: VY018076.D
Acq: 29 Apr 2024 18:18




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 65 Resp: 129743
Ion Ratio Lower Upper
65 100
67 58.2 0.0 109.6

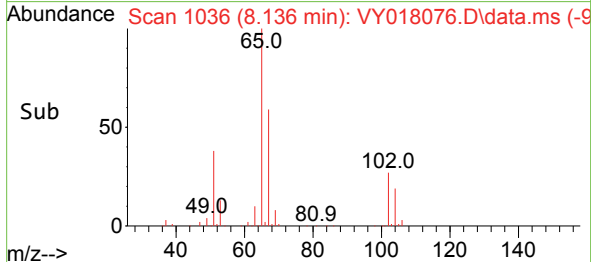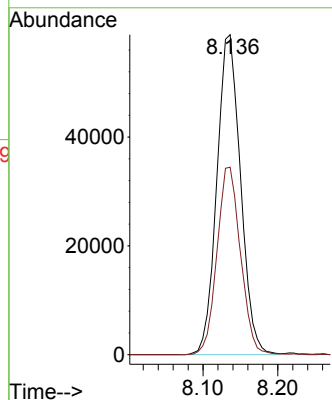

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.685 min Scan# 1126
Delta R.T. -0.006 min
Lab File: VY018076.D
Acq: 29 Apr 2024 18:18


Tgt Ion:114 Resp: 521517
Ion Ratio Lower Upper
114 100
63 16.5 0.0 35.0
88 13.4 0.0 27.2

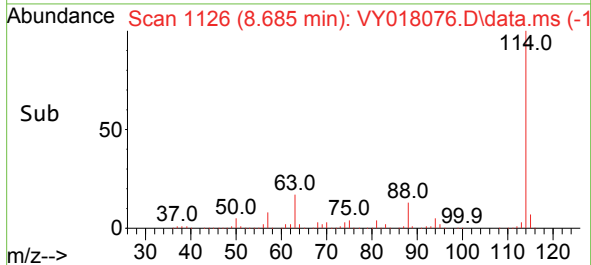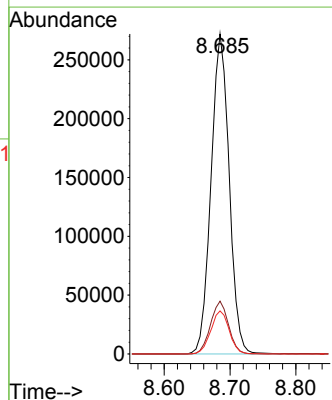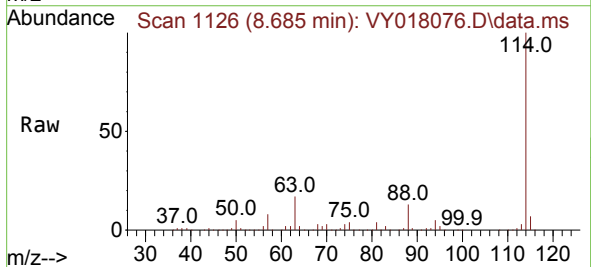



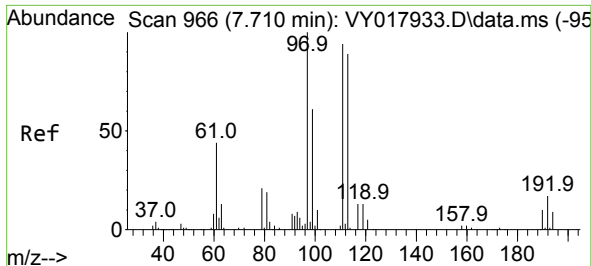


#35
Dibromofluoromethane
Concen: 52.406 ug/l
RT: 7.709 min Scan# 90
Delta R.T. -0.012 min
Lab File: VY018076.D
Acq: 29 Apr 2024 18:18

Instrument :
MSVOA_Y
ClientSampleId :







Tgt Ion:113 Resp: 168612
Ion Ratio Lower Upper
113 100
111 103.2 82.2 123.4
192 21.4 15.9 23.9

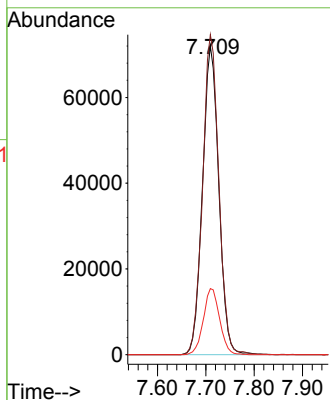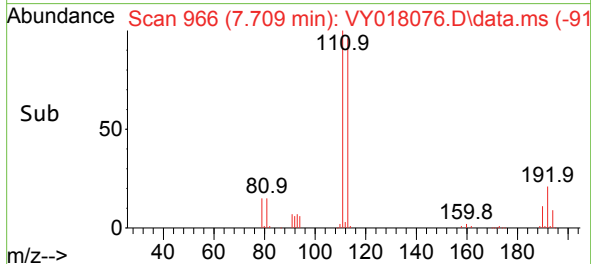

#36
1,1-Dichloropropene
Concen: 3.969 ug/l
RT: 7.782 min Scan# 978
Delta R.T. -0.134 min
Lab File: VY018076.D
Acq: 29 Apr 2024 18:18


Tgt Ion: 75 Resp: 18572
Ion Ratio Lower Upper
75 100
110 8.6 19.0 57.0#
77 0.0 25.3 37.9#

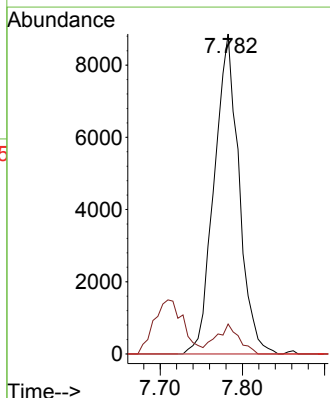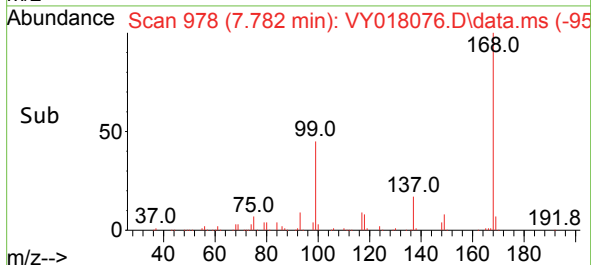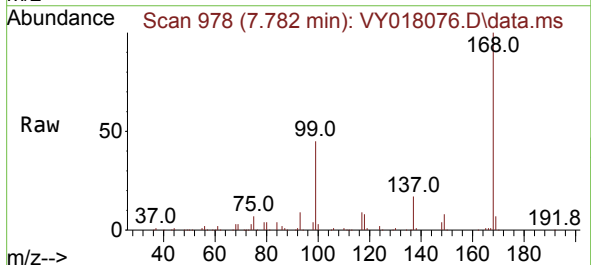



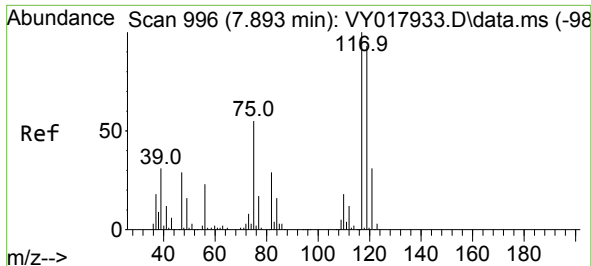


#38
Carbon Tetrachloride
Concen: 5.261 ug/l
RT: 7.782 min Scan# 91
Delta R.T. -0.122 min
Lab File: VY018076.D
Acq: 29 Apr 2024 18:18

Instrument :
MSVOA_Y
ClientSampleId :







Tgt Ion:117 Resp: 24870
Ion Ratio Lower Upper
117 100
119 5.6 75.8 113.6#
121 0.0 24.0 36.0#

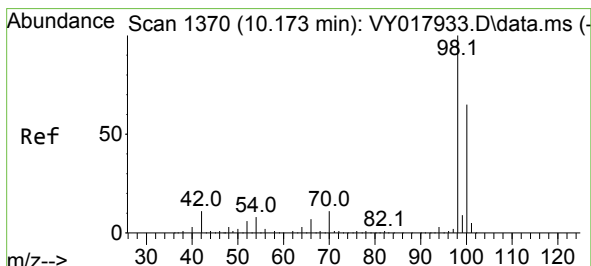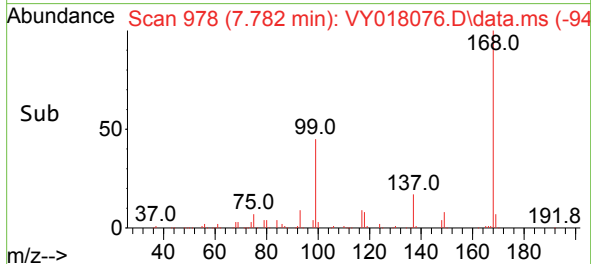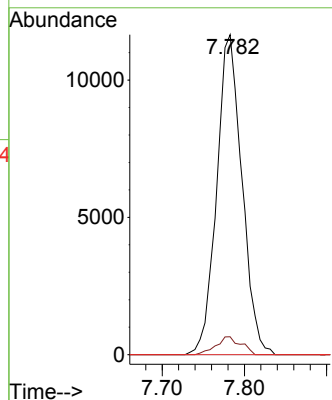

#50
Toluene-d8
Concen: 48.512 ug/l
RT: 10.178 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY018076.D
Acq: 29 Apr 2024 18:18

Tgt Ion: 98 Resp: 592269
Ion Ratio Lower Upper
98 100
100 64.2 52.0 78.0


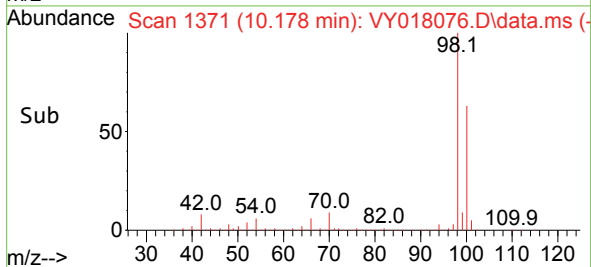
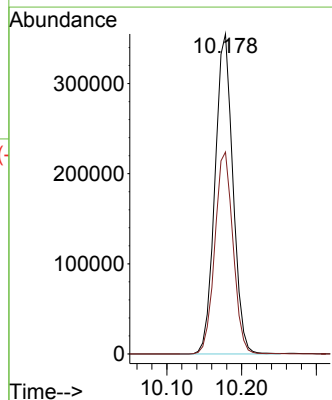
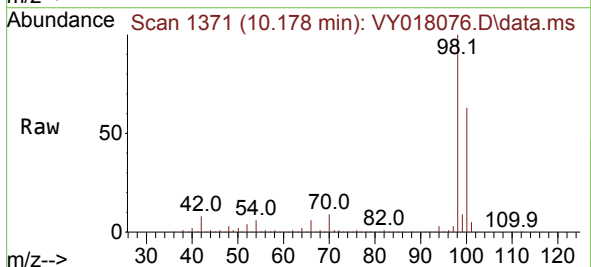




#62
4-Bromofluorobenzene
Concen: 42.274 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.006 min
Lab File: VY018076.D
Acq: 29 Apr 2024 18:18




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 95 Resp: 159839
Ion Ratio Lower Upper
95 100
174 95.3 0.0 175.6
176 90.8 0.0 171.4

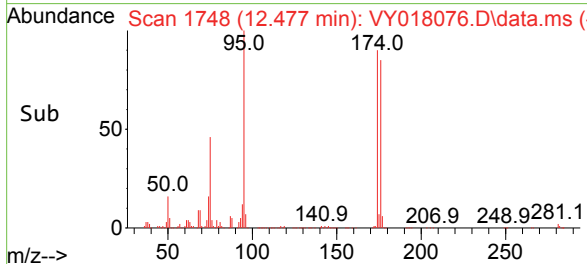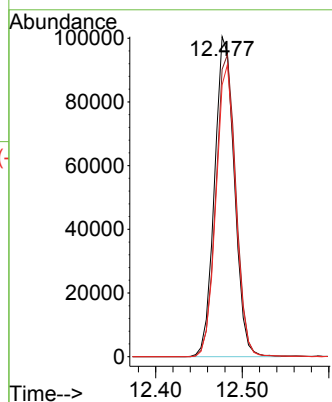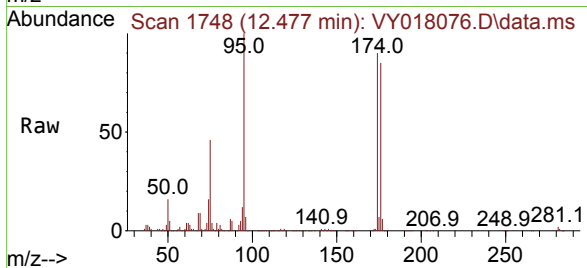

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 1586
Delta R.T. -0.000 min
Lab File: VY018076.D
Acq: 29 Apr 2024 18:18

Tgt Ion: 117 Resp: 467939
Ion Ratio Lower Upper
117 100
82 50.8 42.4 63.6
119 32.2 25.9 38.9

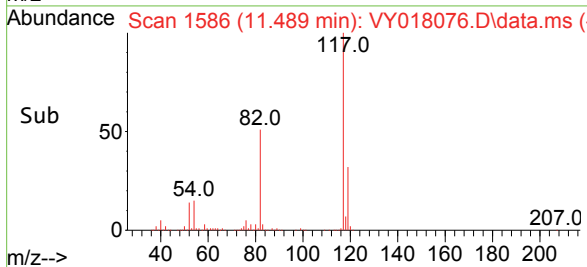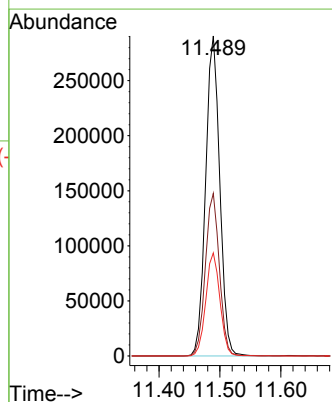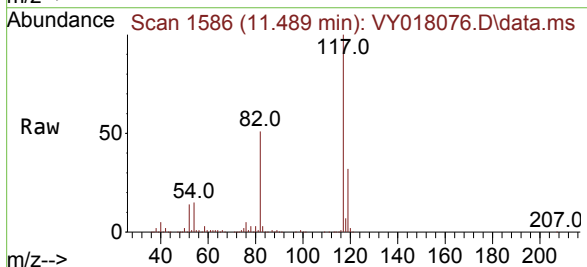



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1903

Delta R.T. -0.000 min

Lab File: VY018076.D

Acq: 29 Apr 2024 18:18

Instrument :

MSVOA_Y

ClientSampleId :





Tgt Ion:152 Resp: 182391

Ion Ratio Lower Upper

152 100

115 53.3 28.2 84.7

150 156.2 0.0 345.6

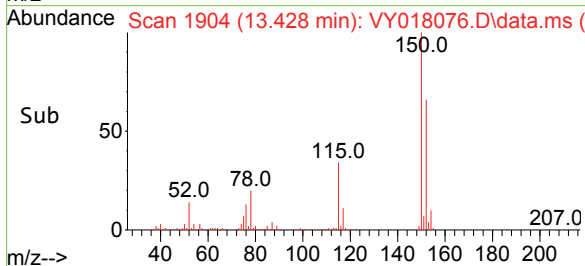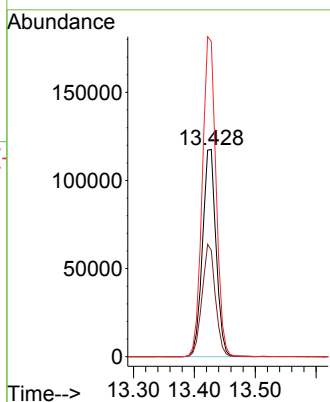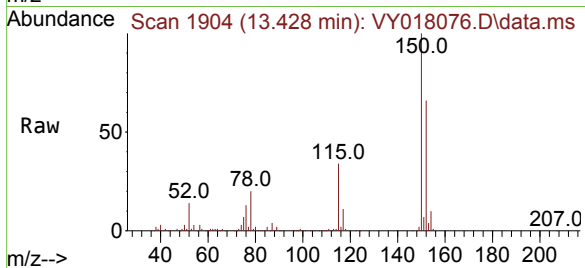

#76

1,2,3-Trichloropropane

Concen: 43.692 ug/l

RT: 12.477 min Scan# 1748

Delta R.T. -0.159 min

Lab File: VY018076.D




Acq: 29 Apr 2024 18:18


Tgt Ion: 75 Resp: 74781

Ion Ratio Lower Upper

75 100


77 1.2 0.0 0.0#

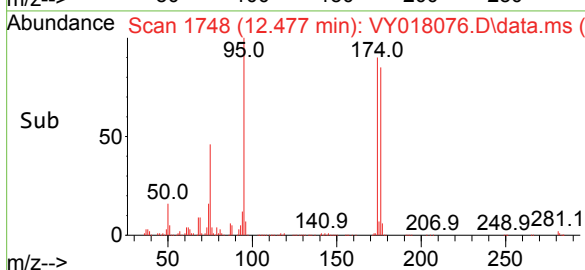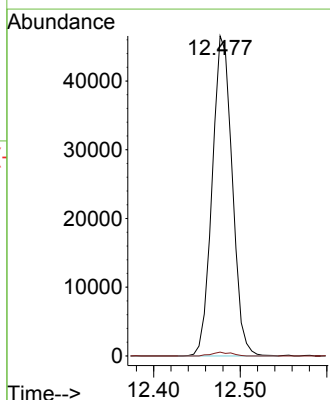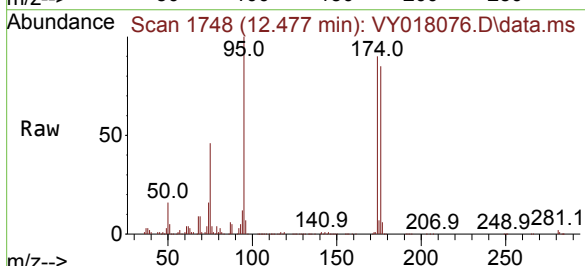



#81
 trans-1,4-Dichloro-2-butene
 Concen: 90.086 ug/l
 RT: 12.477 min Scan# 11
 Delta R.T. 0.097 min
 Lab File: VY018076.D
 Acq: 29 Apr 2024 18:18

Instrument :
 MSVOA_Y
 ClientSampleId :

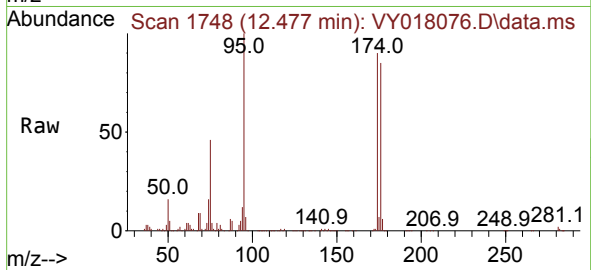

Tgt Ion	Ratio	Lower	Upper
75	100		
53	0.1	66.8	100.2#
89	0.0	35.8	53.6#

