


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY043020\
 Data File : VY002509.D
 Acq On : 30 Apr 2020 13:21
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y043020S.M
 Title : SW846 8260
 Last Update : Mon May 04 12:22:08 2020

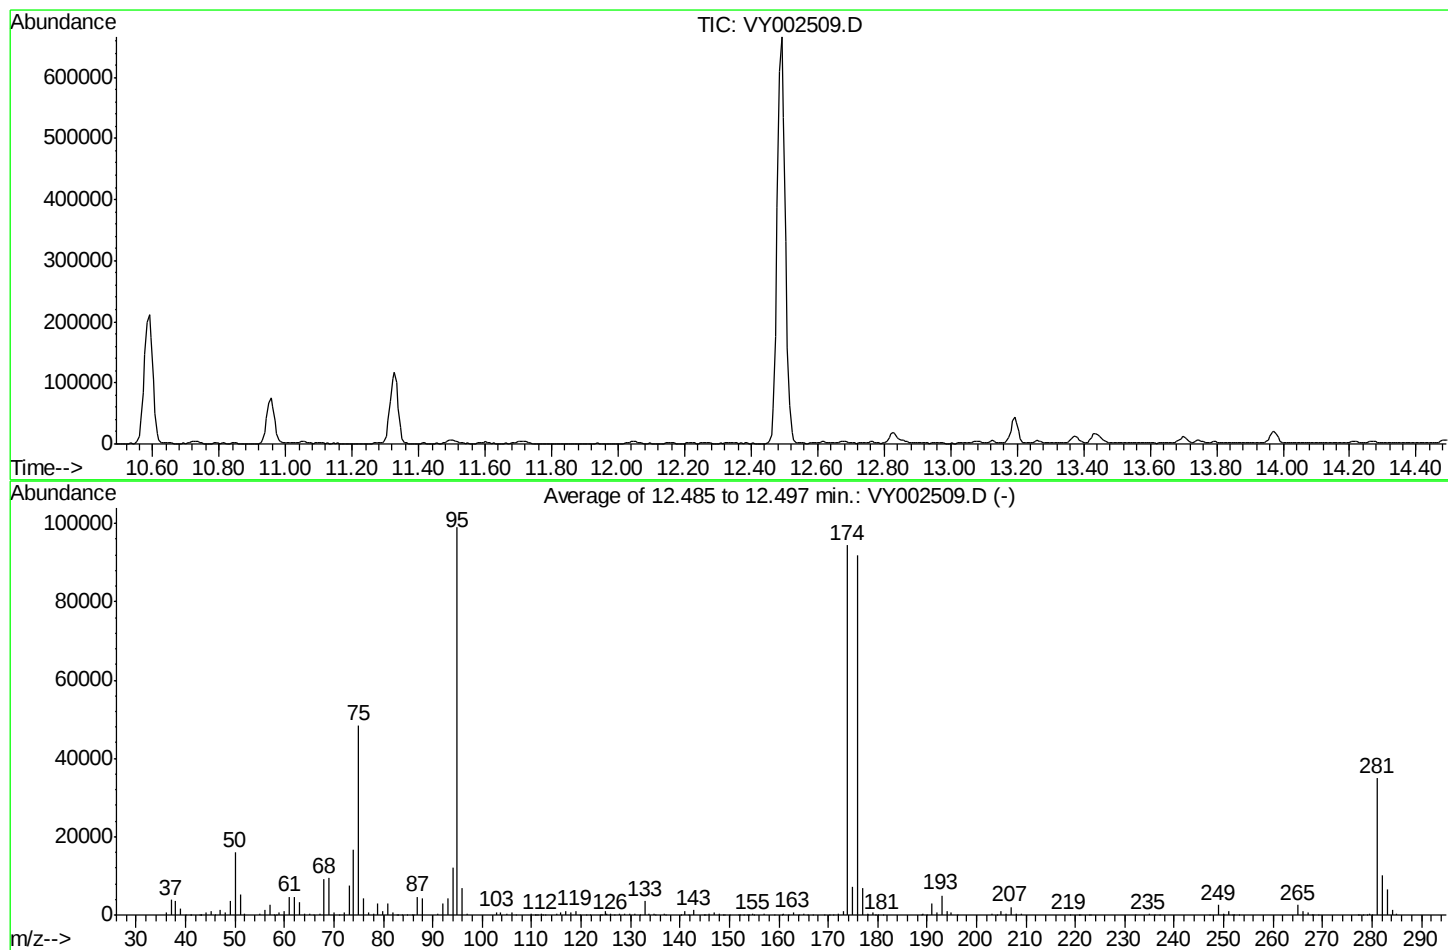

AutoFind: Scans 1763, 1764, 1765; Background Corrected with Scan 1754

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	16010	PASS
75	95	30	60	48.8	48333	PASS
95	95	100	100	100.0	99024	PASS
96	95	5	9	7.0	6901	PASS
173	174	0.00	2	1.1	1011	PASS
174	95	50	100	95.4	94485	PASS
175	174	5	9	7.5	7128	PASS
176	174	95	101	97.1	91762	PASS
177	176	5	9	7.7	7039	PASS