

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050323\
 Data File : VY013575.D
 Acq On : 03 May 2023 12:39
 Operator : KP/MD
 Sample : 02558-07
 Misc : 4.09g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 P001-SS013-0612-01

Quant Time: May 03 15:40:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 25 02:39:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	213982	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	361069	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	354007	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	164288	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	156533	66.731	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	133.460%
35) Dibromofluoromethane	7.716	113	125921	55.448	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	110.900%
50) Toluene-d8	10.179	98	445063	55.091	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	110.180%
62) 4-Bromofluorobenzene	12.483	95	143032	52.517	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	105.040%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050323\
Data File : VY013575.D
Acq On : 03 May 2023 12:39
Operator : KP/MD
Sample : 02558-07
Misc : 4.09g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
P001-SS013-0612-01

Quant Time: May 03 15:40:39 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
Quant Title : SW846 8260
QLast Update : Tue Apr 25 02:39:58 2023
Response via : Initial Calibration




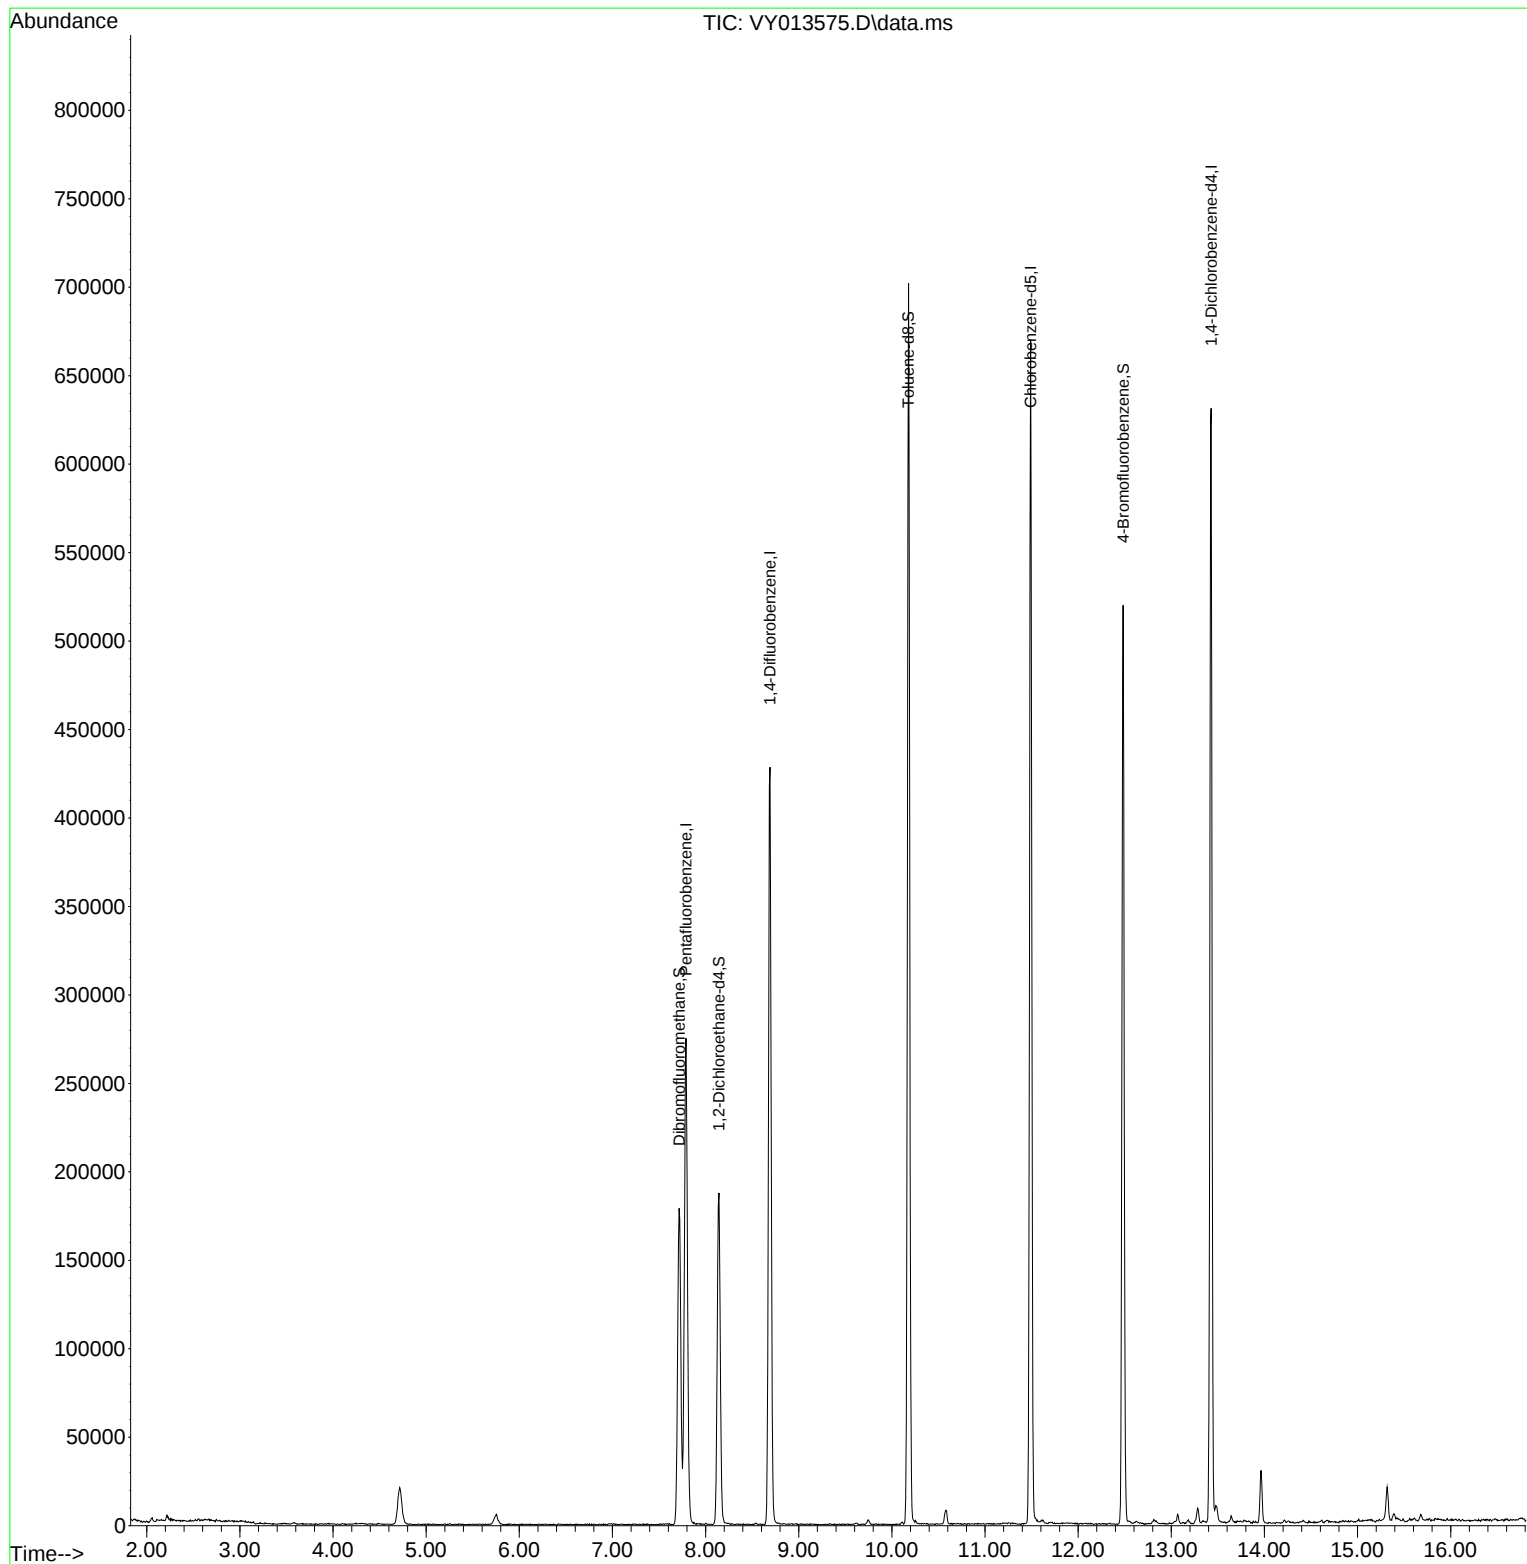




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY013575.D
Acq: 03 May 2023 12:39




Instrument :
MSVOA_Y
ClientSampleId :
P001-SS013-0612-01


Tgt Ion:168 Resp: 213982
Ion Ratio Lower Upper
168 100
99 50.5 41.8 62.6

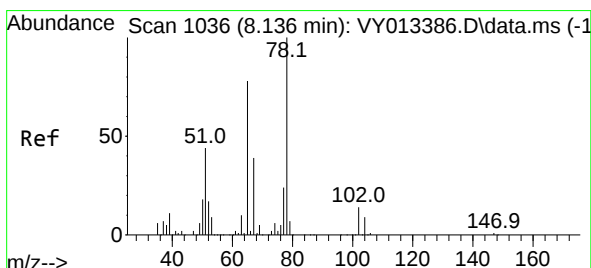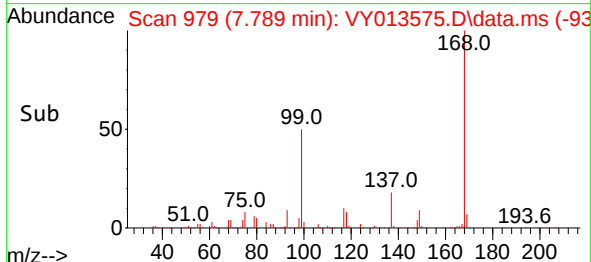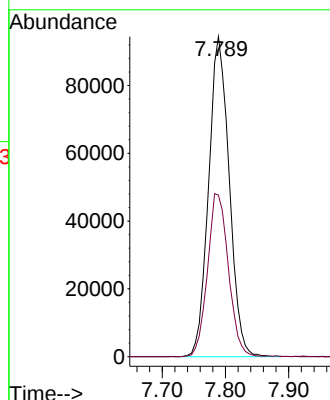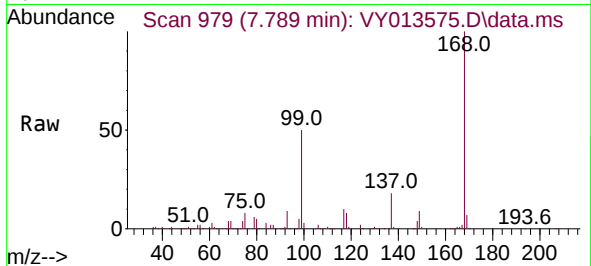

#33
1,2-Dichloroethane-d4
Concen: 66.731 ug/l
RT: 8.142 min Scan# 1037
Delta R.T. 0.006 min
Lab File: VY013575.D
Acq: 03 May 2023 12:39

Tgt Ion: 65 Resp: 156533
Ion Ratio Lower Upper
65 100
67 50.5 0.0 103.4


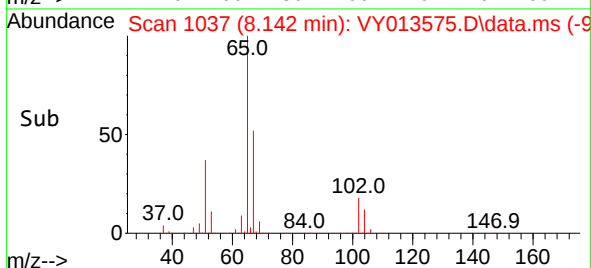
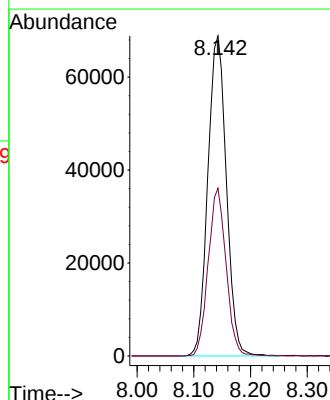
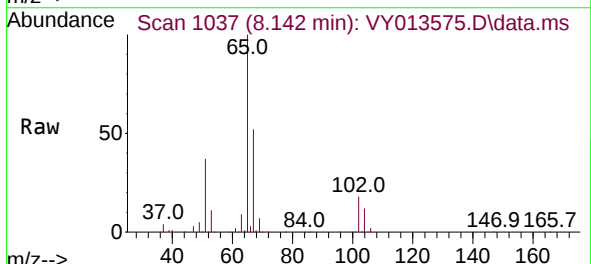


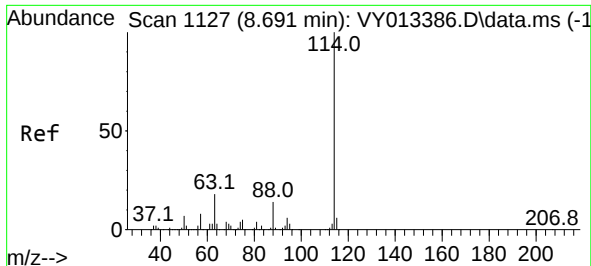

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.691 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VY013575.D
Acq: 03 May 2023 12:39




Instrument :
MSVOA_Y
ClientSampleId :
P001-SS013-0612-01


Tgt Ion:	114	Resp:	361069
Ion Ratio	Lower	Upper	
114	100		
63	20.8	0.0	36.6
88	14.5	0.0	28.8

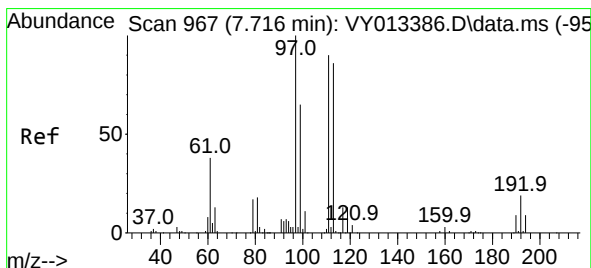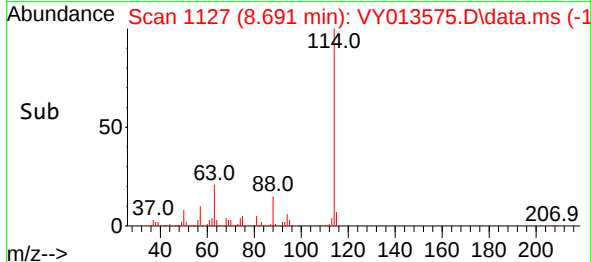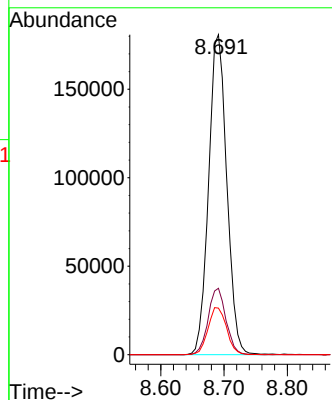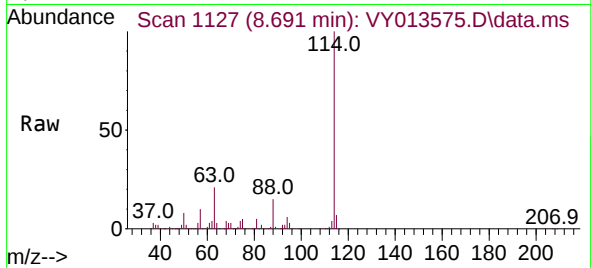

#35
Dibromofluoromethane
Concen: 55.448 ug/l
RT: 7.716 min Scan# 967
Delta R.T. -0.000 min
Lab File: VY013575.D
Acq: 03 May 2023 12:39

Tgt Ion:	113	Resp:	125921
Ion Ratio	Lower	Upper	
113	100		
111	101.8	82.2	123.2
192	21.1	16.7	25.1

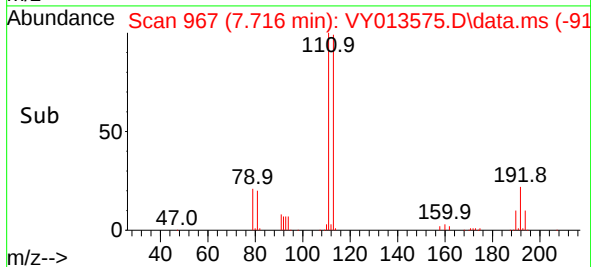
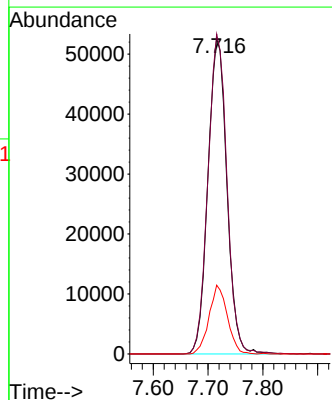
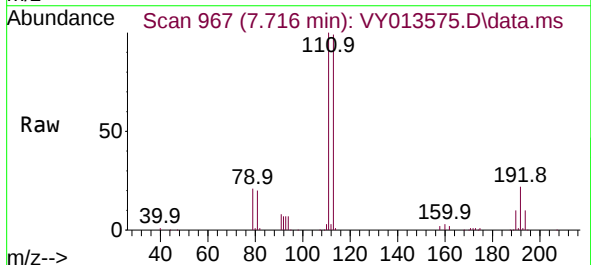


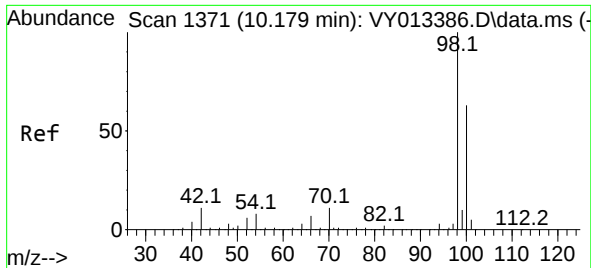

#50
Toluene-d8
Concen: 55.091 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY013575.D
Acq: 03 May 2023 12:39




Instrument :
MSVOA_Y
ClientSampleId :
P001-SS013-0612-01


Tgt Ion: 98 Resp: 445063
Ion Ratio Lower Upper
98 100
100 63.2 50.5 75.7

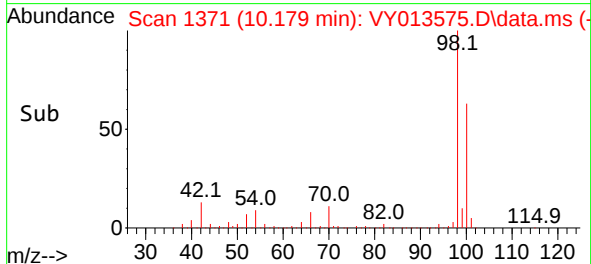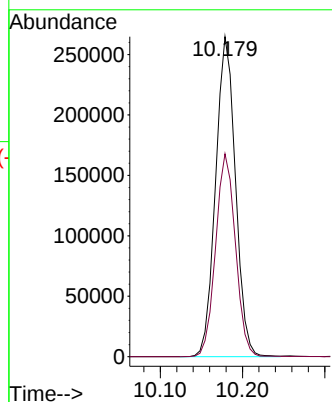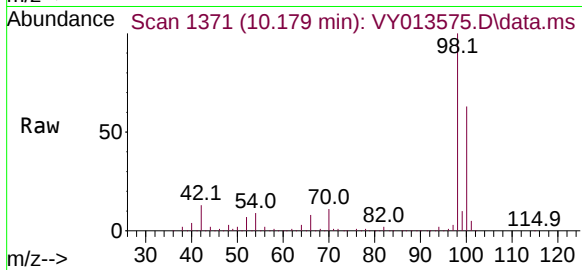

#62
4-Bromofluorobenzene
Concen: 52.517 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.006 min
Lab File: VY013575.D
Acq: 03 May 2023 12:39

Tgt Ion: 95 Resp: 143032
Ion Ratio Lower Upper
95 100
174 92.3 0.0 182.0
176 91.3 0.0 175.4

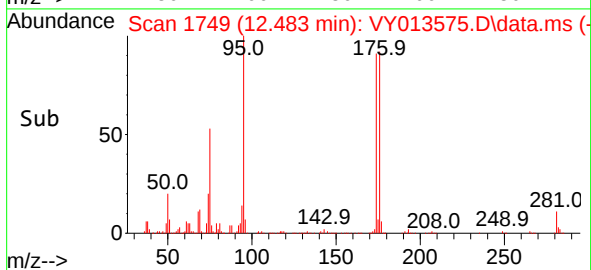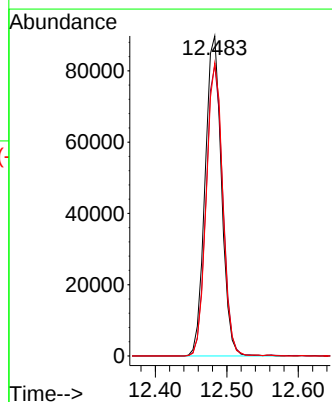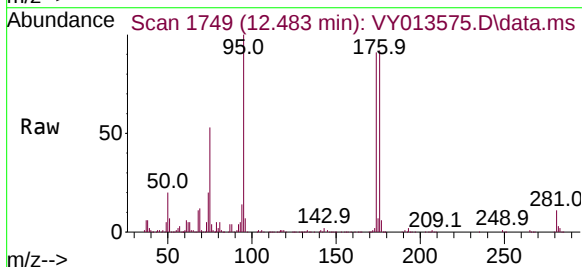

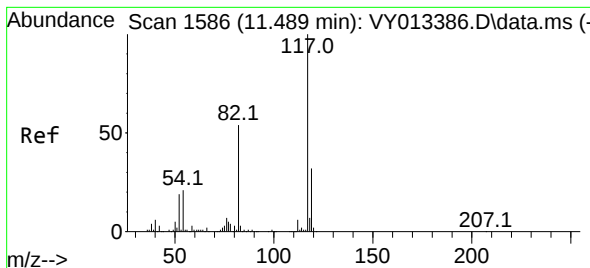

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.489 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY013575.D

Acq: 03 May 2023 12:39

Instrument :

MSVOA_Y

ClientSampleId :

P001-SS013-0612-01





Tgt Ion:117 Resp: 354007

Ion Ratio Lower Upper

117 100

82 53.8 43.0 64.6

119 32.2 25.5 38.3

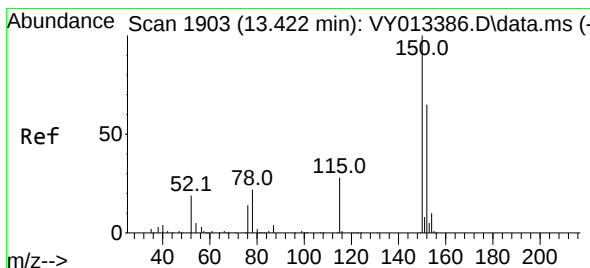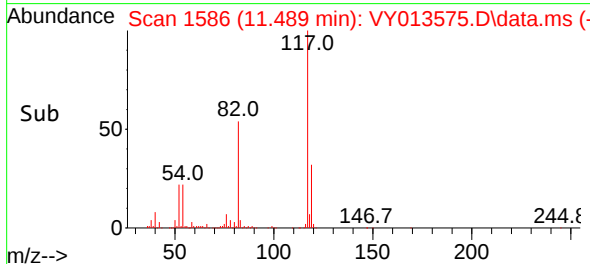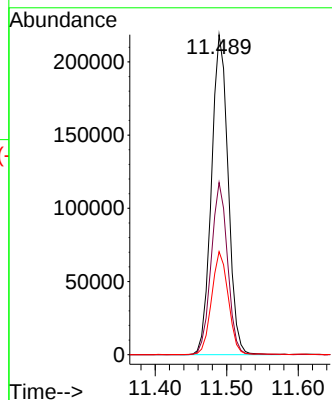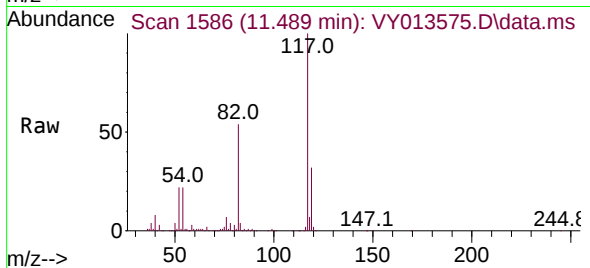

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.006 min

Lab File: VY013575.D

Acq: 03 May 2023 12:39

Tgt Ion:152 Resp: 164288

Ion Ratio Lower Upper

152 100

115 56.8 28.1 84.2

150 157.7 0.0 352.0

