

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050323\
 Data File : VY013586.D
 Acq On : 03 May 2023 16:57
 Operator : KP/MD
 Sample : 02584-01
 Misc : 5.05g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TR-05-050123

Quant Time: May 04 01:21:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 25 02:39:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	193232	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	320340	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	314303	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	144123	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	132657	62.626	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	125.260%
35) Dibromofluoromethane	7.716	113	111332	55.257	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	110.520%
50) Toluene-d8	10.179	98	397798	55.501	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	111.000%
62) 4-Bromofluorobenzene	12.483	95	126735	52.450	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	104.900%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050323\
Data File : VY013586.D
Acq On : 03 May 2023 16:57
Operator : KP/MD
Sample : 02584-01
Misc : 5.05g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TR-05-050123

Quant Time: May 04 01:21:26 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
Quant Title : SW846 8260
QLast Update : Tue Apr 25 02:39:58 2023
Response via : Initial Calibration




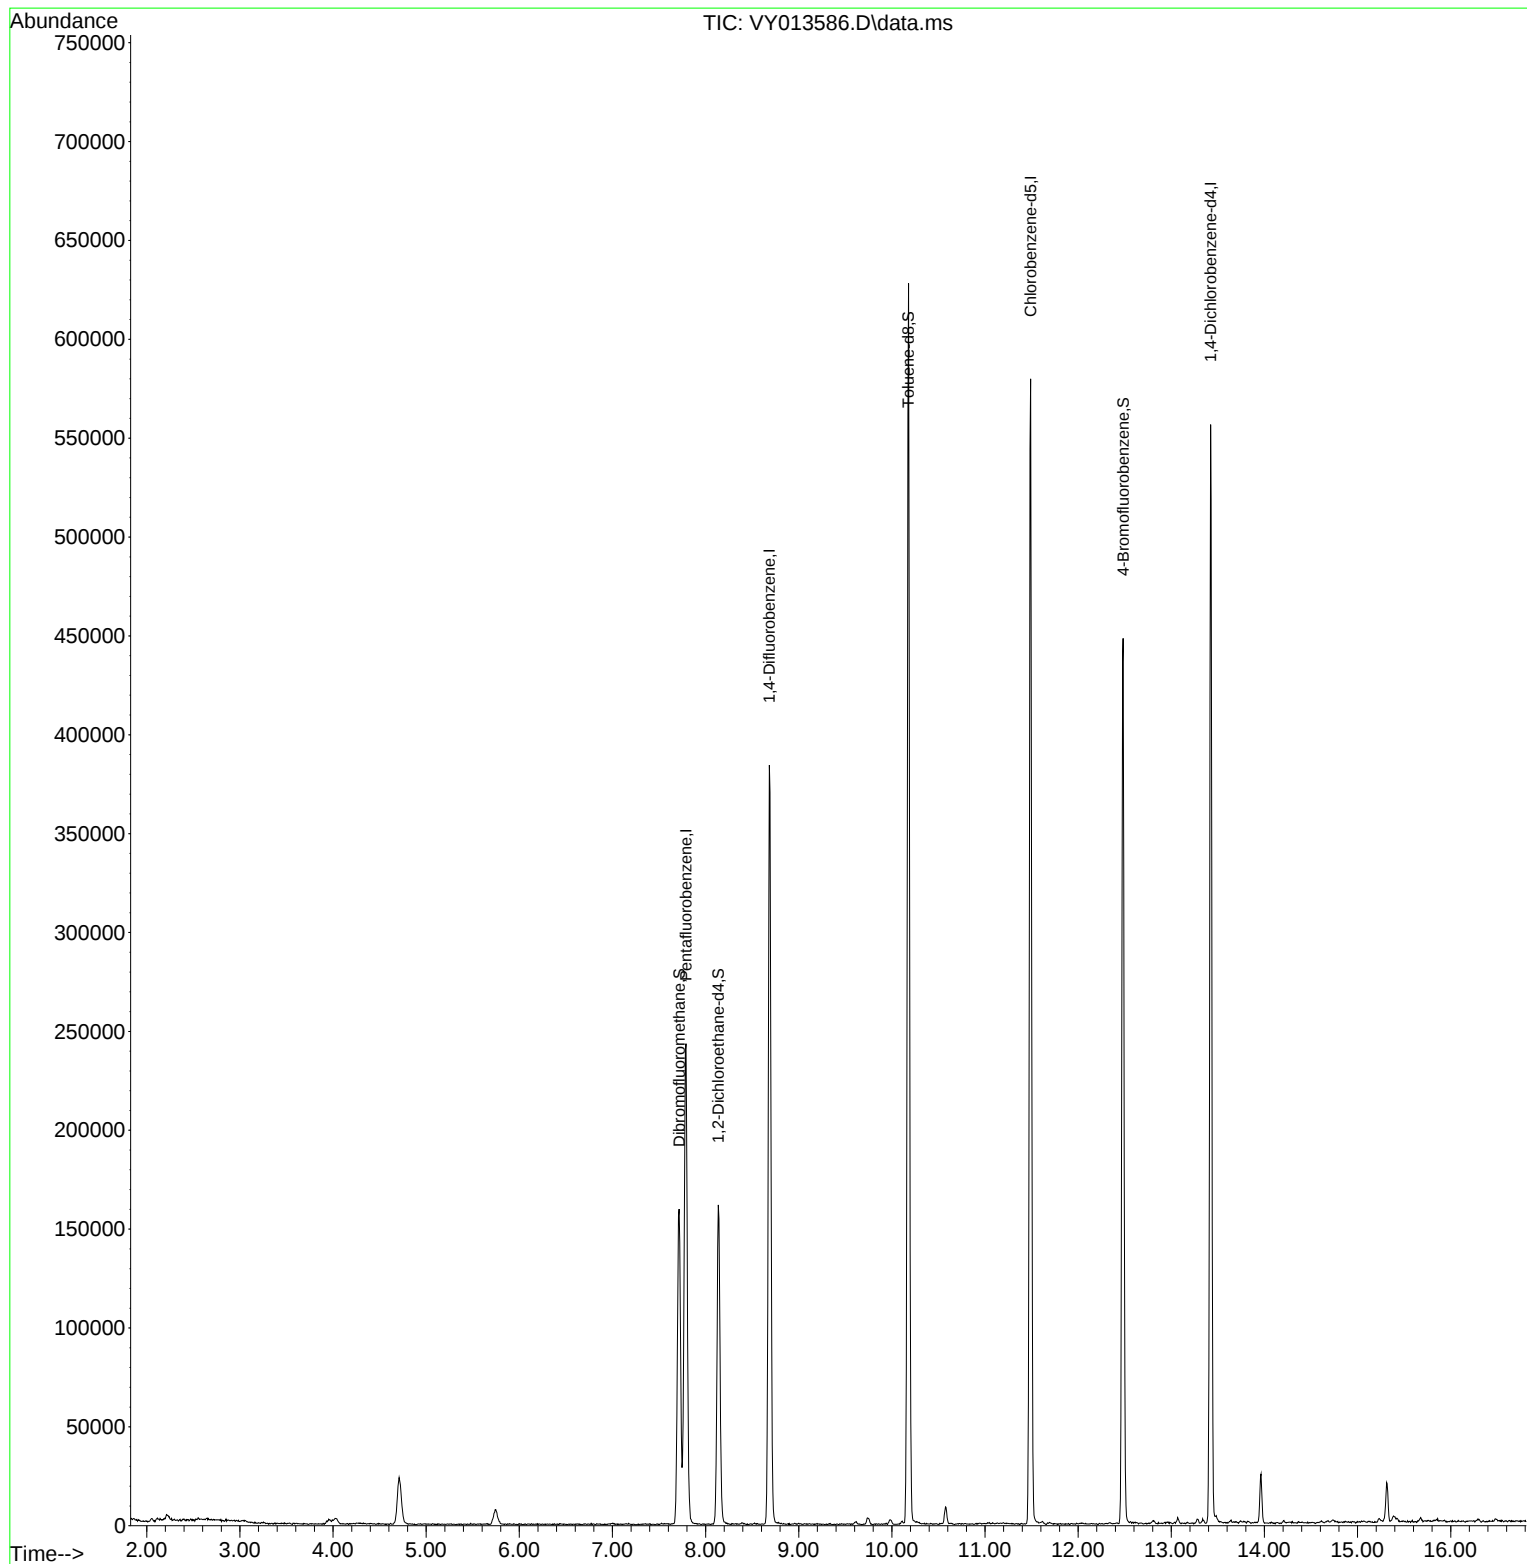




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY013586.D
Acq: 03 May 2023 16:57




Instrument :
MSVOA_Y
ClientSampleId :
TR-05-050123

Tgt Ion:168 Resp: 193232
Ion Ratio Lower Upper
168 100
99 51.2 41.8 62.6

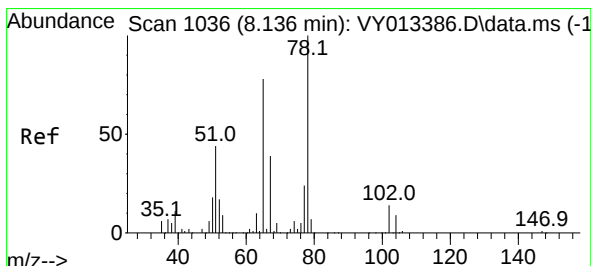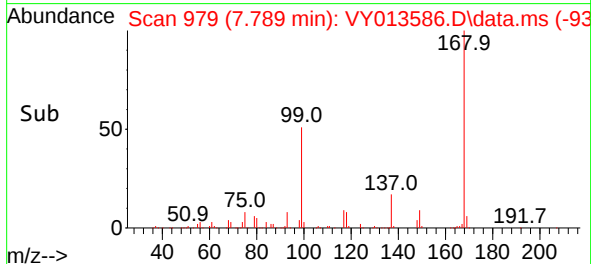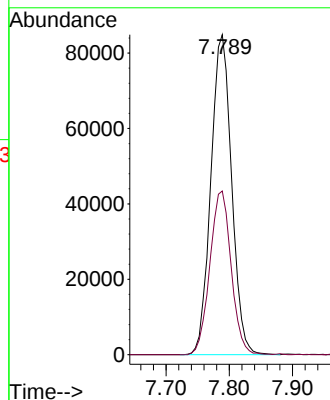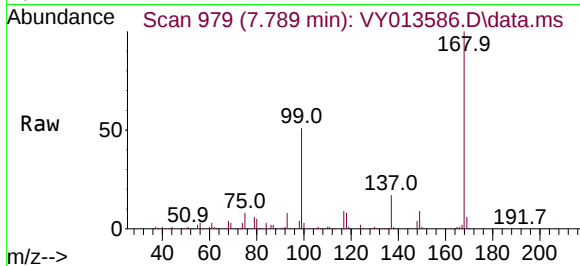

#33
1,2-Dichloroethane-d4
Concen: 62.626 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. 0.000 min
Lab File: VY013586.D
Acq: 03 May 2023 16:57

Tgt Ion: 65 Resp: 132657
Ion Ratio Lower Upper
65 100
67 50.6 0.0 103.4

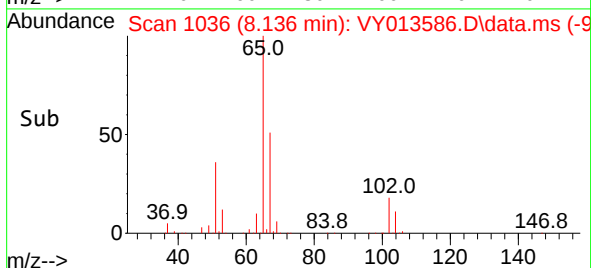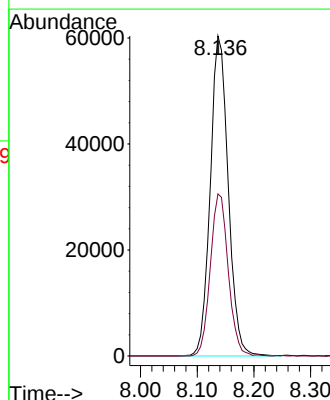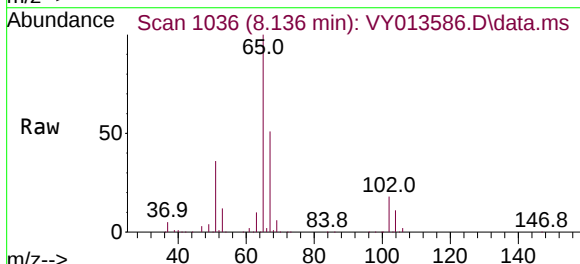



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.006 min

Lab File: VY013586.D

Acq: 03 May 2023 16:57

Instrument :

MSVOA_Y

ClientSampleId :

TR-05-050123




Tgt Ion:114 Resp: 320340

Ion Ratio Lower Upper

114 100

63 20.0 0.0 36.6

88 15.1 0.0 28.8

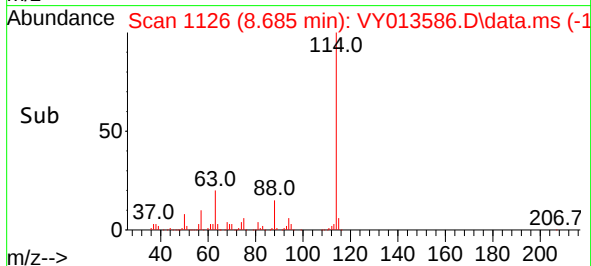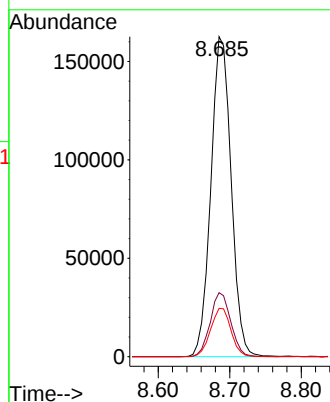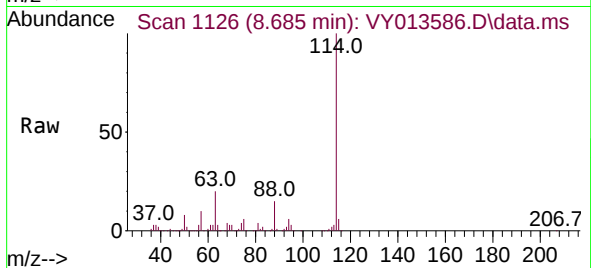

#35

Dibromofluoromethane

Concen: 55.257 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY013586.D

Acq: 03 May 2023 16:57




Tgt Ion:113 Resp: 111332


Ion Ratio Lower Upper

113 100

111 101.7 82.2 123.2

192 20.9 16.7 25.1


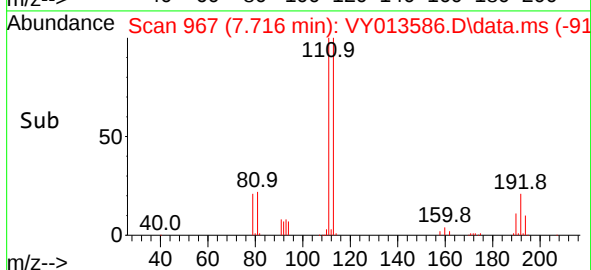
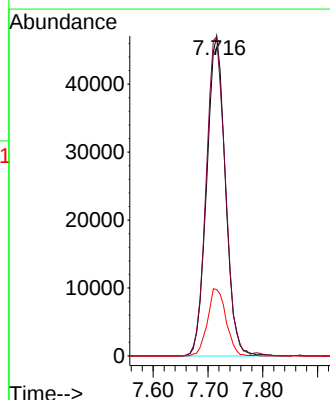
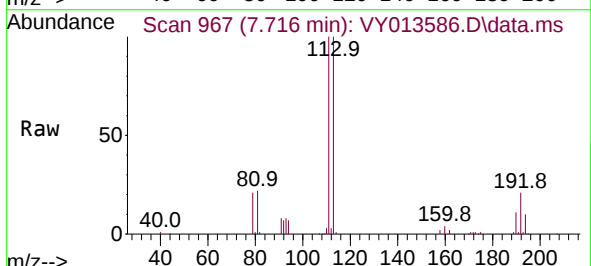


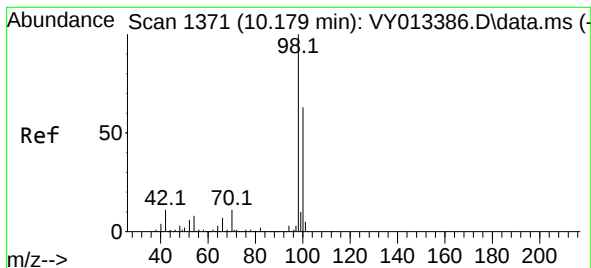

#50
Toluene-d8
Concen: 55.501 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY013586.D
Acq: 03 May 2023 16:57




Instrument :
MSVOA_Y
ClientSampleId :
TR-05-050123


Tgt Ion: 98 Resp: 397798
Ion Ratio Lower Upper
98 100
100 62.6 50.5 75.7

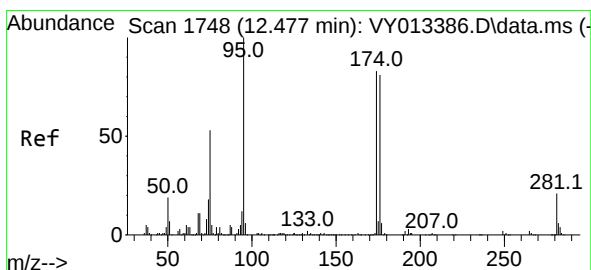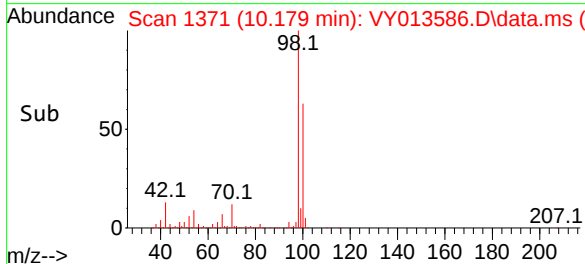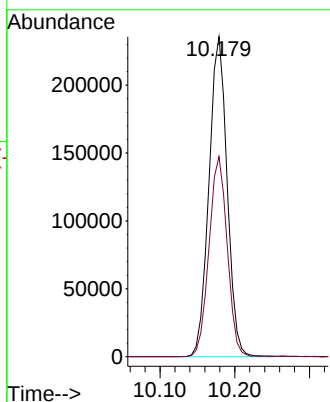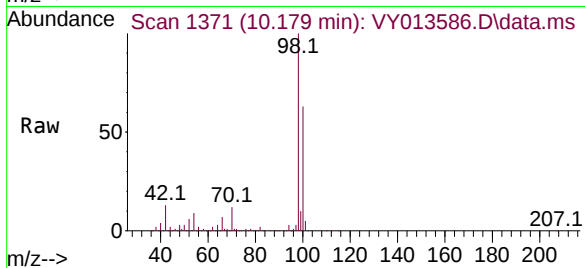

#62
4-Bromofluorobenzene
Concen: 52.450 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.006 min
Lab File: VY013586.D
Acq: 03 May 2023 16:57

Tgt Ion: 95 Resp: 126735
Ion Ratio Lower Upper
95 100
174 92.1 0.0 182.0
176 89.2 0.0 175.4

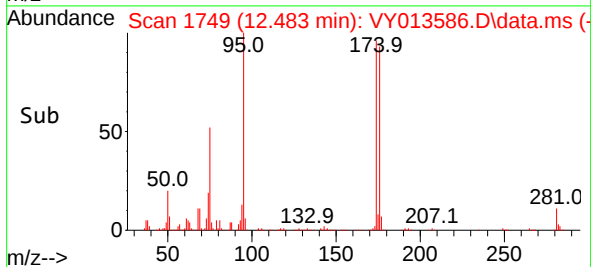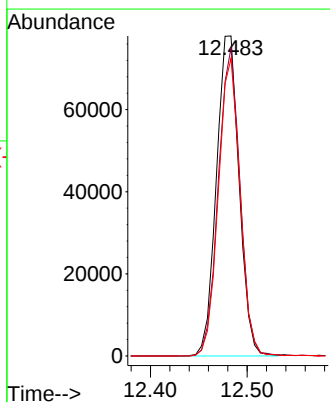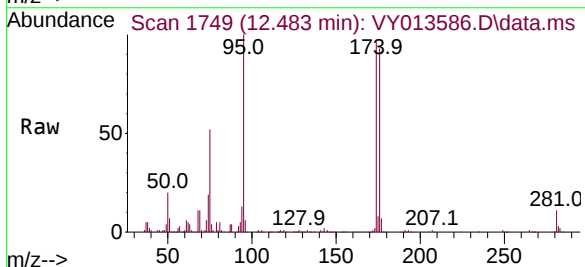

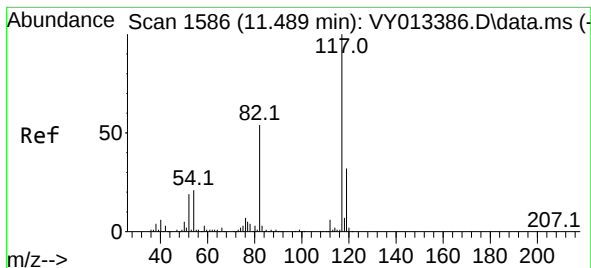

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.490 min Scan# 11

Delta R.T. 0.001 min

Lab File: VY013586.D

Acq: 03 May 2023 16:57

Instrument :

MSVOA_Y

ClientSampleId :

TR-05-050123





Tgt Ion:117 Resp: 314303

Ion Ratio Lower Upper

117 100

82 53.8 43.0 64.6

119 31.7 25.5 38.3

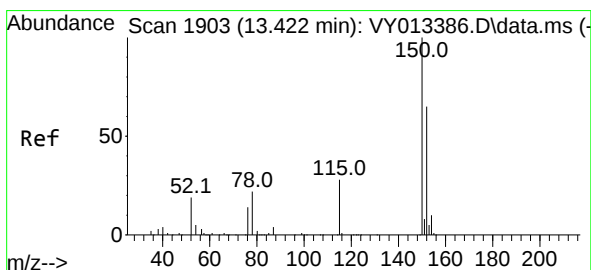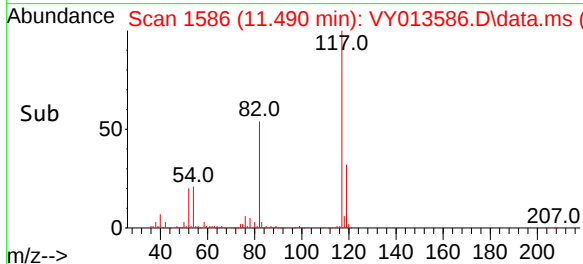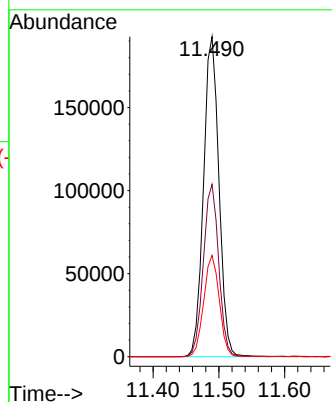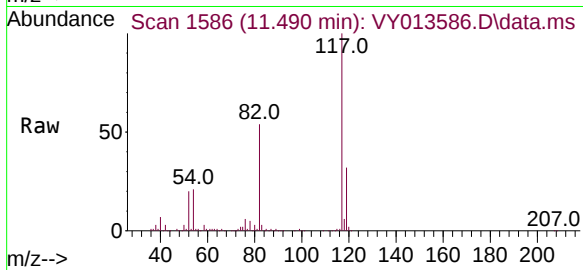

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.422 min Scan# 1903

Delta R.T. 0.000 min

Lab File: VY013586.D

Acq: 03 May 2023 16:57

Tgt Ion:152 Resp: 144123

Ion Ratio Lower Upper

152 100

115 55.0 28.1 84.2

150 154.1 0.0 352.0

