

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050421\
 Data File : VY004702.D
 Acq On : 04 May 2021 09:45
 Operator : SY/MD
 Sample : VY0504SBL01
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0504SBL01

Quant Time: May 05 01:30:40 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041221S.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 13 03:38:02 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.795	168	155897	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	276978	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	264263	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	121902	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.148	65	104036	60.06	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 120.12%	
35) Dibromofluoromethane	7.722	113	83879	54.57	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 109.14%	
50) Toluene-d8	10.179	98	342411	52.37	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 104.74%	
62) 4-Bromofluorobenzene	12.483	95	115965	52.27	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 104.54%	
Target Compounds						
						Qvalue
3) Chloromethane	2.119	50	2567	1.23	ug/l	100
11) Tert butyl alcohol	4.954	59	1738	10.18	ug/l #	76
20) Methylene Chloride	4.716	84	11450	6.84	ug/l	97
37) Ethyl Acetate	7.088	43	2059	1.16	ug/l #	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050421\
Data File : VY004702.D
Acq On : 04 May 2021 09:45
Operator : SY/MD
Sample : VY0504SBL01
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0504SBL01

Quant Time: May 05 01:30:40 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041221S.M
Quant Title : SW846 8260
QLast Update : Tue Apr 13 03:38:02 2021
Response via : Initial Calibration




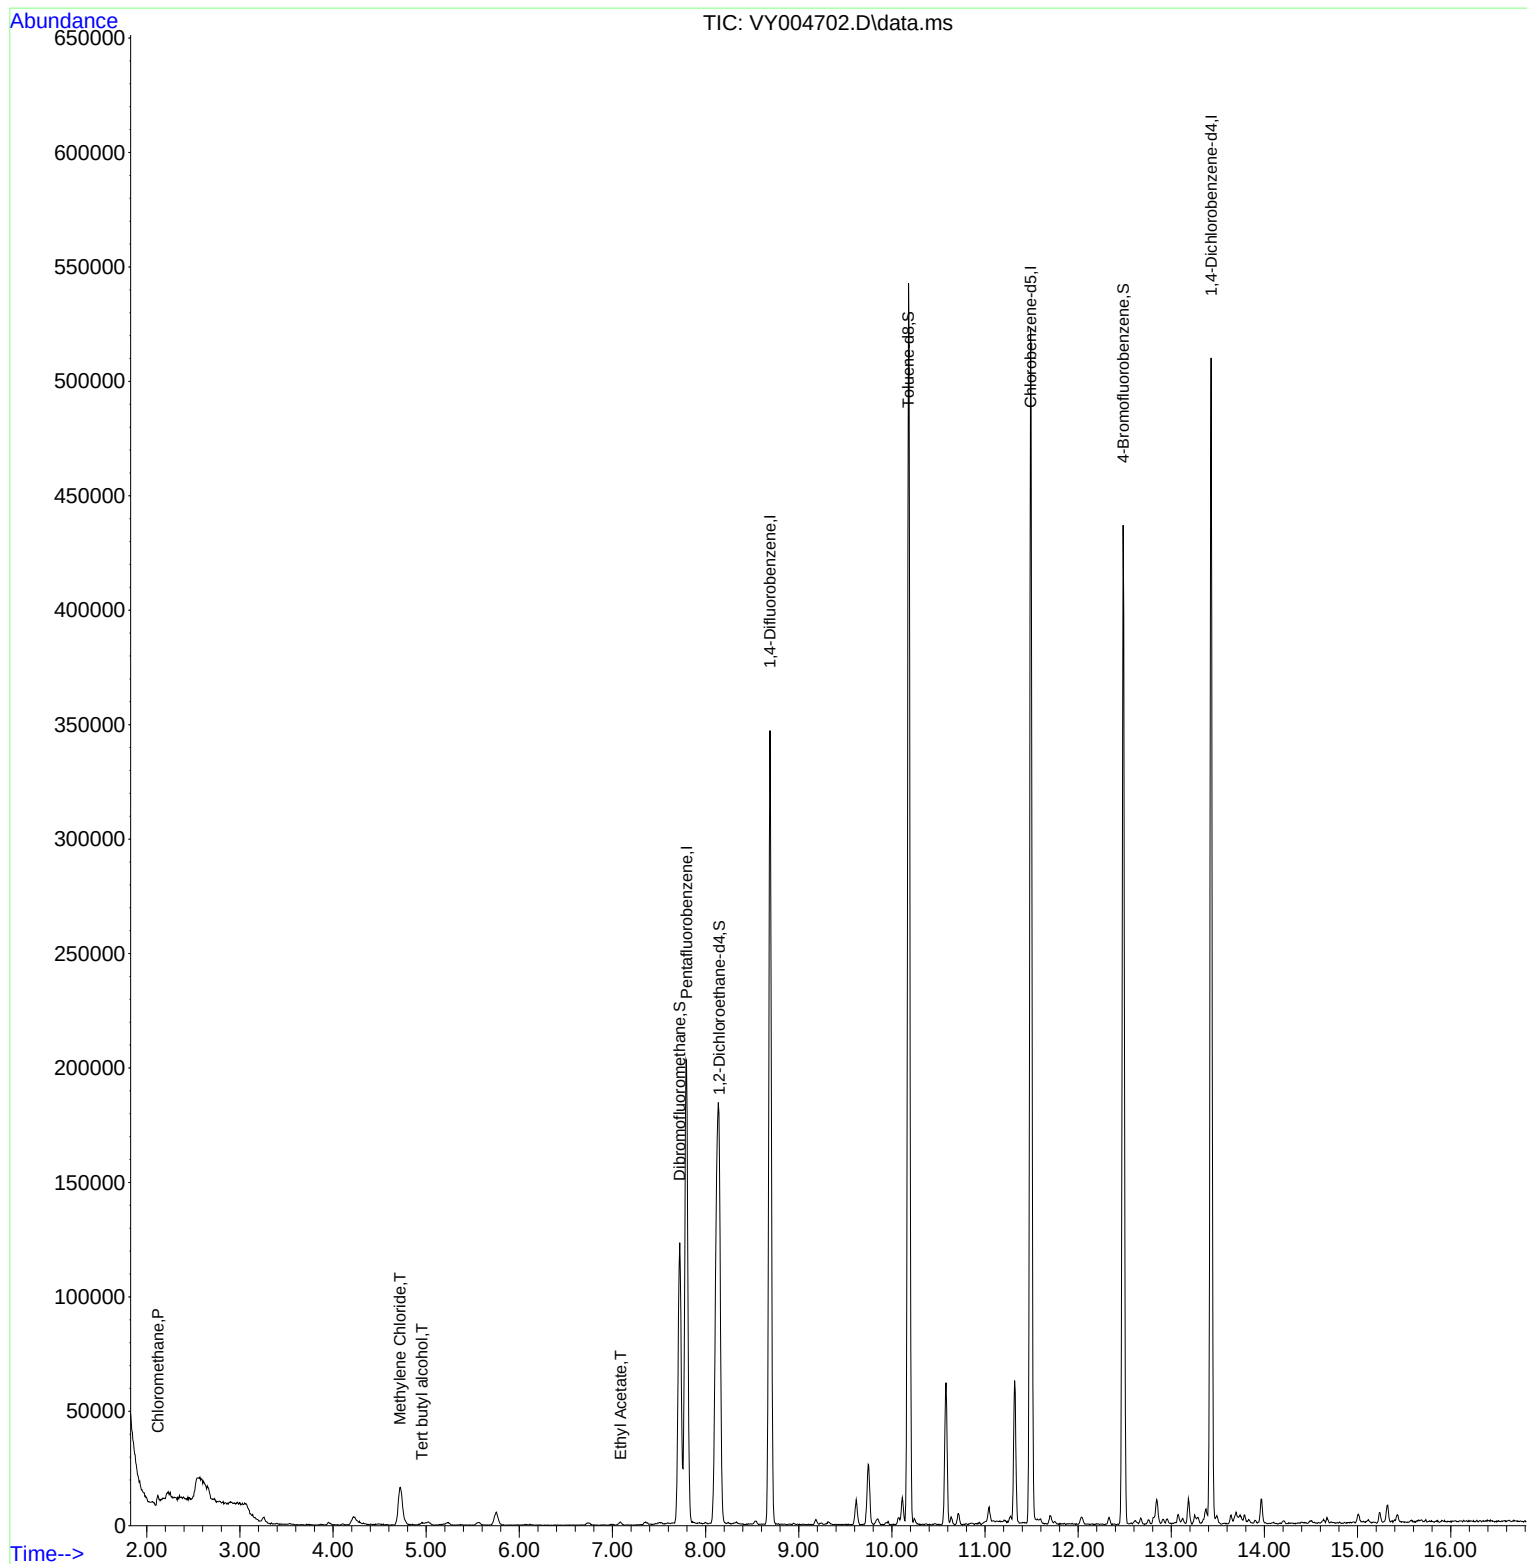




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.795 min Scan# 980
Delta R.T. -0.006 min
Lab File: VY004702.D
Acq: 04 May 2021 09:45




Instrument :
MSVOA_Y
ClientSampleId :
VY0504SBL01


Tgt Ion:168 Resp: 155897
Ion Ratio Lower Upper
168 100
99 54.5 45.5 68.3

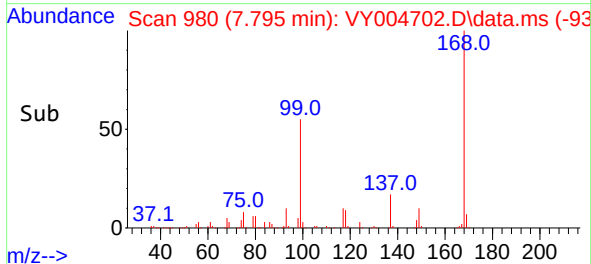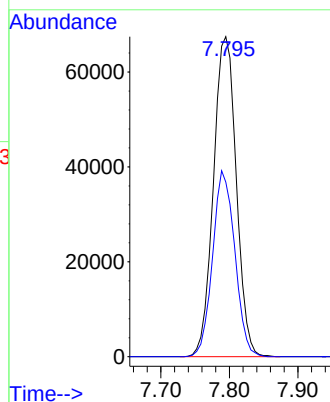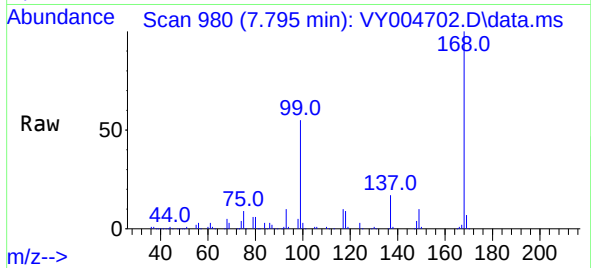

#3
Chloromethane
Concen: 1.23 ug/l
RT: 2.119 min Scan# 49
Delta R.T. 0.000 min
Lab File: VY004702.D
Acq: 04 May 2021 09:45

Tgt Ion: 50 Resp: 2567
Ion Ratio Lower Upper
50 100
52 33.4 26.6 39.8


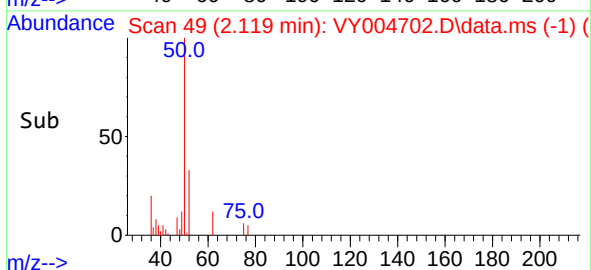
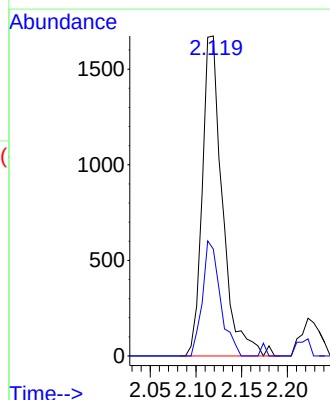





#11
Tert butyl alcohol
Concen: 10.18 ug/l
RT: 4.954 min Scan# 514
Delta R.T. -0.024 min
Lab File: VY004702.D
Acq: 04 May 2021 09:45




Instrument :
MSVOA_Y
ClientSampleId :
VY0504SBL01


Tgt Ion: 59 Resp: 1738
Ion Ratio Lower Upper
59 100
57 1.3 8.1 12.1#

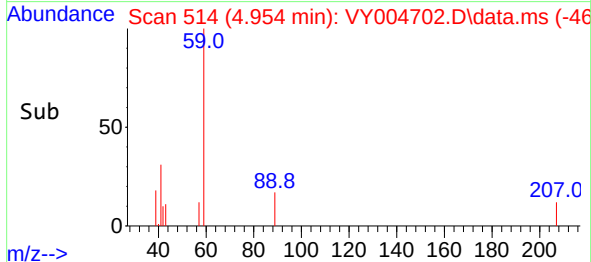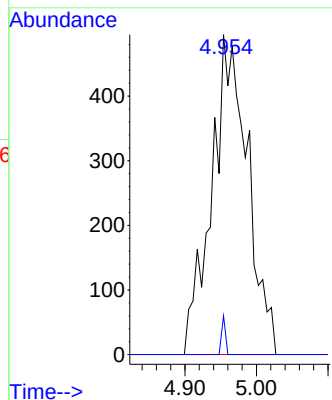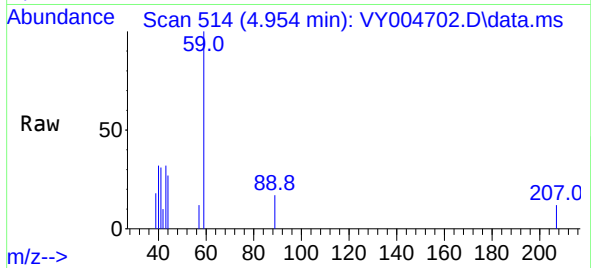

#20
Methylene Chloride
Concen: 6.84 ug/l
RT: 4.716 min Scan# 475
Delta R.T. -0.018 min
Lab File: VY004702.D
Acq: 04 May 2021 09:45

Tgt Ion: 84 Resp: 11450
Ion Ratio Lower Upper
84 100
49 141.1 111.2 166.8
51 44.7 33.4 50.2
86 61.2 52.7 79.1


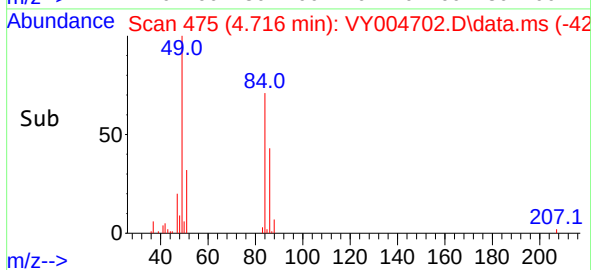
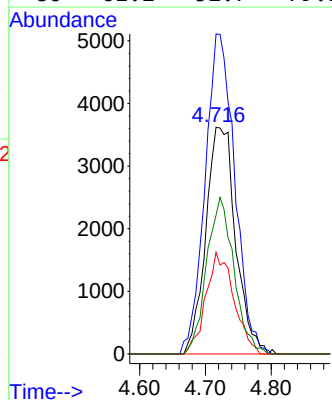
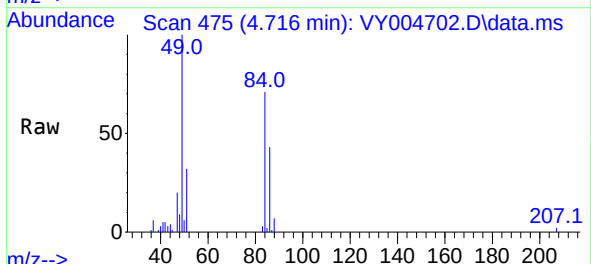




#33
1,2-Dichloroethane-d4
Concen: 60.06 ug/l
RT: 8.148 min Scan# 1038
Delta R.T. -0.006 min
Lab File: VY004702.D
Acq: 04 May 2021 09:45




Instrument :
MSVOA_Y
ClientSampleId :
VY0504SBL01


Tgt Ion: 65 Resp: 104036
Ion Ratio Lower Upper
65 100
67 53.2 0.0 106.4

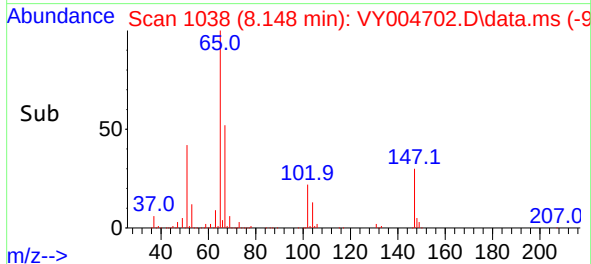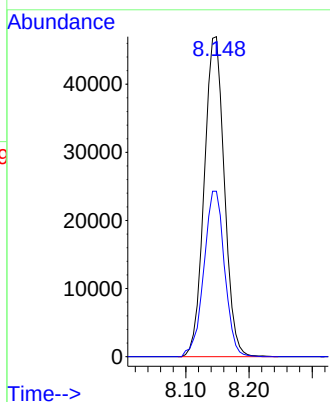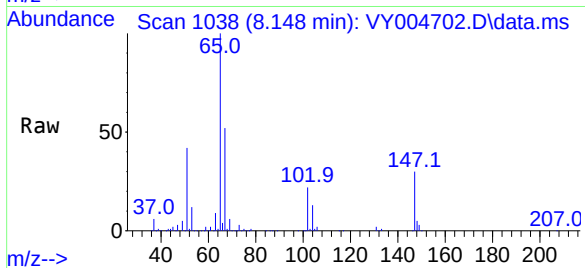

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.691 min Scan# 1127
Delta R.T. -0.006 min
Lab File: VY004702.D
Acq: 04 May 2021 09:45

Tgt Ion: 114 Resp: 276978
Ion Ratio Lower Upper
114 100
63 21.2 0.0 42.4
88 14.5 0.0 30.8


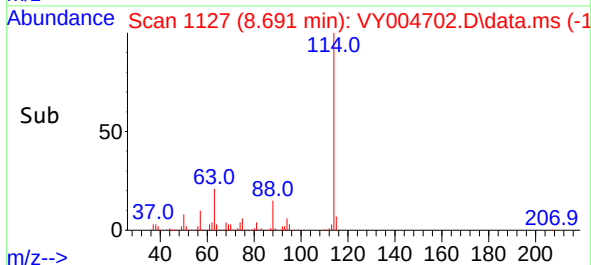
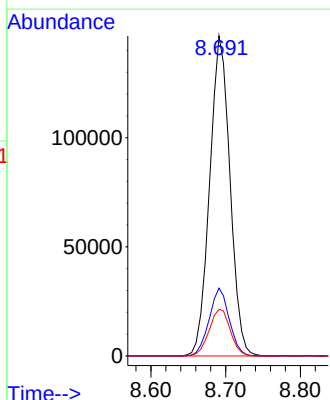
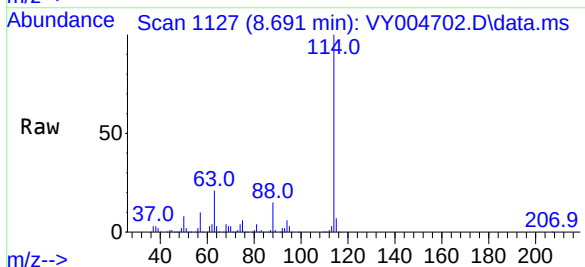


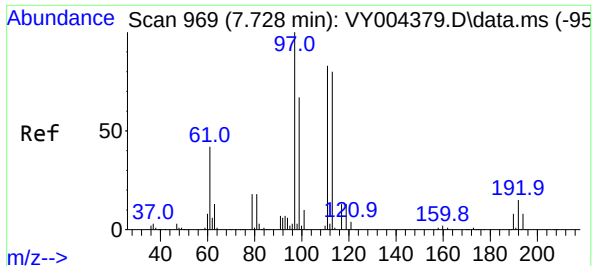

#35
Dibromofluoromethane
Concen: 54.57 ug/l
RT: 7.722 min Scan# 968
Delta R.T. -0.006 min
Lab File: VY004702.D
Acq: 04 May 2021 09:45




Instrument :
MSVOA_Y
ClientSampleId :
VY0504SBL01


Tgt Ion:	113	Resp:	83879
Ion	Ratio	Lower	Upper
113	100		
111	102.3	82.6	123.8
192	19.6	16.1	24.1

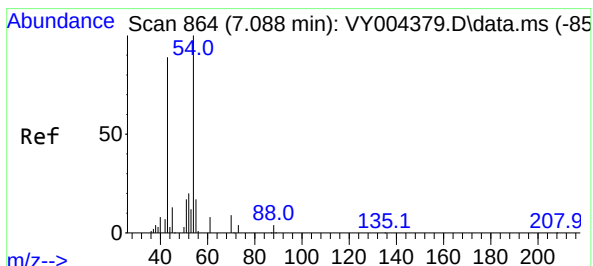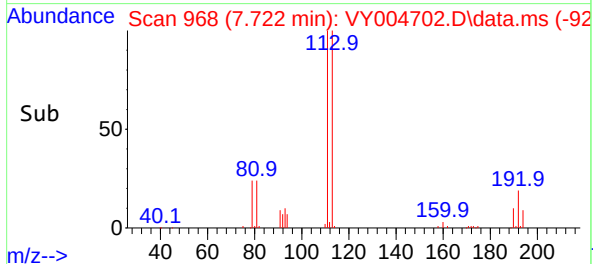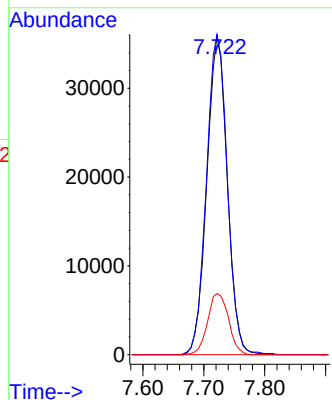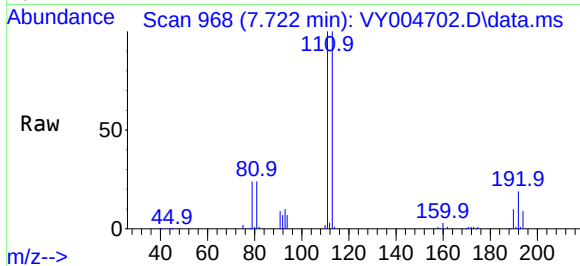

#37
Ethyl Acetate
Concen: 1.16 ug/l
RT: 7.088 min Scan# 864
Delta R.T. 0.000 min
Lab File: VY004702.D
Acq: 04 May 2021 09:45

Tgt Ion:	43	Resp:	2059
Ion	Ratio	Lower	Upper
43	100		
61	4.4	10.4	15.6#
70	3.2	7.5	11.3#


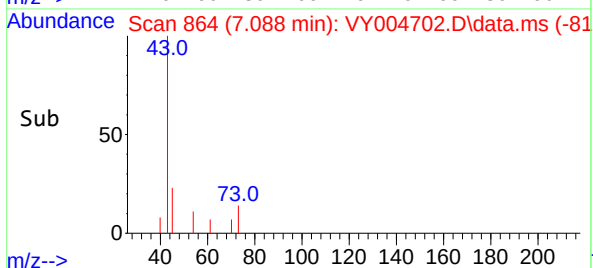
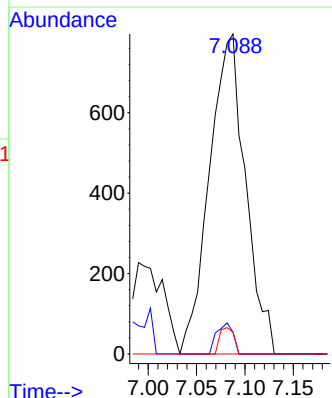
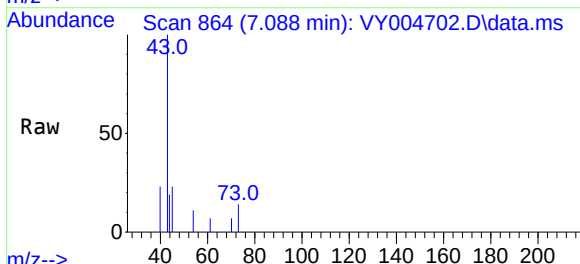




#50
Toluene-d8
Concen: 52.37 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.006 min
Lab File: VY004702.D
Acq: 04 May 2021 09:45




Instrument :
MSVOA_Y
ClientSampleId :
VY0504SBL01


Tgt Ion: 98 Resp: 342411
Ion Ratio Lower Upper
98 100
100 64.9 51.8 77.6

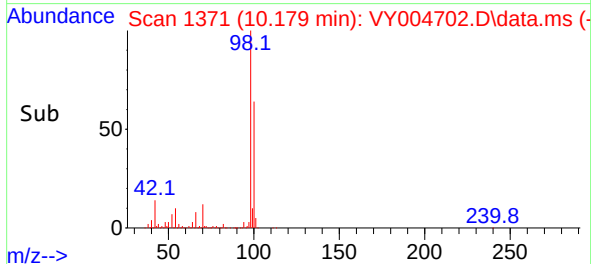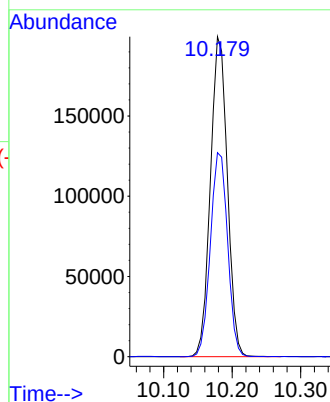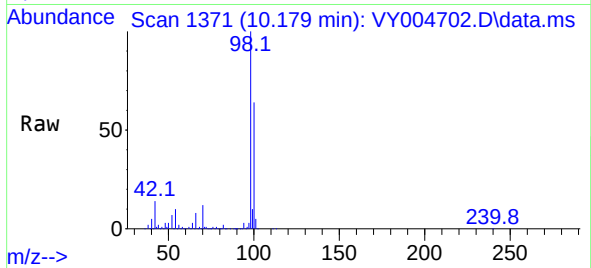

#62
4-Bromofluorobenzene
Concen: 52.27 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY004702.D
Acq: 04 May 2021 09:45

Tgt Ion: 95 Resp: 115965
Ion Ratio Lower Upper
95 100
174 84.8 0.0 162.4
176 80.4 0.0 156.0


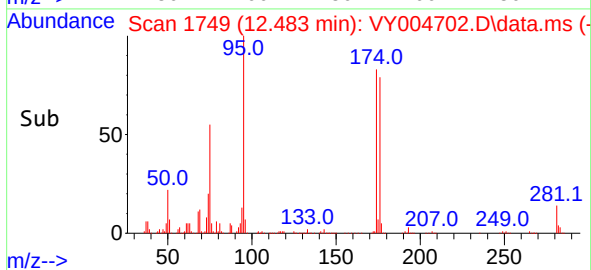
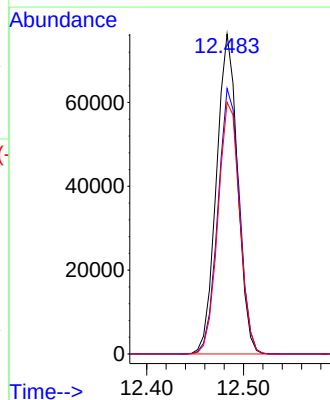
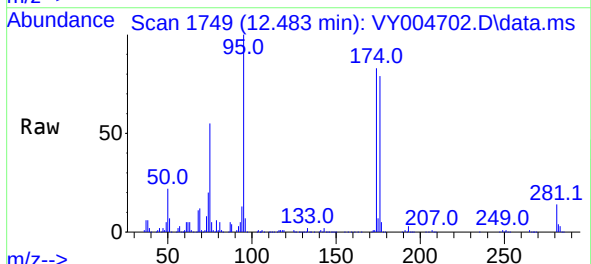




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.489 min Scan# 1586
Delta R.T. -0.006 min
Lab File: VY004702.D
Acq: 04 May 2021 09:45

Instrument :
MSVOA_Y
ClientSampleId :
VY0504SBL01

Tgt Ion:117 Resp: 264263
Ion Ratio Lower Upper
117 100
82 55.2 44.9 67.3
119 33.8 25.4 38.0

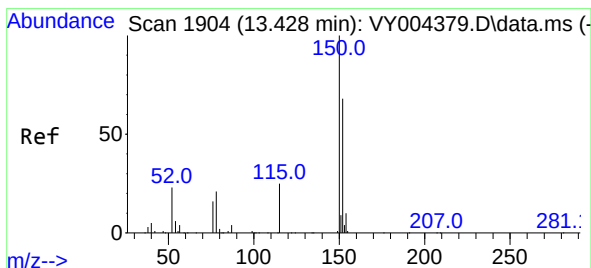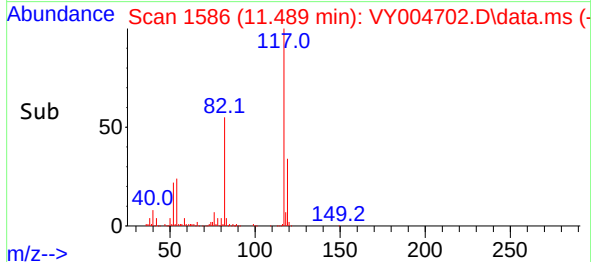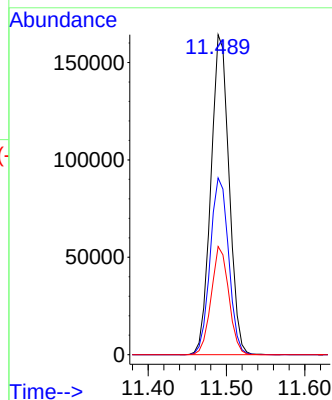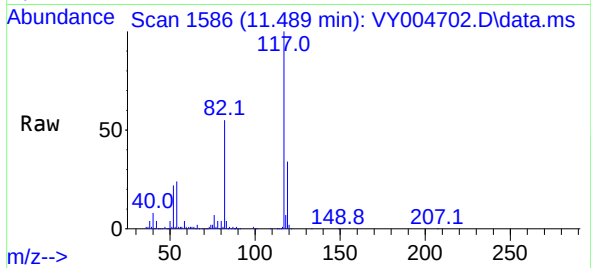

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY004702.D
Acq: 04 May 2021 09:45

Tgt Ion:152 Resp: 121902
Ion Ratio Lower Upper
152 100
115 58.0 29.6 88.8
150 157.3 0.0 348.4

