
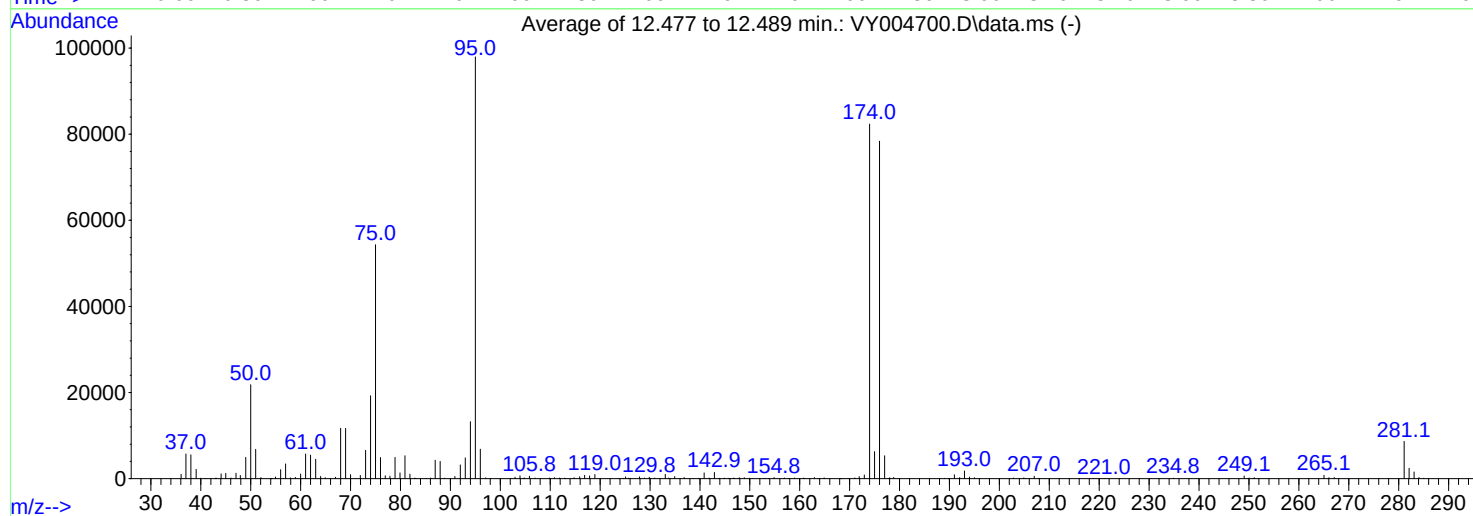


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050421\
Data File : VY004700.D
Acq On : 04 May 2021 08:27
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041221S.M
Title : SW846 8260
Last Update : Tue Apr 13 03:38:02 2021

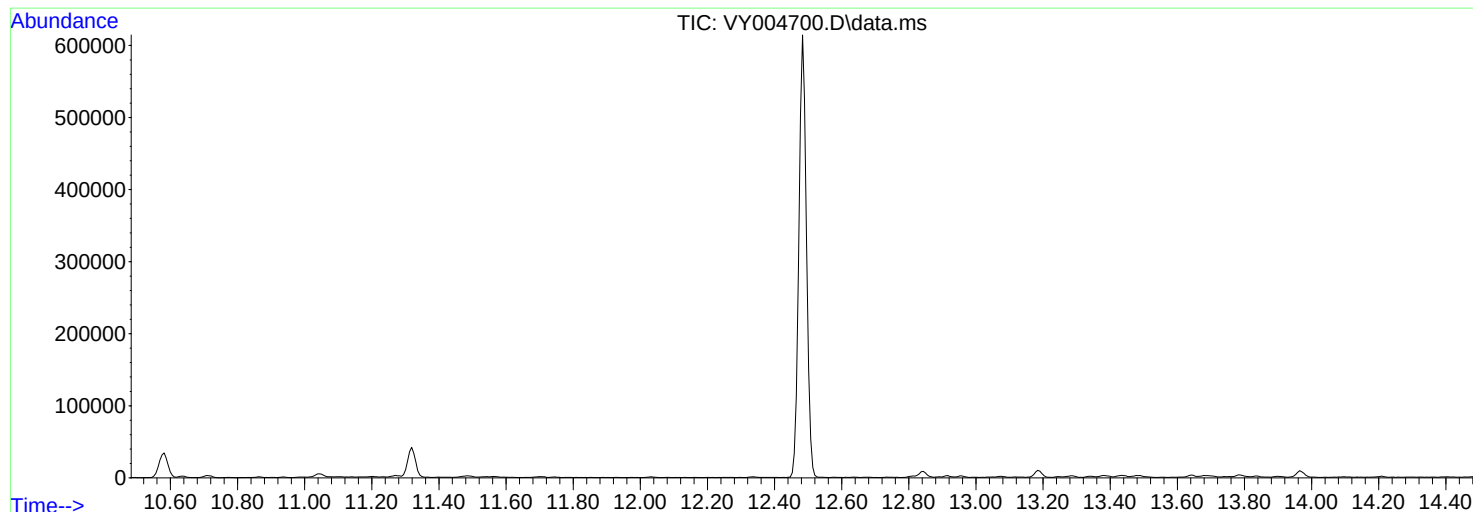

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.3	21816	PASS
75	95	30	60	55.5	54339	PASS
95	95	100	100	100.0	97965	PASS
96	95	5	9	7.0	6848	PASS
173	174	0.00	2	1.0	860	PASS
174	95	50	100	84.1	82347	PASS
175	174	5	9	7.6	6298	PASS
176	174	95	101	95.2	78389	PASS
177	176	5	9	6.8	5334	PASS