

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY050520\  
 Data File : VY002587.D  
 Acq On : 05 May 2020 15:29  
 Operator : SY/MD  
 Sample : L2463-08RE  
 Misc : 4.93G/5ML/MSVOA Y/SOIL  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 NORTH-AOC14-CAR-WASH

Quant Time: May 06 03:20:17 2020  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_Y\METHODS\82Y043020S.M  
 Quant Title : SW846 8260  
 QLast Update : Mon May 04 12:22:08 2020  
 Response via : Initial Calibration

| Internal Standards         | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|----------------------------|-------|------|----------|-------|-------|----------|
| 1) Pentafluorobenzene      | 7.81  | 168  | 339276   | 50.00 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 8.70  | 114  | 533204   | 50.00 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 11.50 | 117  | 455209   | 50.00 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 13.43 | 152  | 182751   | 50.00 | ug/l  | 0.00     |

| System Monitoring Compounds | R.T.  | QIon | Response | Conc  | Units   | Dev(Min) |
|-----------------------------|-------|------|----------|-------|---------|----------|
| 33) 1,2-Dichloroethane-d4   | 8.16  | 65   | 156422   | 54.83 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 109.66% |          |
| 35) Dibromofluoromethane    | 7.73  | 113  | 160208   | 52.54 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 105.08% |          |
| 50) Toluene-d8              | 10.19 | 98   | 619261   | 52.00 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 104.00% |          |
| 62) 4-Bromofluorobenzene    | 12.49 | 95   | 179683   | 44.47 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 88.94%  |          |


| Target Compounds               | R.T.  | QIon | Response | Conc    | Units  | Qvalue |
|--------------------------------|-------|------|----------|---------|--------|--------|
| 2) Dichlorodifluoromethane     | 1.91  | 85   | 95       | 1.817   | ug/l # | 43     |
| 11) Tert butyl alcohol         | 4.96  | 59   | 481      | 1.639   | ug/l # | 74     |
| 13) Acrolein                   | 3.75  | 56   | 215      | 1.059   | ug/l # | 74     |
| 16) Acetone                    | 3.97  | 43   | 72684    | 123.458 | ug/l   | 97     |
| 20) Methylene Chloride         | 4.73  | 84   | 7356     | 2.234   | ug/l   | 95     |
| 25) 2-Butanone                 | 7.00  | 43   | 25901    | 26.876  | ug/l   | 94     |
| 31) Cyclohexane                | 7.80  | 56   | 5877     | 1.146   | ug/l # | 1      |
| 36) 1,1-Dichloropropene        | 7.80  | 75   | 22242    | 4.976   | ug/l # | 49     |
| 37) Ethyl Acetate              | 7.00  | 43   | 25901    | 11.276  | ug/l # | 67     |
| 38) Carbon Tetrachloride       | 7.80  | 117  | 29993    | 6.146   | ug/l # | 16     |
| 76) 1,2,3-Trichloropropane     | 12.49 | 75   | 87447    | 53.845  | ug/l # | 100    |
| 81) trans-1,4-Dichloro-2-buten | 12.49 | 75   | 87447    | 107.970 | ug/l # | 16     |
| 95) Naphthalene                | 15.24 | 128  | 12718    | 1.922   | ug/l # | 95     |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY050520\  
Data File : VY002587.D  
Acq On : 05 May 2020 15:29  
Operator : SY/MD  
Sample : L2463-08RE  
Misc : 4.93G/5ML/MSVOA Y/SOIL  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
NORTH-AOC14-CAR-WASH

Quant Time: May 06 03:20:17 2020  
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_Y\METHODS\82Y043020S.M  
Quant Title : SW846 8260  
QLast Update : Mon May 04 12:22:08 2020  
Response via : Initial Calibration

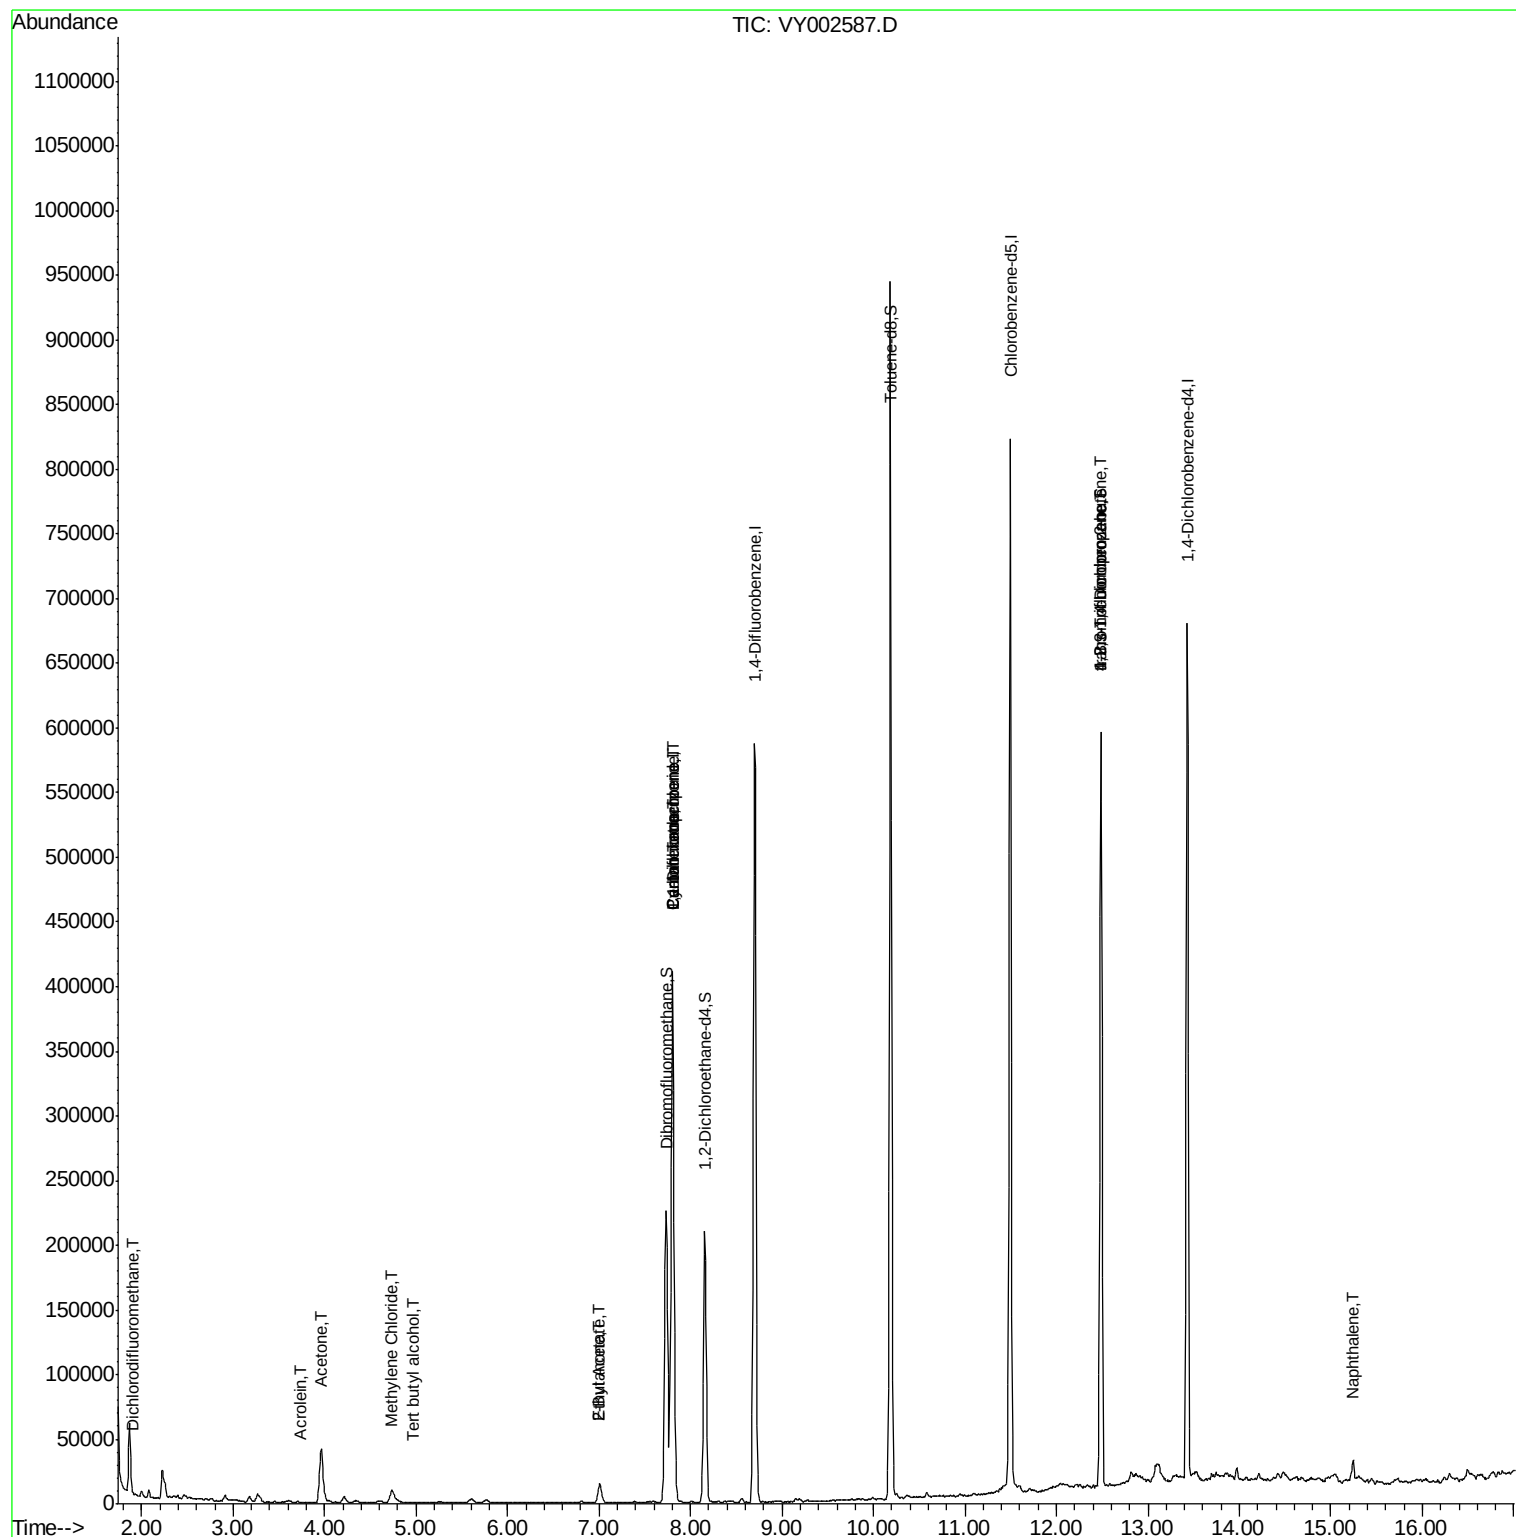

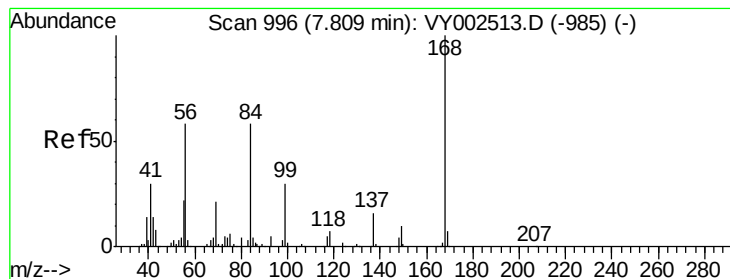

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.81 min Scan# 996

Delta R.T. -0.00 min

Lab File: VY002587.D

Acq: 05 May 2020 15:29

Instrument :

MSVOA\_Y

ClientSampleId :


NORTH-AOC14-CAR-WASH

Tot Ion:168 Resp: 339276

Ion Ratio Lower Upper

168 100

99 48.6 39.2 58.8



Abundance Ion 167.90 (167.60 to 168.60): VY002513.D (-985) (-)

Ion 98.90 (98.60 to 99.60): VY002513.D (-985) (-)

7.81



150000

100000

50000

0

Time-->



#2

Dichlorodifluoromethane

Concen: 1.817 ug/l

RT: 1.91 min Scan# 29

Delta R.T. 0.01 min

Lab File: VY002587.D


Acq: 05 May 2020 15:29

Tgt Ion: 85 Resp: 95

Ion Ratio Lower Upper

85 100

87 0.0 15.8 47.4#



Abundance Ion 84.90 (84.60 to 85.60): VY002513.D (-22) (-)

Ion 86.90 (86.60 to 87.60): VY002513.D (-22) (-)

1.91

120

100

80


60


40

20

0

Time-->



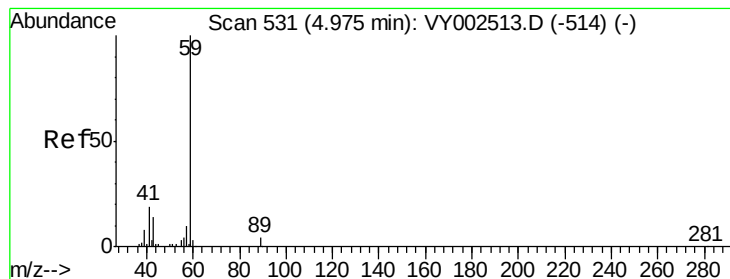

#11

Tert butyl alcohol

Concen: 1.639 ug/l

RT: 4.96 min Scan# 529

Delta R.T. -0.01 min

Lab File: VY002587.D

Acq: 05 May 2020 15:29

Instrument :

MSVOA\_Y

ClientSampleId :


NORTH-AOC14-CAR-WASH

Tot Ion: 59 Resp: 481

Ion Ratio Lower Upper




59 100

57 0.0 7.8 11.6#



Abundance Ion 59.00 (58.70 to 59.70): VY0

Ion 57.00 (56.70 to 57.70): VY0

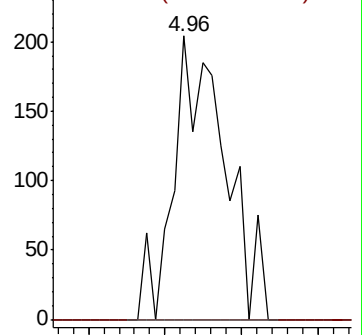

#13

Acrolein

Concen: 1.059 ug/l

RT: 3.75 min Scan# 330

Delta R.T. 0.01 min

Lab File: VY002587.D


Acq: 05 May 2020 15:29

Tgt Ion: 56 Resp: 215

Ion Ratio Lower Upper



56 100


55 46.0 53.8 80.6#



Abundance Ion 56.00 (55.70 to 56.70): VY0

Ion 55.00 (54.70 to 55.70): VY0

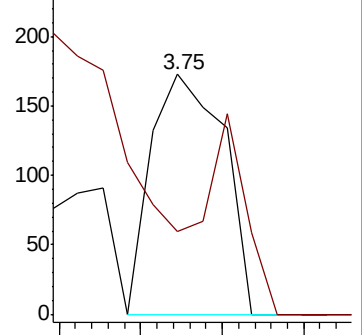



#16

Acetone

Concen: 123.458 ug/l

RT: 3.97 min Scan# 366

Delta R.T. 0.01 min

Lab File: VY002587.D

Acq: 05 May 2020 15:29

Instrument :

MSVOA\_Y

ClientSampleId :





NORTH-AOC14-CAR-WASH

Tot Ion: 43 Resp: 72684

Ion Ratio Lower Upper

43 100

58 32.1 26.9 40.3

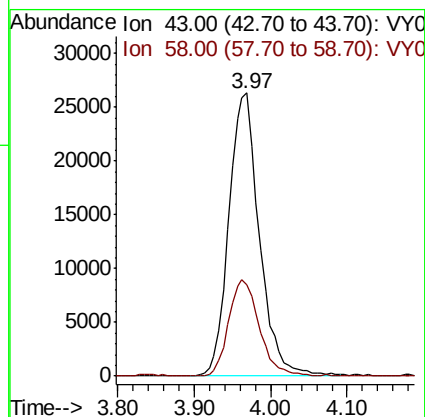

#20

Methylene Chloride

Concen: 2.234 ug/l

RT: 4.73 min Scan# 491

Delta R.T. -0.01 min

Lab File: VY002587.D

Acq: 05 May 2020 15:29

Tgt Ion: 84 Resp: 7356




Ion Ratio Lower Upper


84 100

49 120.8 90.5 135.7

51 36.0 28.3 42.5

86 61.1 49.9 74.9



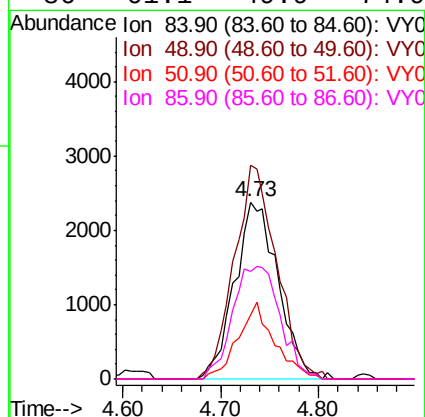





#25  
2-Butanone  
Concen: 26.876 ug/l  
RT: 7.00 min Scan# 864  
Delta R.T. -0.01 min  
Lab File: VY002587.D  
Acq: 05 May 2020 15:29




Instrument :  
MSVOA\_Y  
ClientSampleId :  
NORTH-AOC14-CAR-WASH


Tot Ion: 43 Resp: 25901  
Ion Ratio Lower Upper  
43 100  
72 26.8 24.1 36.1

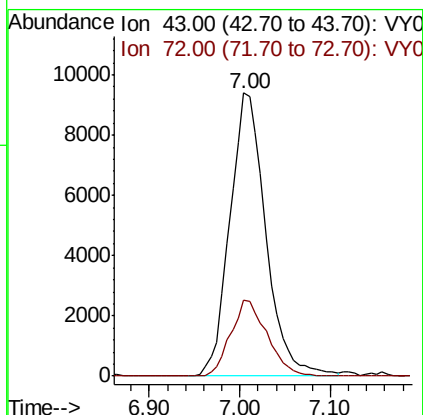

#31  
Cyclohexane  
Concen: 1.146 ug/l  
RT: 7.80 min Scan# 995  
Delta R.T. -0.00 min  
Lab File: VY002587.D  
Acq: 05 May 2020 15:29

Tgt Ion: 56 Resp: 5877  
Ion Ratio Lower Upper  
56 100  
69 158.1 27.6 41.4#  
84 176.4 77.7 116.5#



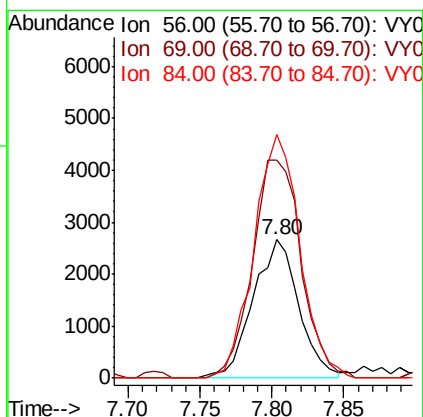





#33  
 1,2-Dichloroethane-d4  
 Concen: 54.833 ug/l  
 RT: 8.16 min Scan# 1053  
 Delta R.T. -0.01 min  
 Lab File: VY002587.D  
 Acq: 05 May 2020 15:29




Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 NORTH-AOC14-CAR-WASH


Tot Ion: 65 Resp: 156422  
 Ion Ratio Lower Upper  
 65 100  
 67 53.9 0.0 107.2

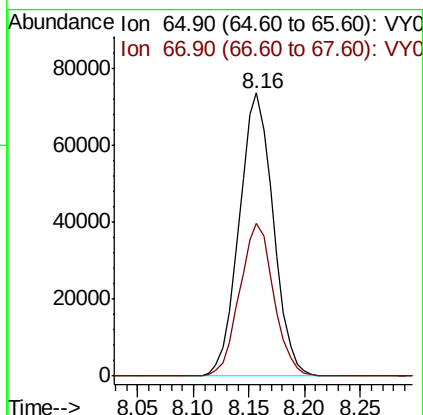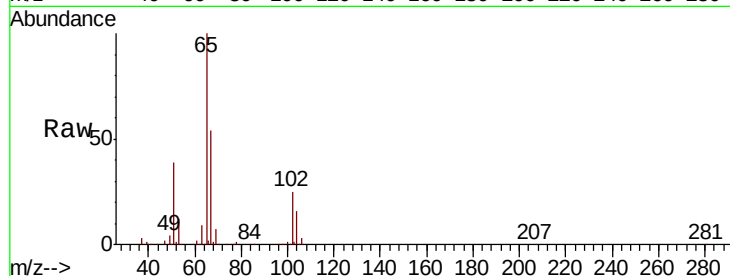

#34  
 1,4-Difluorobenzene  
 Concen: 50.000 ug/l  
 RT: 8.70 min Scan# 1142  
 Delta R.T. -0.01 min  
 Lab File: VY002587.D  
 Acq: 05 May 2020 15:29

Tgt Ion: 114 Resp: 533204  
 Ion Ratio Lower Upper  
 114 100  
 63 19.1 0.0 36.4  
 88 15.2 0.0 29.6

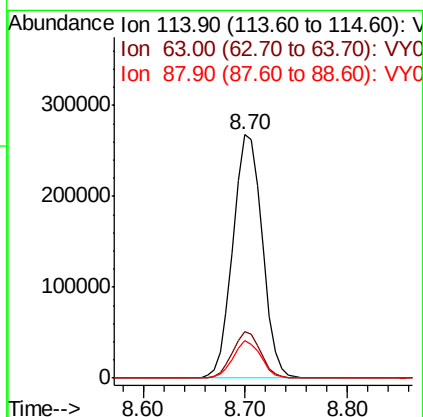

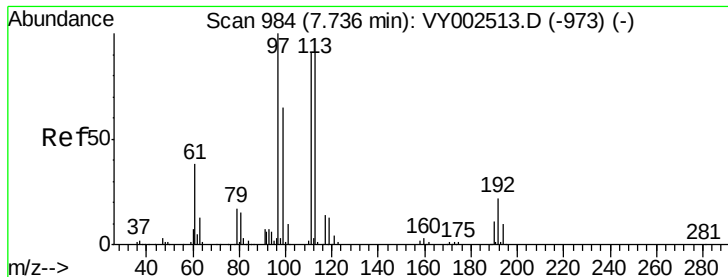

#35

Dibromofluoromethane

Concen: 52.537 ug/l

RT: 7.73 min Scan# 983

Delta R.T. -0.01 min

Lab File: VY002587.D

Acq: 05 May 2020 15:29

Instrument :

MSVOA\_Y

ClientSampleId :

NORTH-AOC14-CAR-WASH


Tot Ion:113 Resp: 160208

Ion Ratio Lower Upper

113 100

111 103.8 81.8 122.6




192 22.8 18.2 27.4

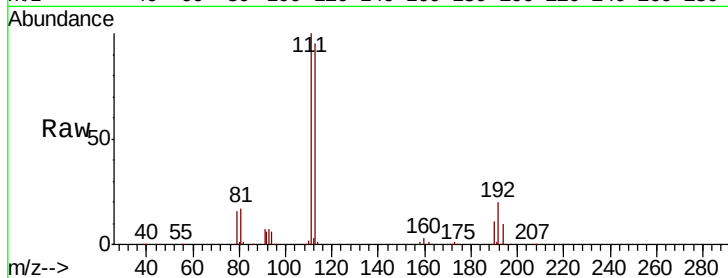

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

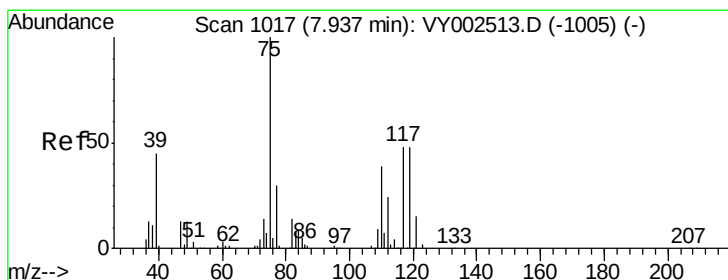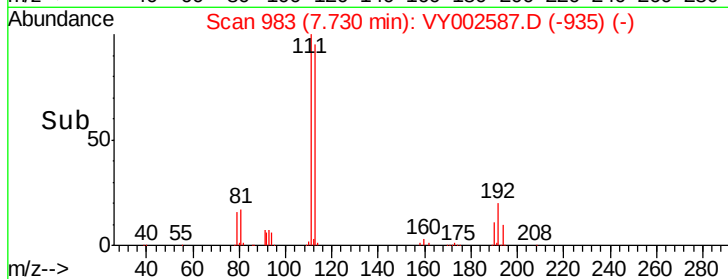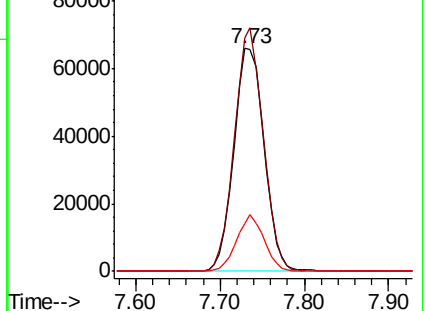

#36

1,1-Dichloropropene

Concen: 4.976 ug/l

RT: 7.80 min Scan# 995

Delta R.T. -0.13 min

Lab File: VY002587.D

Acq: 05 May 2020 15:29


Tgt Ion: 75 Resp: 22242

Ion Ratio Lower Upper

75 100

110 9.4 19.1 57.3#



77 0.0 24.6 37.0#

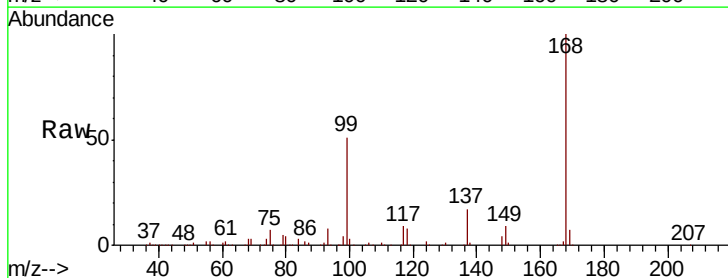


Abundance Ion 74.90 (74.60 to 75.60): VY0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VY0

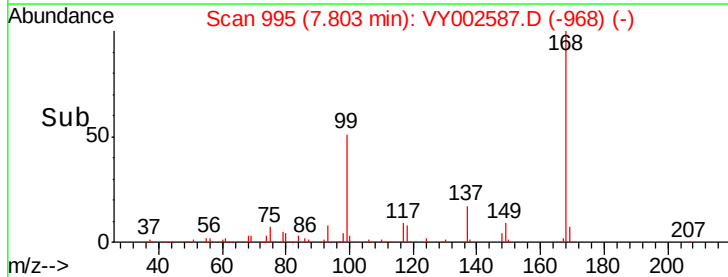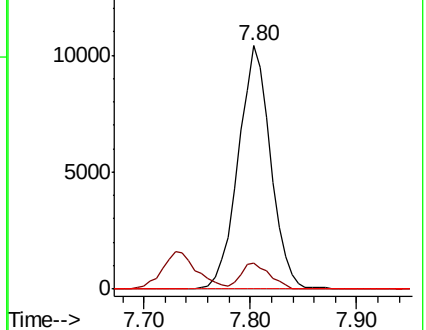









#37  
Ethyl Acetate  
Concen: 11.276 ug/l  
RT: 7.00 min Scan# 864  
Delta R.T. -0.09 min  
Lab File: VY002587.D  
Acq: 05 May 2020 15:29

Instrument :  
MSVOA\_Y  
ClientSampleId :  
NORTH-AOC14-CAR-WASH

Tot Ion: 43 Resp: 25901  
Ion Ratio Lower Upper  
43 100  
61 0.0 11.6 17.4#  
70 0.0 9.0 13.6#

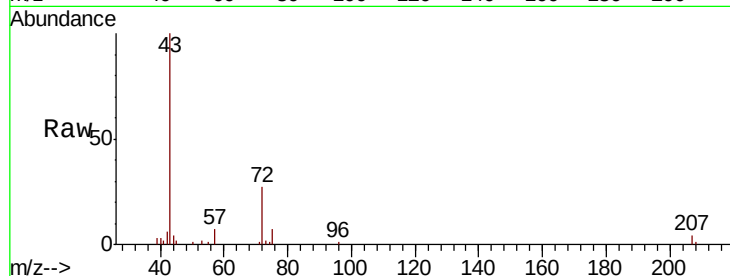


Abundance Ion 43.00 (42.70 to 43.70): VY0  
Ion 60.90 (60.60 to 61.60): VY0  
Ion 70.00 (69.70 to 70.70): VY0


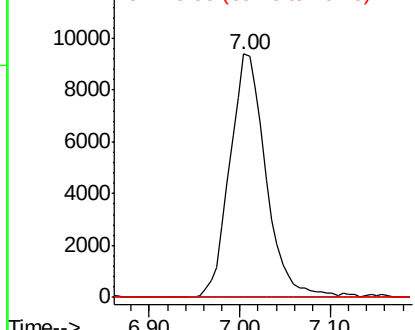



#38  
Carbon Tetrachloride  
Concen: 6.146 ug/l  
RT: 7.80 min Scan# 995  
Delta R.T. -0.12 min  
Lab File: VY002587.D  
Acq: 05 May 2020 15:29

Tgt Ion: 117 Resp: 29993  
Ion Ratio Lower Upper  
117 100  
119 4.9 77.1 115.7#  
121 0.0 25.2 37.8#



Abundance Ion 116.80 (116.50 to 117.50): V  
Ion 118.80 (118.50 to 119.50): V  
Ion 120.80 (120.50 to 121.50): V




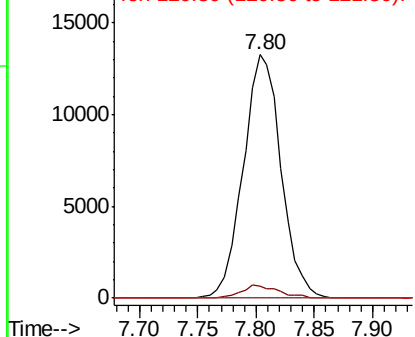




#50  
Toluene-d8  
Concen: 52.002 ug/l  
RT: 10.19 min Scan# 1386  
Delta R.T. -0.01 min  
Lab File: VY002587.D  
Acq: 05 May 2020 15:29




Instrument :  
MSVOA\_Y  
ClientSampleId :  
NORTH-AOC14-CAR-WASH


Tot Ion: 98 Resp: 619261  
Ion Ratio Lower Upper  
98 100  
100 65.5 52.2 78.2

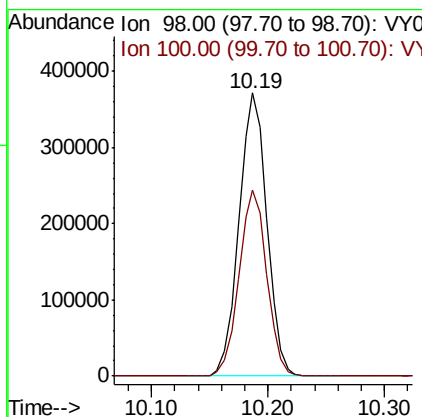

#62  
4-Bromofluorobenzene  
Concen: 44.467 ug/l  
RT: 12.49 min Scan# 1763  
Delta R.T. -0.01 min  
Lab File: VY002587.D  
Acq: 05 May 2020 15:29

Tgt Ion: 95 Resp: 179683  
Ion Ratio Lower Upper  
95 100  
174 92.7 0.0 188.8  
176 90.0 0.0 183.2

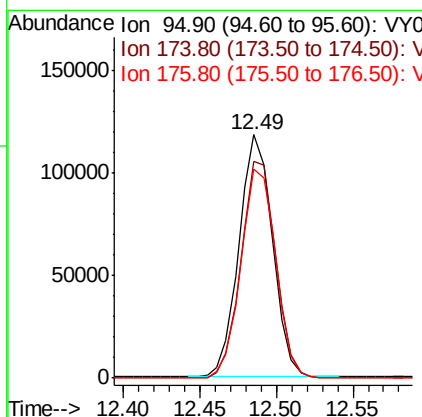




#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.50 min Scan# 1601  
Delta R.T. -0.00 min  
Lab File: VY002587.D  
Acq: 05 May 2020 15:29

Instrument :  
MSVOA\_Y  
ClientSampleId :  
NORTH-AOC14-CAR-WASH

| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 117     | 100   |       |       |
| 82      | 51.7  | 41.3  | 61.9  |
| 119     | 33.2  | 26.0  | 39.0  |



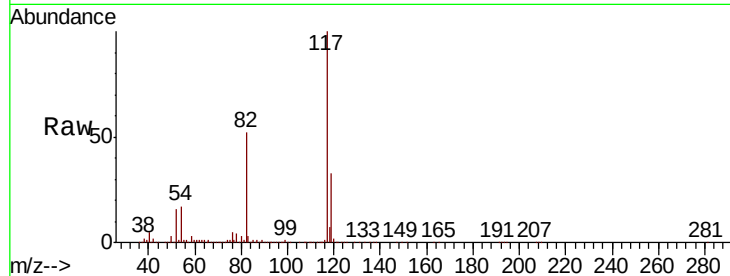


Abundance

Ion 116.90 (116.60 to 117.60): V


Ion 82.00 (81.70 to 82.70): VY0

Ion 118.90 (118.60 to 119.60): V

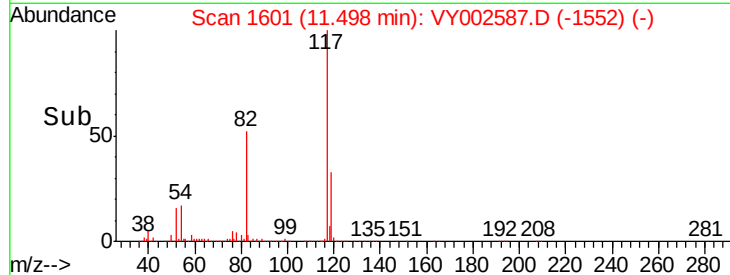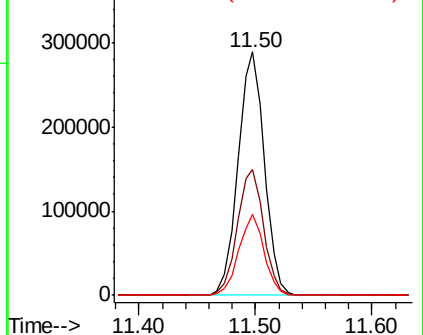

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 13.43 min Scan# 1918  
Delta R.T. -0.01 min  
Lab File: VY002587.D  
Acq: 05 May 2020 15:29

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 152     | 100   |       |       |
| 115     | 53.9  | 27.5  | 82.4  |
| 150     | 155.3 | 0.0   | 346.4 |


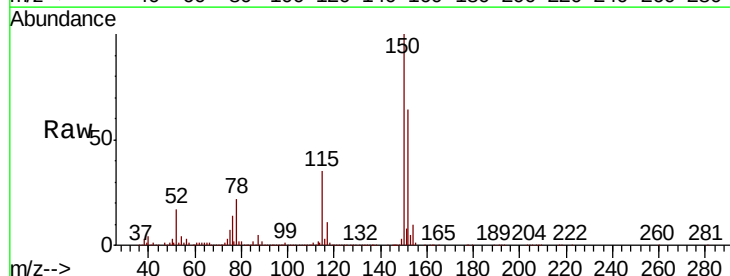



Abundance

Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

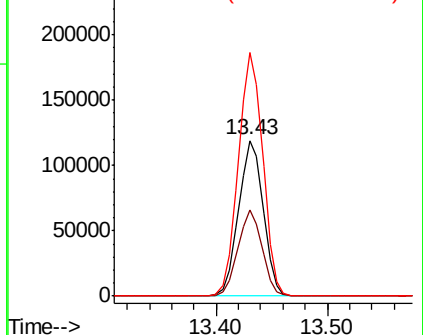

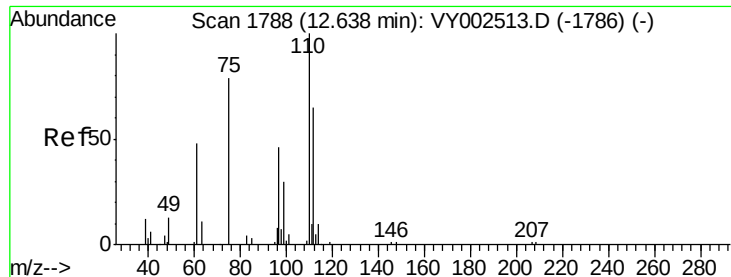

#76

1,2,3-Trichloropropane

Concen: 53.845 ug/l

RT: 12.49 min Scan# 1763

Delta R.T. -0.15 min

Lab File: VY002587.D

Acq: 05 May 2020 15:29

Instrument :

MSVOA\_Y

ClientSampleId :


NORTH-AOC14-CAR-WASH

Tot Ion: 75 Resp: 87447

Ion Ratio Lower Upper




75 100

77 1.6 0.0 0.0#

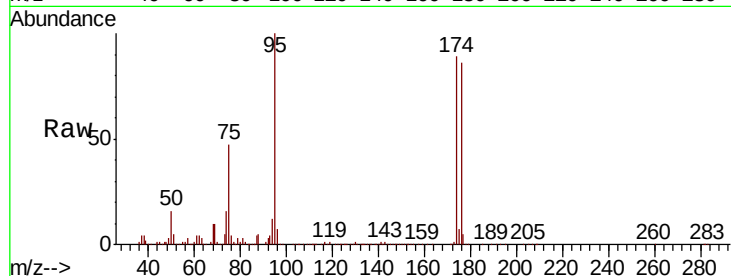

Abundance Ion 74.90 (74.60 to 75.60): VY0

Ion 77.00 (76.70 to 77.70): VY0

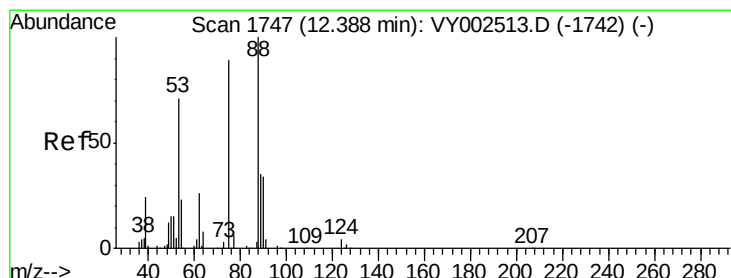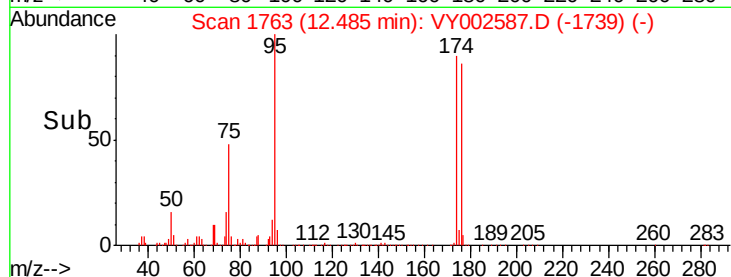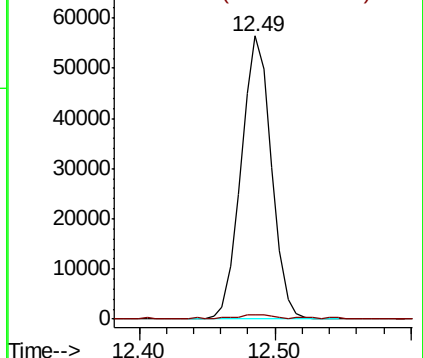

#81

trans-1,4-Dichloro-2-butene

Concen: 107.970 ug/l

RT: 12.49 min Scan# 1763

Delta R.T. 0.10 min

Lab File: VY002587.D

Acq: 05 May 2020 15:29


Tgt Ion: 75 Resp: 87447

Ion Ratio Lower Upper

75 100

53 0.3 67.4 101.0#



89 0.0 37.4 56.0#

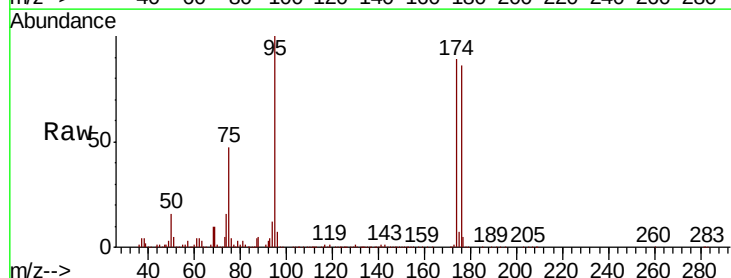


Abundance Ion 74.90 (74.60 to 75.60): VY0

Ion 53.00 (52.70 to 53.70): VY0

Ion 88.90 (88.60 to 89.60): VY0

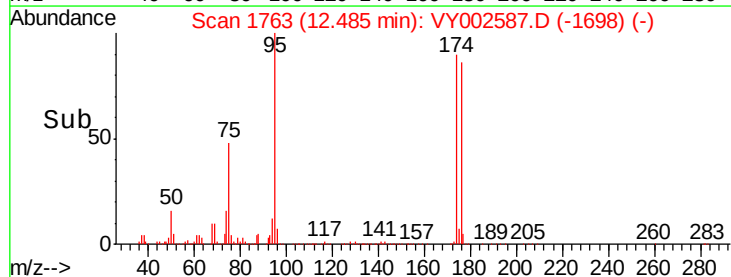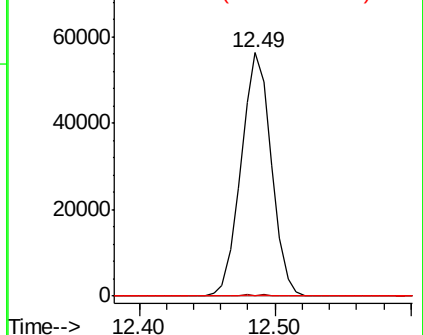


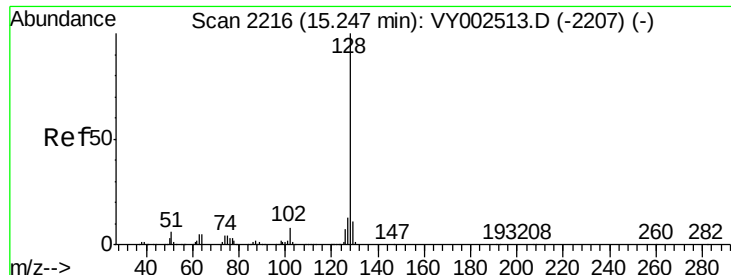

#95  
Naphthalene  
Concen: 1.922 ug/l  
RT: 15.24 min Scan# 2215  
Delta R.T. -0.01 min  
Lab File: VY002587.D  
Acq: 05 May 2020 15:29

Instrument :  
MSVOA\_Y  
ClientSampleId :  
NORTH-AOC14-CAR-WASH

| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 128     | 100   |       |       |
| 127     | 16.6  | 10.5  | 15.7# |
| 129     | 11.1  | 8.8   | 13.2  |

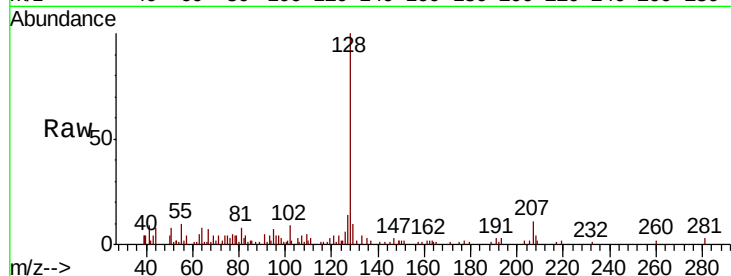

Abundance

Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

