


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY050820\
 Data File : VY002632.D
 Acq On : 08 May 2020 10:03
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y043020S.M
 Title : SW846 8260
 Last Update : Mon May 04 12:22:08 2020

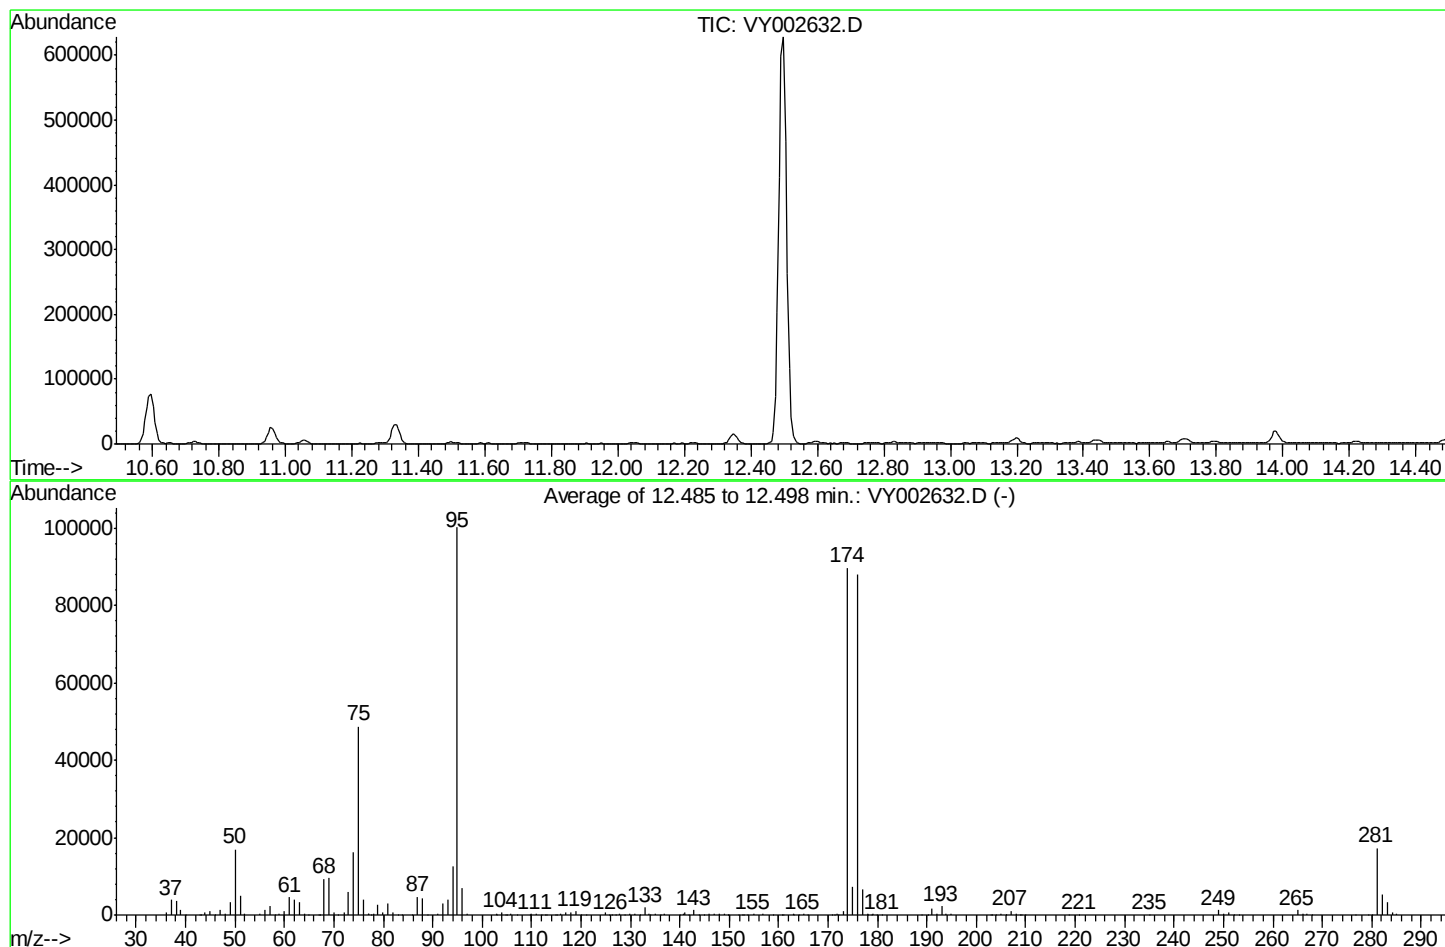

AutoFind: Scans 1763, 1764, 1765; Background Corrected with Scan 1754

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	16907	PASS
75	95	30	60	48.6	48632	PASS
95	95	100	100	100.0	100157	PASS
96	95	5	9	7.0	7013	PASS
173	174	0.00	2	1.1	970	PASS
174	95	50	100	89.6	89757	PASS
175	174	5	9	7.9	7131	PASS
176	174	95	101	97.9	87914	PASS
177	176	5	9	7.4	6498	PASS