

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050824\
 Data File : VY018185.D
 Acq On : 08 May 2024 13:55
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VIBLK

Quant Time: May 09 02:25:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y050724S.M
 Quant Title : SW846 8260
 QLast Update : Wed May 08 01:40:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.783	168	196599	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	356296	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	319277	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	125034	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.137	65	87180	60.277	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	120.560%
35) Dibromofluoromethane	7.710	113	102551	54.767	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	109.540%
50) Toluene-d8	10.179	98	401877	54.464	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	108.920%
62) 4-Bromofluorobenzene	12.477	95	123506	51.830	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	103.660%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050824\
Data File : VY018185.D
Acq On : 08 May 2024 13:55
Operator : SY/MD
Sample : VIBLK
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VIBLK


Quant Time: May 09 02:25:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y050724S.M
Quant Title : SW846 8260
QLast Update : Wed May 08 01:40:14 2024
Response via : Initial Calibration

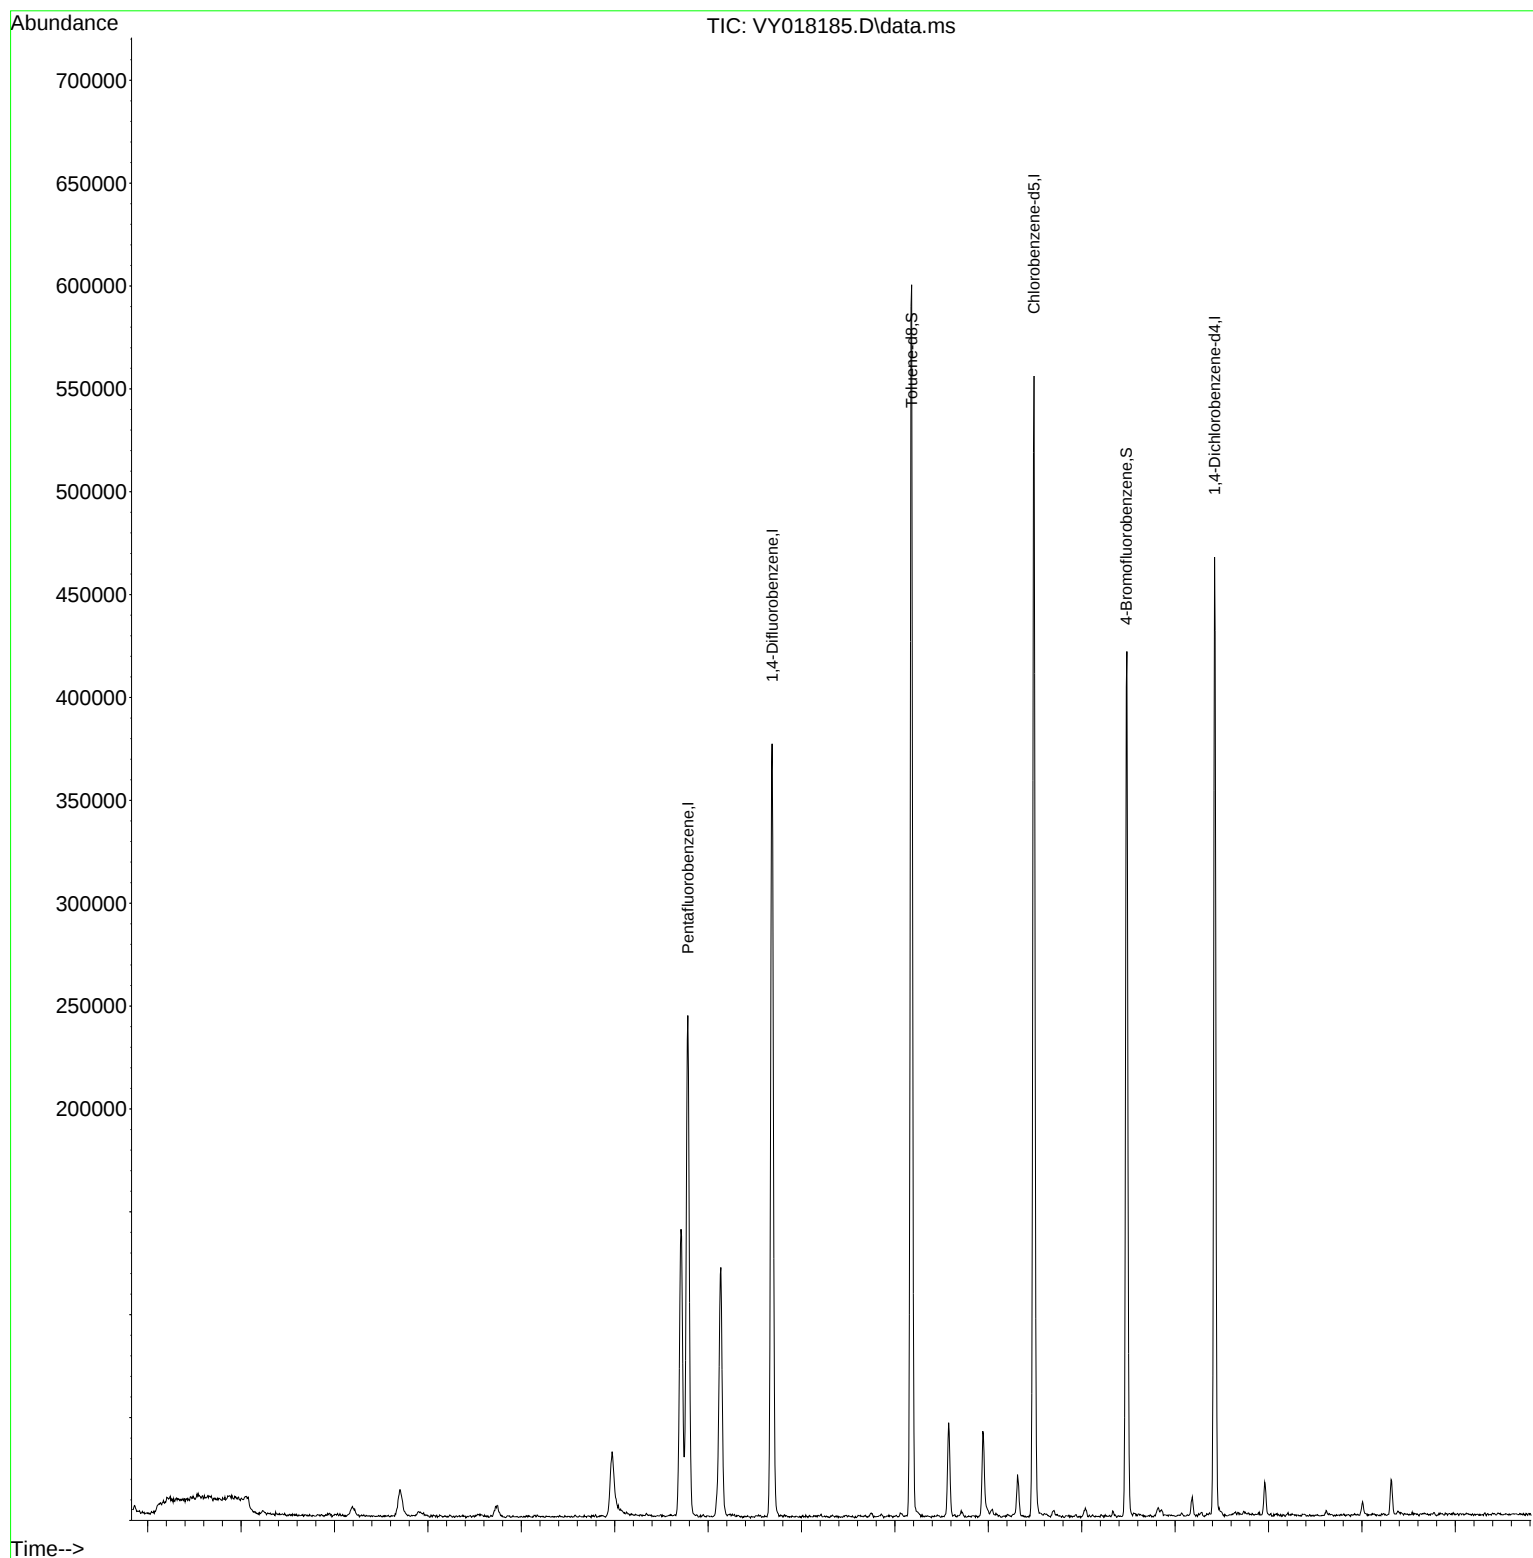



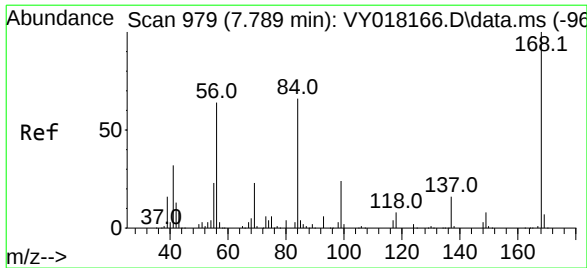


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 979
Delta R.T. -0.006 min
Lab File: VY018185.D
Acq: 08 May 2024 13:55

Instrument :
MSVOA_Y
ClientSampleId :
VIBLK



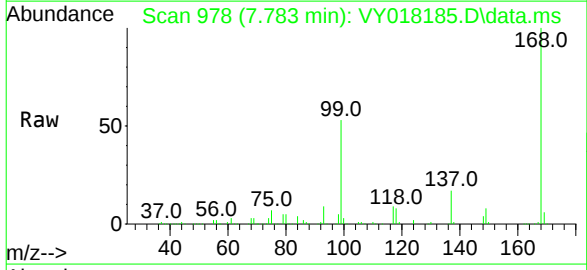



Tgt Ion:168 Resp: 196599
Ion Ratio Lower Upper
168 100
99 52.5 39.1 58.7

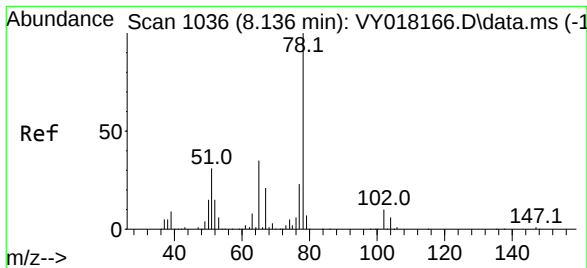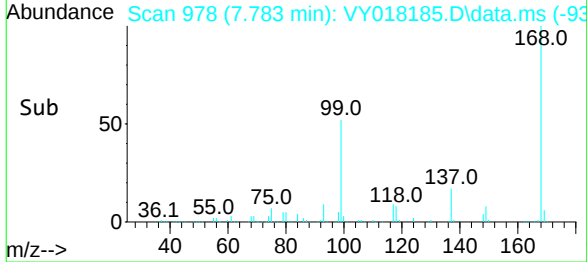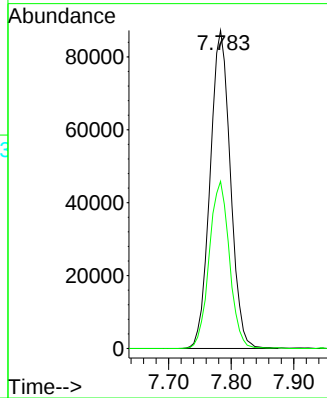

#33
1,2-Dichloroethane-d4
Concen: 60.277 ug/l
RT: 8.137 min Scan# 1036
Delta R.T. 0.000 min
Lab File: VY018185.D
Acq: 08 May 2024 13:55

Tgt Ion: 65 Resp: 87180
Ion Ratio Lower Upper
65 100
67 54.7 0.0 109.6


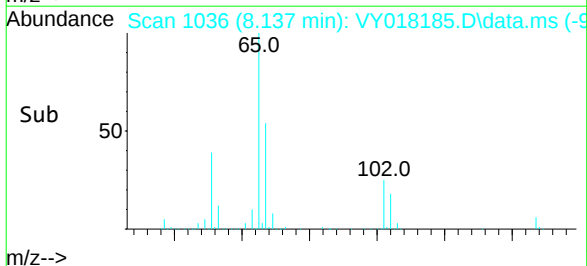
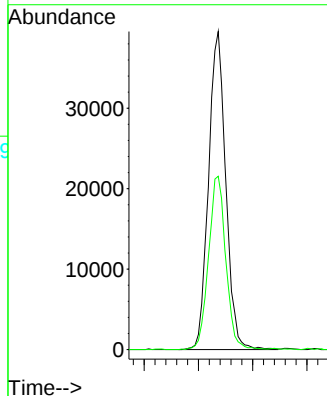
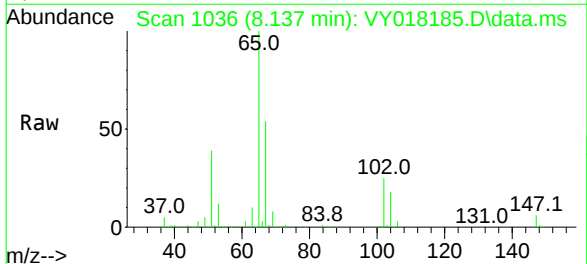


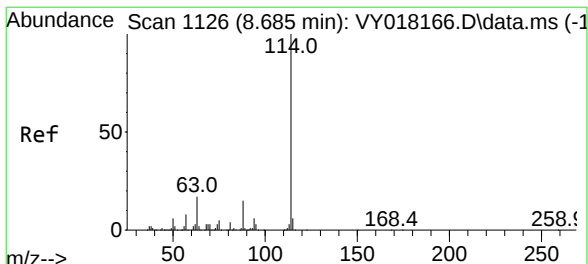

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.685 min Scan# 111
 Delta R.T. 0.000 min
 Lab File: VY018185.D
 Acq: 08 May 2024 13:55




Instrument :
 MSVOA_Y
 ClientSampleId :
 VIBLK


Tgt Ion:	114	Resp:	356296
Ion Ratio	Lower	Upper	
114	100		
63	17.2	0.0	35.0
88	15.0	0.0	27.2

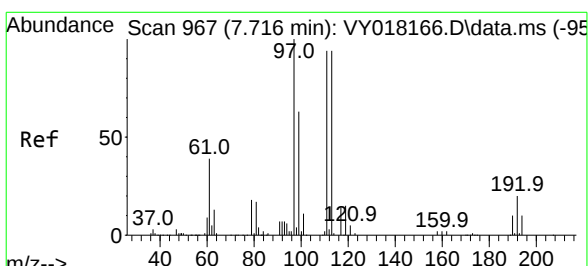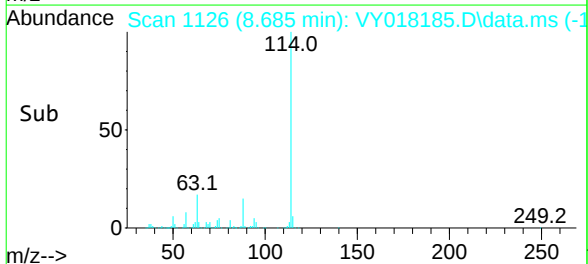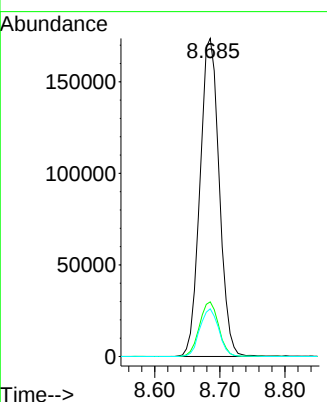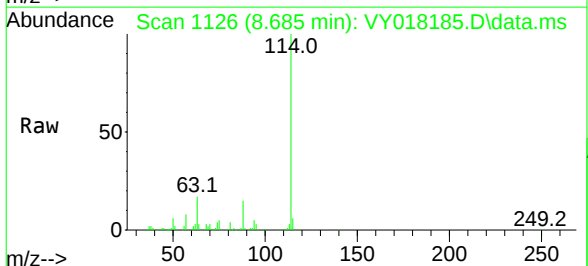

#35
 Dibromofluoromethane
 Concen: 54.767 ug/l
 RT: 7.710 min Scan# 966
 Delta R.T. -0.006 min
 Lab File: VY018185.D
 Acq: 08 May 2024 13:55

Tgt Ion:	113	Resp:	102551
Ion Ratio	Lower	Upper	
113	100		
111	102.2	82.2	123.4
192	20.1	15.9	23.9

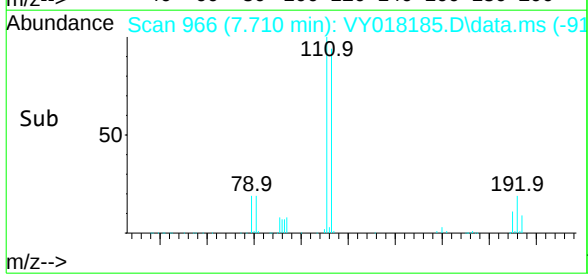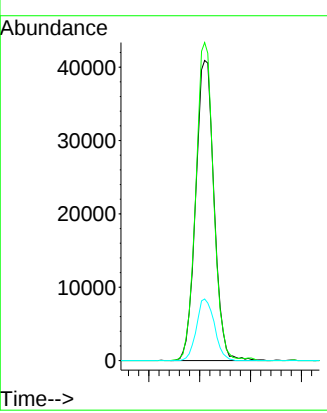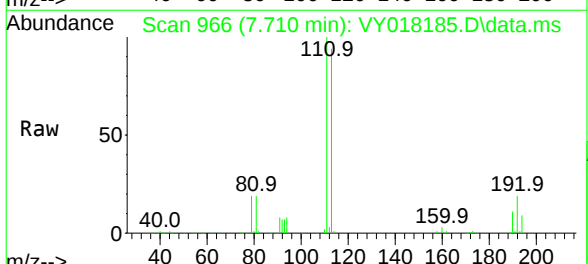

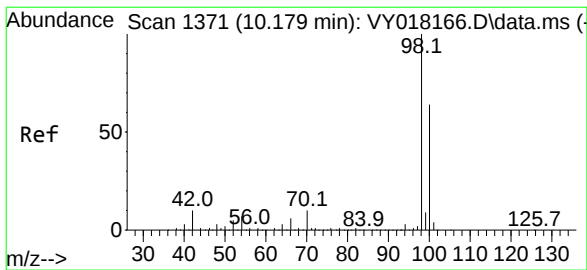

#50

Toluene-d8

Concen: 54.464 ug/l

RT: 10.179 min Scan# 1371

Delta R.T. 0.000 min

Lab File: VY018185.D

Acq: 08 May 2024 13:55

Instrument :

MSVOA_Y

ClientSampleId :





VIBLK

Tgt Ion: 98 Resp: 401877

Ion Ratio Lower Upper

98 100

100 66.3 52.0 78.0

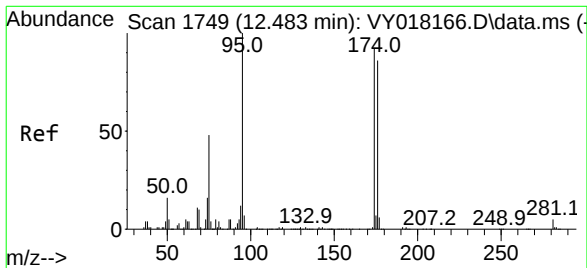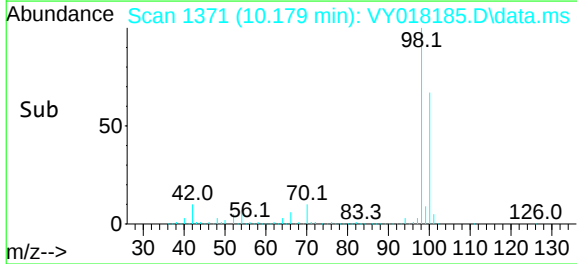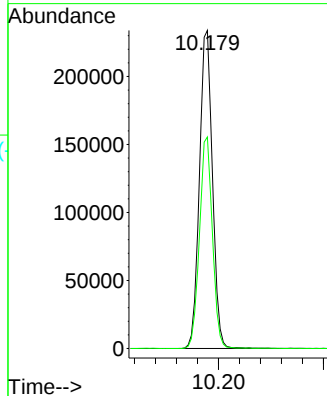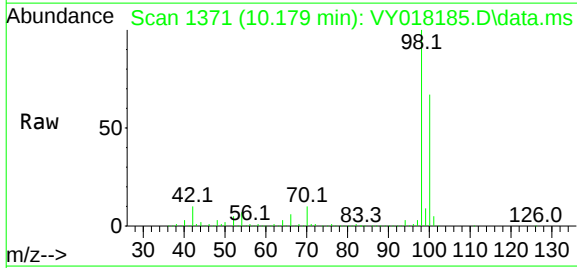

#62

4-Bromofluorobenzene

Concen: 51.830 ug/l

RT: 12.477 min Scan# 1748

Delta R.T. -0.006 min

Lab File: VY018185.D

Acq: 08 May 2024 13:55




Tgt Ion: 95 Resp: 123506


Ion Ratio Lower Upper

95 100

174 86.3 0.0 175.6

176 83.0 0.0 171.4

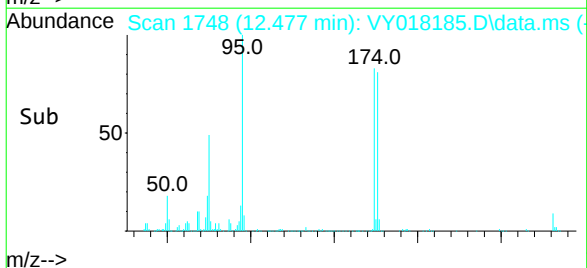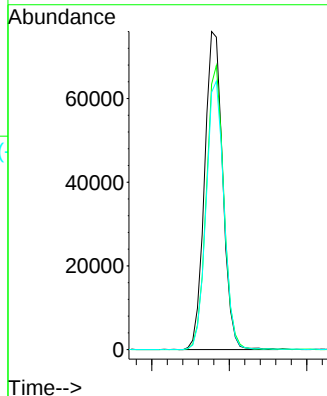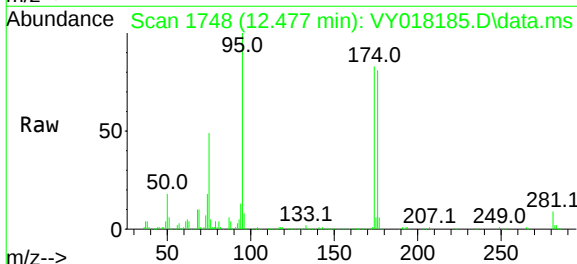

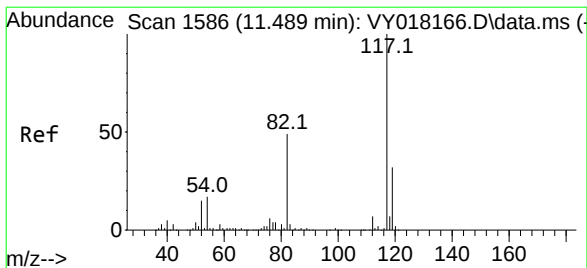

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.490 min Scan# 15

Delta R.T. 0.000 min

Lab File: VY018185.D

Acq: 08 May 2024 13:55

Instrument :

MSVOA_Y

ClientSampleId :

VIBLK





Tgt Ion:117 Resp: 319277

Ion Ratio Lower Upper

117 100

82 48.7 42.4 63.6

119 32.3 25.9 38.9

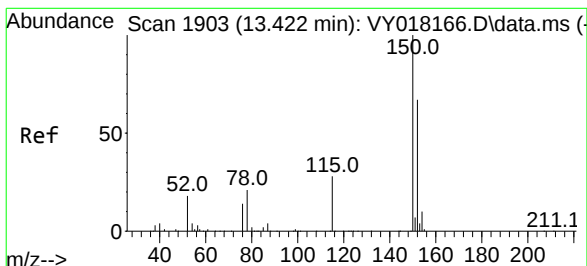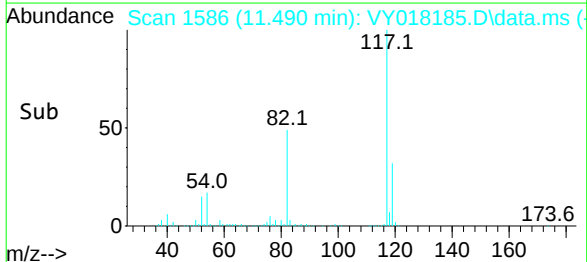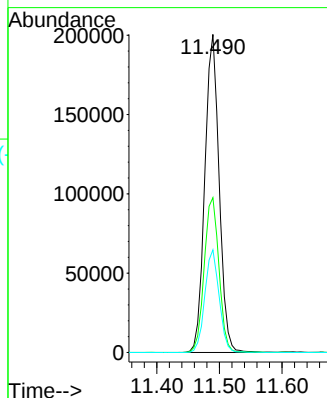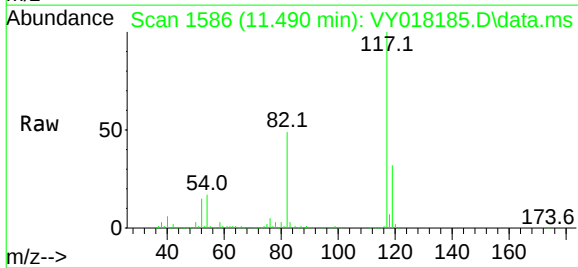

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.422 min Scan# 1903

Delta R.T. 0.000 min

Lab File: VY018185.D

Acq: 08 May 2024 13:55

Tgt Ion:152 Resp: 125034

Ion Ratio Lower Upper

152 100

115 56.5 28.2 84.7

150 155.6 0.0 345.6

