

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050924\
 Data File : VY018207.D
 Acq On : 09 May 2024 13:20
 Operator : SY/MD
 Sample : P2423-07
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 WC-HH-VOC

Quant Time: May 10 01:17:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y050724S.M
 Quant Title : SW846 8260
 QLast Update : Wed May 08 01:40:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.783	168	185681	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	350793	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	316913	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	122270	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.137	65	91109	66.698	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	133.400%
35) Dibromofluoromethane	7.710	113	105489	57.220	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	114.440%
50) Toluene-d8	10.179	98	395569	54.450	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	108.900%
62) 4-Bromofluorobenzene	12.483	95	124007	52.856	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	105.720%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050924\
Data File : VY018207.D
Acq On : 09 May 2024 13:20
Operator : SY/MD
Sample : P2423-07
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
WC-HH-VOC

Quant Time: May 10 01:17:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y050724S.M
Quant Title : SW846 8260
QLast Update : Wed May 08 01:40:14 2024
Response via : Initial Calibration




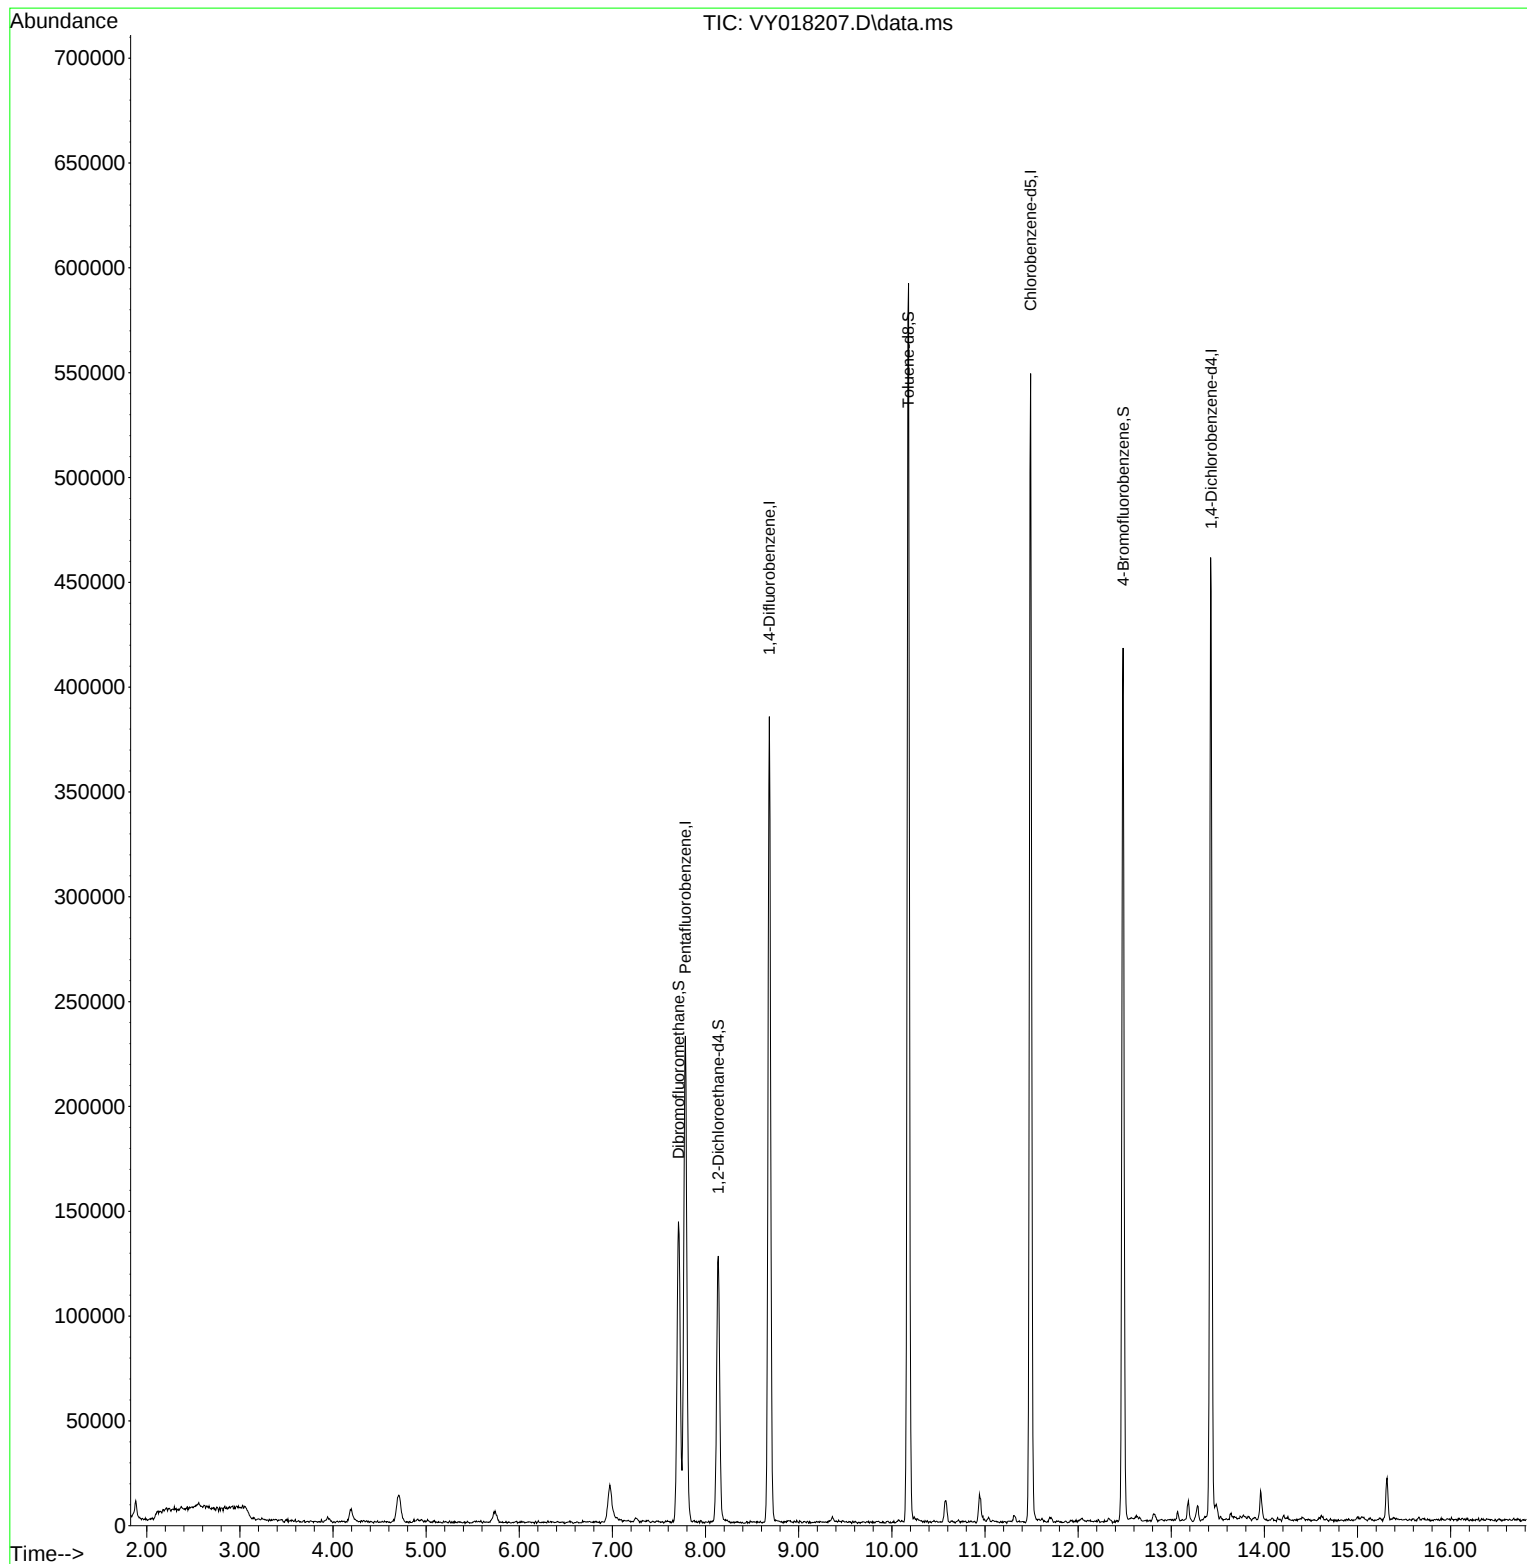


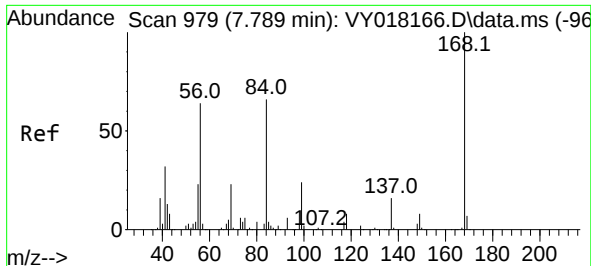

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY018207.D
Acq: 09 May 2024 13:20




Instrument :
MSVOA_Y
ClientSampleId :
WC-HH-VOC


Tgt Ion:168 Resp: 185681
Ion Ratio Lower Upper
168 100
99 51.2 39.1 58.7

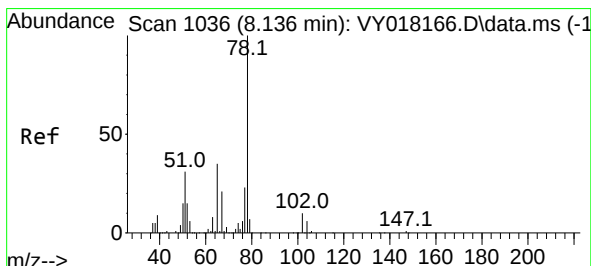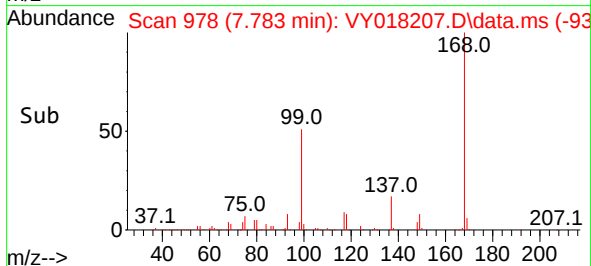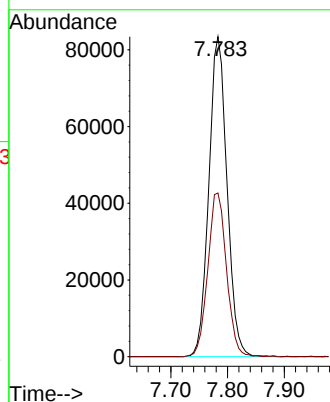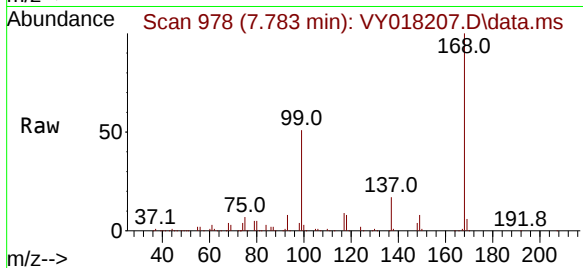

#33
1,2-Dichloroethane-d4
Concen: 66.698 ug/l
RT: 8.137 min Scan# 1036
Delta R.T. 0.000 min
Lab File: VY018207.D
Acq: 09 May 2024 13:20

Tgt Ion: 65 Resp: 91109
Ion Ratio Lower Upper
65 100
67 56.4 0.0 109.6

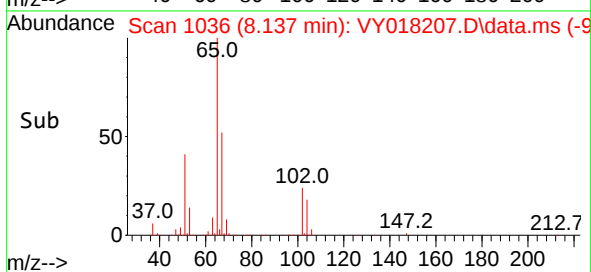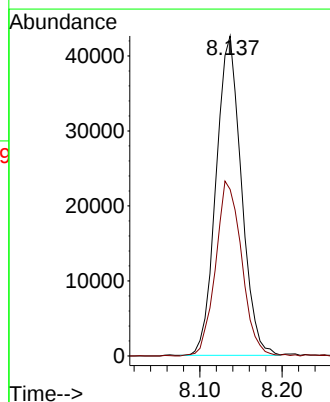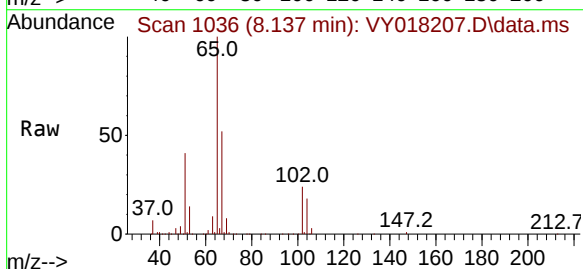

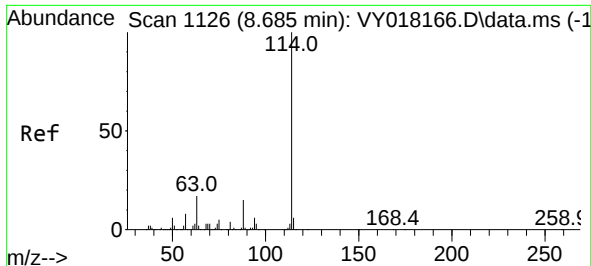

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. 0.000 min

Lab File: VY018207.D

Acq: 09 May 2024 13:20

Instrument :

MSVOA_Y

ClientSampleId :

WC-HH-VOC





Tgt Ion:114 Resp: 350793

Ion Ratio Lower Upper

114 100

63 17.1 0.0 35.0

88 14.0 0.0 27.2

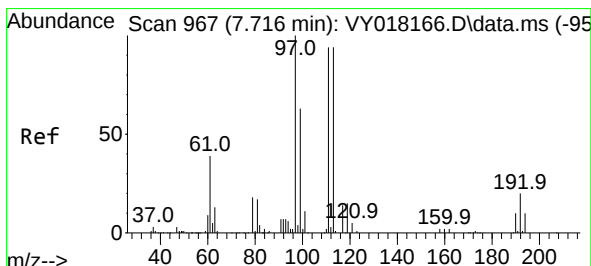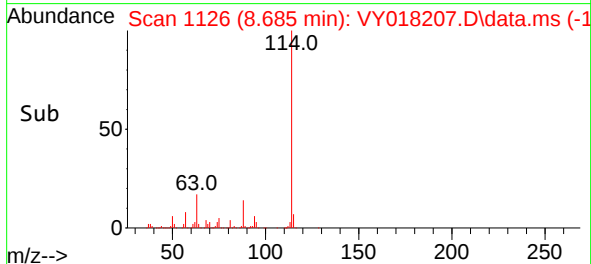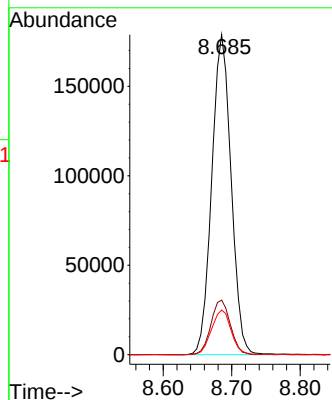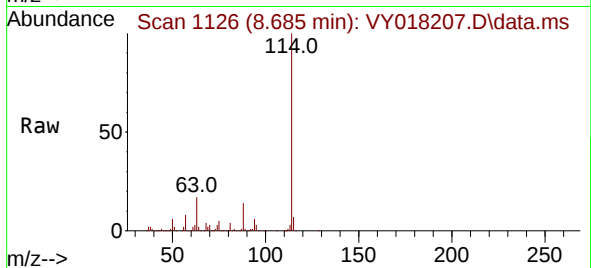

#35

Dibromofluoromethane

Concen: 57.220 ug/l

RT: 7.710 min Scan# 966

Delta R.T. -0.006 min

Lab File: VY018207.D

Acq: 09 May 2024 13:20




Tgt Ion:113 Resp: 105489


Ion Ratio Lower Upper

113 100

111 101.2 82.2 123.4

192 19.4 15.9 23.9


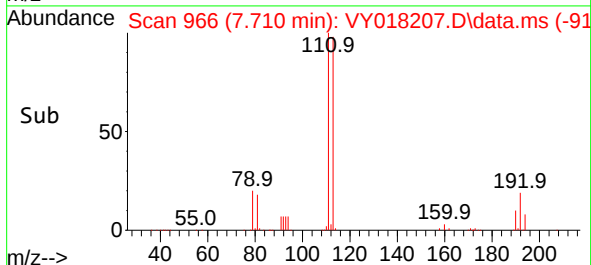
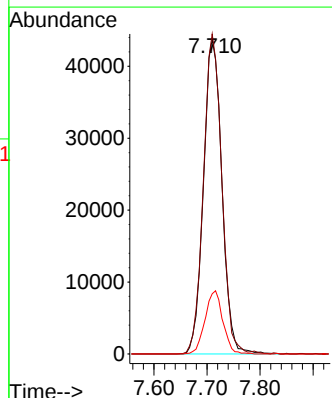
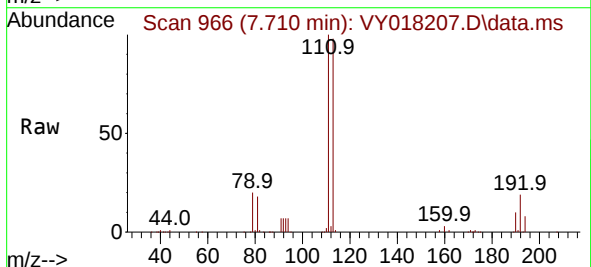


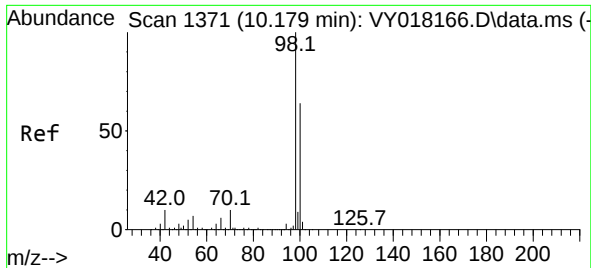

#50
Toluene-d8
Concen: 54.450 ug/l
RT: 10.179 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY018207.D
Acq: 09 May 2024 13:20




Instrument :
MSVOA_Y
ClientSampleId :
WC-HH-VOC


Tgt Ion: 98 Resp: 395569
Ion Ratio Lower Upper
98 100
100 66.6 52.0 78.0

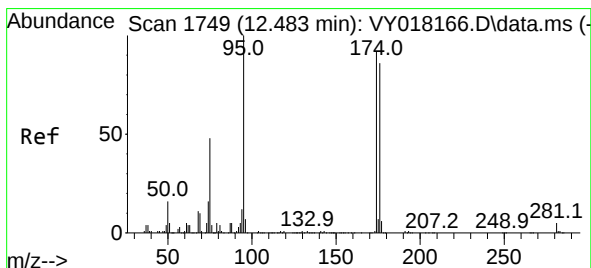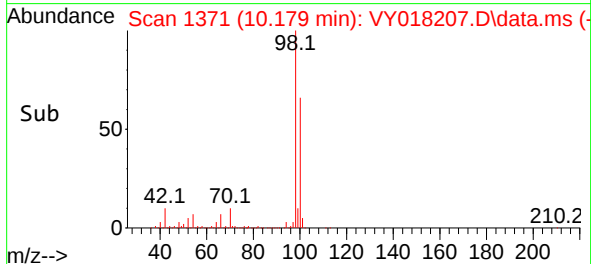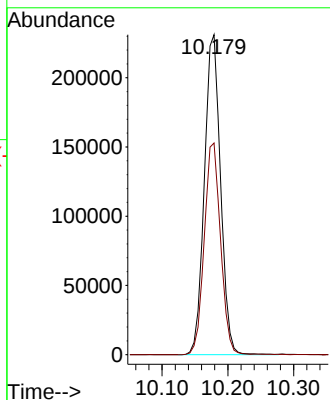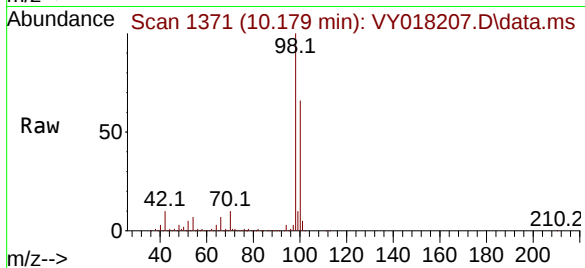

#62
4-Bromofluorobenzene
Concen: 52.856 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY018207.D
Acq: 09 May 2024 13:20

Tgt Ion: 95 Resp: 124007
Ion Ratio Lower Upper
95 100
174 84.6 0.0 175.6
176 82.8 0.0 171.4

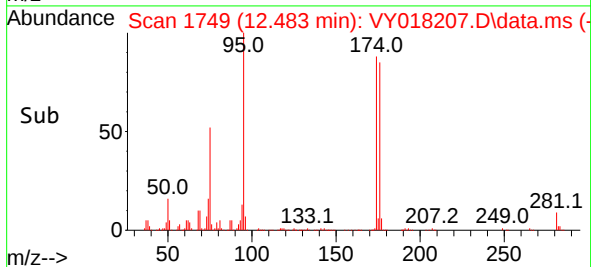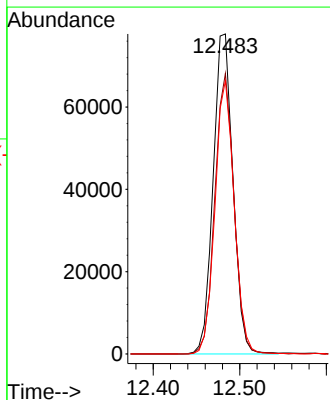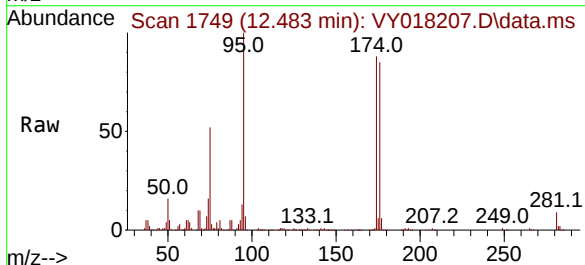

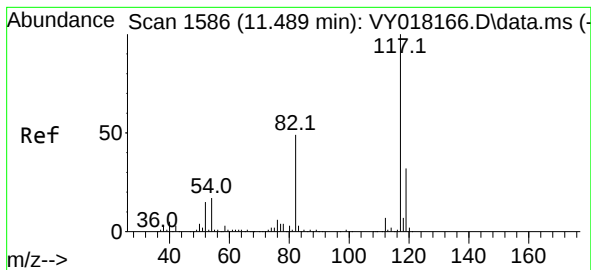

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.490 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY018207.D

Acq: 09 May 2024 13:20

Instrument :

MSVOA_Y

ClientSampleId :

WC-HH-VOC





Tgt Ion:117 Resp: 316913

Ion Ratio Lower Upper

117 100

82 50.0 42.4 63.6

119 33.0 25.9 38.9

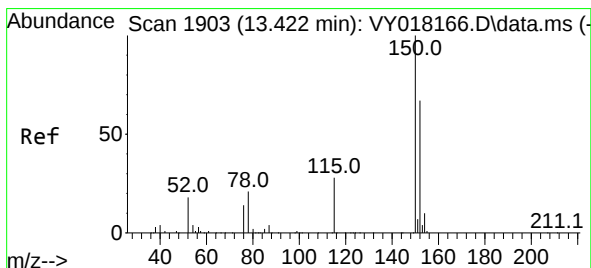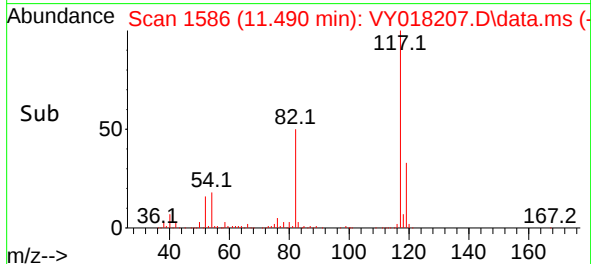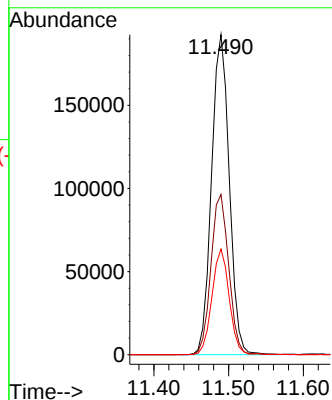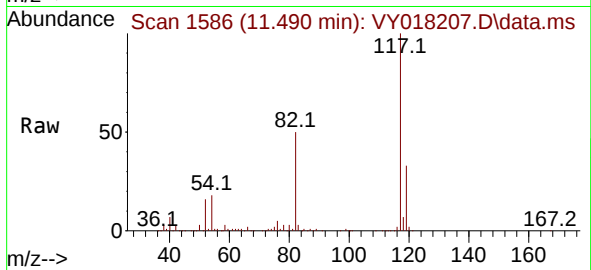

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.006 min

Lab File: VY018207.D

Acq: 09 May 2024 13:20

Tgt Ion:152 Resp: 122270

Ion Ratio Lower Upper

152 100

115 58.3 28.2 84.7

150 158.1 0.0 345.6

