


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\vy051120\
Data File : VY002650.D
Acq On : 11 May 2020 09:31
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y043020S.M
Title : SW846 8260
Last Update : Mon May 04 12:22:08 2020

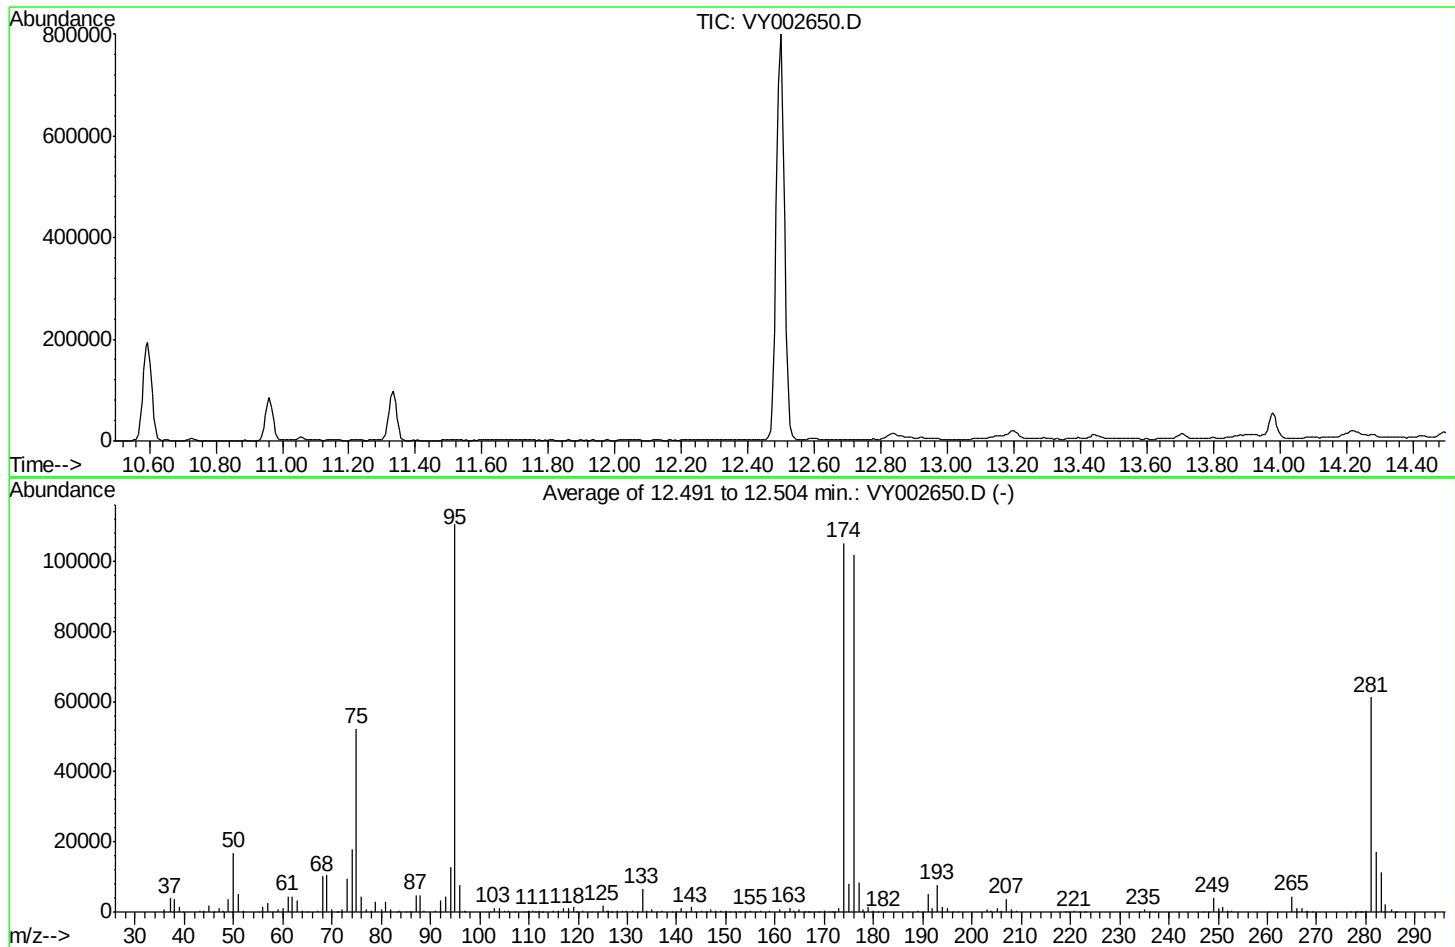

AutoFind: Scans 1764, 1765, 1766; Background Corrected with Scan 1754

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	16889	PASS
75	95	30	60	47.3	52290	PASS
95	95	100	100	100.0	110584	PASS
96	95	5	9	7.0	7781	PASS
173	174	0.00	2	1.2	1211	PASS
174	95	50	100	95.2	105304	PASS
175	174	5	9	7.5	7915	PASS
176	174	95	101	96.8	101882	PASS
177	176	5	9	8.3	8480	PASS