

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051123\
 Data File : VY013709.D
 Acq On : 11 May 2023 11:53
 Operator : KP/MD
 Sample : 02719-10
 Misc : 6.12g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-01_10-12_20230509

Quant Time: May 12 04:40:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 25 02:39:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	56601	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	80724	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	66970	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	26102	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	29277	47.185	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	94.380%
35) Dibromofluoromethane	7.716	113	26950	53.081	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	106.160%
50) Toluene-d8	10.179	98	95810	53.046	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	106.100%
62) 4-Bromofluorobenzene	12.483	95	23555	38.684	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	77.360%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051123\
Data File : VY013709.D
Acq On : 11 May 2023 11:53
Operator : KP/MD
Sample : 02719-10
Misc : 6.12g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SB-01_10-12_20230509

Quant Time: May 12 04:40:15 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
Quant Title : SW846 8260
QLast Update : Tue Apr 25 02:39:58 2023
Response via : Initial Calibration




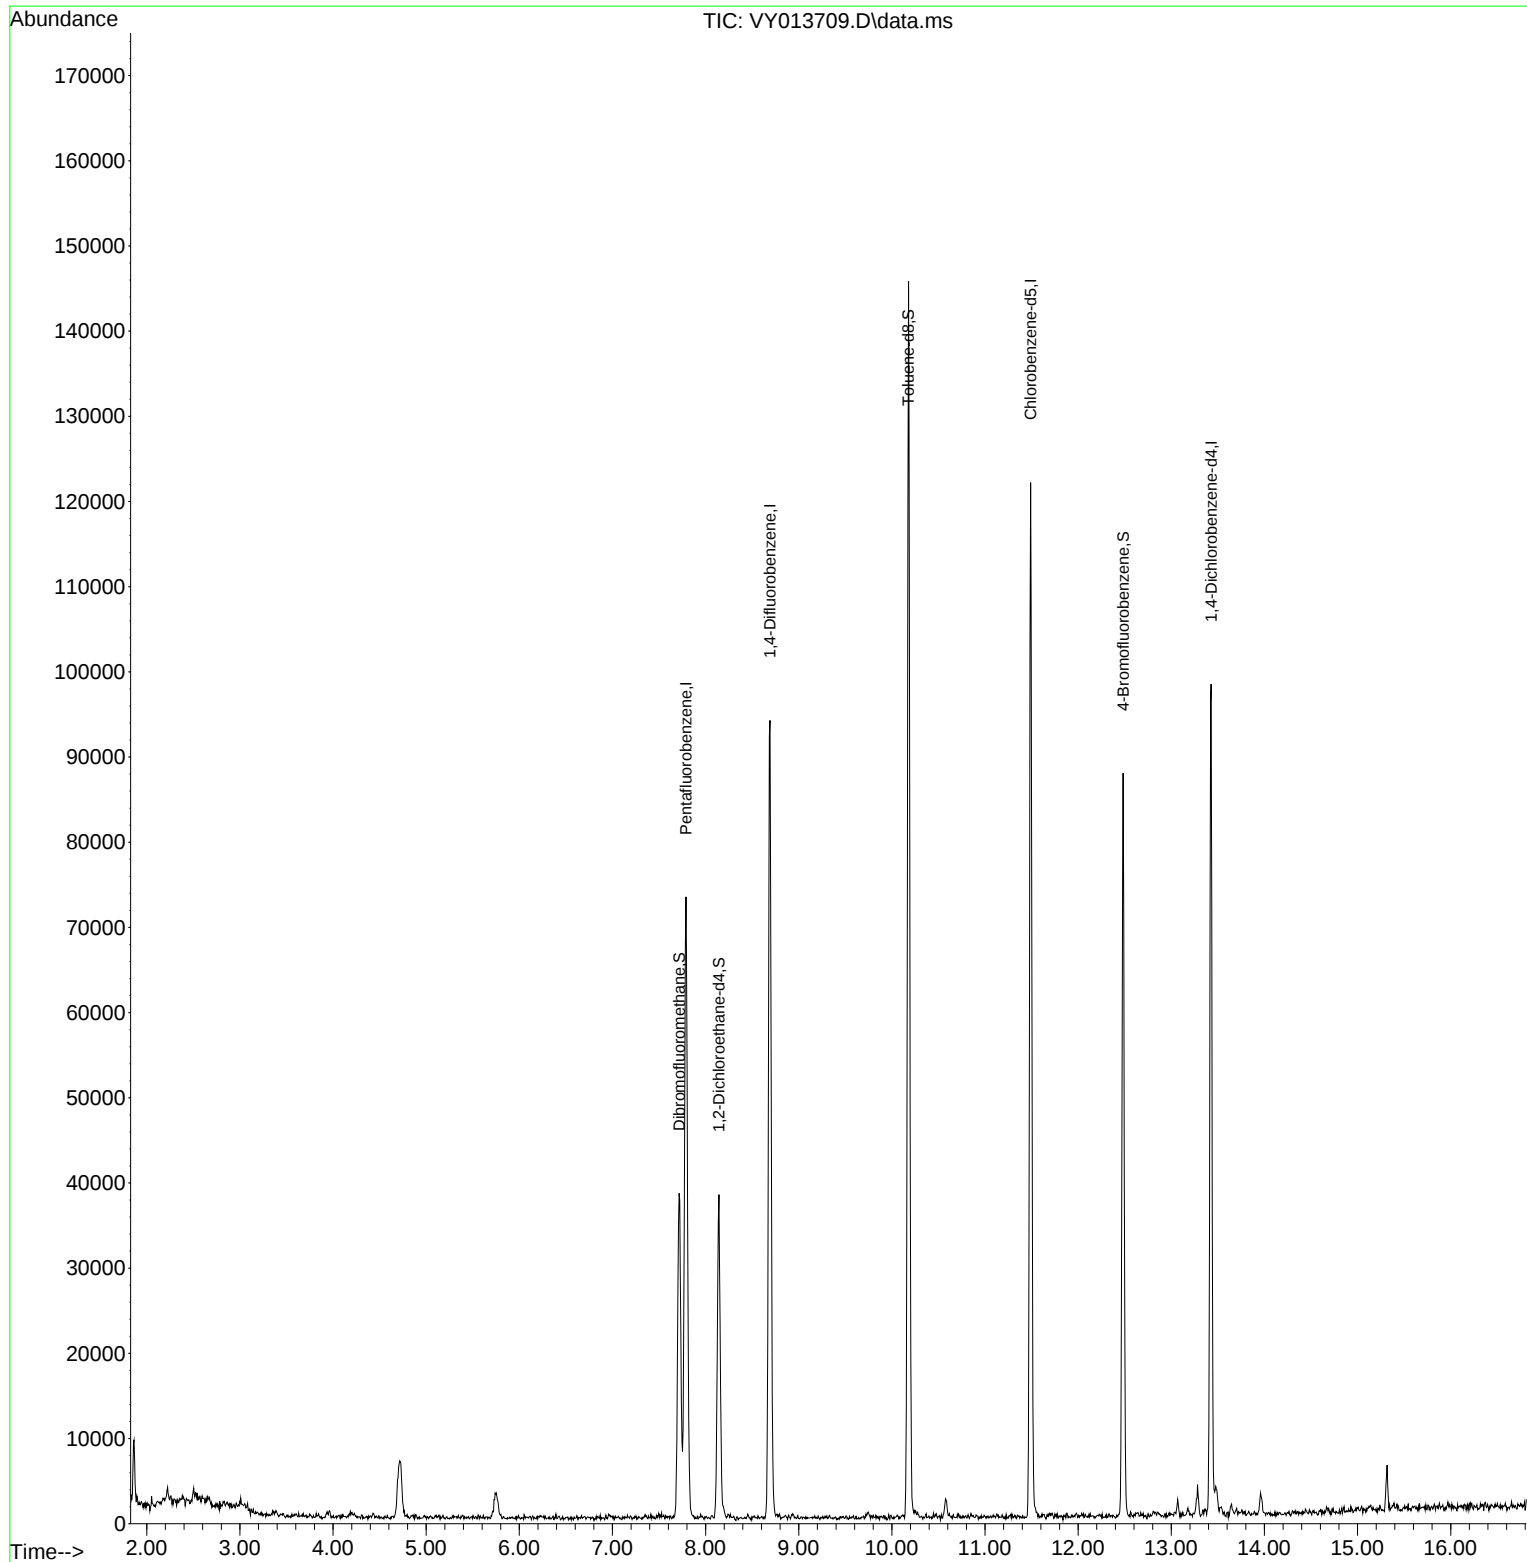


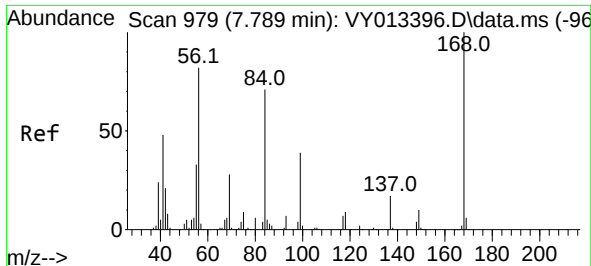

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY013709.D
Acq: 11 May 2023 11:53




Instrument :
MSVOA_Y
ClientSampleId :
SB-01_10-12_20230509


Tgt Ion:168 Resp: 56601
Ion Ratio Lower Upper
168 100
99 51.9 41.8 62.6

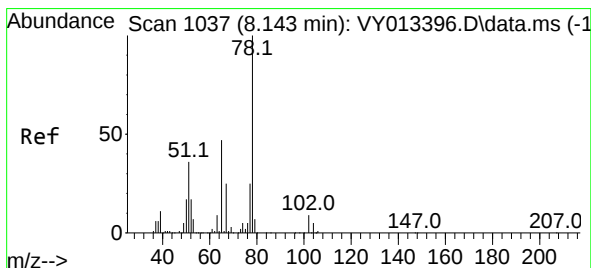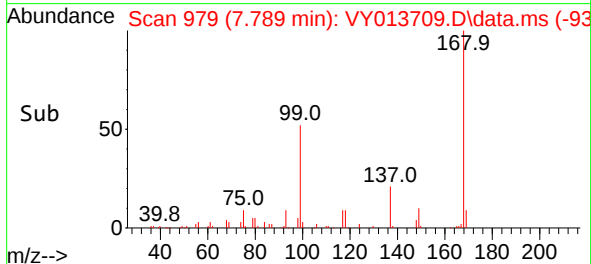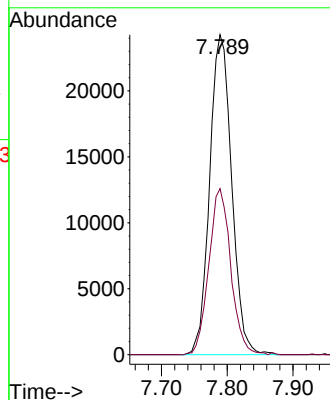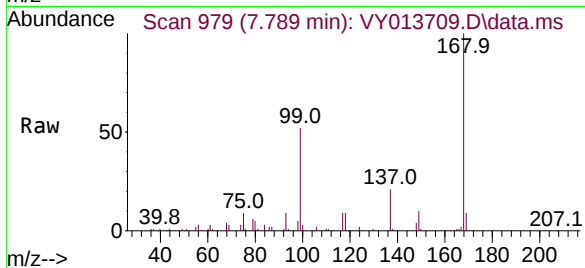

#33
1,2-Dichloroethane-d4
Concen: 47.185 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. 0.007 min
Lab File: VY013709.D
Acq: 11 May 2023 11:53

Tgt Ion: 65 Resp: 29277
Ion Ratio Lower Upper
65 100
67 51.1 0.0 103.4

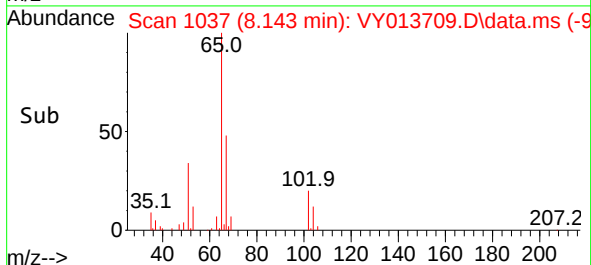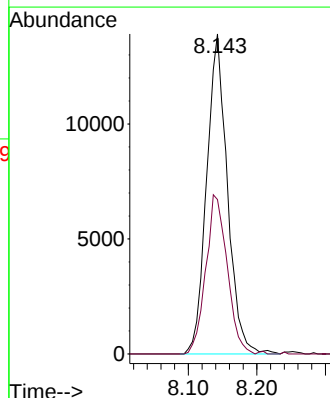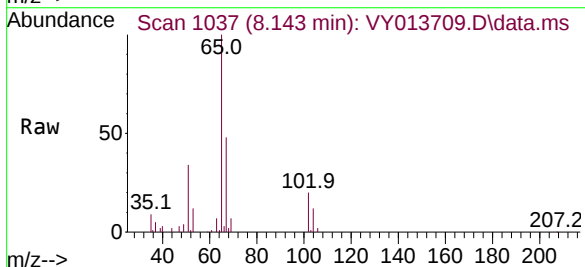

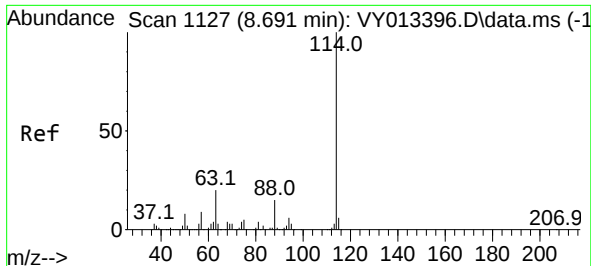

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY013709.D

Acq: 11 May 2023 11:53

Instrument :

MSVOA_Y

ClientSampleId :

SB-01_10-12_20230509





Tgt Ion:114 Resp: 80724

Ion Ratio Lower Upper

114 100

63 19.2 0.0 36.6

88 13.5 0.0 28.8

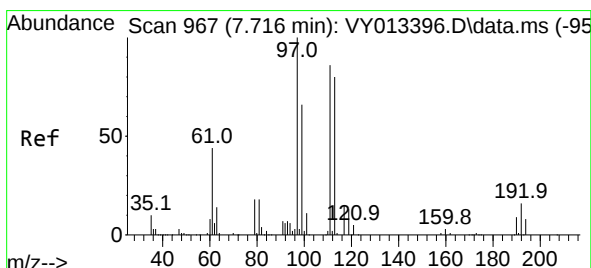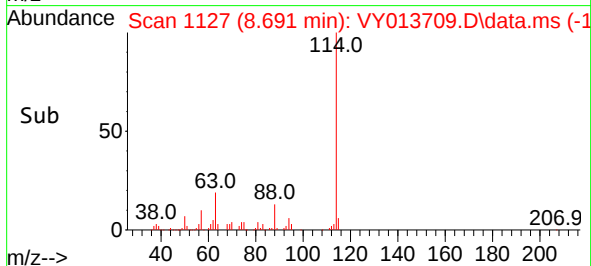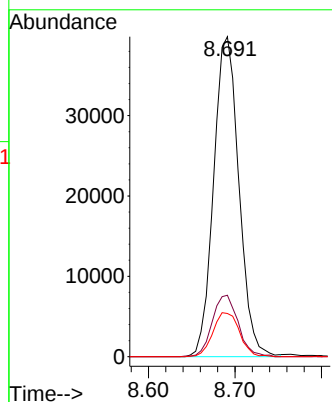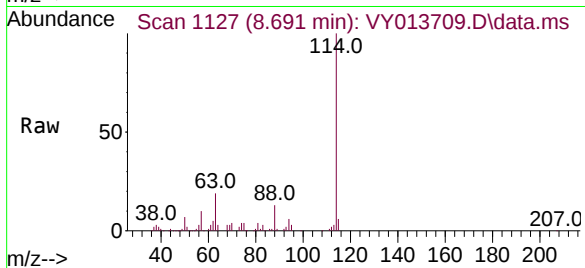

#35

Dibromofluoromethane

Concen: 53.081 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY013709.D

Acq: 11 May 2023 11:53




Tgt Ion:113 Resp: 26950


Ion Ratio Lower Upper

113 100

111 101.8 82.2 123.2

192 21.6 16.7 25.1


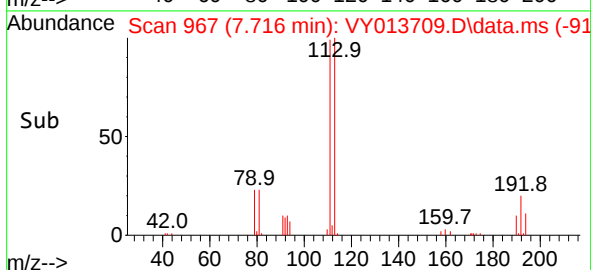
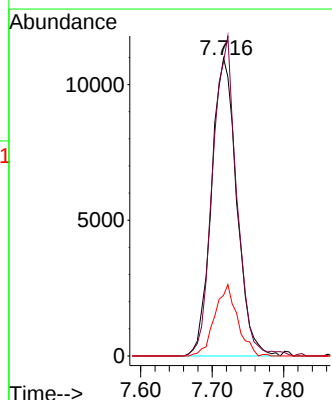
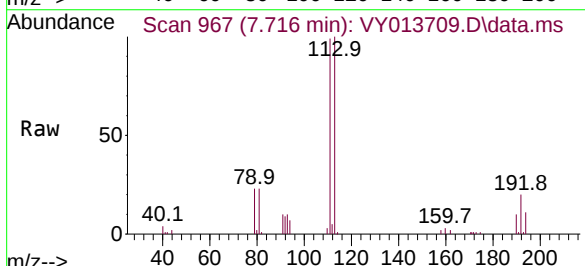


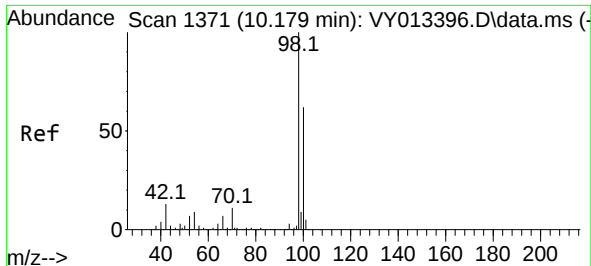

#50
Toluene-d8
Concen: 53.046 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY013709.D
Acq: 11 May 2023 11:53




Instrument :
MSVOA_Y
ClientSampleId :
SB-01_10-12_20230509


Tgt Ion: 98 Resp: 95810
Ion Ratio Lower Upper
98 100
100 61.1 50.5 75.7

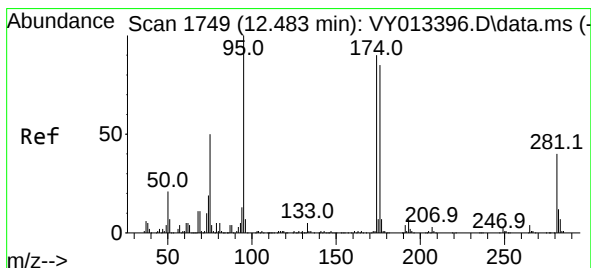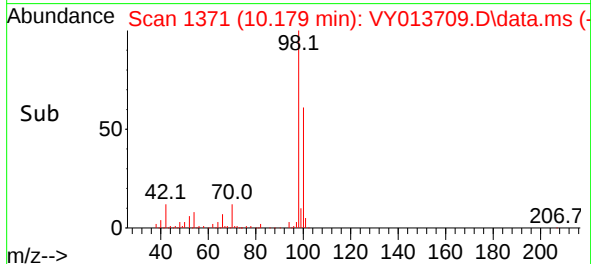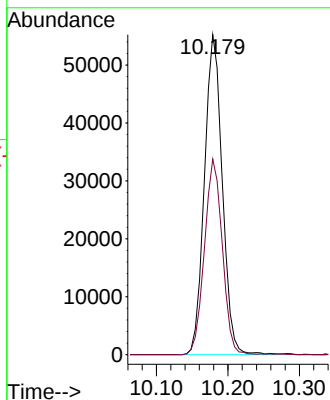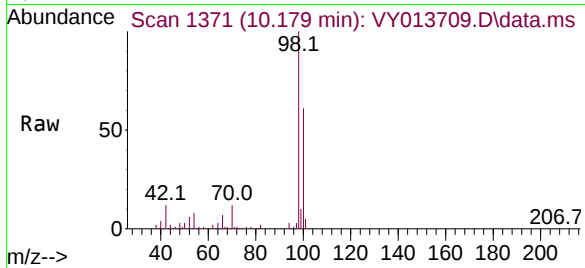

#62
4-Bromofluorobenzene
Concen: 38.684 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.006 min
Lab File: VY013709.D
Acq: 11 May 2023 11:53

Tgt Ion: 95 Resp: 23555
Ion Ratio Lower Upper
95 100
174 99.8 0.0 182.0
176 90.0 0.0 175.4

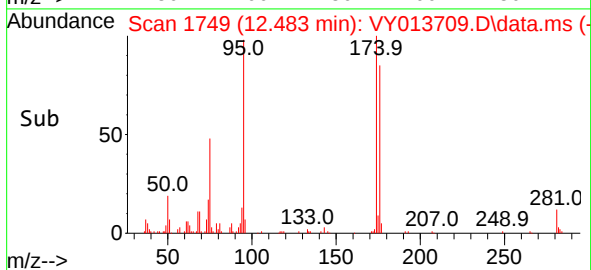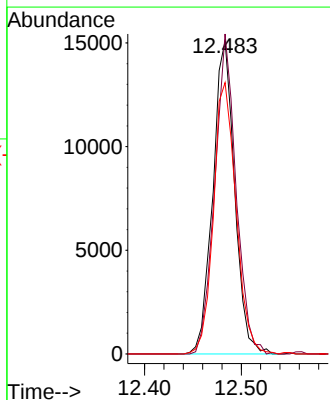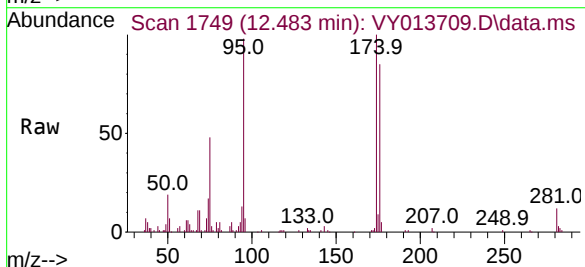

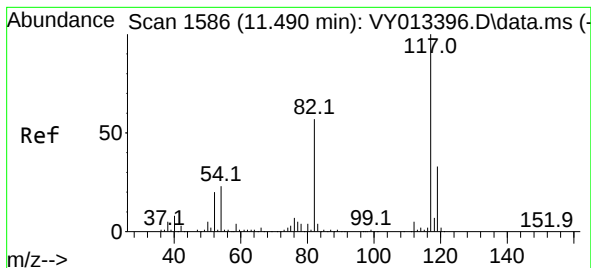

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.489 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY013709.D

Acq: 11 May 2023 11:53

Instrument :

MSVOA_Y

ClientSampleId :

SB-01_10-12_20230509





Tgt Ion:117 Resp: 66970

Ion Ratio Lower Upper

117 100

82 52.9 43.0 64.6

119 31.2 25.5 38.3

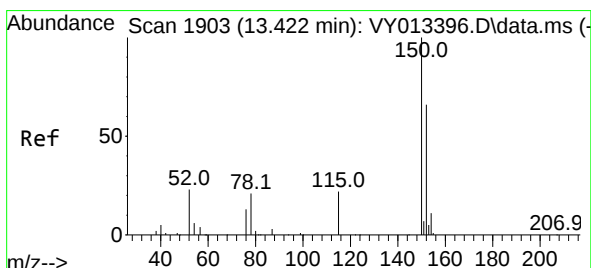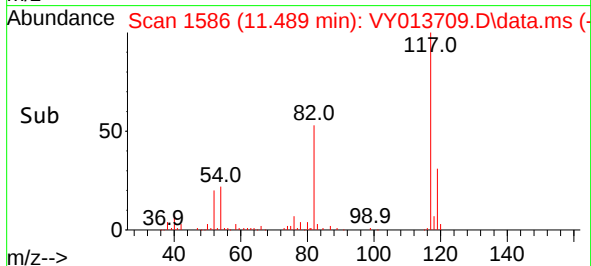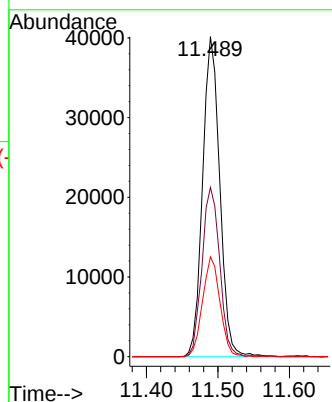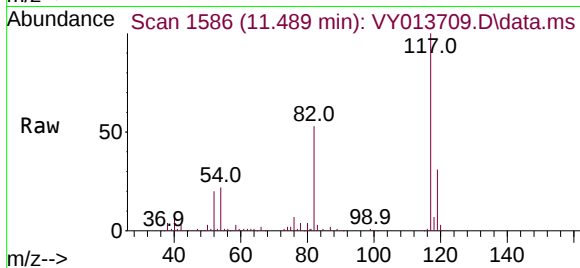

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.006 min

Lab File: VY013709.D

Acq: 11 May 2023 11:53

Tgt Ion:152 Resp: 26102

Ion Ratio Lower Upper

152 100

115 57.1 28.1 84.2

150 159.7 0.0 352.0

