

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051123\
 Data File : VY013711.D
 Acq On : 11 May 2023 12:40
 Operator : KP/MD
 Sample : 02719-08
 Misc : 6.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-02_5-7_20230509

Quant Time: May 12 04:41:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 25 02:39:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	140065	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	229387	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	222392	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	99445	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.137	65	95606	62.267	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	124.540%
35) Dibromofluoromethane	7.716	113	81396	56.418	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	112.840%
50) Toluene-d8	10.179	98	283018	55.143	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	110.280%
62) 4-Bromofluorobenzene	12.483	95	87126	50.354	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	100.700%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051123\
Data File : VY013711.D
Acq On : 11 May 2023 12:40
Operator : KP/MD
Sample : 02719-08
Misc : 6.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SB-02_5-7_20230509

Quant Time: May 12 04:41:01 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
Quant Title : SW846 8260
QLast Update : Tue Apr 25 02:39:58 2023
Response via : Initial Calibration




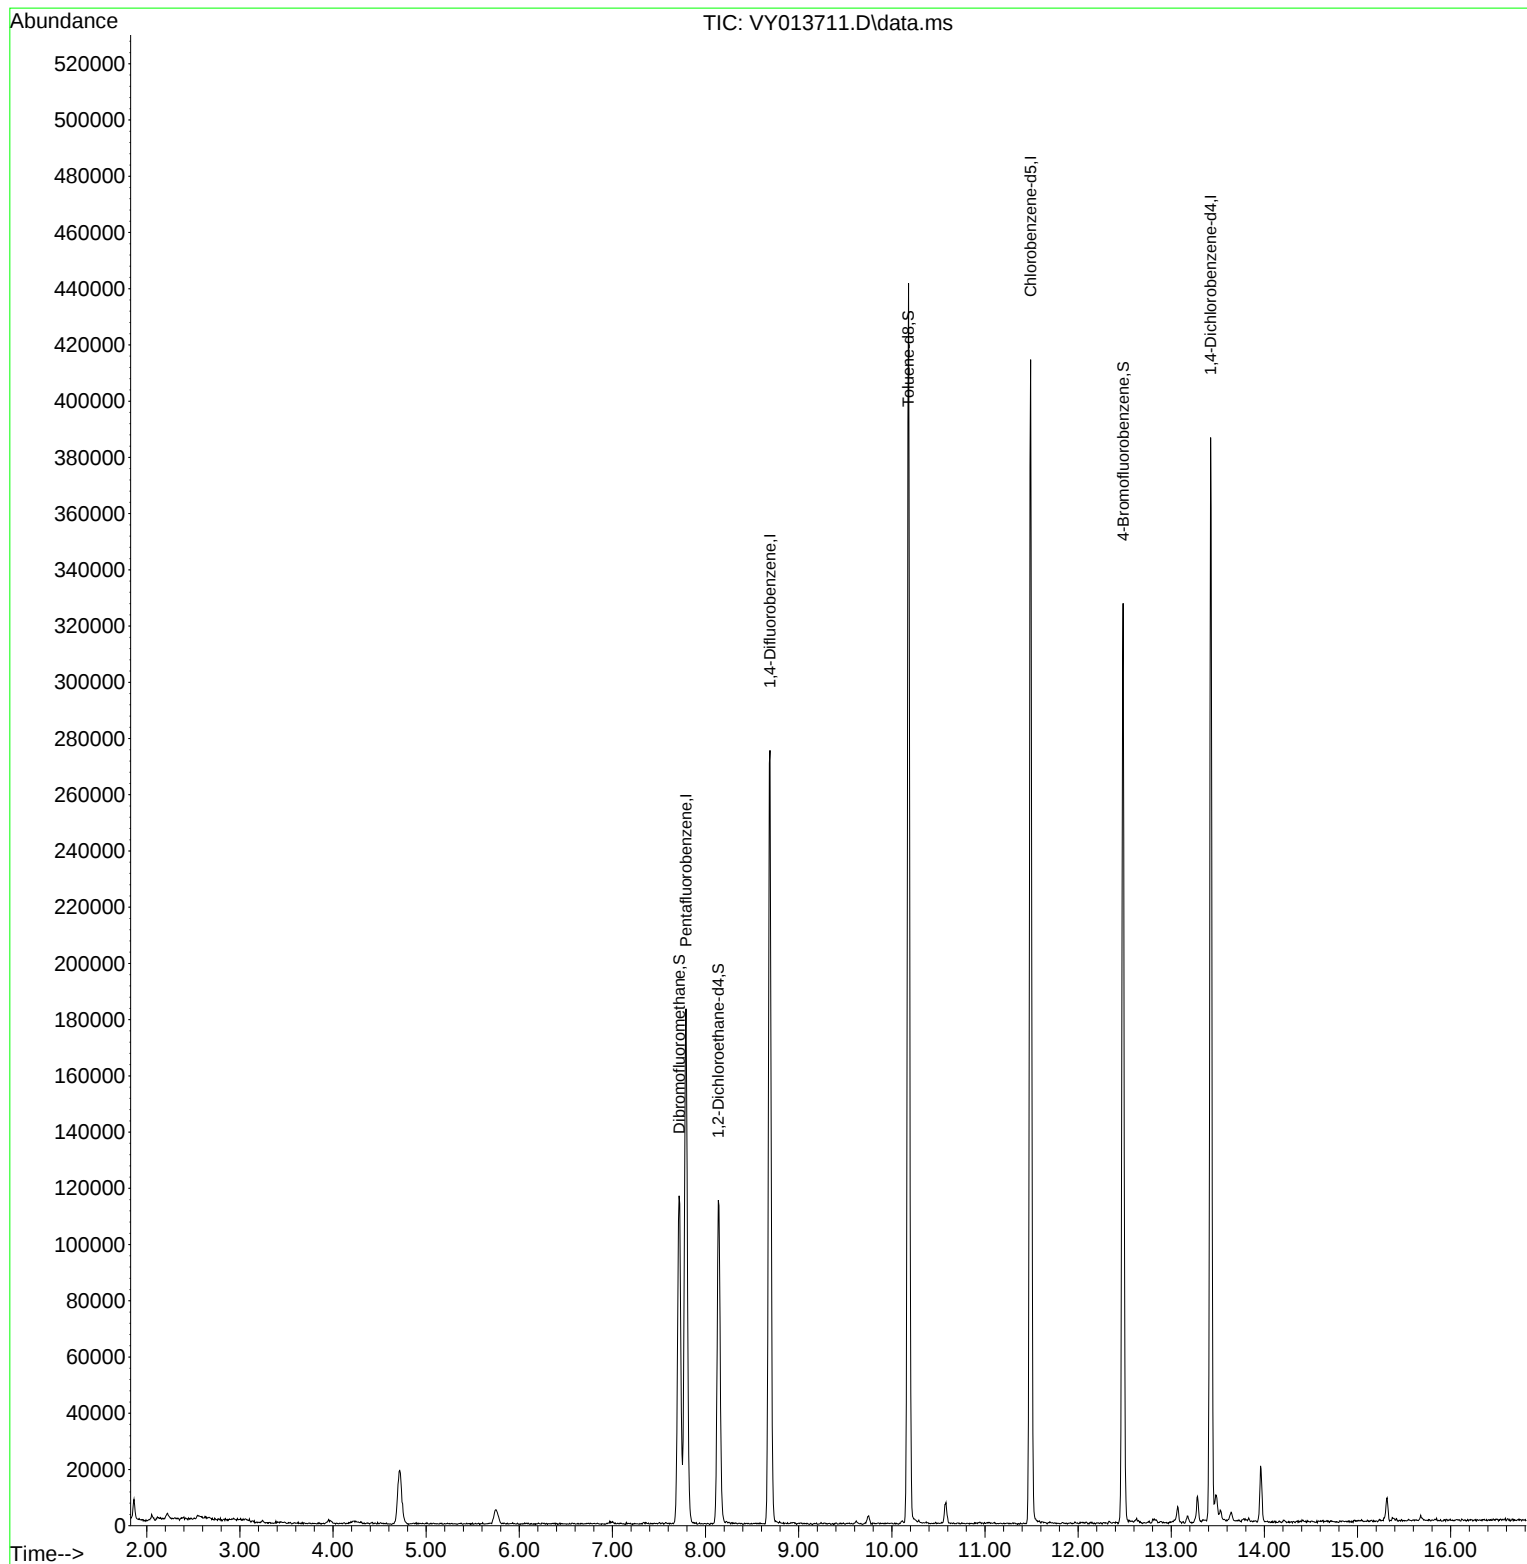


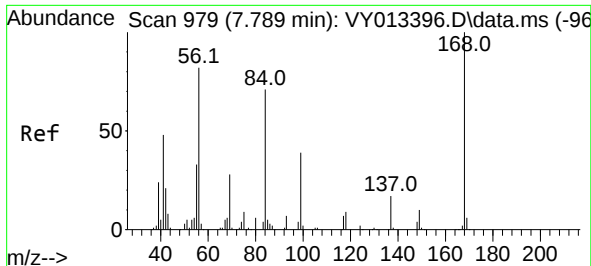

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY013711.D
Acq: 11 May 2023 12:40




Instrument :
MSVOA_Y
ClientSampleId :
SB-02_5-7_20230509


Tgt Ion:168 Resp: 140065
Ion Ratio Lower Upper
168 100
99 52.4 41.8 62.6

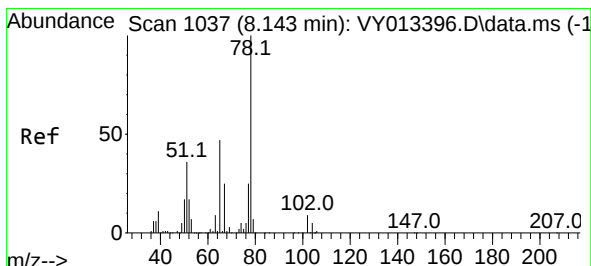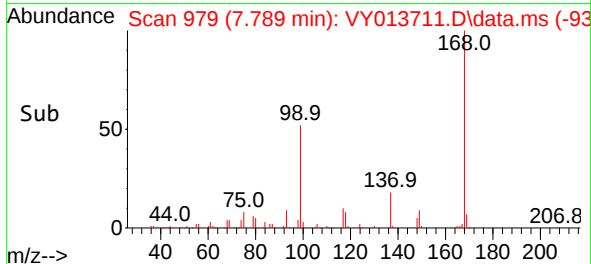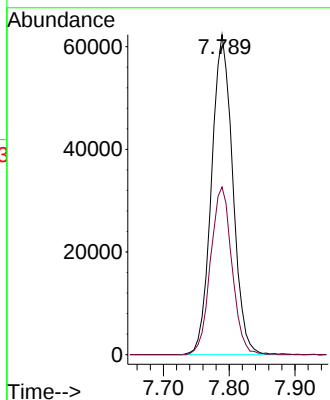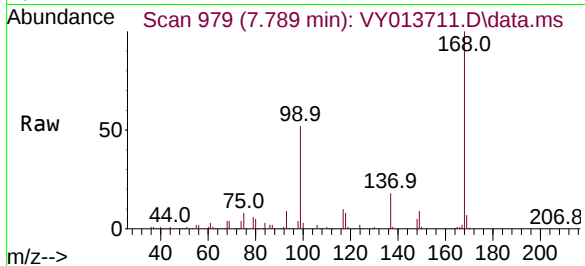

#33
1,2-Dichloroethane-d4
Concen: 62.267 ug/l
RT: 8.137 min Scan# 1036
Delta R.T. 0.001 min
Lab File: VY013711.D
Acq: 11 May 2023 12:40

Tgt Ion: 65 Resp: 95606
Ion Ratio Lower Upper
65 100
67 50.4 0.0 103.4

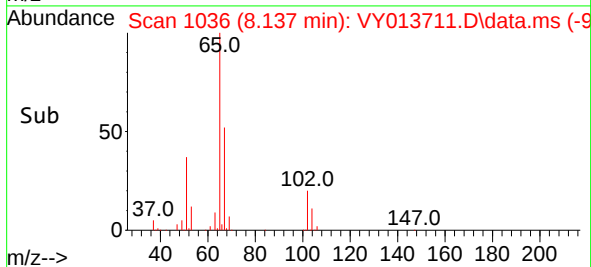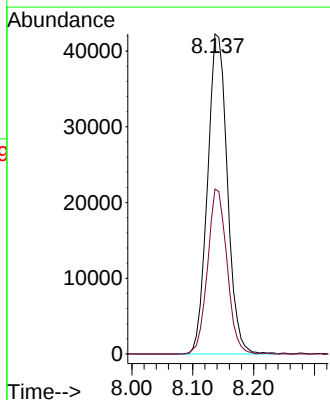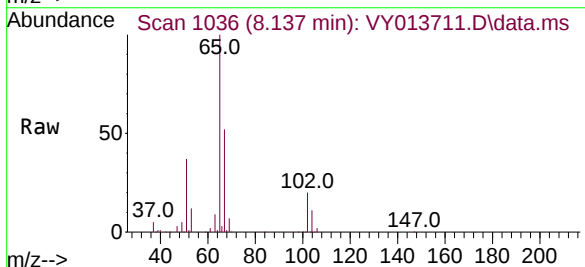

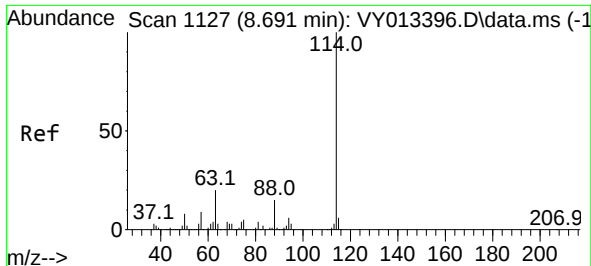

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY013711.D

Acq: 11 May 2023 12:40

Instrument :

MSVOA_Y

ClientSampleId :

SB-02_5-7_20230509





Tgt Ion:114 Resp: 229387

Ion Ratio Lower Upper

114 100

63 19.6 0.0 36.6

88 14.2 0.0 28.8

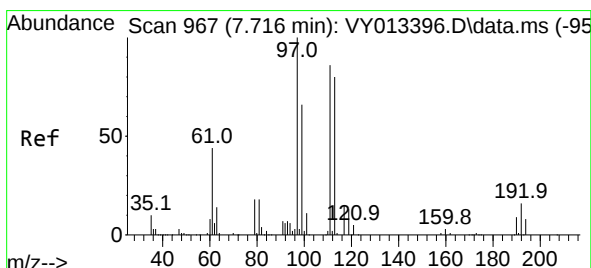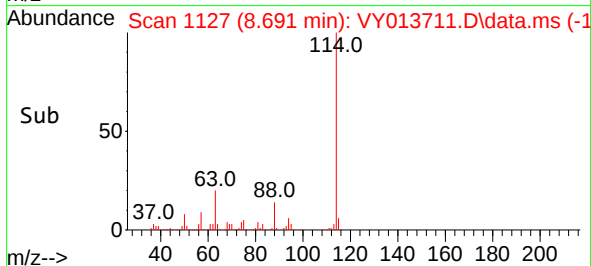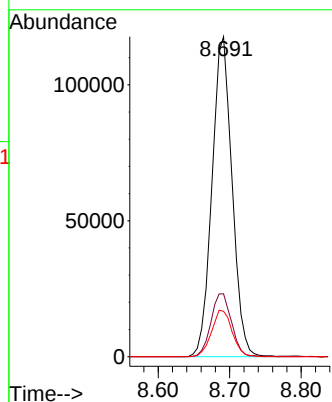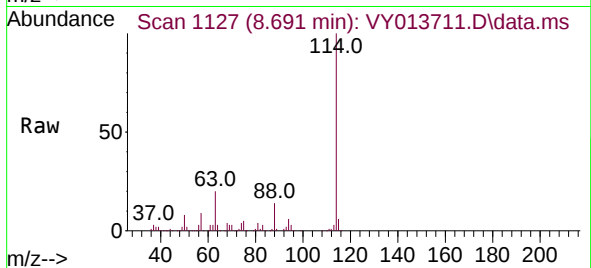

#35

Dibromofluoromethane

Concen: 56.418 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY013711.D

Acq: 11 May 2023 12:40




Tgt Ion:113 Resp: 81396


Ion Ratio Lower Upper

113 100

111 103.1 82.2 123.2

192 21.1 16.7 25.1

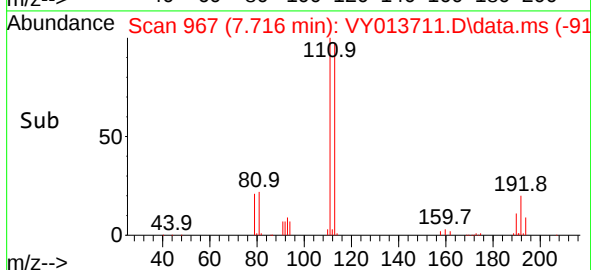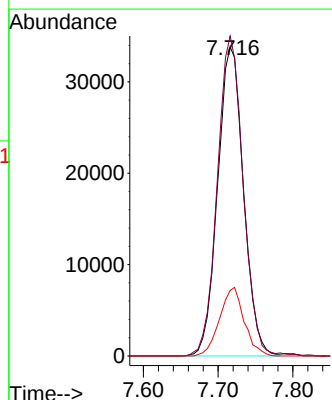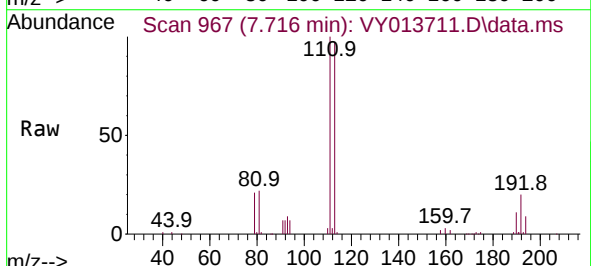

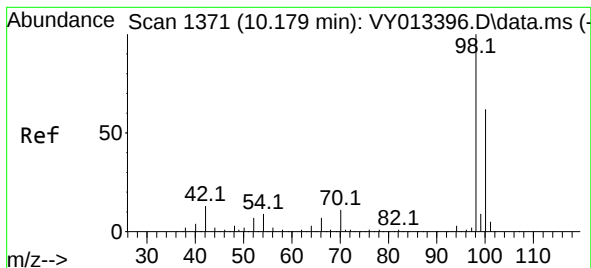

#50

Toluene-d8

Concen: 55.143 ug/l

RT: 10.179 min Scan# 1371

Delta R.T. -0.000 min

Lab File: VY013711.D

Acq: 11 May 2023 12:40

Instrument :

MSVOA_Y

ClientSampleId :





SB-02_5-7_20230509

Tgt Ion: 98 Resp: 283018

Ion Ratio Lower Upper

98 100

100 62.8 50.5 75.7

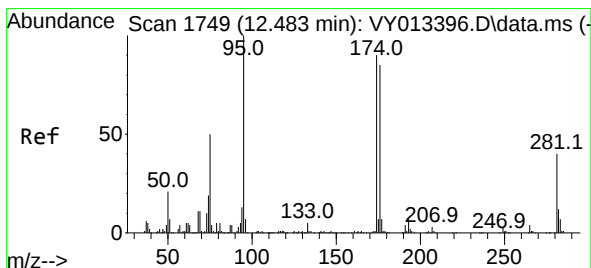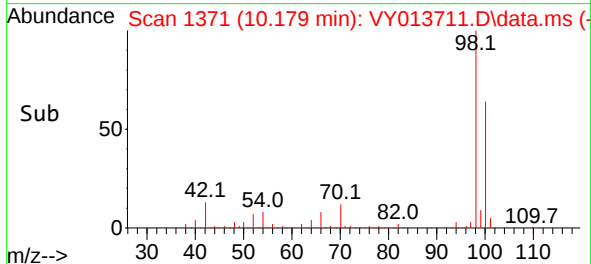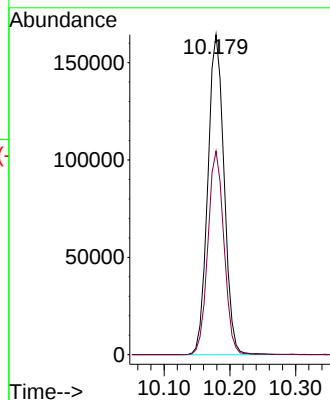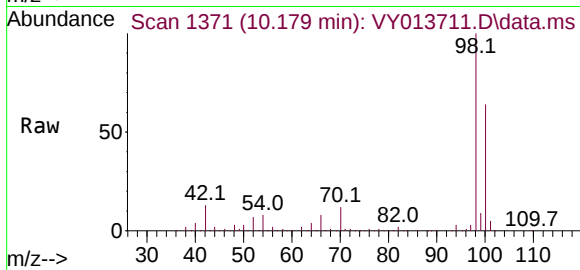

#62

4-Bromofluorobenzene

Concen: 50.354 ug/l

RT: 12.483 min Scan# 1749

Delta R.T. 0.006 min

Lab File: VY013711.D

Acq: 11 May 2023 12:40




Tgt Ion: 95 Resp: 87126


Ion Ratio Lower Upper

95 100

174 94.5 0.0 182.0

176 90.6 0.0 175.4

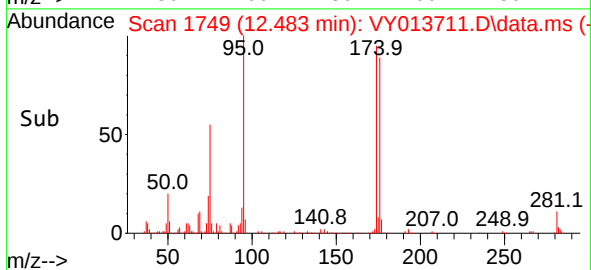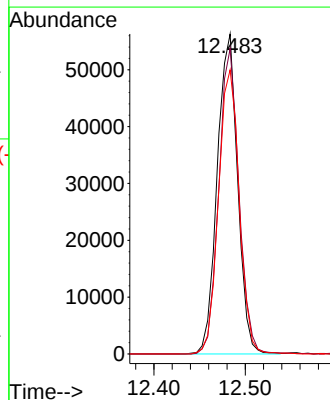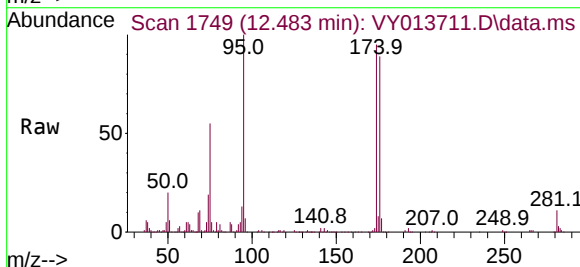

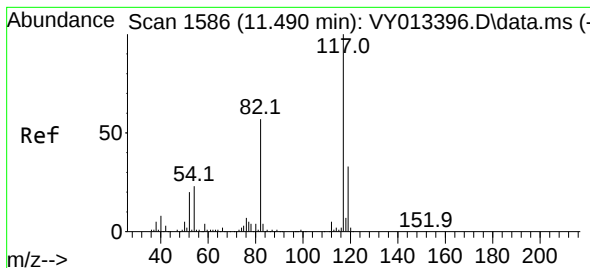

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.490 min Scan# 11

Delta R.T. 0.001 min

Lab File: VY013711.D

Acq: 11 May 2023 12:40

Instrument :

MSVOA_Y

ClientSampleId :

SB-02_5-7_20230509





Tgt Ion:117 Resp: 222392

Ion Ratio Lower Upper

117 100

82 52.7 43.0 64.6

119 33.8 25.5 38.3

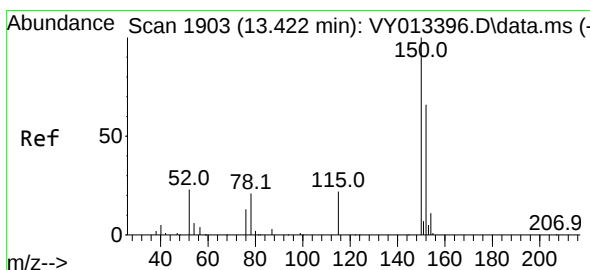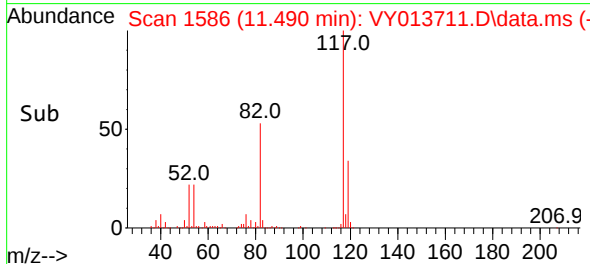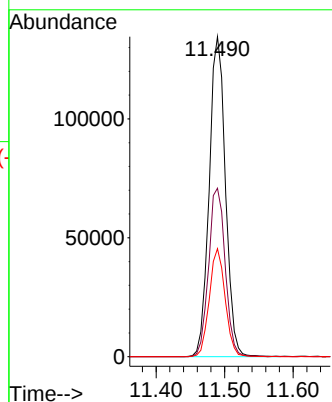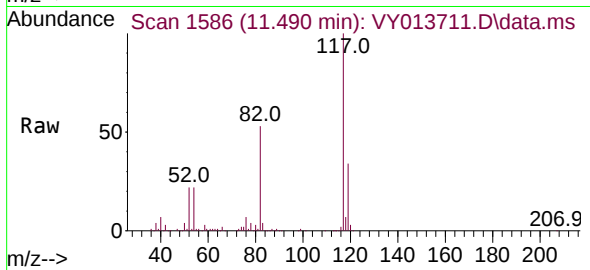

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.422 min Scan# 1903

Delta R.T. 0.000 min

Lab File: VY013711.D

Acq: 11 May 2023 12:40

Tgt Ion:152 Resp: 99445

Ion Ratio Lower Upper

152 100

115 55.8 28.1 84.2

150 157.4 0.0 352.0

