


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv051220\
Data File : VY002657.D
Acq On : 12 May 2020 09:32
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y043020S.M
Title : SW846 8260
Last Update : Mon May 04 12:22:08 2020

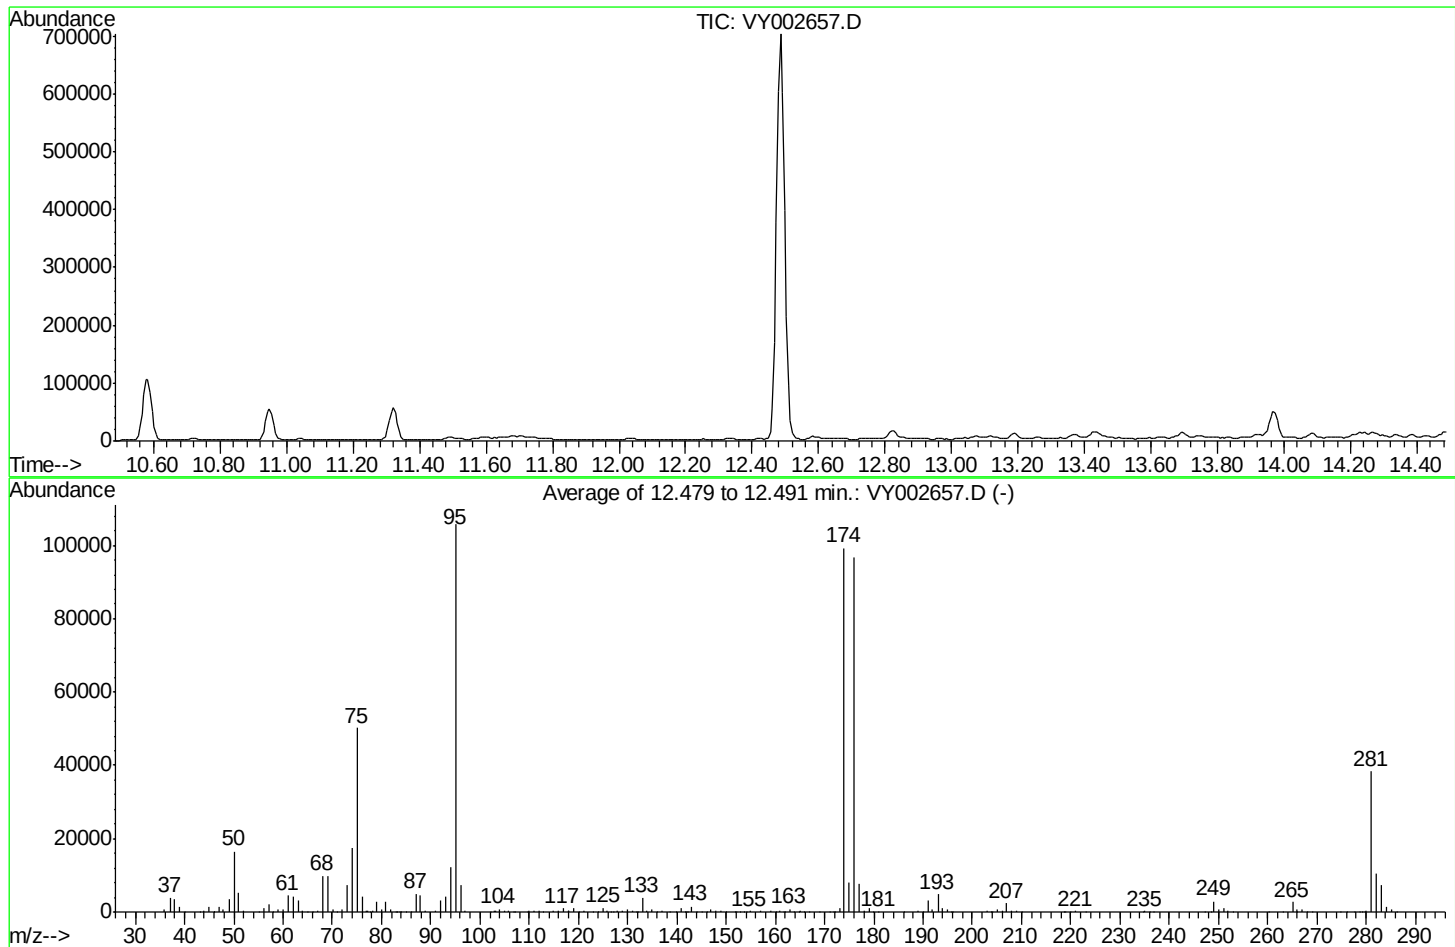

AutoFind: Scans 1762, 1763, 1764; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	16531	PASS
75	95	30	60	47.4	50152	PASS
95	95	100	100	100.0	105750	PASS
96	95	5	9	7.1	7467	PASS
173	174	0.00	2	1.0	1023	PASS
174	95	50	100	93.8	99221	PASS
175	174	5	9	8.1	8002	PASS
176	174	95	101	97.5	96760	PASS
177	176	5	9	7.9	7625	PASS