
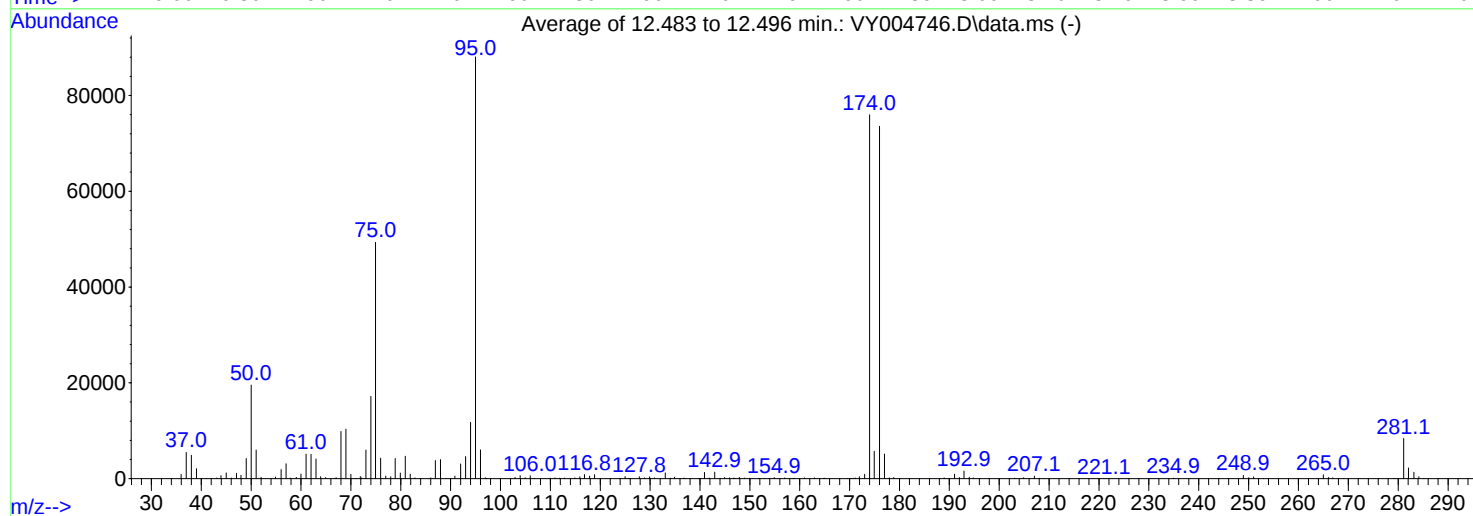


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051221\
 Data File : VY004746.D
 Acq On : 12 May 2021 09:45
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051021S.M
 Title : SW846 8260
 Last Update : Tue May 11 04:13:44 2021

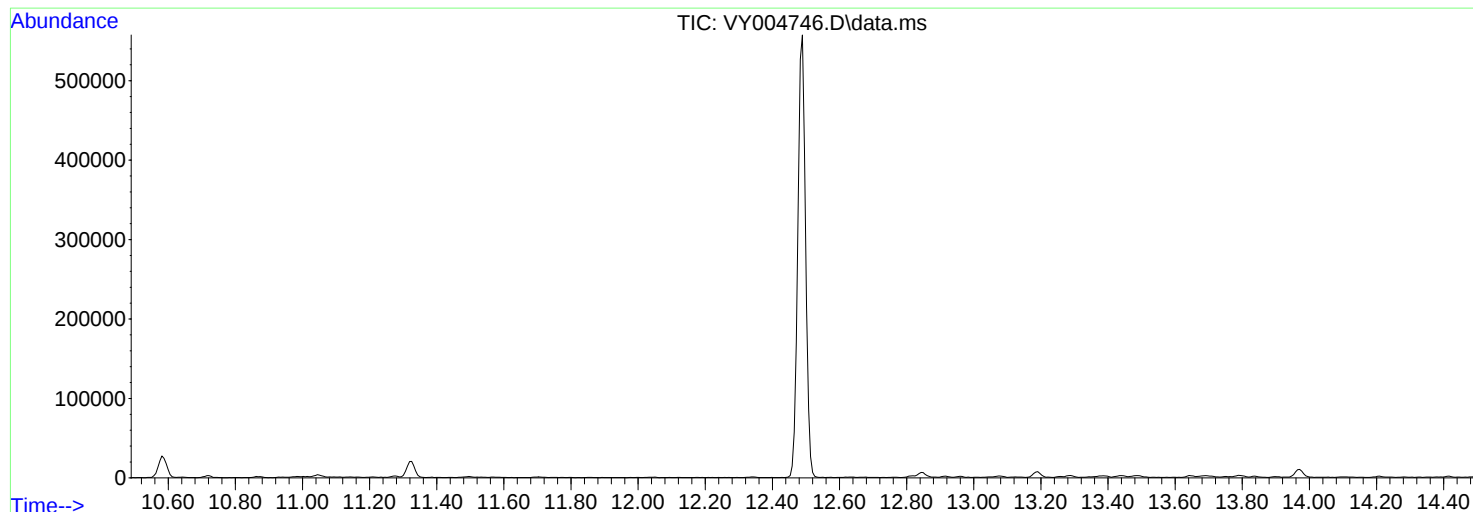

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	19559	PASS
75	95	30	60	56.0	49357	PASS
95	95	100	100	100.0	88069	PASS
96	95	5	9	6.8	6006	PASS
173	174	0.00	2	1.2	899	PASS
174	95	50	100	86.3	75968	PASS
175	174	5	9	7.5	5706	PASS
176	174	95	101	96.8	73557	PASS
177	176	5	9	7.0	5148	PASS