
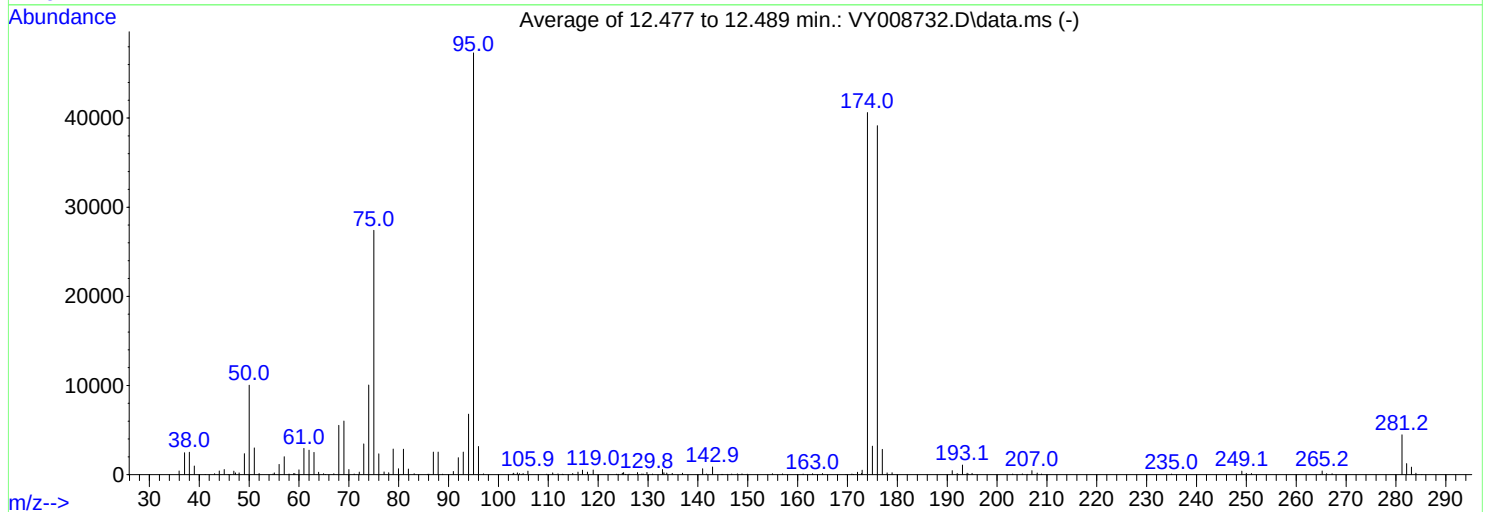


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051222\
Data File : VY008732.D
Acq On : 12 May 2022 14:00
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051222S.M
Title : SW846 8260
Last Update : Fri May 13 02:08:33 2022

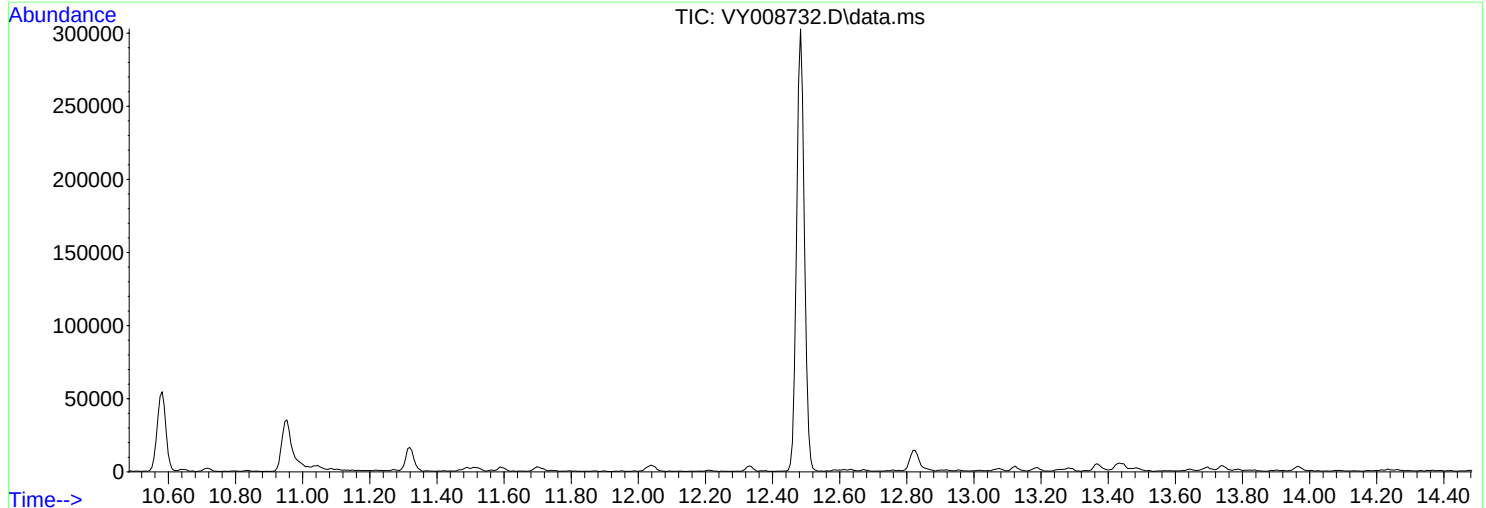

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.2	10034	PASS
75	95	30	60	57.9	27403	PASS
95	95	100	100	100.0	47315	PASS
96	95	5	9	6.7	3159	PASS
173	174	0.00	2	1.3	512	PASS
174	95	50	100	85.8	40611	PASS
175	174	5	9	7.9	3191	PASS
176	174	95	101	96.4	39141	PASS
177	176	5	9	7.3	2838	PASS