
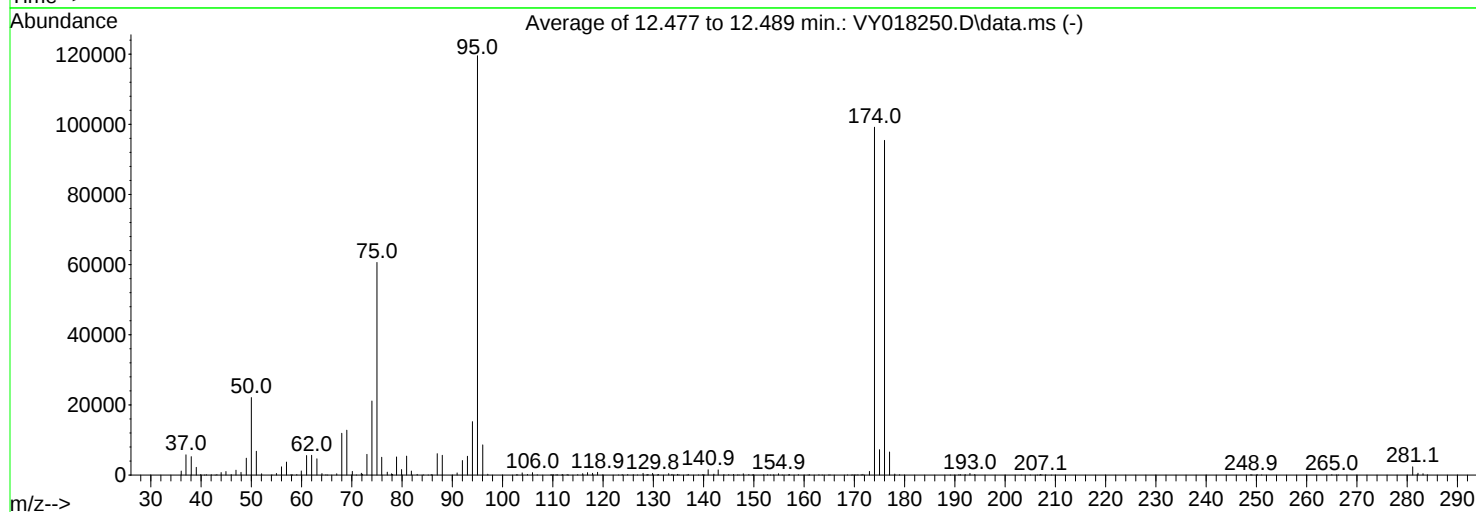


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051424\
Data File : VY018250.D
Acq On : 14 May 2024 08:23
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y050724S.M
Title : SW846 8260
Last Update : Wed May 08 01:40:14 2024

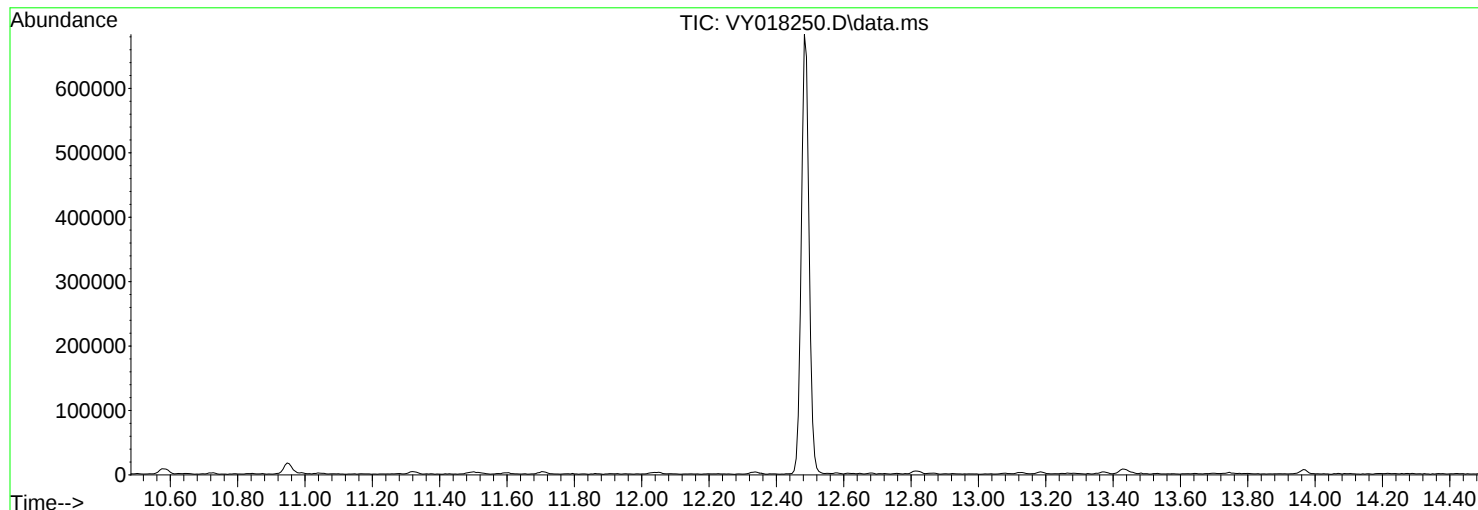

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	22096	PASS
75	95	30	60	50.7	60627	PASS
95	95	100	100	100.0	119555	PASS
96	95	5	9	7.2	8604	PASS
173	174	0.00	2	1.0	1040	PASS
174	95	50	100	83.0	99173	PASS
175	174	5	9	7.3	7239	PASS
176	174	95	101	96.2	95427	PASS
177	176	5	9	6.9	6587	PASS