
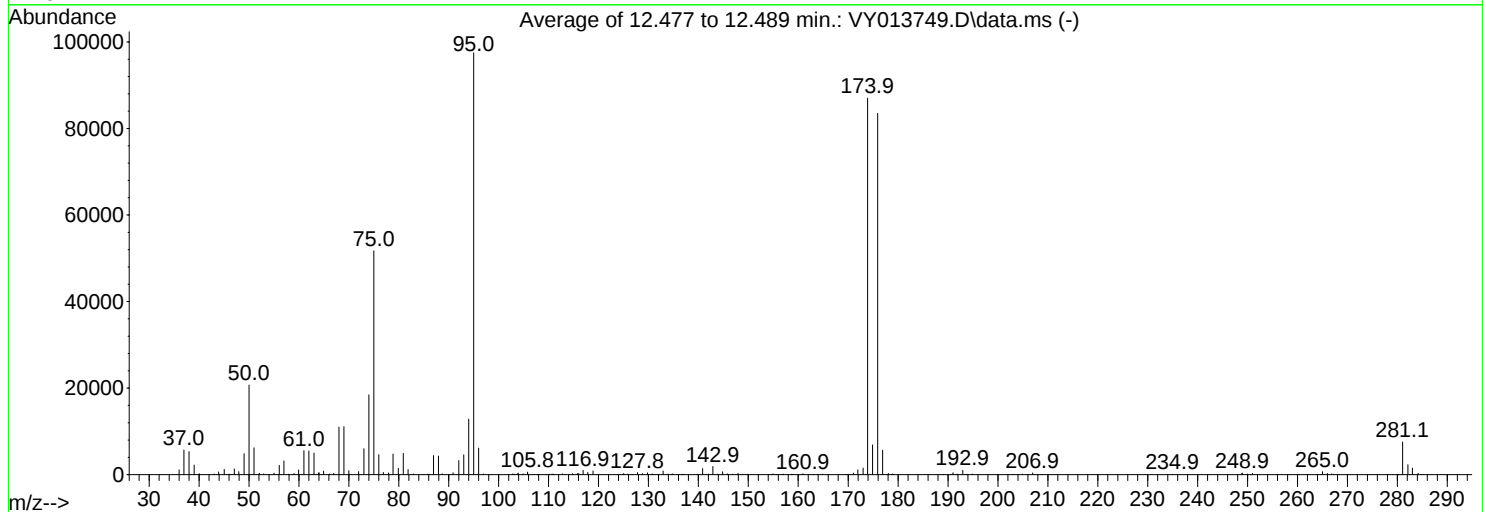


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051623\
Data File : VY013749.D
Acq On : 16 May 2023 09:11
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
Title : SW846 8260
Last Update : Tue Apr 25 02:39:58 2023

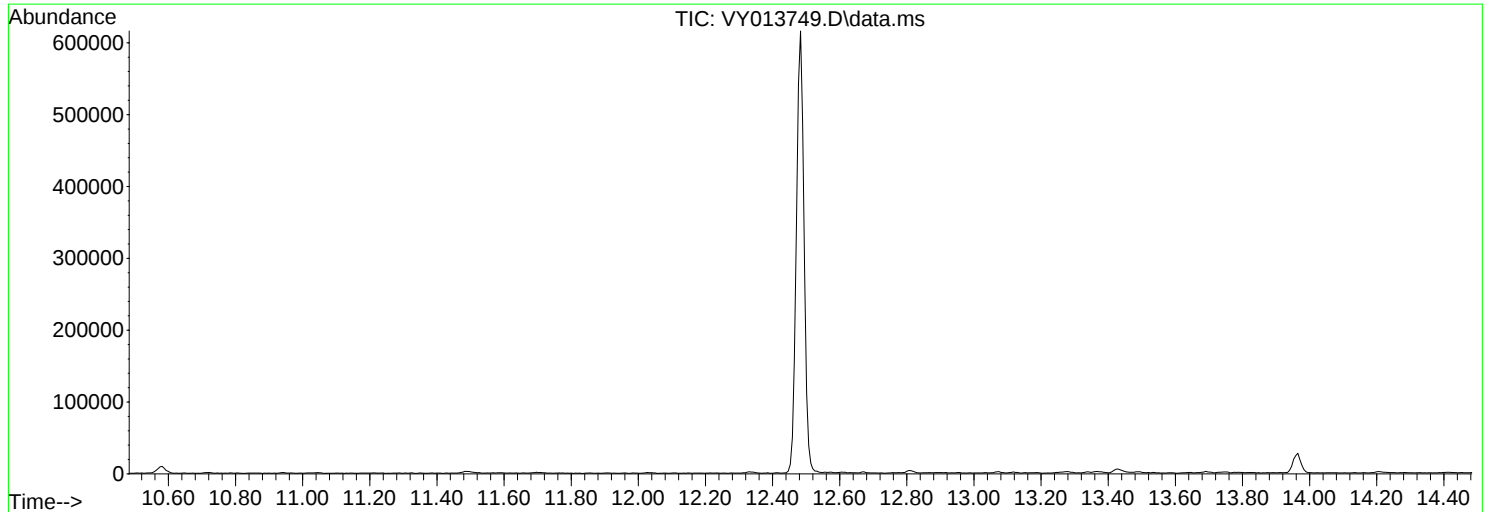

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1739

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.2	20704	PASS
75	95	30	60	53.1	51723	PASS
95	95	100	100	100.0	97485	PASS
96	95	5	9	6.3	6159	PASS
173	174	0.00	2	1.8	1524	PASS
174	95	50	100	89.3	87019	PASS
175	174	5	9	7.9	6886	PASS
176	174	95	101	95.9	83493	PASS
177	176	5	9	6.8	5666	PASS