
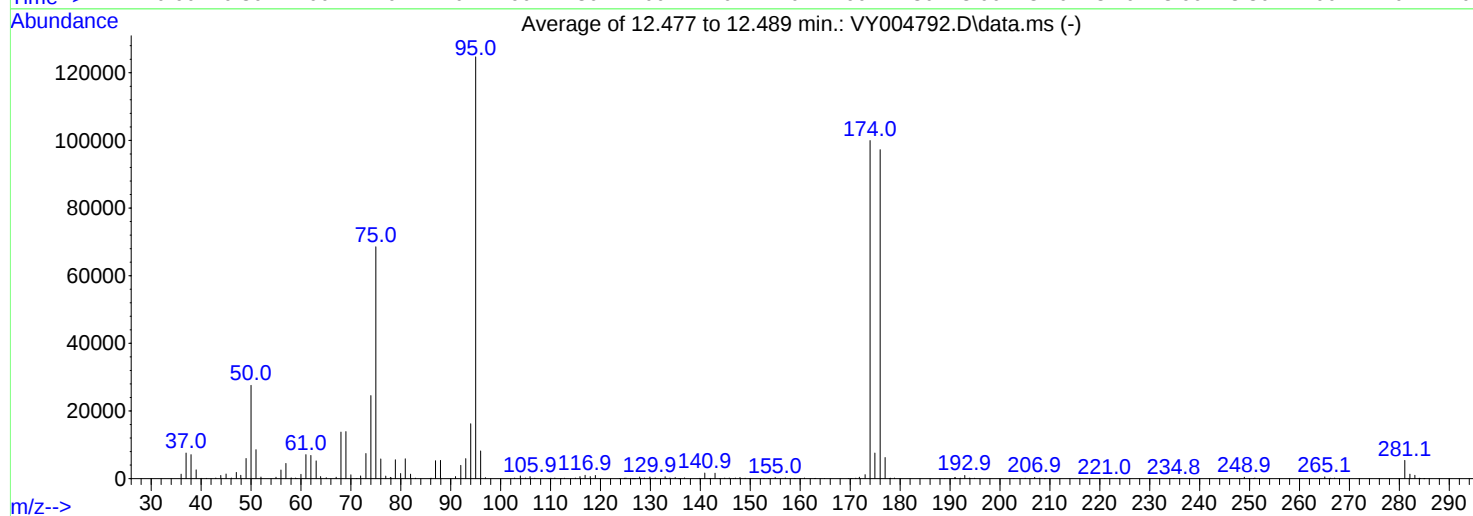


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051721\
 Data File : VY004792.D
 Acq On : 17 May 2021 09:33
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051021S.M
 Title : SW846 8260
 Last Update : Tue May 11 04:13:44 2021

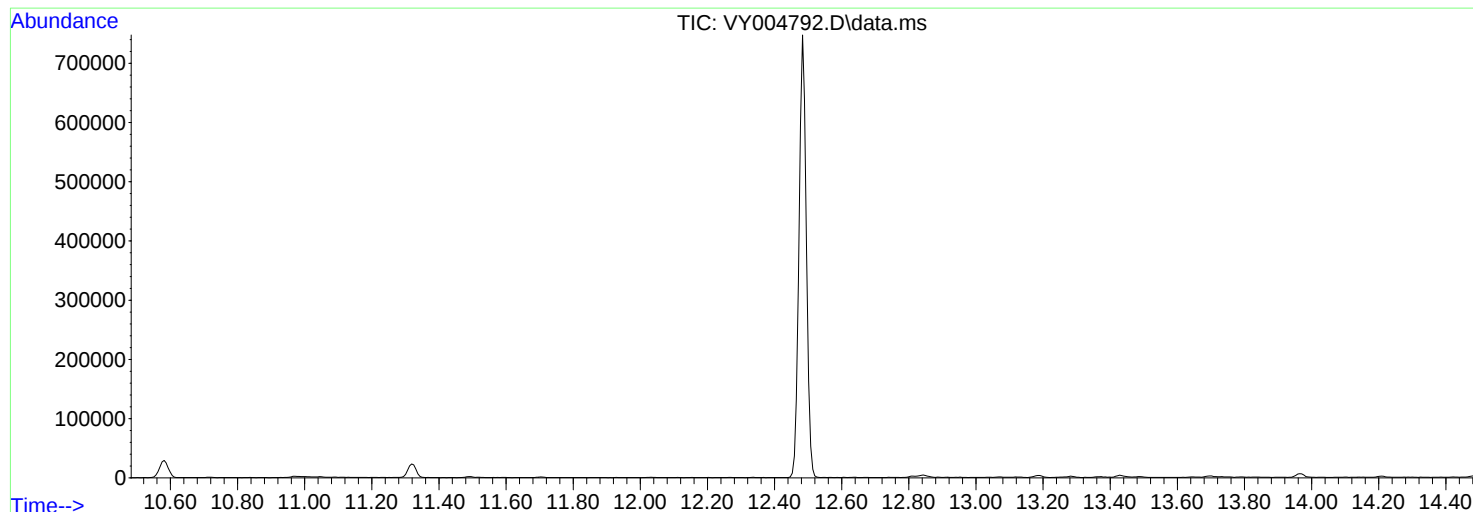

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	27581	PASS
75	95	30	60	54.9	68525	PASS
95	95	100	100	100.0	124707	PASS
96	95	5	9	6.6	8211	PASS
173	174	0.00	2	1.2	1205	PASS
174	95	50	100	80.2	99968	PASS
175	174	5	9	7.6	7573	PASS
176	174	95	101	97.3	97245	PASS
177	176	5	9	6.4	6262	PASS