

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY051820\
 Data File : VY002707.D
 Acq On : 18 May 2020 13:56
 Operator : SY/MD
 Sample : L2686-01
 Misc : 5.36G/5ML/MSVOA Y/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VNJ-214

Quant Time: May 18 23:53:15 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y051520S.M
 Quant Title : SW846 8260
 QLast Update : Sat May 16 04:52:36 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-7.80
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-8.69
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-11.49
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-13.42

System Monitoring Compounds		R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4		0.00	65	0	0.00	ug/l	
Spiked Amount	50.000			Recovery	=	0.00%	
35) Dibromofluoromethane		0.00	113	0	0.00	ug/l	
Spiked Amount	50.000			Recovery	=	0.00%	
50) Toluene-d8		0.00	98	0	0.00	ug/l	
Spiked Amount	50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene		0.00	95	0	0.00	ug/l	
Spiked Amount	50.000			Recovery	=	0.00%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY051820\
Data File : VY002707.D
Acq On : 18 May 2020 13:56
Operator : SY/MD
Sample : L2686-01
Misc : 5.36G/5ML/MSVOA Y/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VNJ-214

Quant Time: May 18 23:53:15 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y051520S.M
Quant Title : SW846 8260
QLast Update : Sat May 16 04:52:36 2020
Response via : Initial Calibration

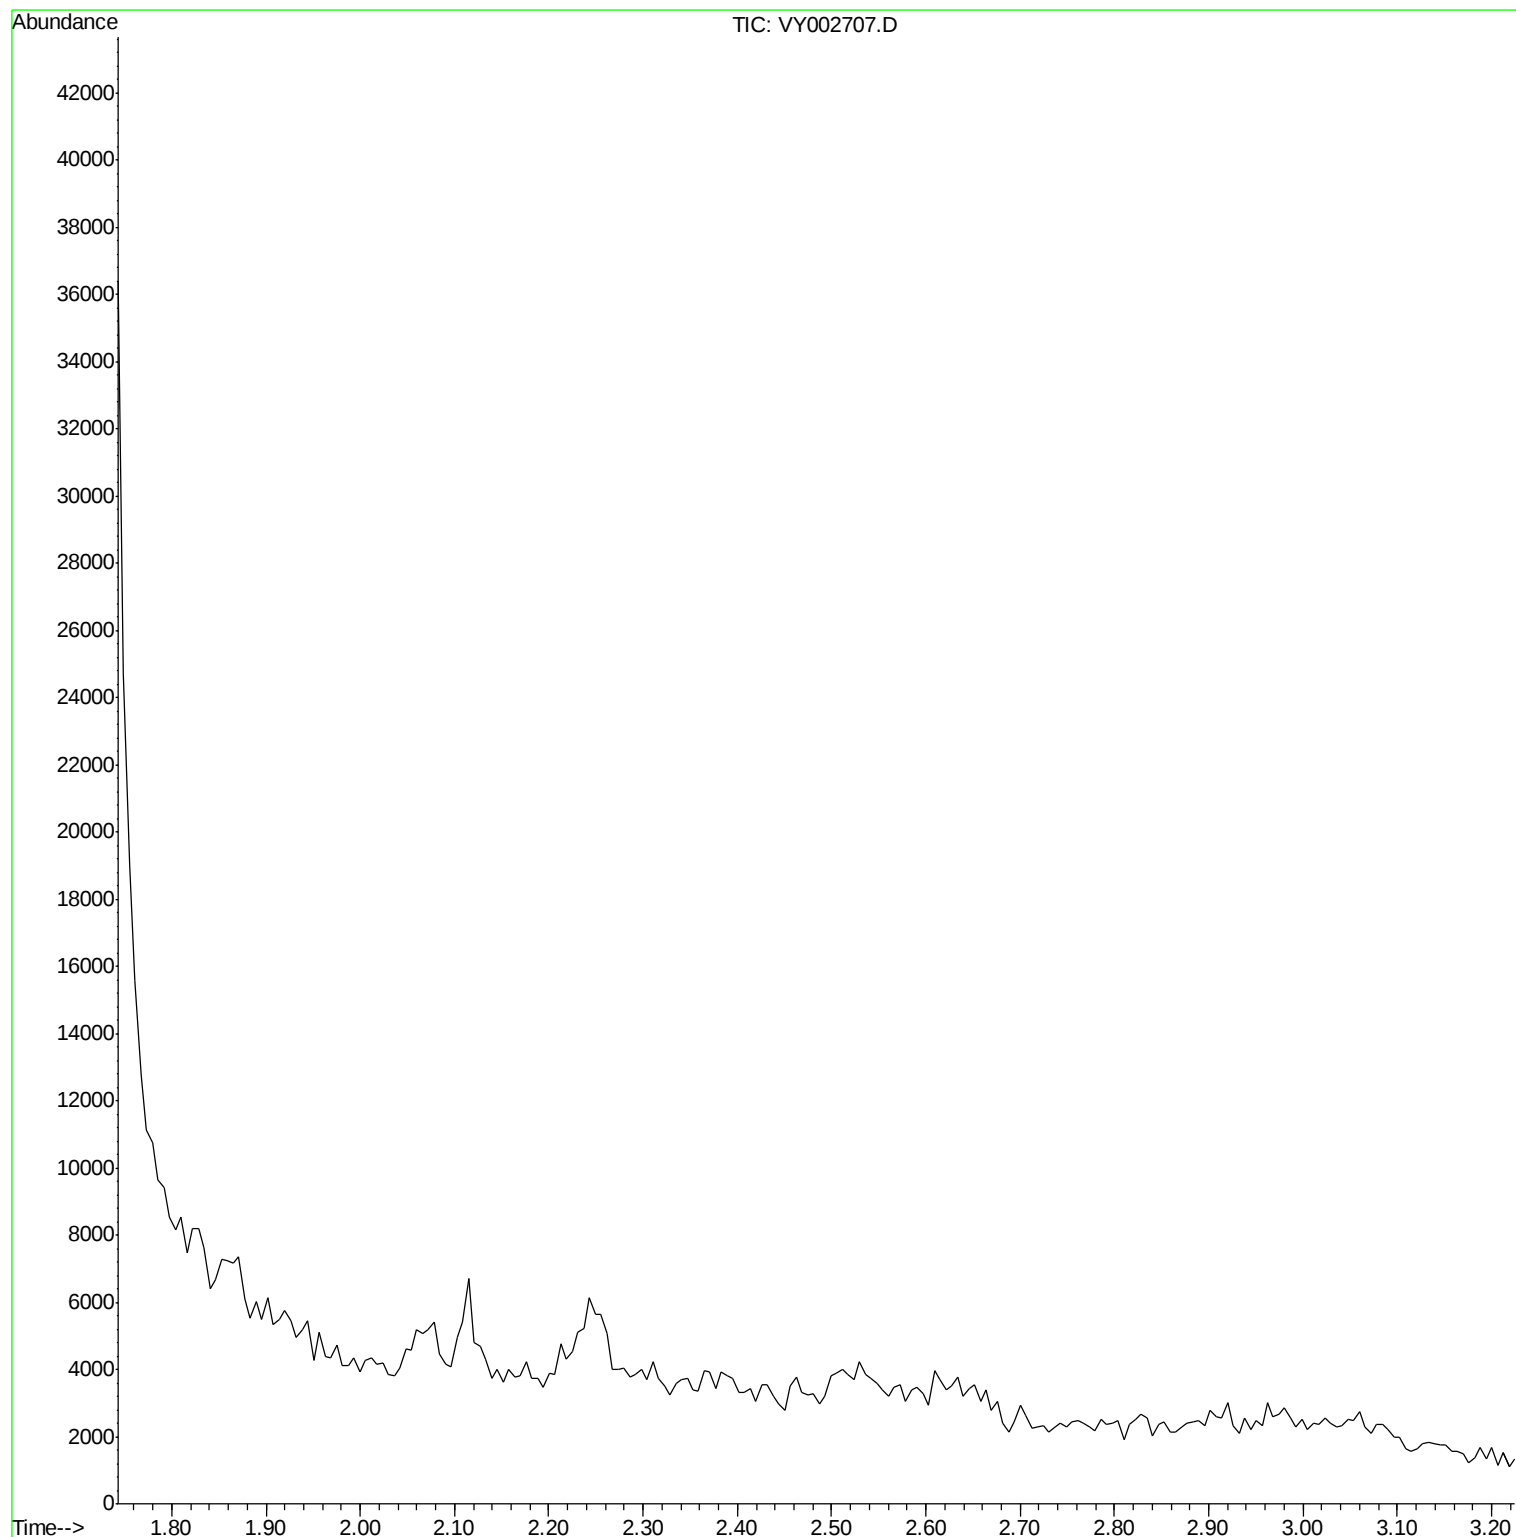


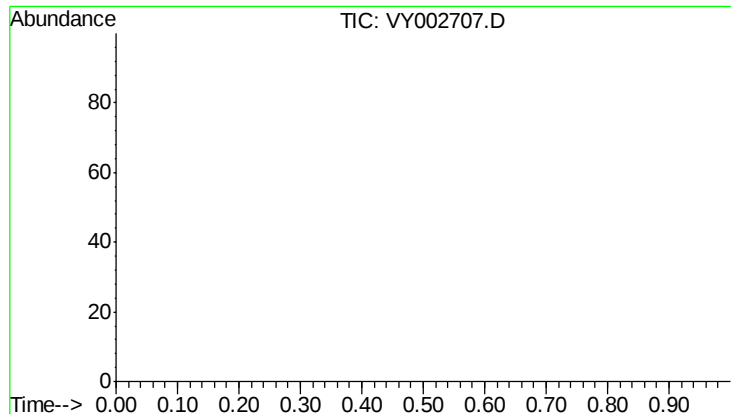


#1
Pentafluorobenzene
Concen: 0.000 ug/l
Expected RT: 7.80 min

Lab File: VY002707.D
Acq: 18 May 2020 13:56

Instrument :
MSVOA_Y
ClientSampleId :
VNJ-214


Tot Ion: 168
Sig Exp Ratio
168 100
99 49.0

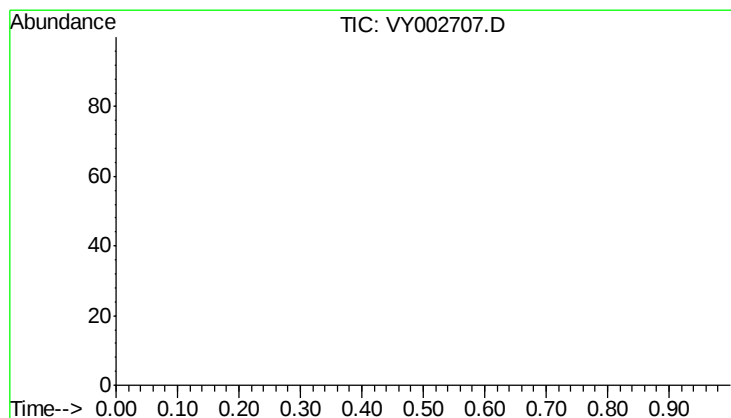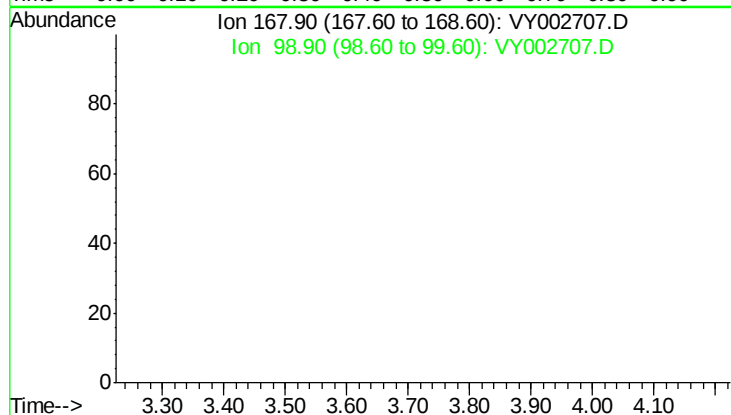


#33
1,2-Dichloroethane-d4
Concen: 0.000 ug/l
Expected RT: 8.15 min

Lab File: VY002707.D
Acq: 18 May 2020 13:56

Tgt Ion: 65
Sig Exp Ratio
65 100
67 54.5


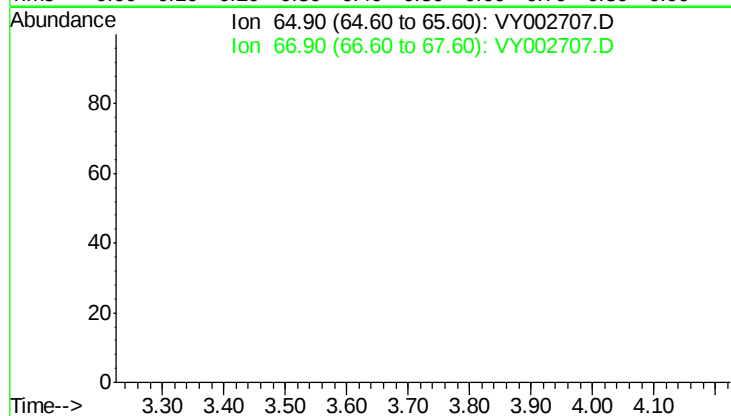


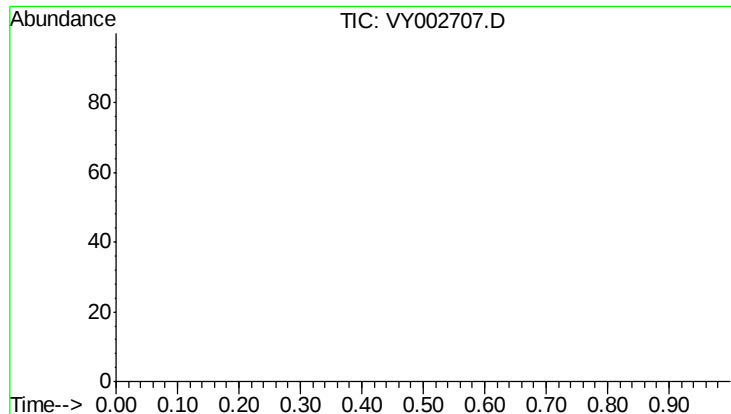

#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 8.69 min
 Lab File: VY002707.D
 Acq: 18 May 2020 13:56


Instrument :
 MSVOA_Y
 ClientSampleId :
 VNJ-214


Tot Ion	114
Sig	Exp Ratio
114	100
63	17.7
88	14.7

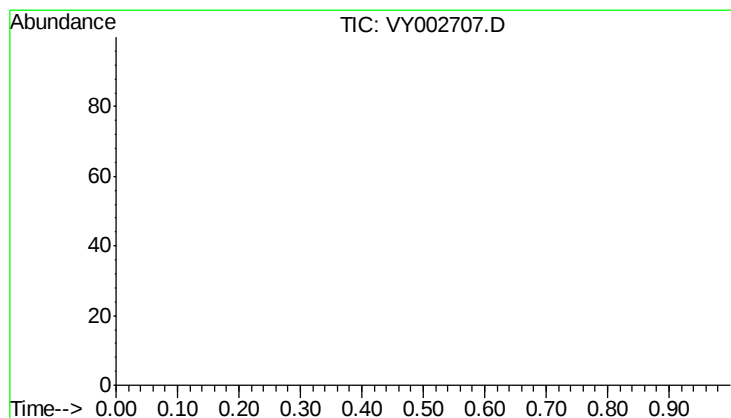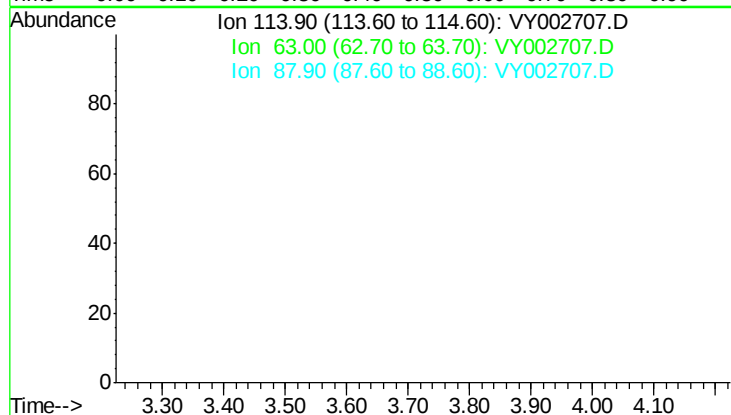

#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 7.72 min
 Lab File: VY002707.D
 Acq: 18 May 2020 13:56

Tgt Ion	113
Sig	Exp Ratio
113	100
111	102.4
192	23.2

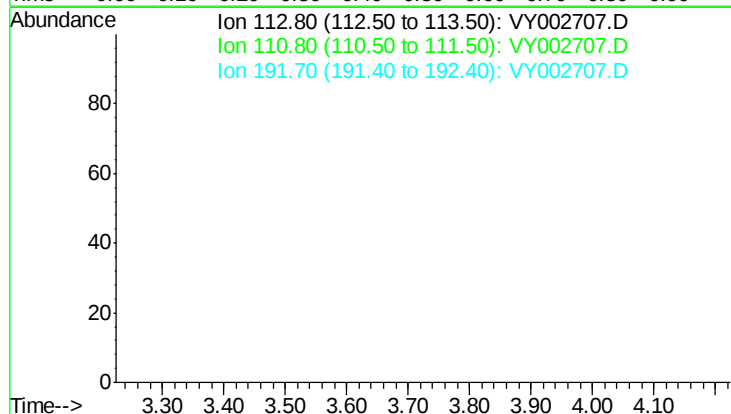


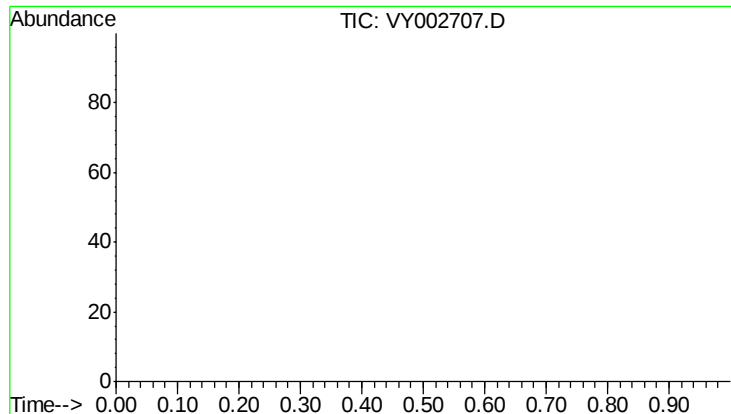


#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 10.18 min

Lab File: VY002707.D
Acq: 18 May 2020 13:56

Instrument :
MSVOA_Y
ClientSampleId :
VNJ-214


Tot Ion	Sig	Exp Ratio
98	100	
100	65.4	

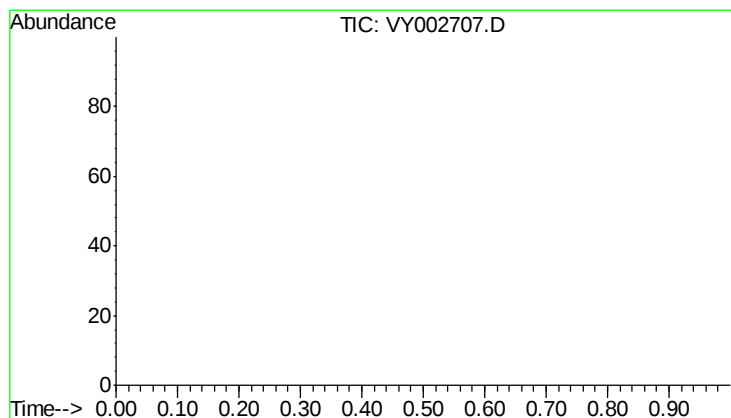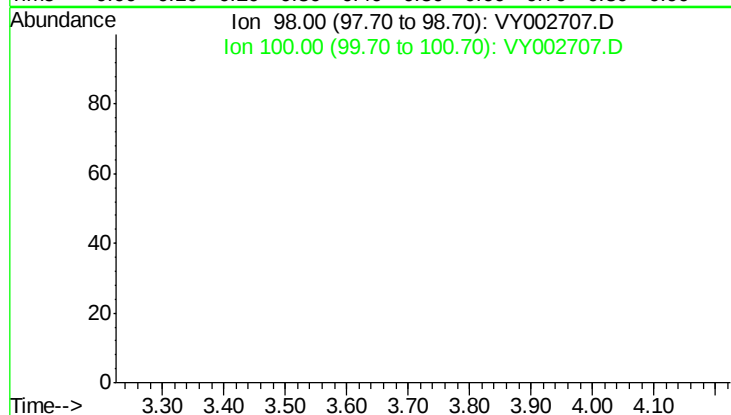


#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
Expected RT: 12.48 min

Lab File: VY002707.D
Acq: 18 May 2020 13:56

Tgt Ion	Sig	Exp Ratio
95	100	
174	95.7	
176	93.0	


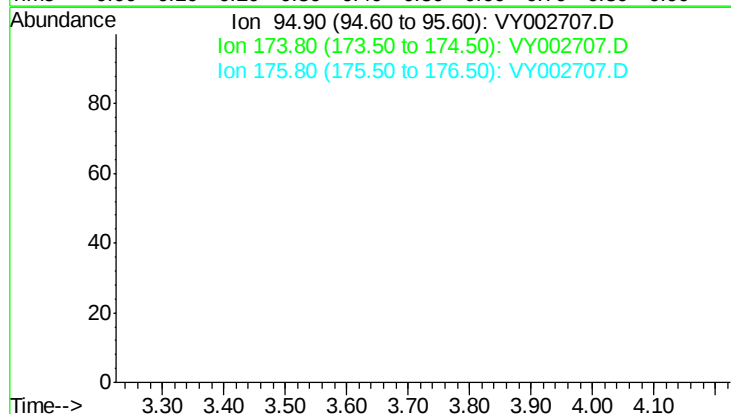


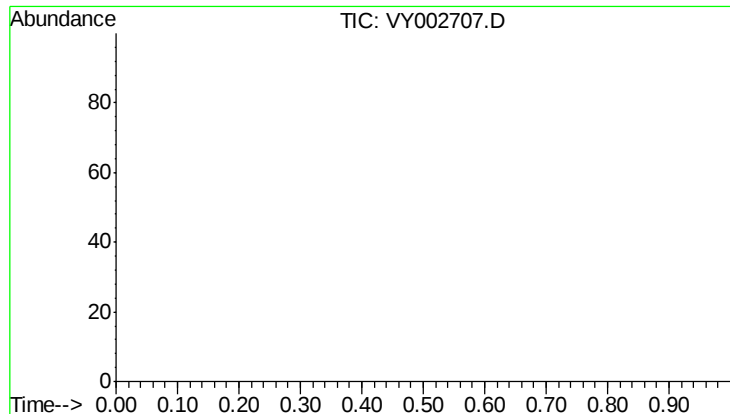

#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 11.49 min
 Lab File: VY002707.D
 Acq: 18 May 2020 13:56

Instrument :
 MSVOA_Y
 ClientSampleId :
 VNJ-214

Tot Ion: 117
 Sig Exp Ratio
 117 100
 82 50.4
 119 32.8

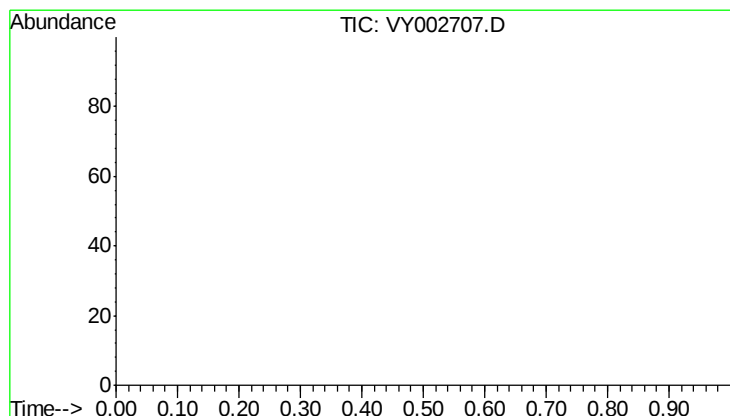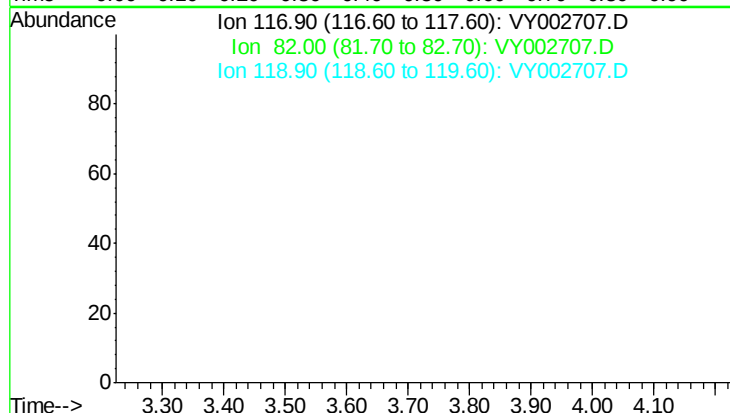

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 13.42 min
 Lab File: VY002707.D
 Acq: 18 May 2020 13:56

Tgt Ion: 152
 Sig Exp Ratio
 152 100
 115 54.4
 150 171.9

