

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051821\
 Data File : VY004818.D
 Acq On : 18 May 2021 11:22
 Operator : SY/MD
 Sample : VY0518SBL01
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0518SBL01

Quant Time: May 19 01:01:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051021S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 11 04:13:44 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.795	168	166071	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	305768	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	298818	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	134363	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	117180	59.28	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	118.56%
35) Dibromofluoromethane	7.728	113	96607	57.71	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	115.42%
50) Toluene-d8	10.185	98	384589	50.86	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	101.72%
62) 4-Bromofluorobenzene	12.483	95	130979	51.32	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	102.64%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051821\
Data File : VY004818.D
Acq On : 18 May 2021 11:22
Operator : SY/MD
Sample : VY0518SBL01
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0518SBL01

Quant Time: May 19 01:01:19 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051021S.M
Quant Title : SW846 8260
QLast Update : Tue May 11 04:13:44 2021
Response via : Initial Calibration




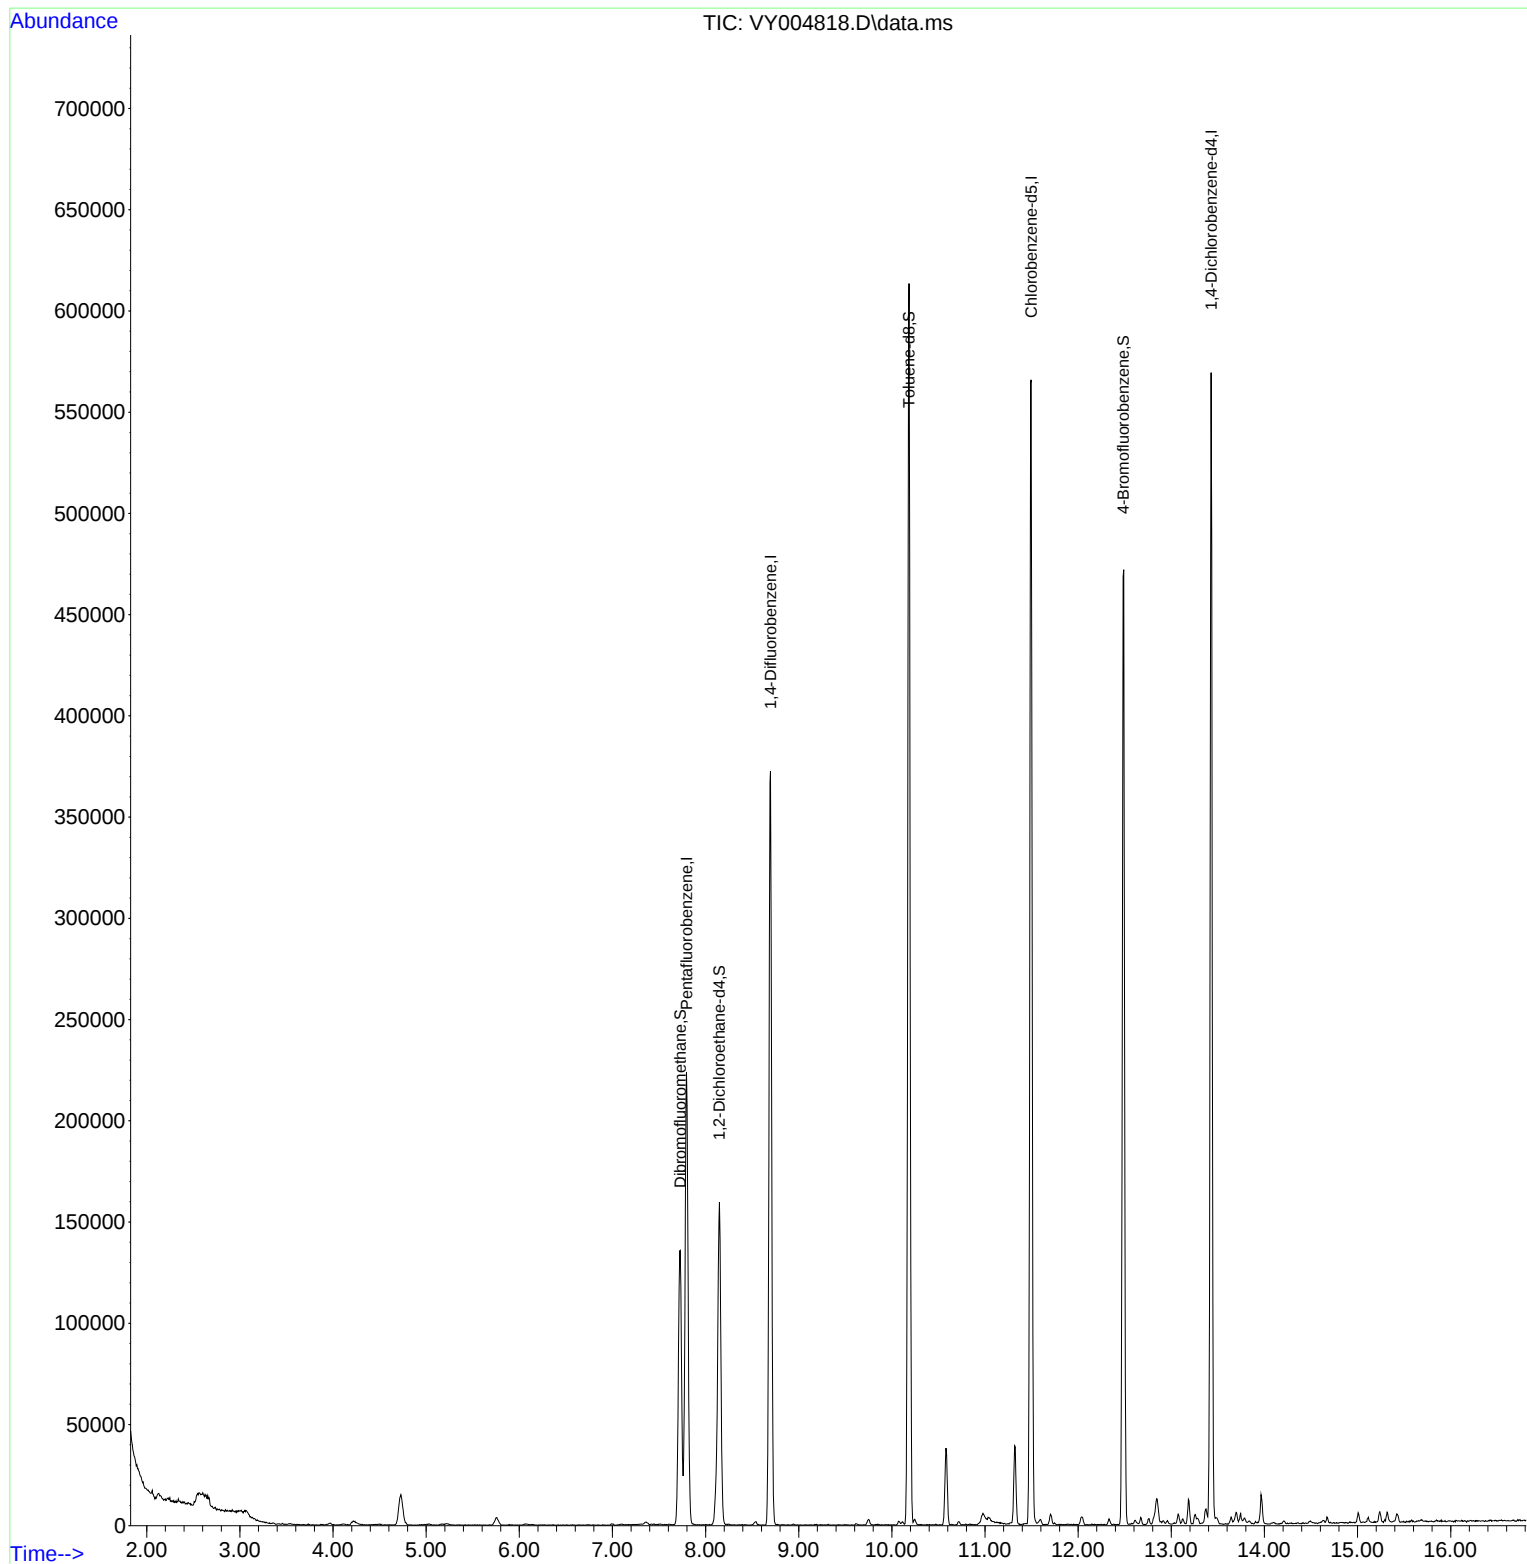


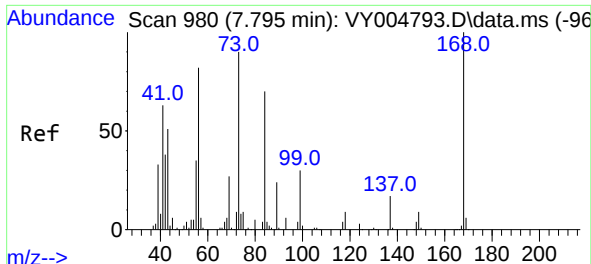

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.795 min Scan# 980
Delta R.T. -0.000 min
Lab File: VY004818.D
Acq: 18 May 2021 11:22




Instrument :
MSVOA_Y
ClientSampleId :
VY0518SBL01


Tgt Ion:168 Resp: 166071
Ion Ratio Lower Upper
168 100
99 57.5 45.6 68.4

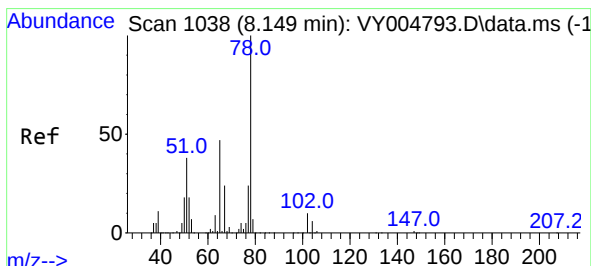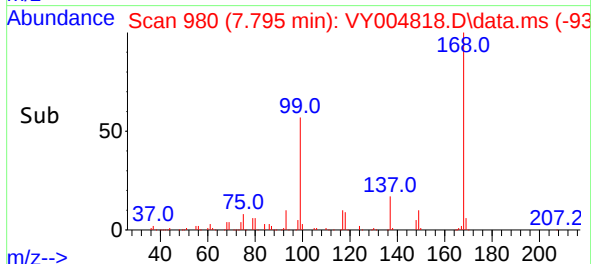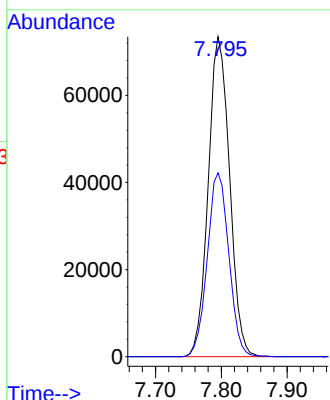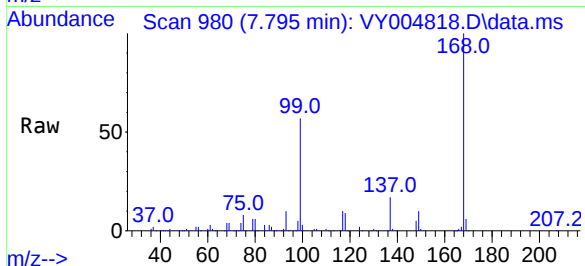

#33
1,2-Dichloroethane-d4
Concen: 59.28 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. -0.000 min
Lab File: VY004818.D
Acq: 18 May 2021 11:22

Tgt Ion: 65 Resp: 117180
Ion Ratio Lower Upper
65 100
67 53.4 0.0 108.0

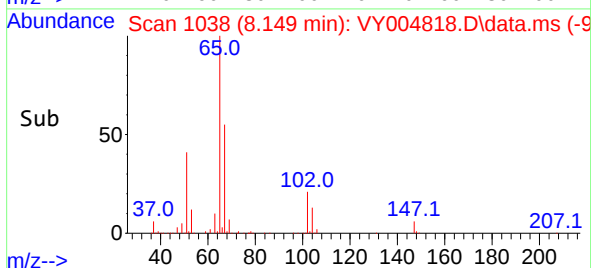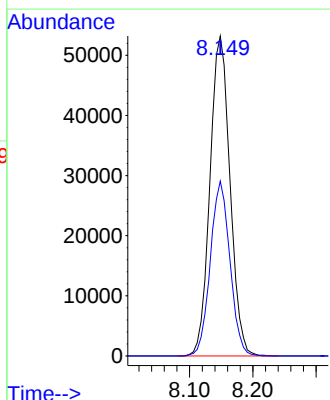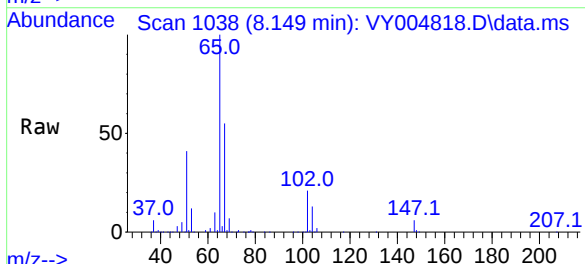




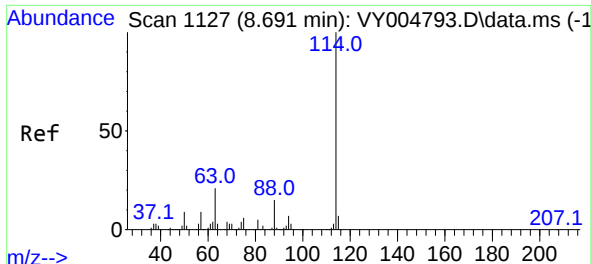


#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. -0.000 min
Lab File: VY004818.D
Acq: 18 May 2021 11:22

Instrument :
MSVOA_Y
ClientSampleId :
VY0518SBL01

Tgt Ion:114 Resp: 305768




Ion	Ratio	Lower	Upper
114	100		
63	20.9	0.0	42.8
88	15.3	0.0	31.0

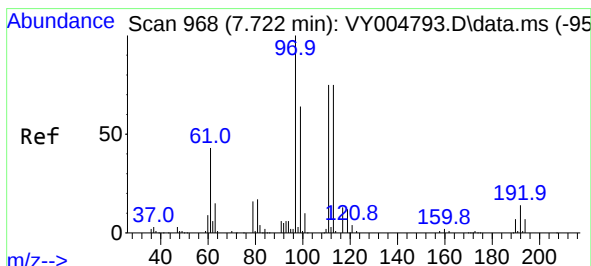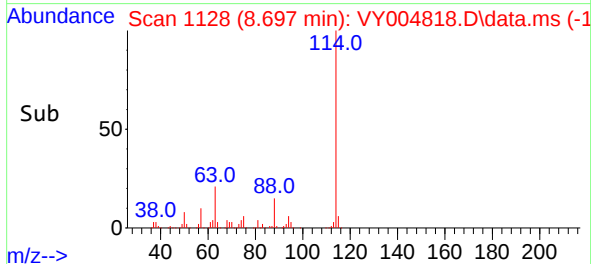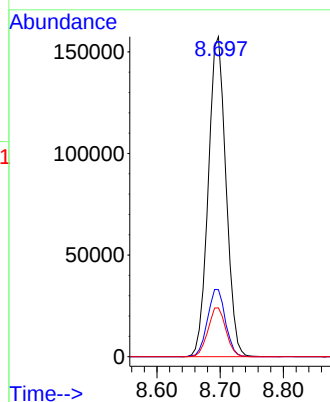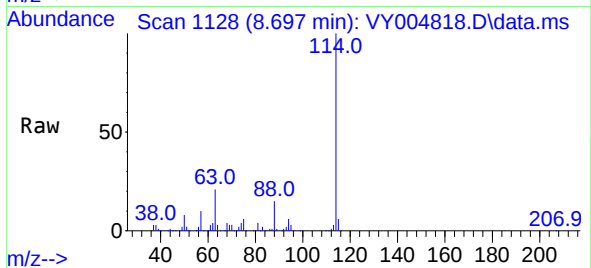


#35
Dibromofluoromethane
Concen: 57.71 ug/l
RT: 7.728 min Scan# 969
Delta R.T. -0.000 min
Lab File: VY004818.D
Acq: 18 May 2021 11:22

Tgt Ion:113 Resp: 96607

Ion	Ratio	Lower	Upper
113	100		
111	102.6	80.5	120.7
192	18.8	15.0	22.6


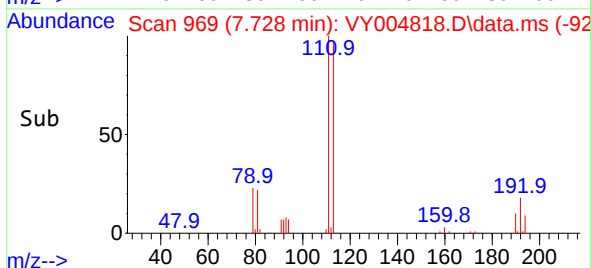
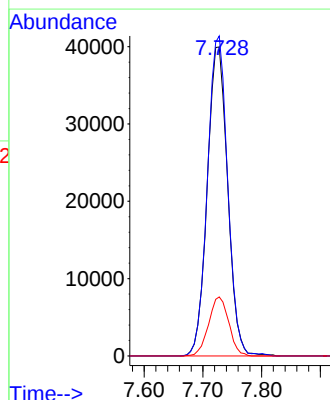
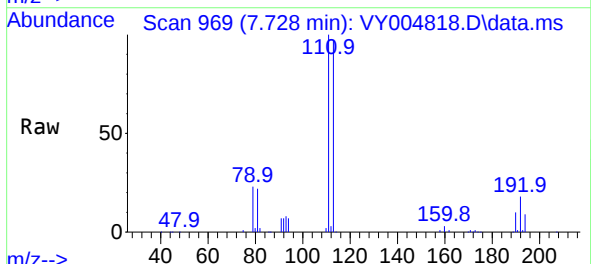


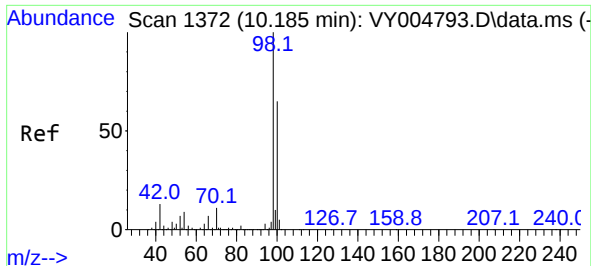

#50
Toluene-d8
Concen: 50.86 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. -0.000 min
Lab File: VY004818.D
Acq: 18 May 2021 11:22




Instrument :
MSVOA_Y
ClientSampleId :
VY0518SBL01


Tgt Ion: 98 Resp: 384589
Ion Ratio Lower Upper
98 100
100 64.1 51.5 77.3

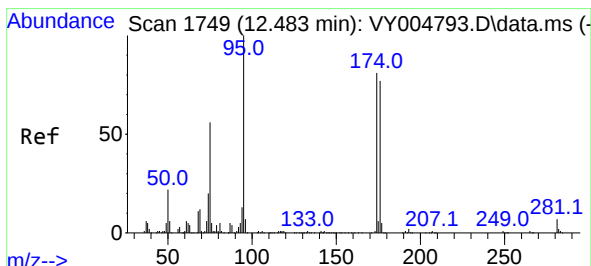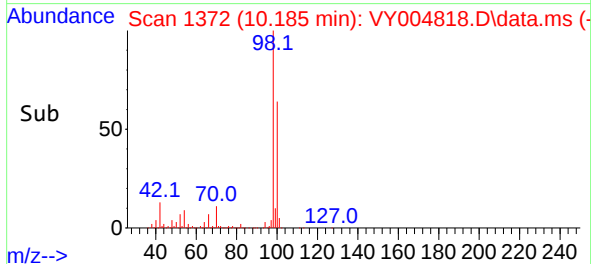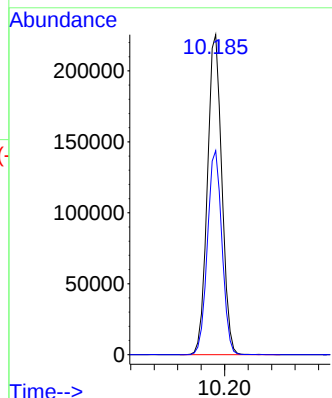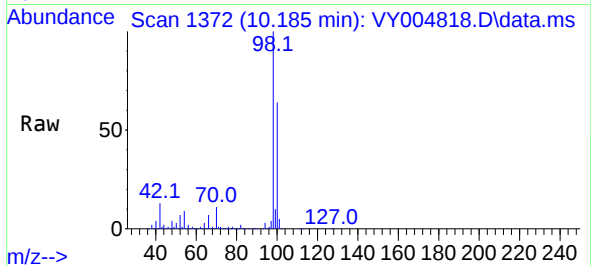

#62
4-Bromofluorobenzene
Concen: 51.32 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY004818.D
Acq: 18 May 2021 11:22

Tgt Ion: 95 Resp: 130979
Ion Ratio Lower Upper
95 100
174 80.3 0.0 164.2
176 77.8 0.0 159.0


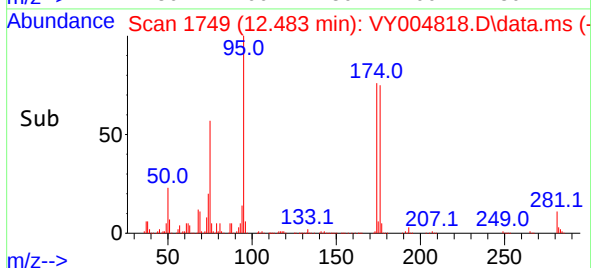
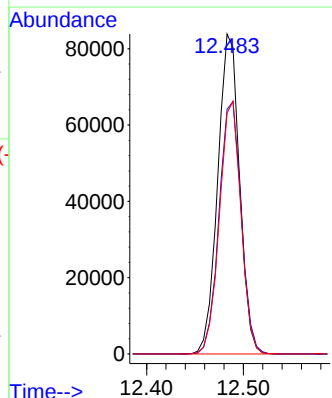
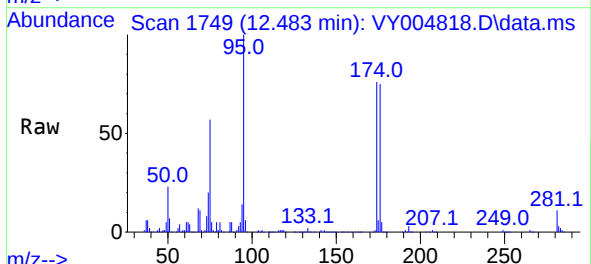


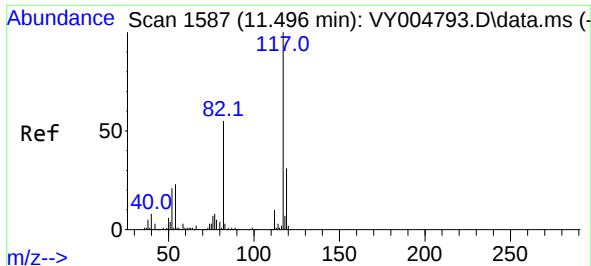

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.496 min Scan# 1587
Delta R.T. 0.006 min
Lab File: VY004818.D
Acq: 18 May 2021 11:22

Instrument :
MSVOA_Y
ClientSampleId :
VY0518SBL01

Tgt Ion:117 Resp: 298818
Ion Ratio Lower Upper
117 100
82 56.1 45.4 68.2
119 32.4 25.8 38.6

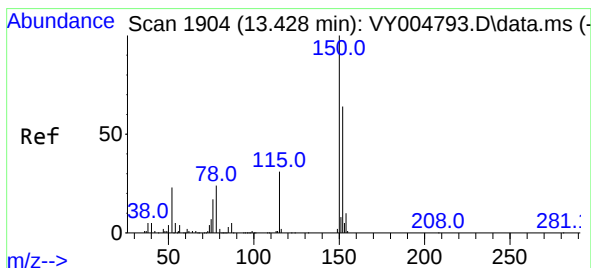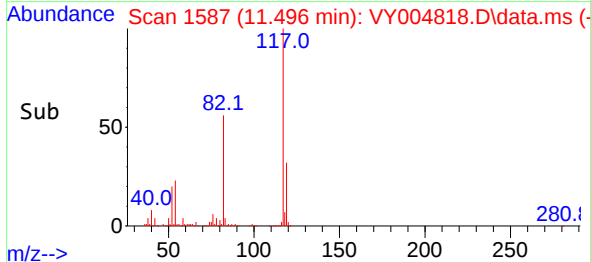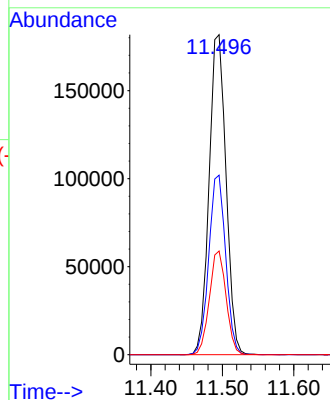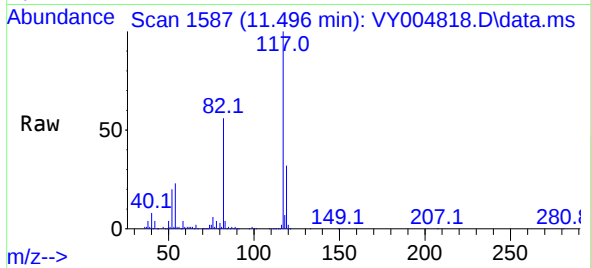

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY004818.D
Acq: 18 May 2021 11:22

Tgt Ion:152 Resp: 134363
Ion Ratio Lower Upper
152 100
115 58.5 29.4 88.3
150 157.2 0.0 349.8

