

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051822\
 Data File : VY008849.D
 Acq On : 19 May 2022 05:42
 Operator : KP/MD
 Sample : N2868-02
 Misc : 5.10g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 P017-SS001-0612-01

Quant Time: May 19 06:57:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051722S.M
 Quant Title : SW846 8260
 QLast Update : Wed May 18 07:32:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	102436	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	180216	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	167045	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	69535	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	60113	63.257	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	126.520%
35) Dibromofluoromethane	7.715	113	56345	53.511	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	107.020%
50) Toluene-d8	10.178	98	224720	48.139	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	96.280%
62) 4-Bromofluorobenzene	12.483	95	61477	37.726	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	75.460%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051822\
Data File : VY008849.D
Acq On : 19 May 2022 05:42
Operator : KP/MD
Sample : N2868-02
Misc : 5.10g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
P017-SS001-0612-01


Quant Time: May 19 06:57:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051722S.M
Quant Title : SW846 8260
QLast Update : Wed May 18 07:32:50 2022
Response via : Initial Calibration

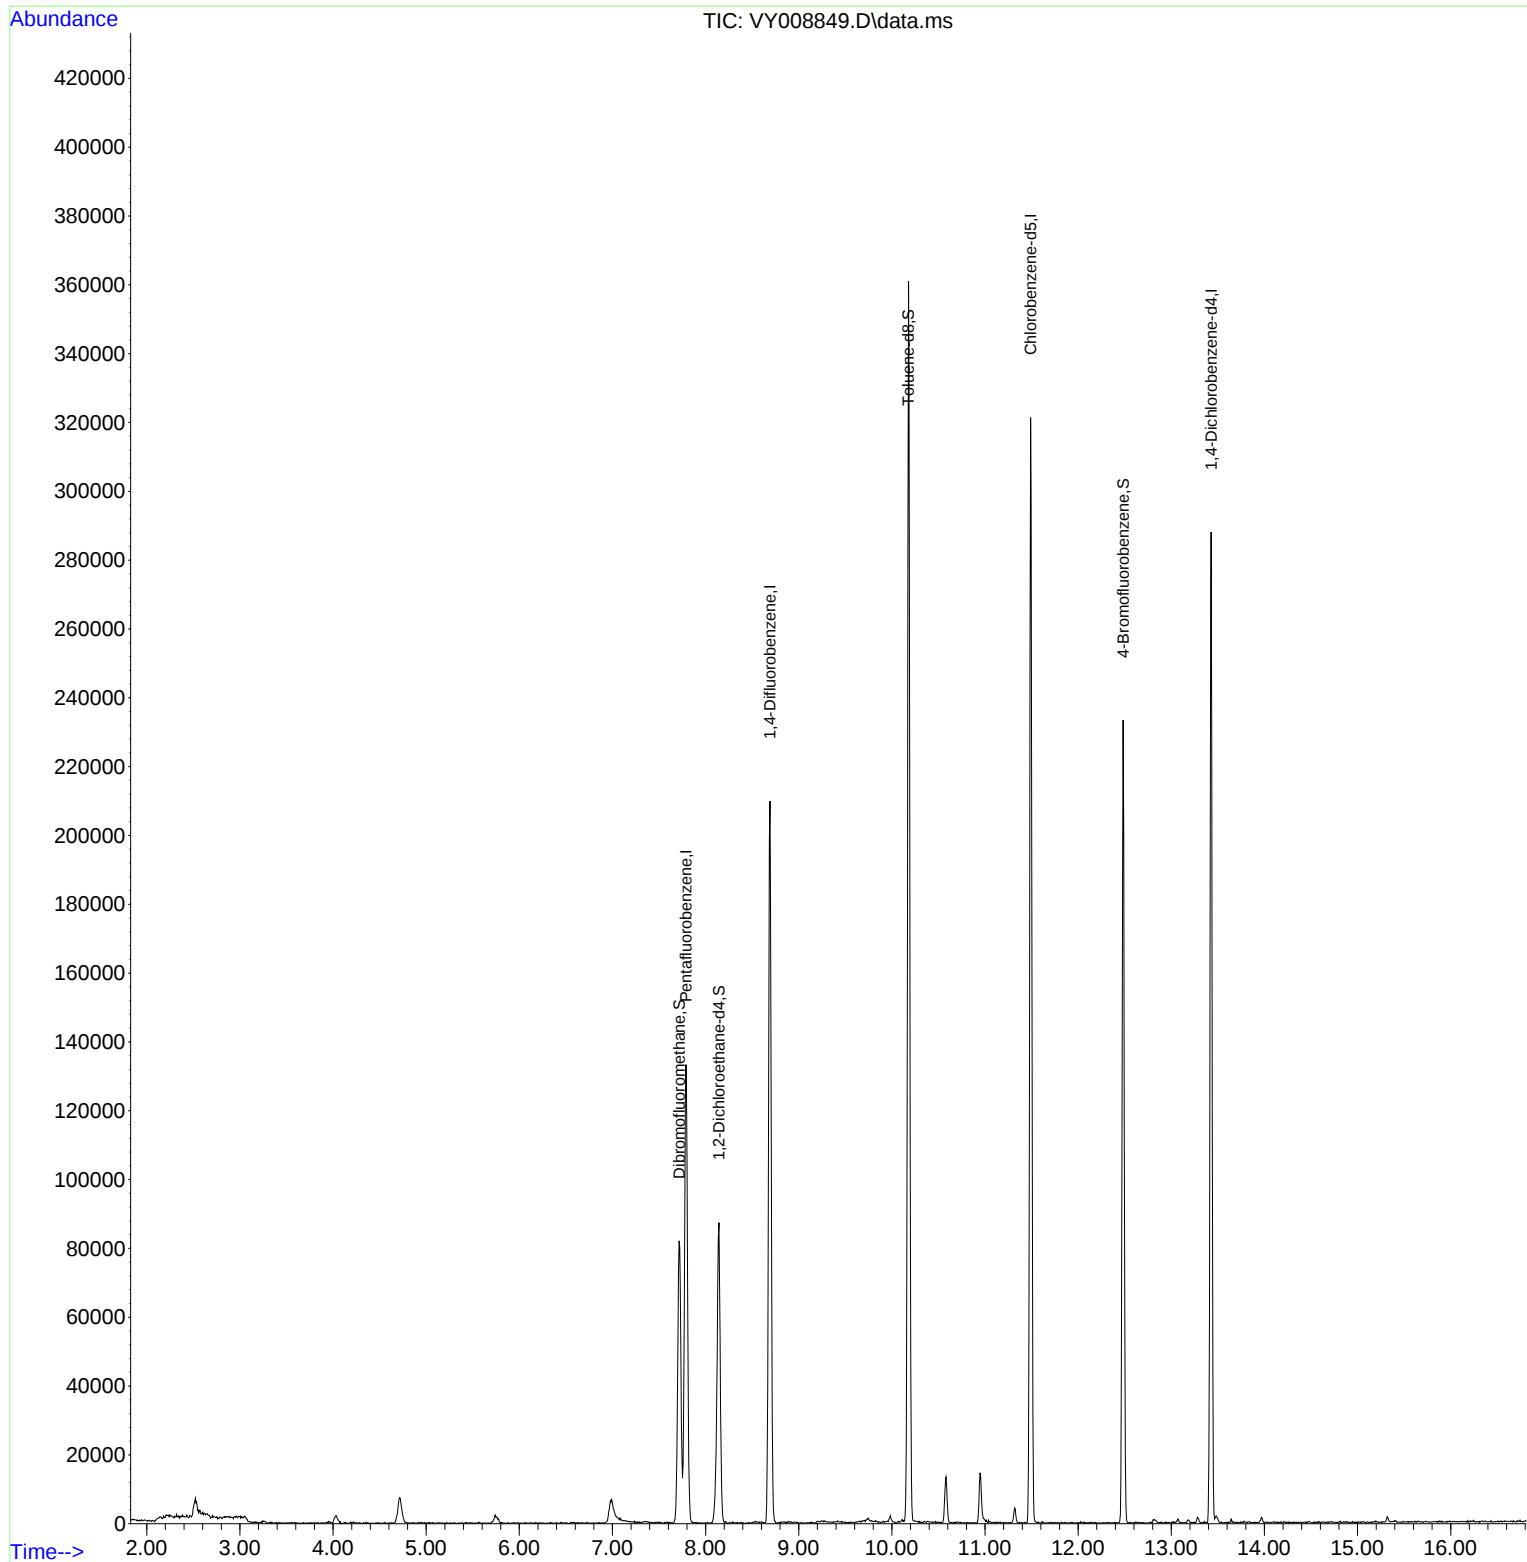



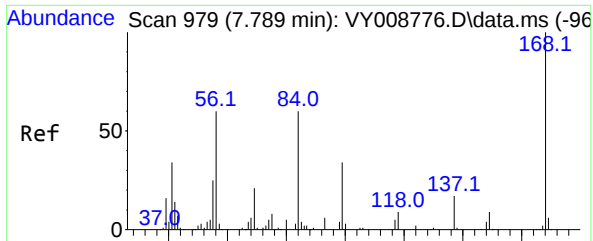


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY008849.D
Acq: 19 May 2022 05:42


Instrument :
MSVOA_Y
ClientSampleId :
P017-SS001-0612-01

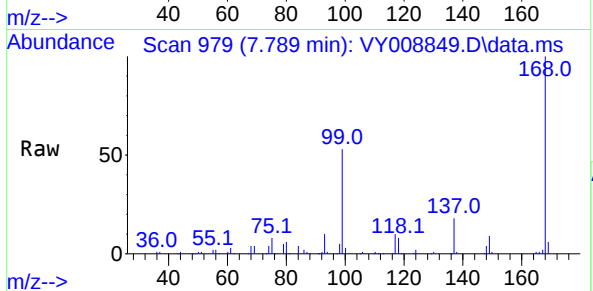



Tgt Ion:168 Resp: 102436
Ion Ratio Lower Upper
168 100
99 53.4 46.9 70.3

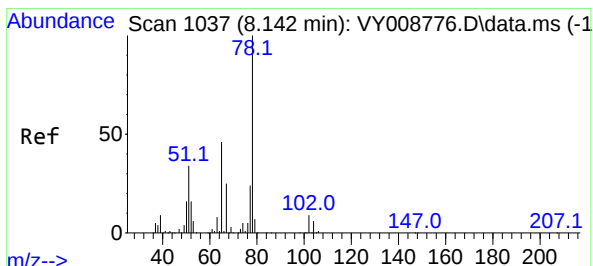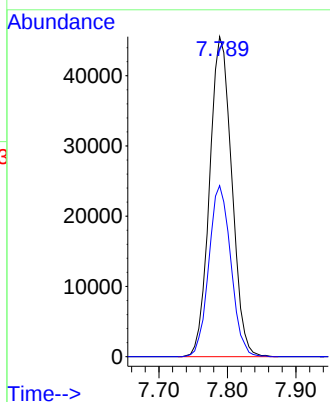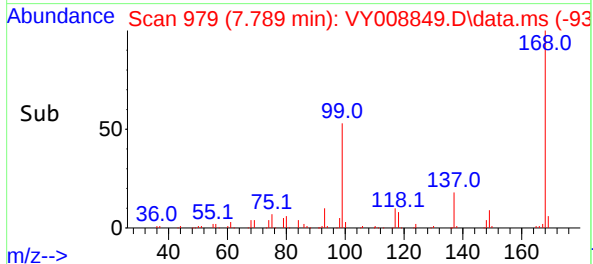


#33
1,2-Dichloroethane-d4
Concen: 63.257 ug/l
RT: 8.142 min Scan# 1037
Delta R.T. -0.000 min
Lab File: VY008849.D
Acq: 19 May 2022 05:42

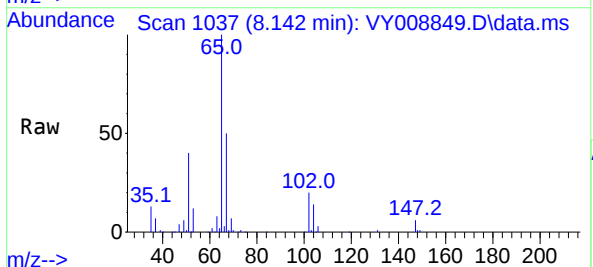

Tgt Ion: 65 Resp: 60113
Ion Ratio Lower Upper
65 100
67 52.8 0.0 99.4

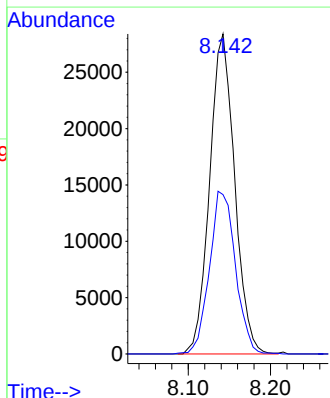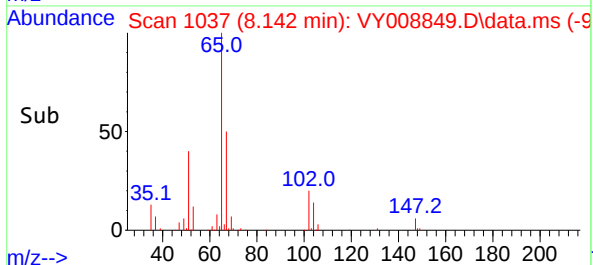

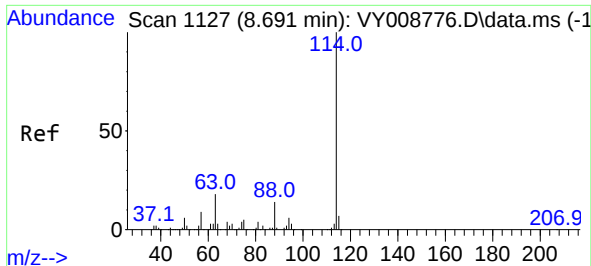

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. -0.000 min

Lab File: VY008849.D

Acq: 19 May 2022 05:42

Instrument :

MSVOA_Y

ClientSampleId :

P017-SS001-0612-01





Tgt Ion:114 Resp: 180216

Ion Ratio Lower Upper

114 100

63 20.0 0.0 43.2

88 14.2 0.0 31.8

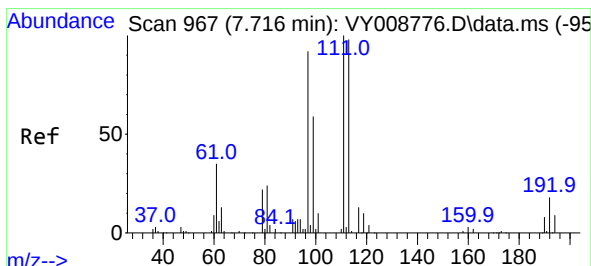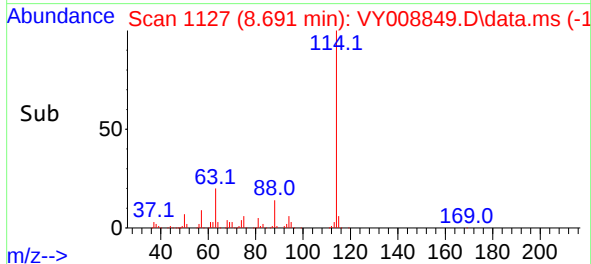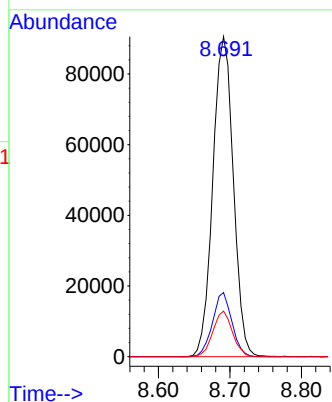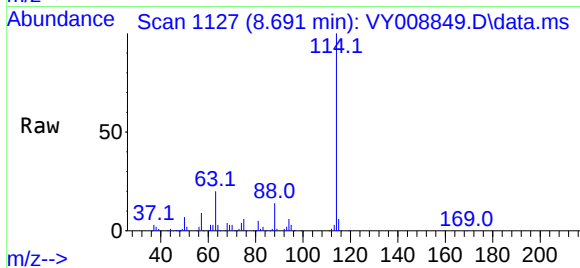

#35

Dibromofluoromethane

Concen: 53.511 ug/l

RT: 7.715 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY008849.D

Acq: 19 May 2022 05:42




Tgt Ion:113 Resp: 56345

Ion Ratio Lower Upper

113 100

111 105.8 82.6 124.0

192 18.9 17.6 26.4

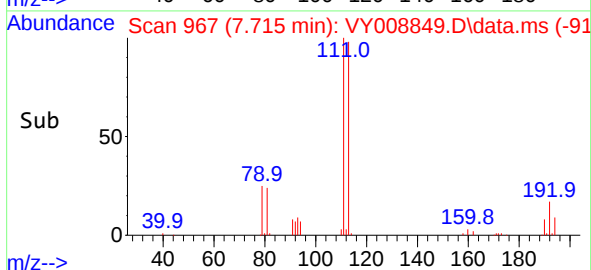
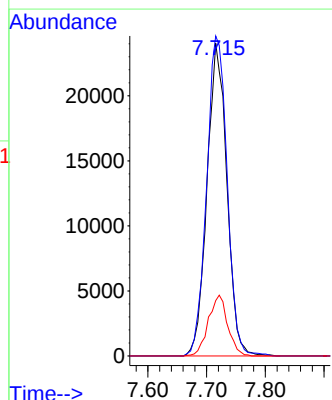
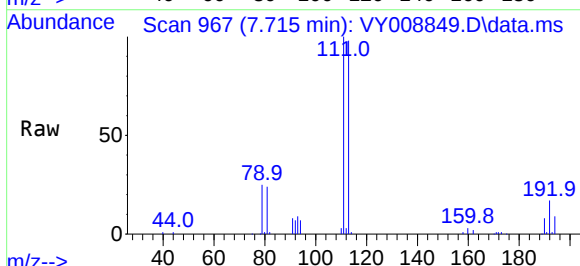




#50
Toluene-d8
Concen: 48.139 ug/l
RT: 10.178 min Scan# 11
Delta R.T. -0.001 min
Lab File: VY008849.D
Acq: 19 May 2022 05:42




Instrument :
MSVOA_Y
ClientSampleId :
P017-SS001-0612-01

Tgt Ion: 98 Resp: 224720
Ion Ratio Lower Upper
98 100
100 64.2 50.2 75.2

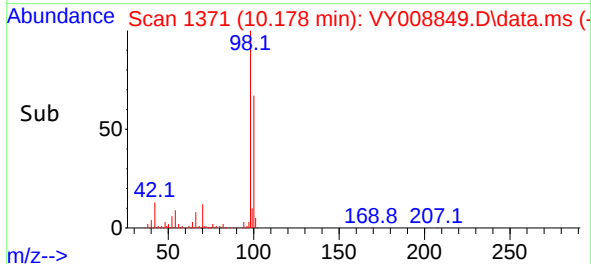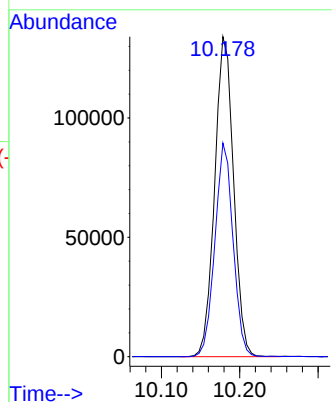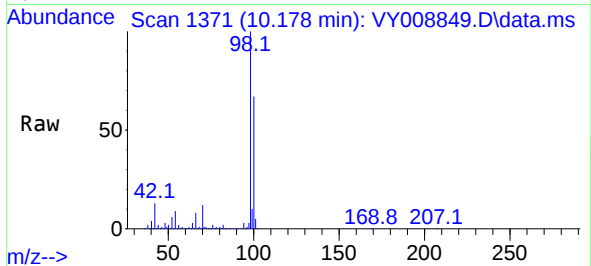

#62
4-Bromofluorobenzene
Concen: 37.726 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY008849.D
Acq: 19 May 2022 05:42

Tgt Ion: 95 Resp: 61477
Ion Ratio Lower Upper
95 100
174 90.3 0.0 177.0
176 87.8 0.0 175.8


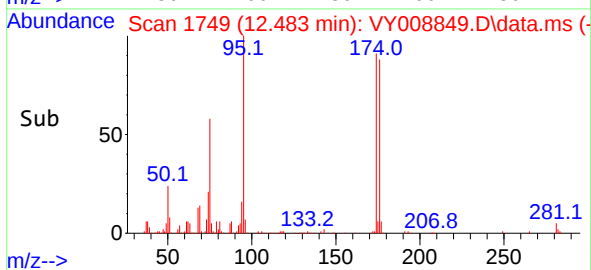
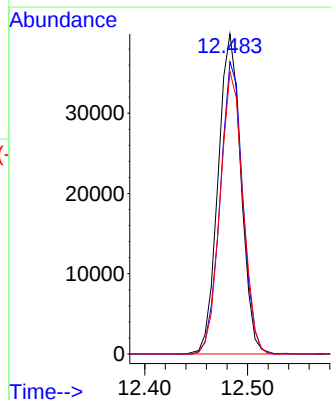
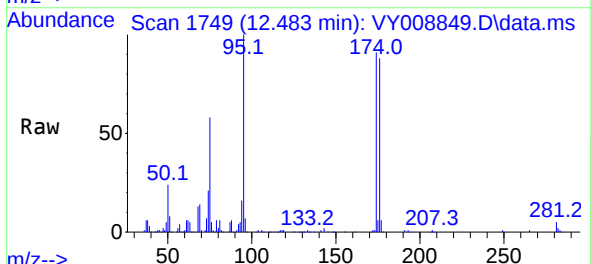




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 117
Delta R.T. -0.000 min
Lab File: VY008849.D
Acq: 19 May 2022 05:42

Instrument :
MSVOA_Y
ClientSampleId :
P017-SS001-0612-01

Tgt Ion:	117	Resp:	167045
Ion	Ratio	Lower	Upper
117	100		
82	53.7	43.0	64.4
119	33.2	25.4	38.0

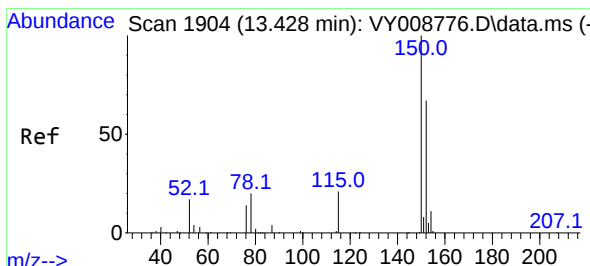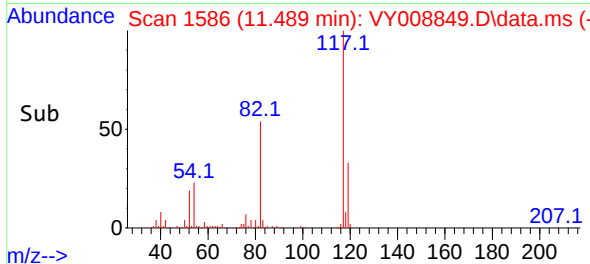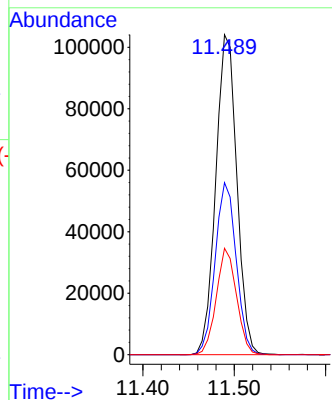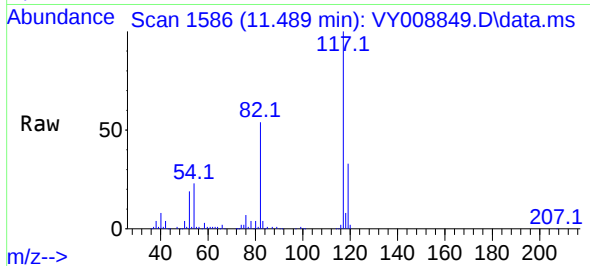

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY008849.D
Acq: 19 May 2022 05:42

Tgt Ion:	152	Resp:	69535
Ion	Ratio	Lower	Upper
152	100		
115	56.3	28.2	84.7
150	155.6	0.0	347.6

