


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051822\
Data File : VY008830.D
Acq On : 18 May 2022 21:54
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051722S.M
Title : SW846 8260
Last Update : Wed May 18 07:32:50 2022

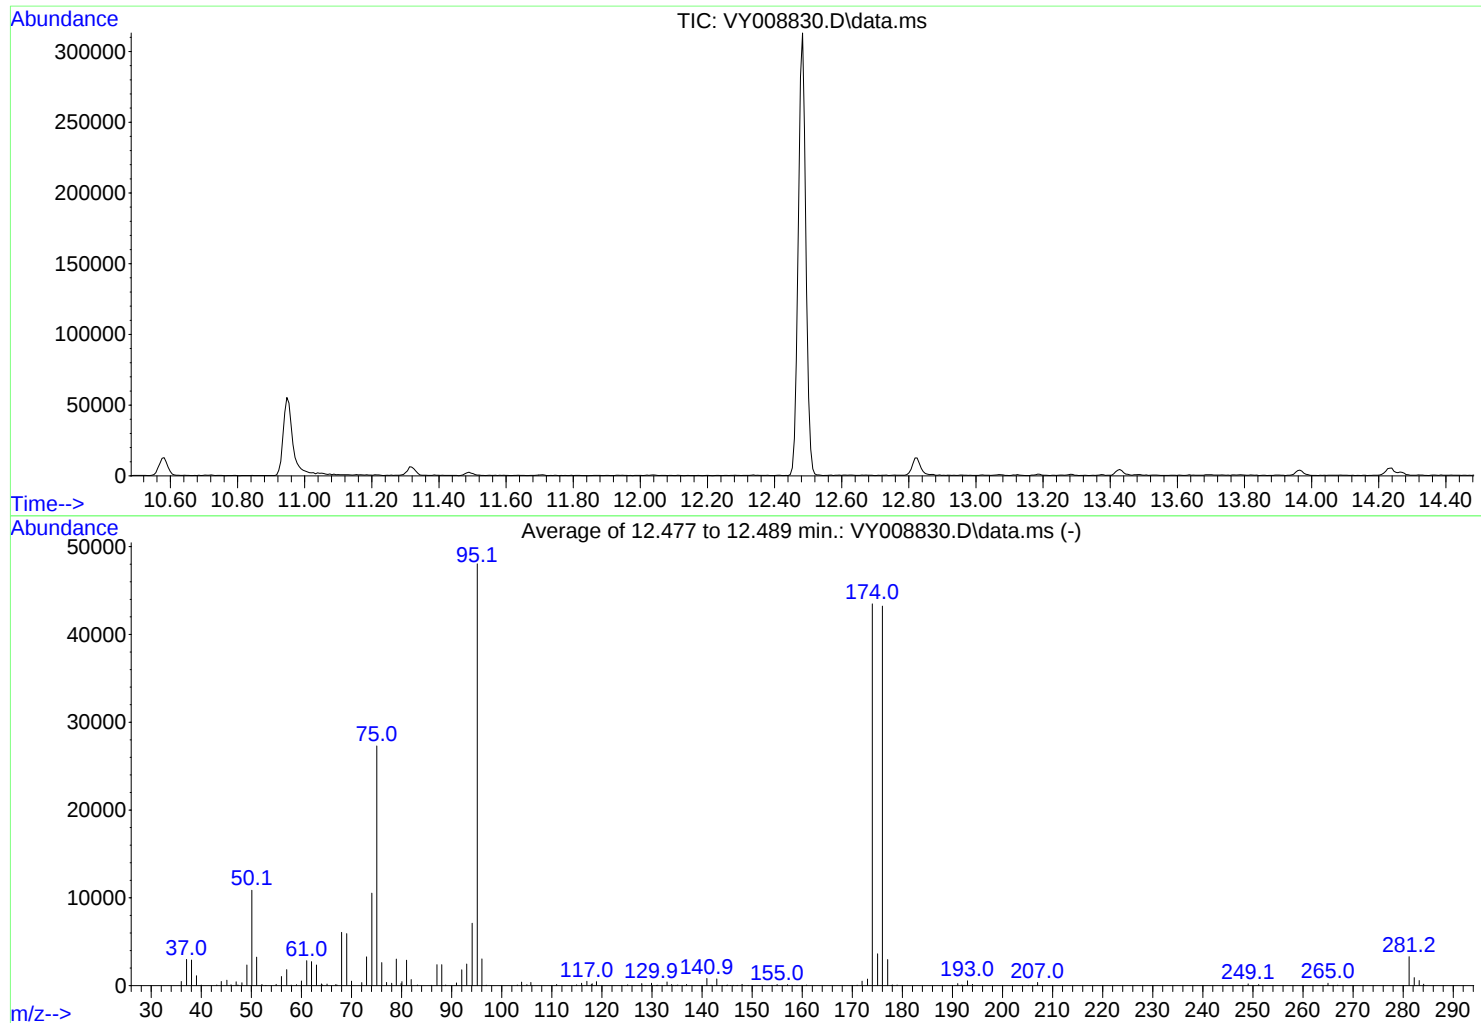

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.6	10859	PASS
75	95	30	60	56.8	27301	PASS
95	95	100	100	100.0	48043	PASS
96	95	5	9	6.3	3037	PASS
173	174	0.00	2	1.7	742	PASS
174	95	50	100	90.5	43488	PASS
175	174	5	9	8.3	3626	PASS
176	174	95	101	99.4	43227	PASS
177	176	5	9	6.9	2980	PASS