

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY052020\
 Data File : VY002729.D
 Acq On : 20 May 2020 14:57
 Operator : SY/MD
 Sample : L2718-02
 Misc : 6.60G/5ML/MSVOA Y/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 72-12017

Quant Time: May 21 04:11:41 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y051520S.M
 Quant Title : SW846 8260
 QLast Update : Sat May 16 04:52:36 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.80	168	352998	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.69	114	555361	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.49	117	505764	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.42	152	245843	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.15	65	155013	56.14	ug/l	0.00
Spiked Amount 50.000			Recovery	=	112.28%	
35) Dibromofluoromethane	7.72	113	164836	53.78	ug/l	0.00
Spiked Amount 50.000			Recovery	=	107.56%	
50) Toluene-d8	10.18	98	648674	52.57	ug/l	0.00
Spiked Amount 50.000			Recovery	=	105.14%	
62) 4-Bromofluorobenzene	12.48	95	216808	51.12	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.24%	
Target Compounds						
95) Naphthalene	15.23	128	15326	1.602	ug/l #	Qvalue 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY052020\
Data File : VY002729.D
Acq On : 20 May 2020 14:57
Operator : SY/MD
Sample : L2718-02
Misc : 6.60G/5ML/MSVOA Y/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
72-12017

Quant Time: May 21 04:11:41 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y051520S.M
Quant Title : SW846 8260
QLast Update : Sat May 16 04:52:36 2020
Response via : Initial Calibration

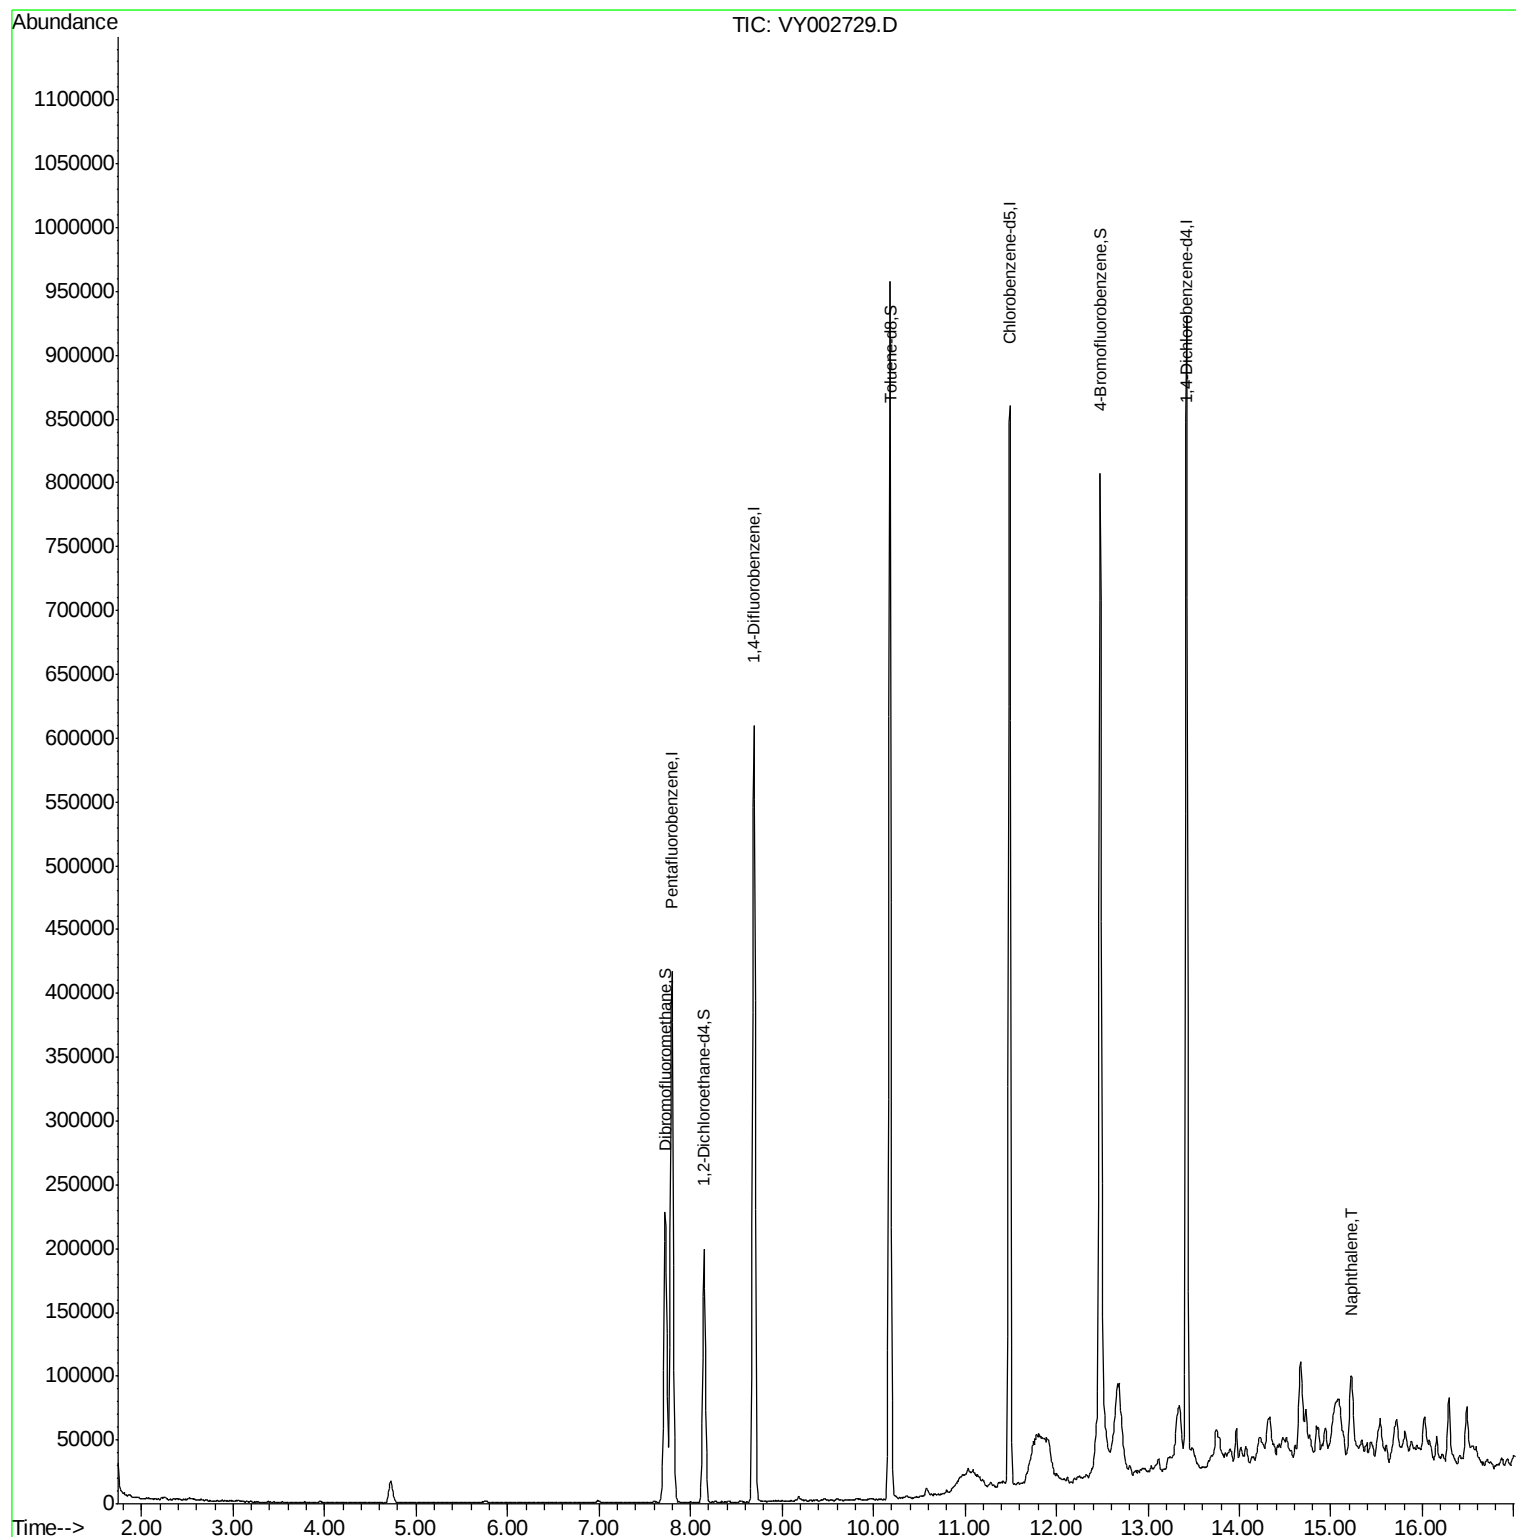

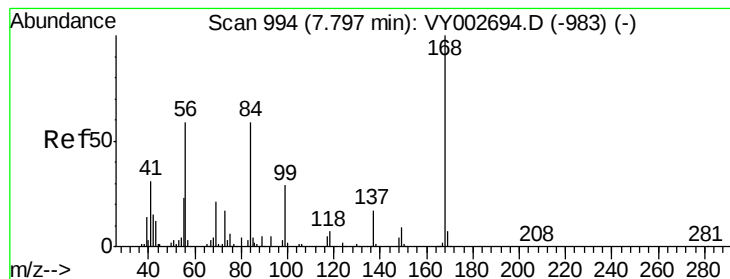

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.80 min Scan# 994

Delta R.T. -0.00 min

Lab File: VY002729.D

Acq: 20 May 2020 14:57

Instrument :

MSVOA_Y

ClientSampleId :


72-12017

Tot Ion:168 Resp: 352998

Ion Ratio Lower Upper

168 100

99 48.6 39.2 58.8



Abundance Ion 167.90 (167.60 to 168.60): VY002729.D (-945) (-)

Ion 98.90 (98.60 to 99.60): VY002729.D (-945) (-)

7.80



150000

100000

50000

0

Time-->

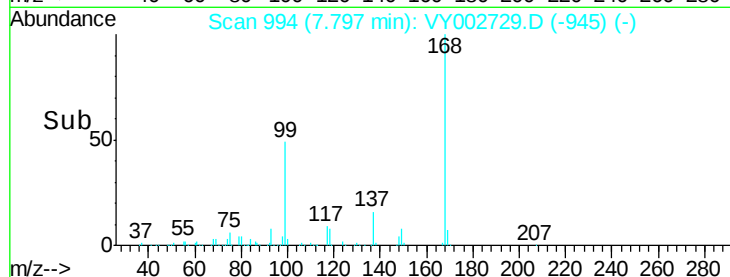

#33

1,2-Dichloroethane-d4

Concen: 56.140 ug/l

RT: 8.15 min Scan# 1052

Delta R.T. -0.00 min

Lab File: VY002729.D


Acq: 20 May 2020 14:57

Tgt Ion: 65 Resp: 155013

Ion Ratio Lower Upper

65 100

67 54.2 0.0 109.0



Abundance Ion 64.90 (64.60 to 65.60): VY002729.D (-1003) (-)

Ion 66.90 (66.60 to 67.60): VY002729.D (-1003) (-)

8.15

80000


60000


40000

20000

0

Time-->

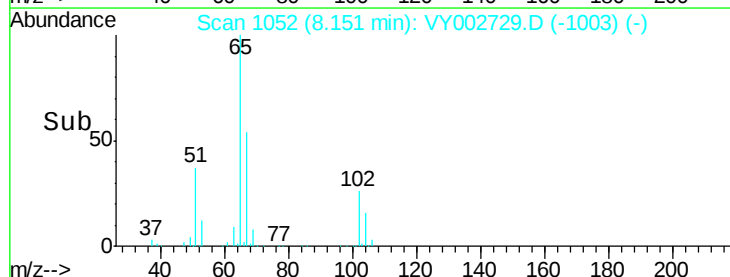

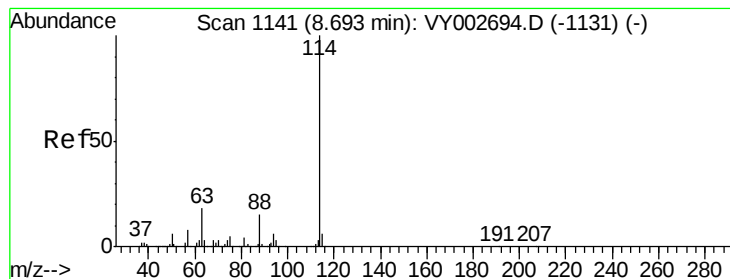

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.69 min Scan# 1141

Delta R.T. -0.00 min

Lab File: VY002729.D

Acq: 20 May 2020 14:57

Instrument :

MSVOA_Y

ClientSampleId :

72-12017


Tot Ion:114 Resp: 555361

Ion Ratio Lower Upper

114 100

63 17.9 0.0 35.4




88 14.5 0.0 29.4



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VY0

Ion 87.90 (87.60 to 88.60): VY0

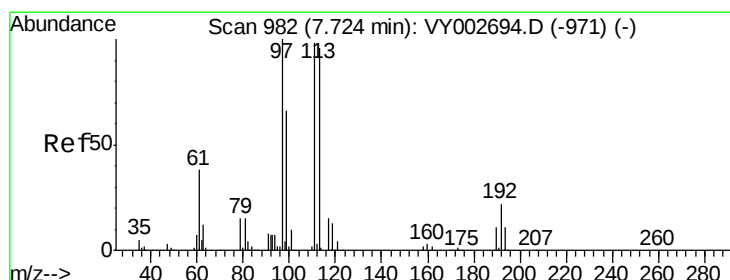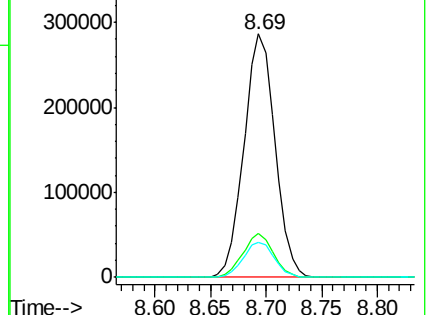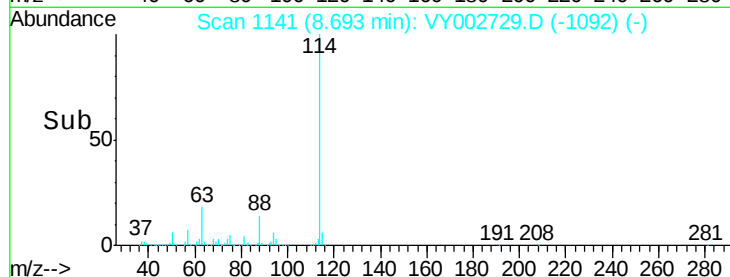

#35

Dibromofluoromethane

Concen: 53.782 ug/l

RT: 7.72 min Scan# 982

Delta R.T. -0.00 min

Lab File: VY002729.D

Acq: 20 May 2020 14:57


Tgt Ion:113 Resp: 164836

Ion Ratio Lower Upper

113 100

111 102.7 81.9 122.9



192 23.3 18.6 27.8




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

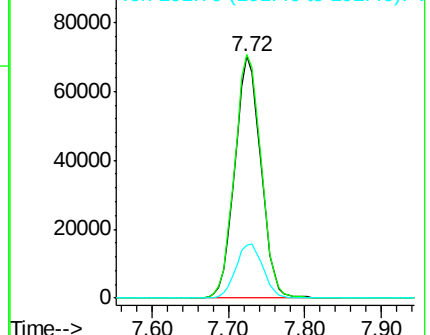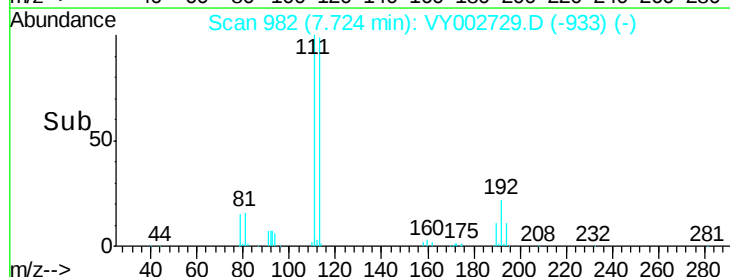

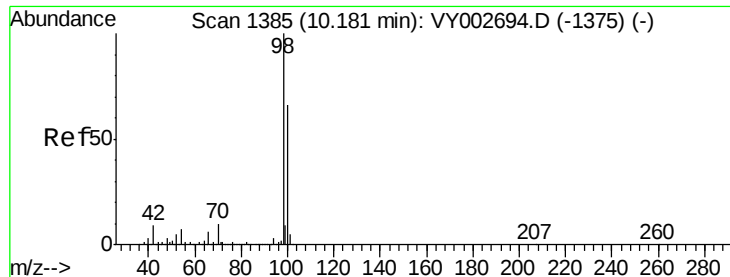

#50

Toluene-d8

Concen: 52.569 ug/l

RT: 10.18 min Scan# 1385

Delta R.T. -0.00 min

Lab File: VY002729.D

Acq: 20 May 2020 14:57

Instrument :

MSVOA_Y

ClientSampleId :





72-12017

Tot Ion: 98 Resp: 648674

Ion Ratio Lower Upper

98 100

100 65.1 52.3 78.5

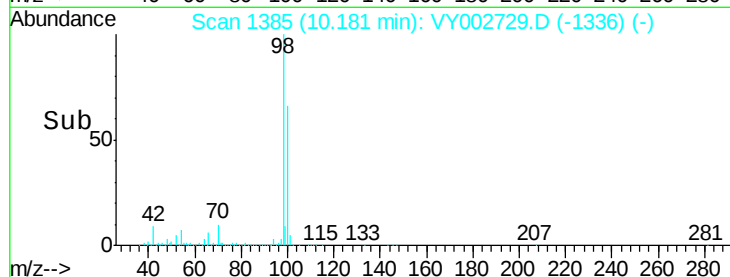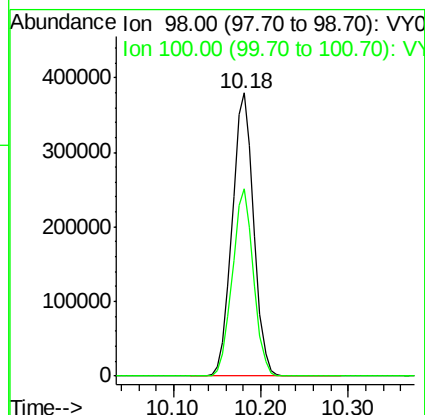

#62

4-Bromofluorobenzene

Concen: 51.120 ug/l

RT: 12.48 min Scan# 1762

Delta R.T. -0.00 min

Lab File: VY002729.D

Acq: 20 May 2020 14:57




Tgt Ion: 95 Resp: 216808


Ion Ratio Lower Upper

95 100

174 93.9 0.0 191.4

176 91.0 0.0 186.0

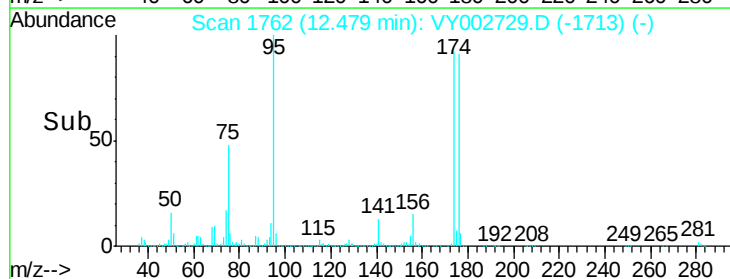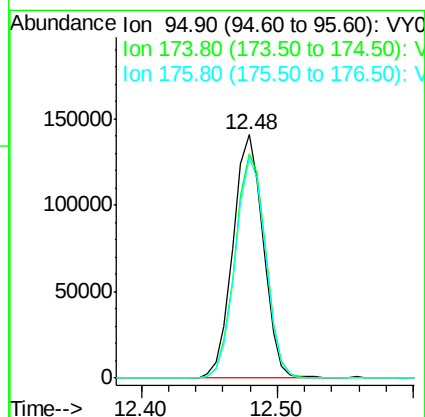

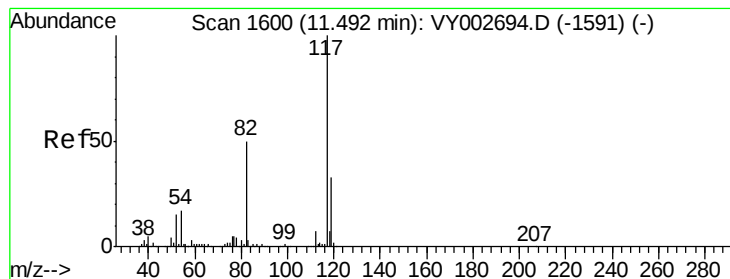

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.49 min Scan# 1600

Delta R.T. -0.00 min

Lab File: VY002729.D

Acq: 20 May 2020 14:57

Instrument :

MSVOA_Y

ClientSampleId :

72-12017


Tot Ion:117 Resp: 505764

Ion Ratio Lower Upper

117 100

82 49.4 40.3 60.5




119 32.1 26.2 39.4



Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VY0

Ion 118.90 (118.60 to 119.60): V

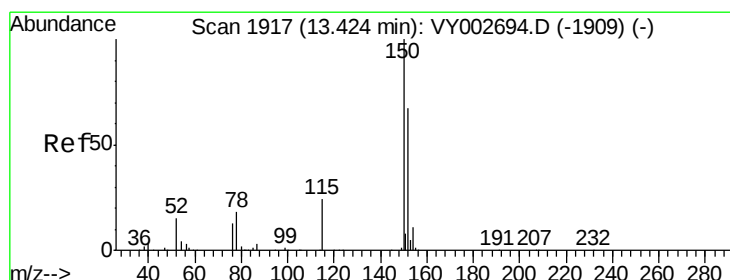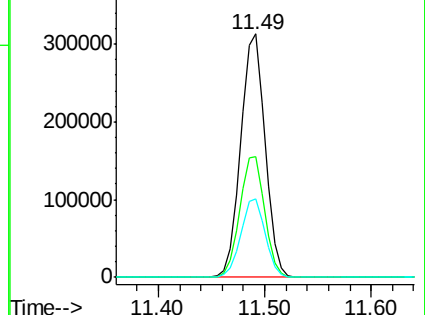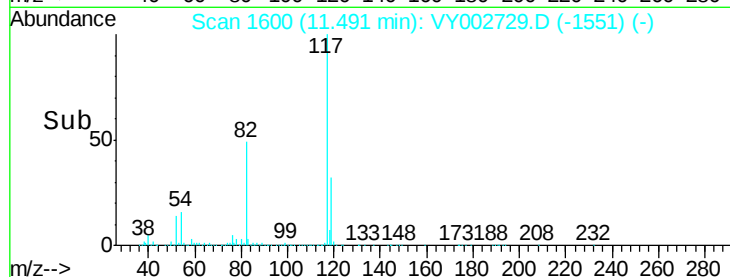

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.42 min Scan# 1917

Delta R.T. -0.00 min

Lab File: VY002729.D

Acq: 20 May 2020 14:57


Tgt Ion:152 Resp: 245843

Ion Ratio Lower Upper

152 100

115 53.7 27.2 81.6



150 156.2 0.0 343.8




Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

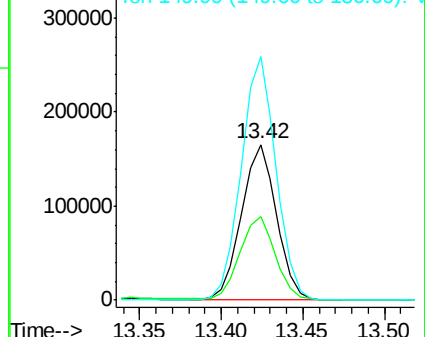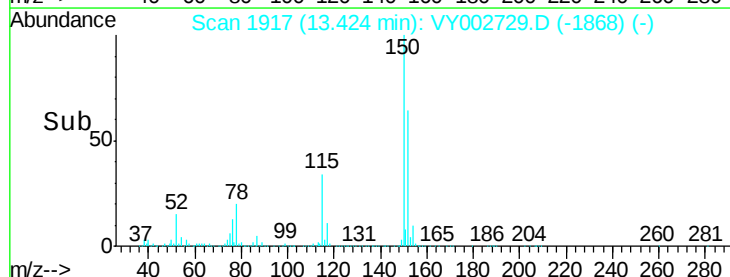

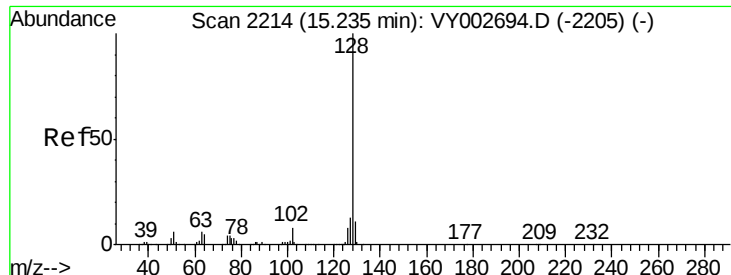

#95

Naphthalene

Concen: 1.602 ug/l

RT: 15.23 min Scan# 2214

Delta R.T. 0.00 min

Lab File: VY002729.D

Acq: 20 May 2020 14:57

Instrument :

MSVOA_Y

ClientSampleId :

72-12017


Tot Ion:128 Resp: 15326

Ion Ratio Lower Upper

128 100

127 18.9 10.3 15.5#

129 17.8 8.7 13.1#

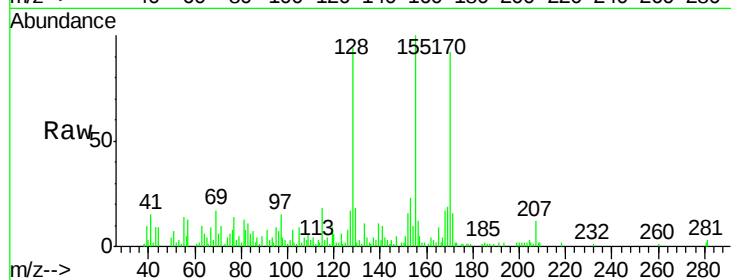

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

