

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052025\
 Data File : VY022338.D
 Acq On : 20 May 2025 13:25
 Operator : SY/MD
 Sample : Q2056-04
 Misc : 6.57g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 GVD14

Quant Time: May 21 01:48:01 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051525S.M
 Quant Title : SW846 8260
 QLast Update : Fri May 16 01:42:09 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	240752	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	423261	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	327850	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	112421	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	129742	49.309	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	98.620%
35) Dibromofluoromethane	7.634	113	127362	50.415	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.840%
50) Toluene-d8	10.103	98	509429	49.237	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	98.480%
62) 4-Bromofluorobenzene	12.408	95	121193	36.955	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	73.900%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052025\
Data File : VY022338.D
Acq On : 20 May 2025 13:25
Operator : SY/MD
Sample : Q2056-04
Misc : 6.57g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
GVD14

Quant Time: May 21 01:48:01 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051525S.M
Quant Title : SW846 8260
QLast Update : Fri May 16 01:42:09 2025
Response via : Initial Calibration




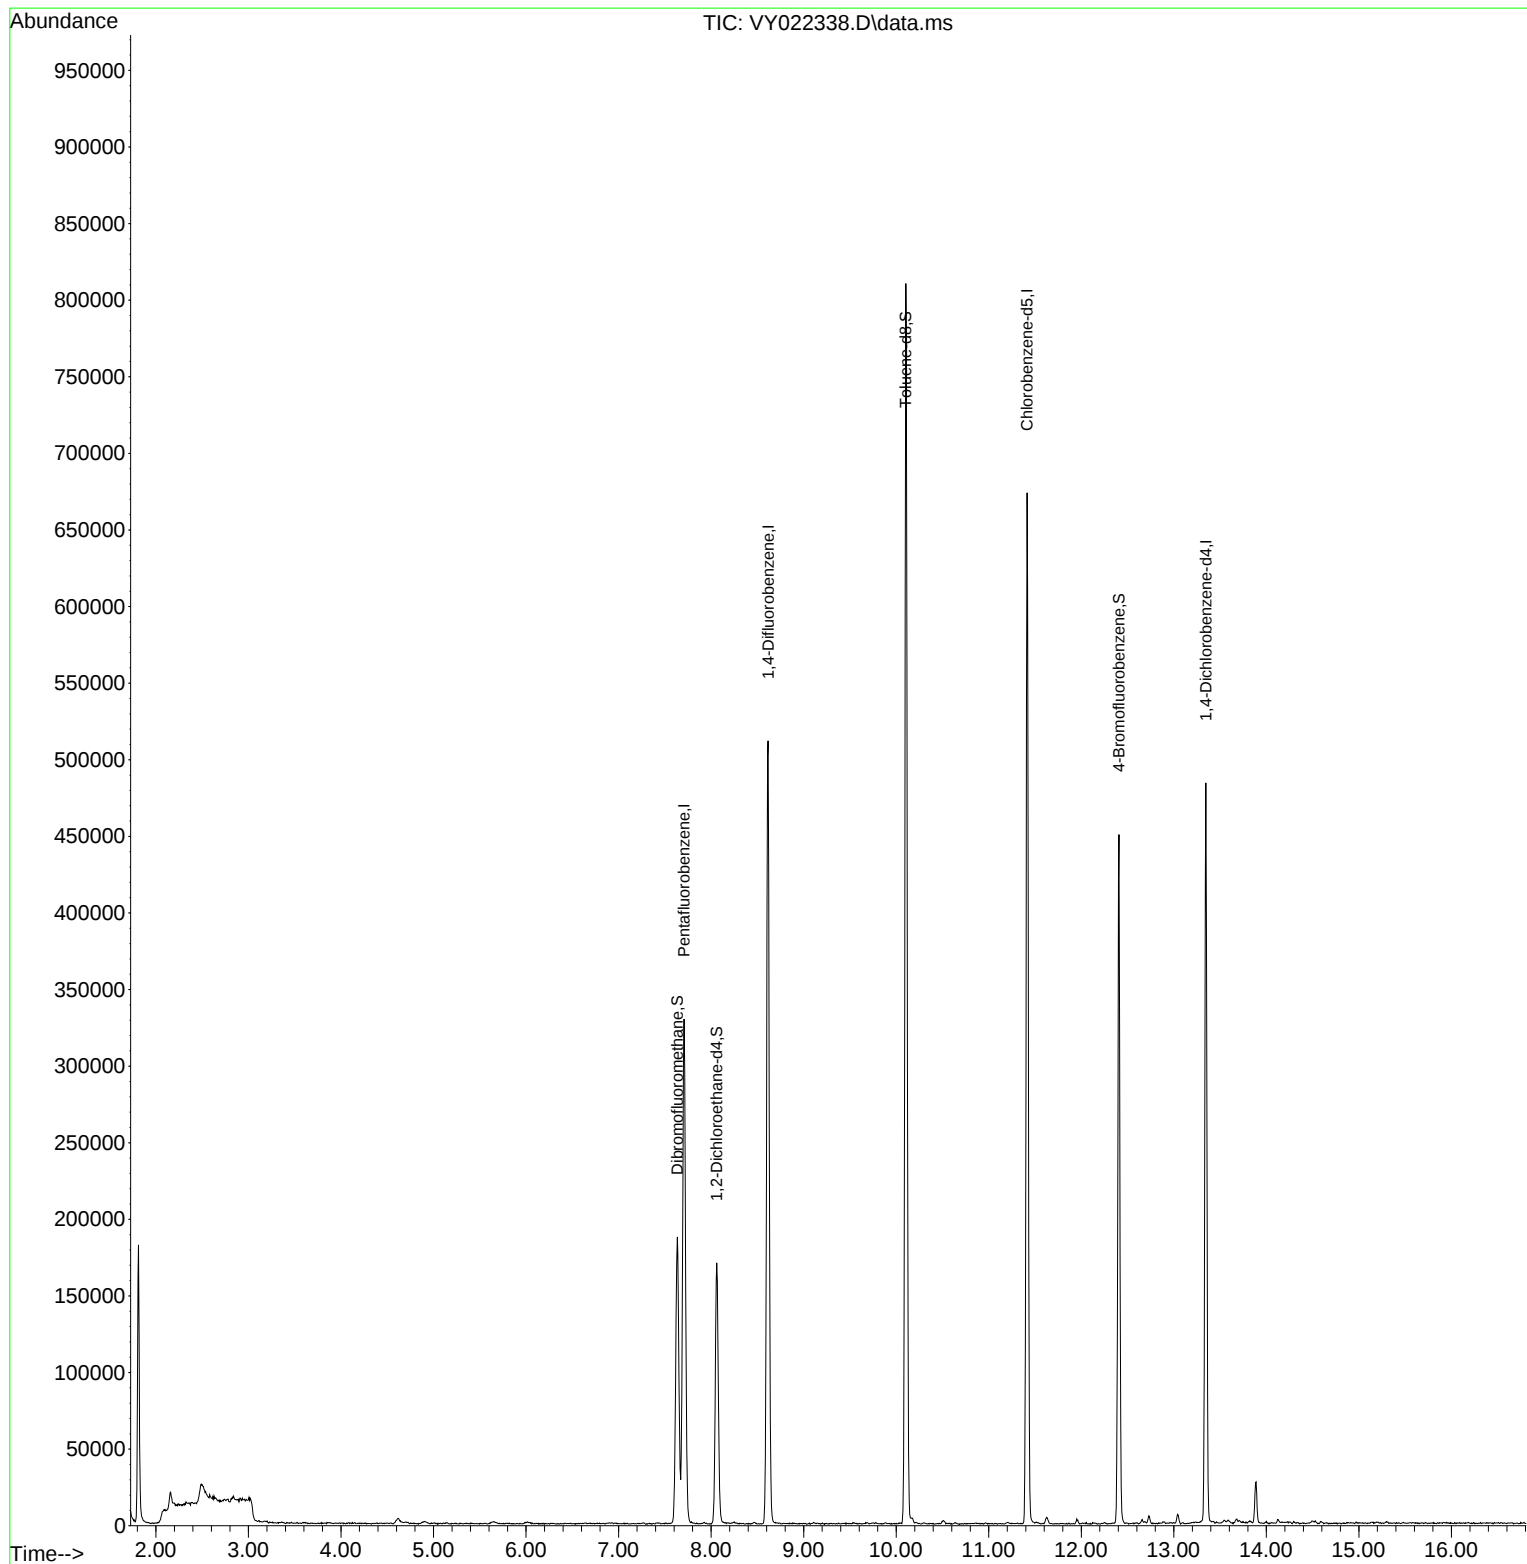


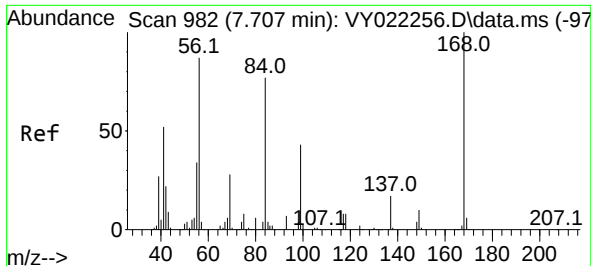

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 982
Delta R.T. 0.000 min
Lab File: VY022338.D
Acq: 20 May 2025 13:25




Instrument :
MSVOA_Y
ClientSampleId :
GVD14

Tgt Ion:168 Resp: 240752
Ion Ratio Lower Upper
168 100
99 55.1 44.2 66.4

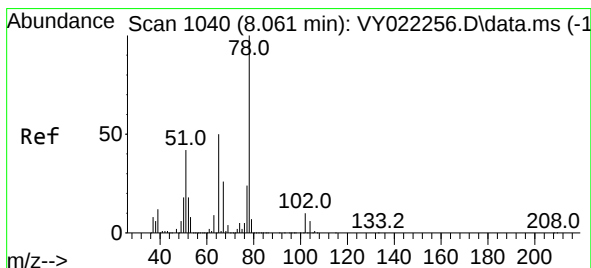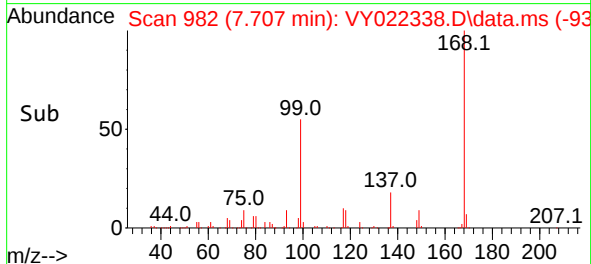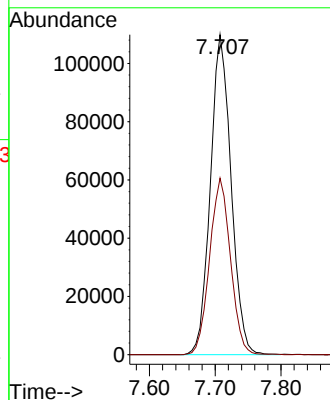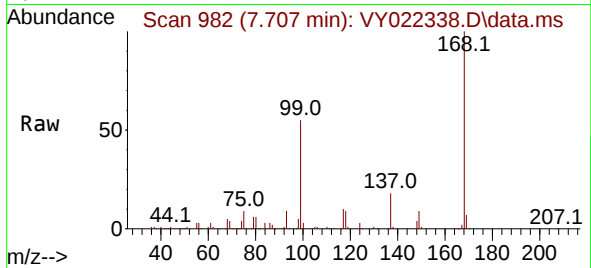

#33
1,2-Dichloroethane-d4
Concen: 49.309 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.000 min
Lab File: VY022338.D
Acq: 20 May 2025 13:25

Tgt Ion: 65 Resp: 129742
Ion Ratio Lower Upper
65 100
67 52.3 0.0 104.6


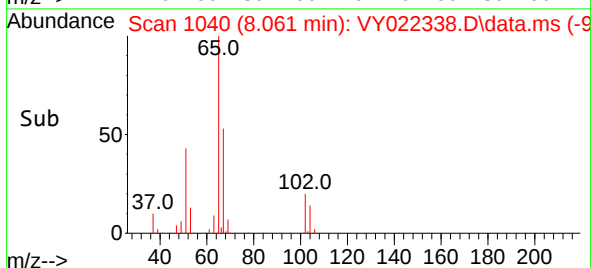
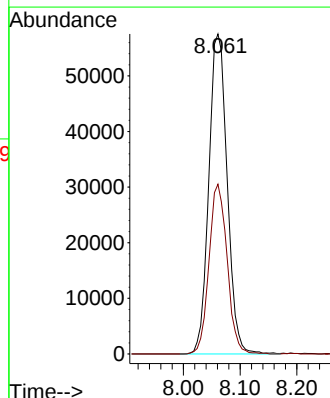
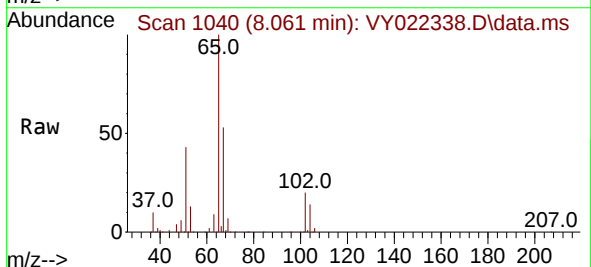




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. 0.000 min
Lab File: VY022338.D
Acq: 20 May 2025 13:25




Instrument :
MSVOA_Y
ClientSampleId :
GVD14

Tgt Ion:114 Resp: 423261
Ion Ratio Lower Upper
114 100
63 20.4 0.0 41.0
88 14.4 0.0 29.4

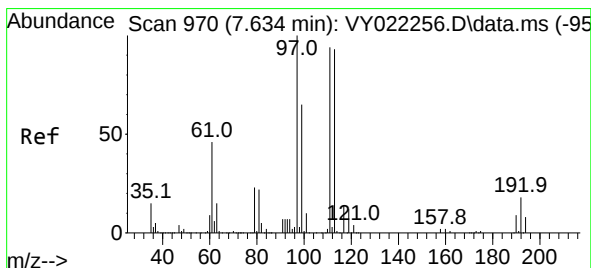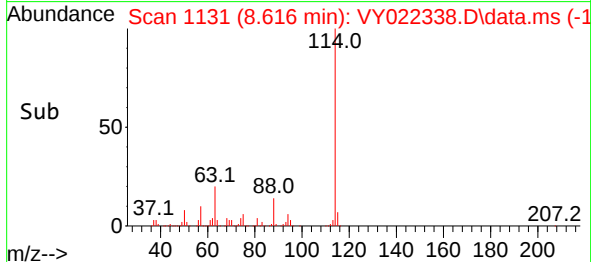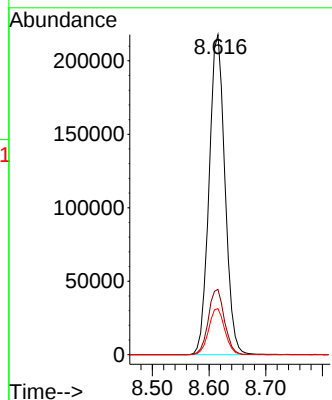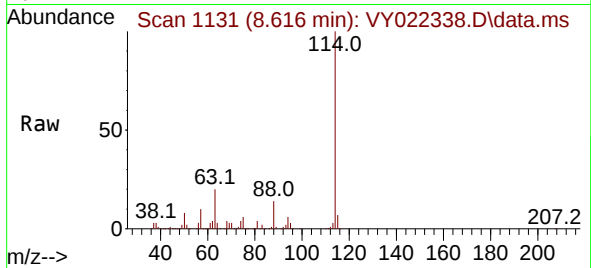

#35
Dibromofluoromethane
Concen: 50.415 ug/l
RT: 7.634 min Scan# 970
Delta R.T. 0.000 min
Lab File: VY022338.D
Acq: 20 May 2025 13:25

Tgt Ion:113 Resp: 127362
Ion Ratio Lower Upper
113 100
111 104.2 82.6 123.8
192 18.1 15.2 22.8

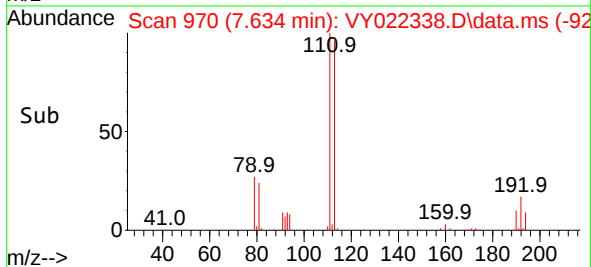
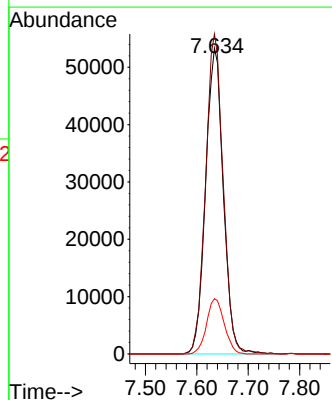
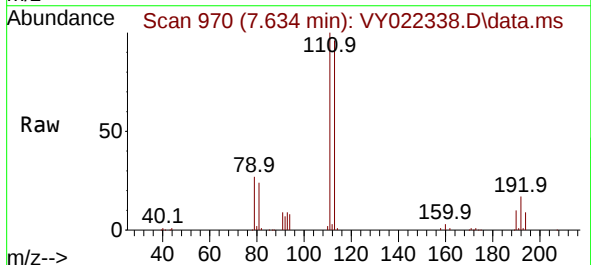




#50
Toluene-d8
Concen: 49.237 ug/l
RT: 10.103 min Scan# 1375
Delta R.T. 0.000 min
Lab File: VY022338.D
Acq: 20 May 2025 13:25




Instrument :
MSVOA_Y
ClientSampleId :
GVD14


Tgt Ion: 98 Resp: 509429
Ion Ratio Lower Upper
98 100
100 63.2 51.8 77.8

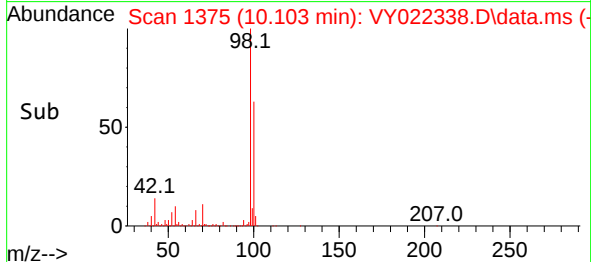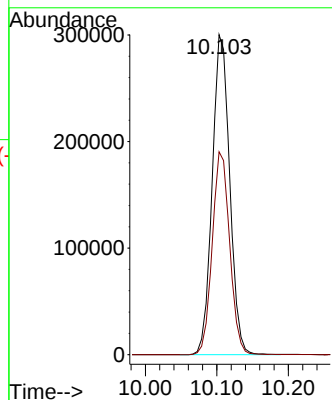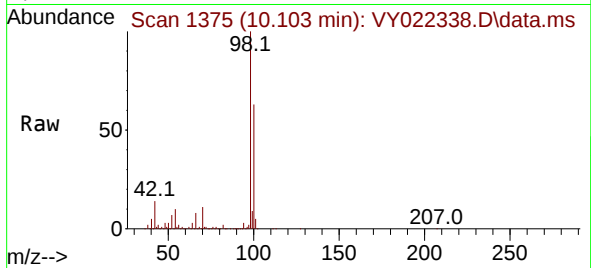

#62
4-Bromofluorobenzene
Concen: 36.955 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.000 min
Lab File: VY022338.D
Acq: 20 May 2025 13:25

Tgt Ion: 95 Resp: 121193
Ion Ratio Lower Upper
95 100
174 85.8 0.0 166.8
176 83.9 0.0 160.8


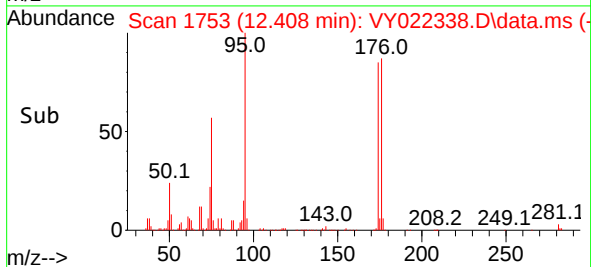
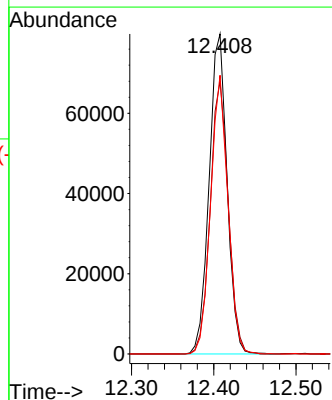
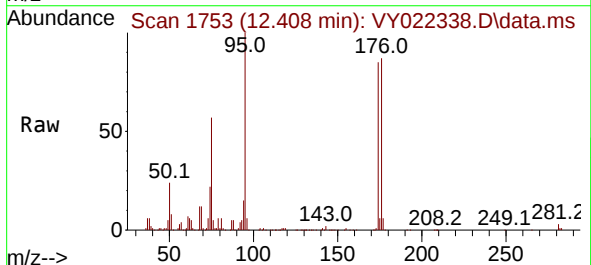


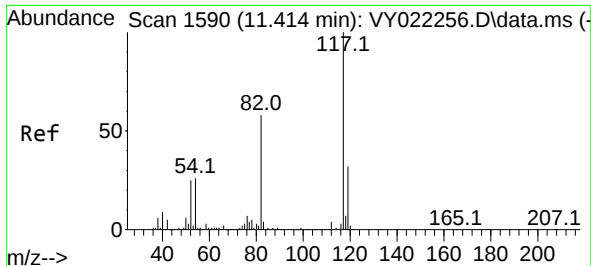

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 117
Delta R.T. 0.000 min
Lab File: VY022338.D
Acq: 20 May 2025 13:25

Instrument :
MSVOA_Y
ClientSampleId :
GVD14

Tgt Ion:117 Resp: 327850
Ion Ratio Lower Upper
117 100
82 57.8 46.6 70.0
119 32.4 25.8 38.6

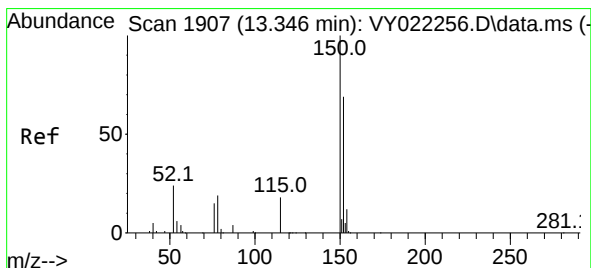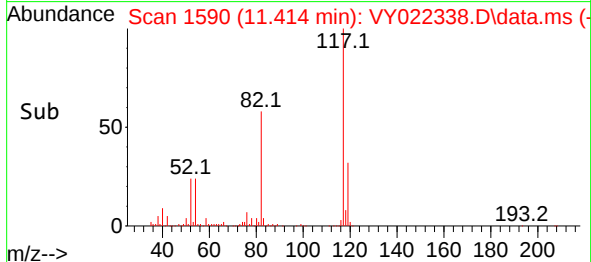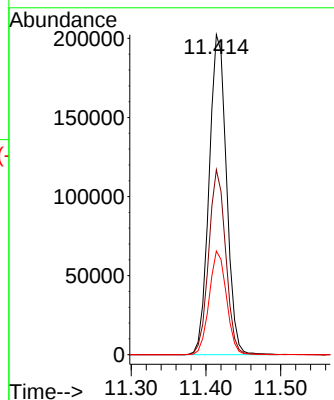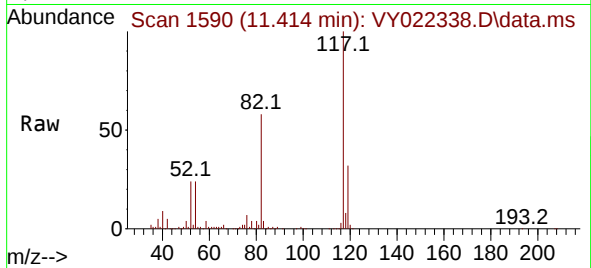

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.346 min Scan# 1907
Delta R.T. 0.000 min
Lab File: VY022338.D
Acq: 20 May 2025 13:25

Tgt Ion:152 Resp: 112421
Ion Ratio Lower Upper
152 100
115 57.5 29.4 88.2
150 153.2 0.0 353.8

